

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110922\
 Data File : VX032691.D
 Acq On : 09 Nov 2022 19:43
 Operator : JC/MD
 Sample : N5551-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EB-2022-11-08

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M

Title : SW846 8260

Signal : TIC: VX032691.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	25	30	44	rBV	13201	36664	6.13%	1.106%
2	2.946	297	305	318	rVB	15505	35617	5.95%	1.075%
3	4.562	561	570	585	rBV2	3795	13287	2.22%	0.401%
4	5.391	694	706	719	rBV	70089	206636	34.53%	6.234%
5	5.556	722	733	748	rVB	115086	330424	55.22%	9.969%
6	5.958	789	799	812	rBV	77296	207348	34.65%	6.256%
7	6.763	920	931	944	rBV	182379	432800	72.32%	13.058%
8	8.647	1234	1240	1256	rBV	378412	598416	100.00%	18.054%
9	10.055	1465	1471	1480	rBV	398200	514295	85.94%	15.516%
10	10.195	1490	1494	1502	rVB	4733	6228	1.04%	0.188%
11	11.079	1634	1639	1650	rBV	348887	444470	74.27%	13.410%
12	12.024	1788	1794	1803	rBV	389107	488336	81.60%	14.733%




Sum of corrected areas: 3314521

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110922\
Data File : VX032691.D
Acq On : 09 Nov 2022 19:43
Operator : JC/MD
Sample : N5551-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2022-11-08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

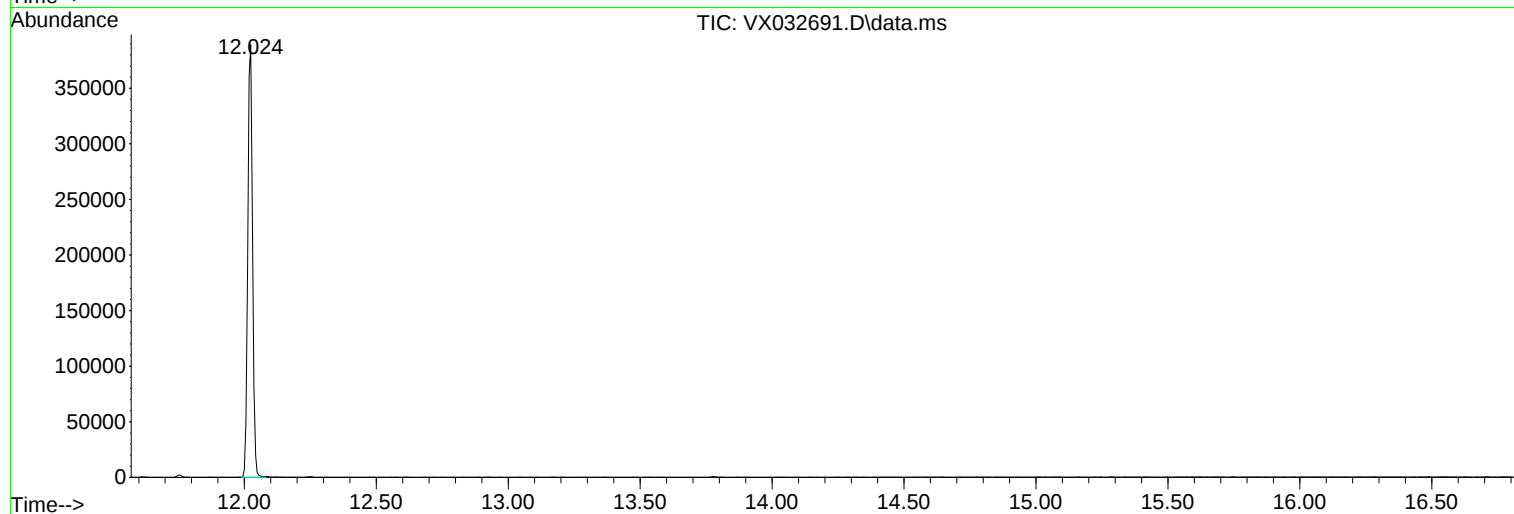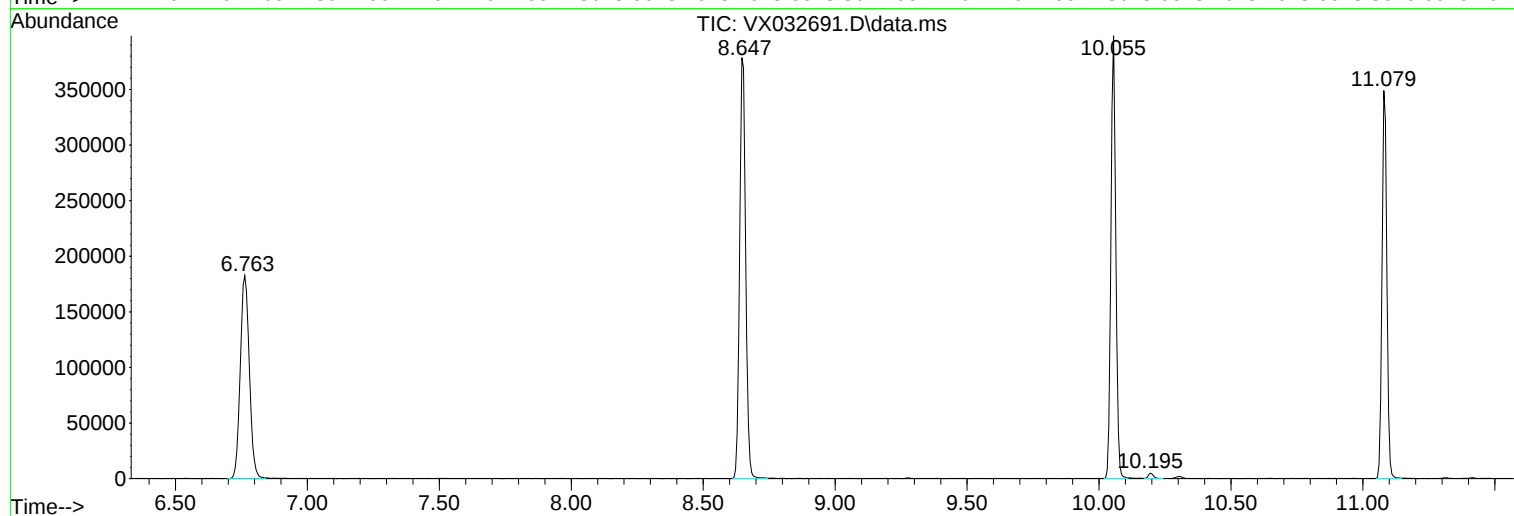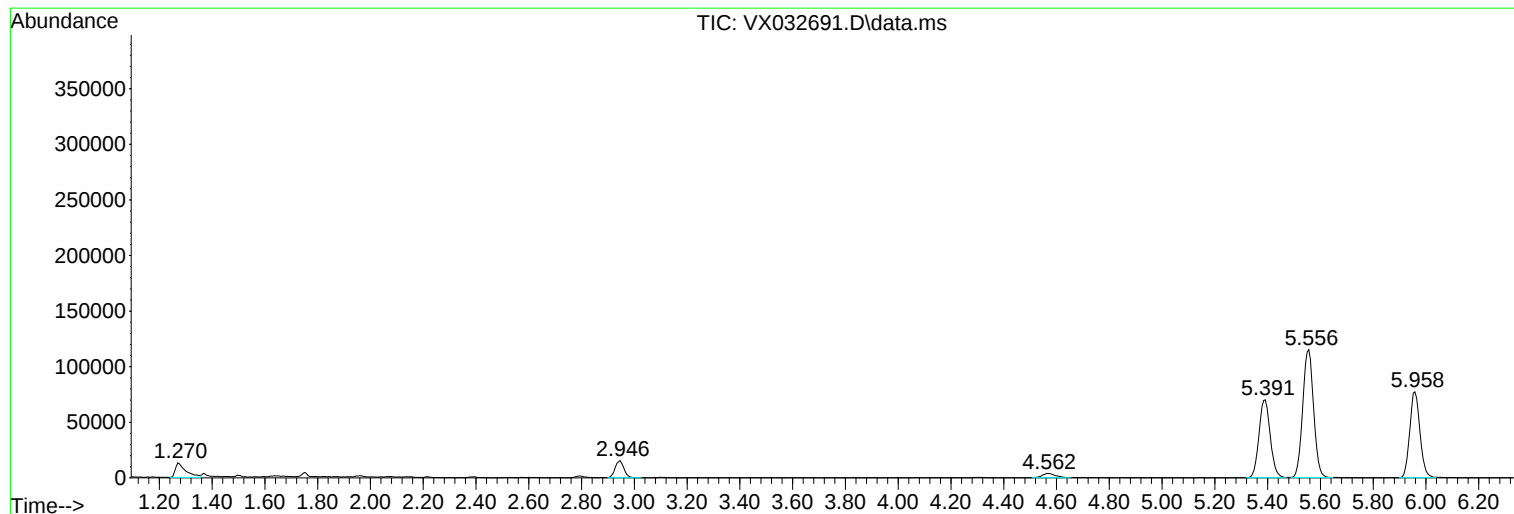

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110922\
Data File : VX032691.D
Acq On : 09 Nov 2022 19:43
Operator : JC/MD
Sample : N5551-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2022-11-08









Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.270	5.55 ug/l	36664	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	90
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
4			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	4
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	3

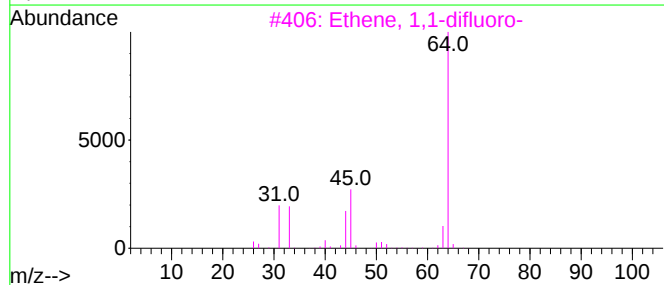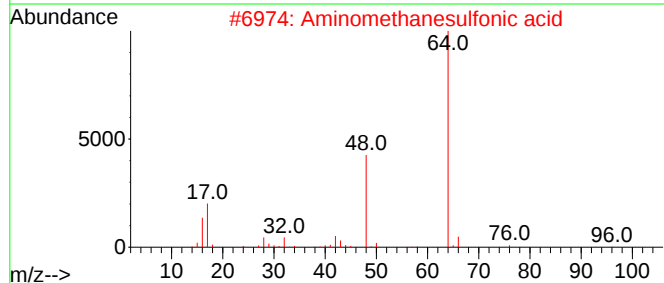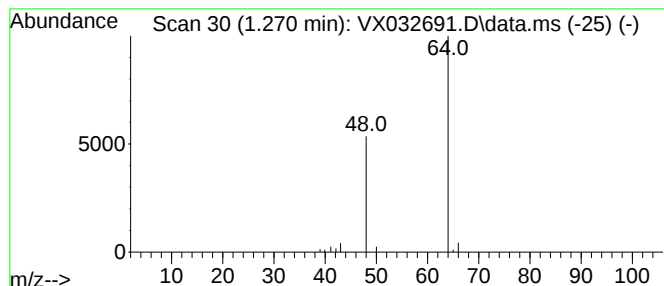

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110922\
Data File : VX032691.D
Acq On : 09 Nov 2022 19:43
Operator : JC/MD
Sample : N5551-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2022-11-08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.270	5.5	ug/l	36664	1	5.556	330424	50.0