



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110922\
Data File : VX032668.D
Acq On : 09 Nov 2022 10:10
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Title : SW846 8260
Last Update : Thu Oct 27 08:28:06 2022

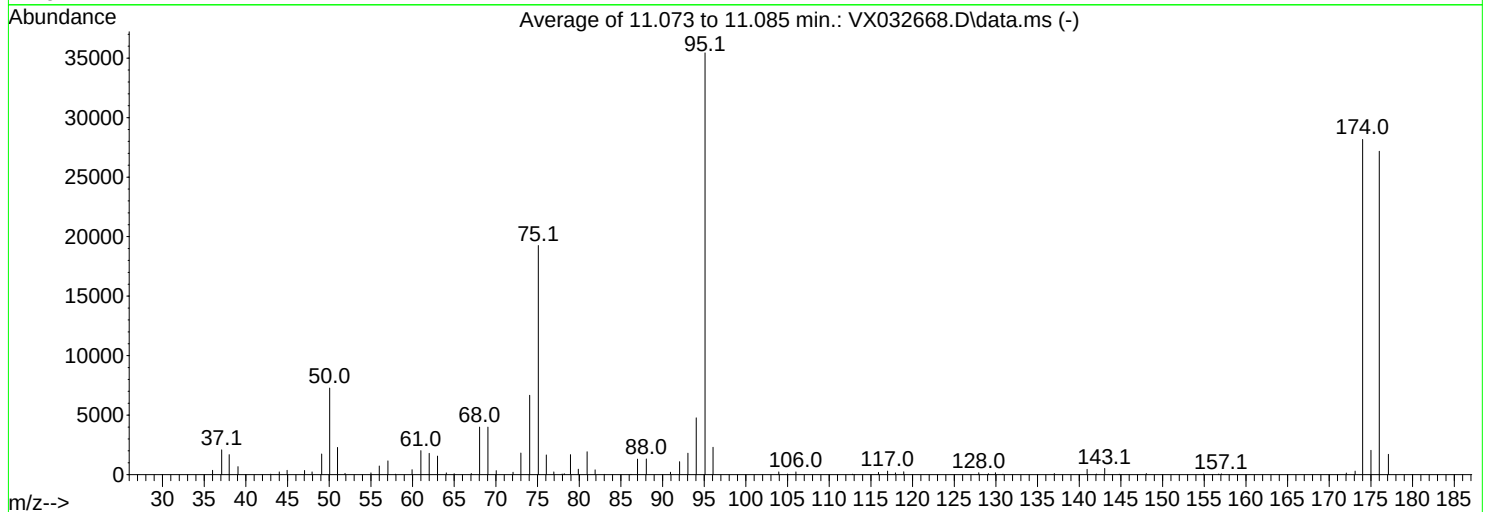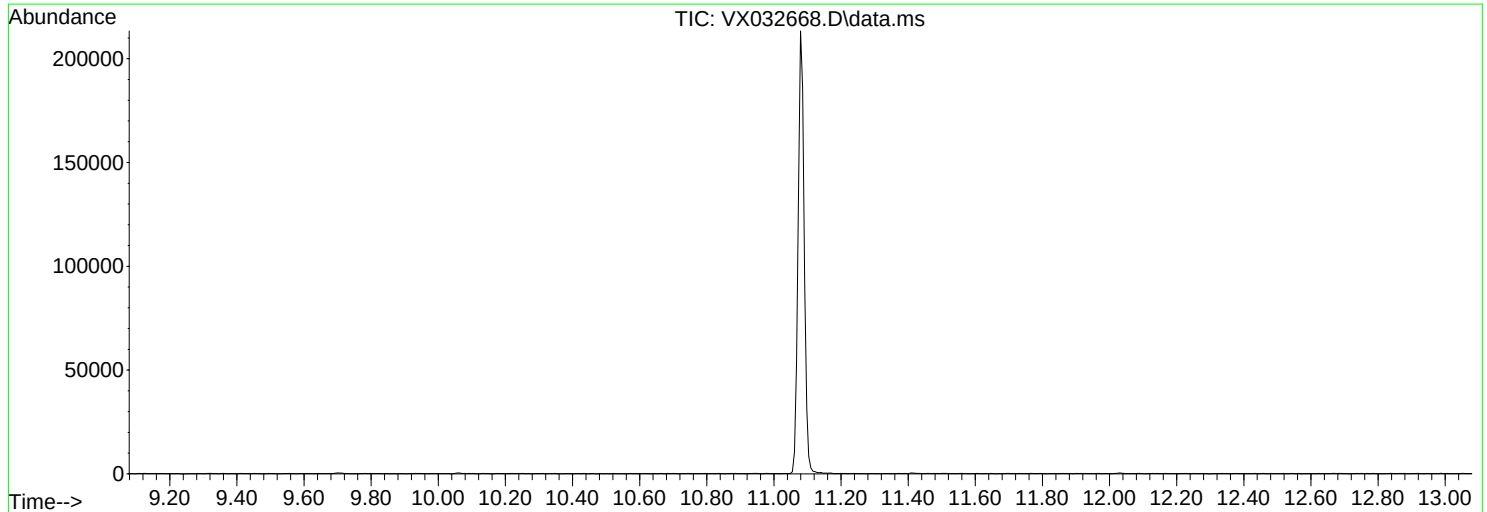

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	7277	PASS
75	95	30	60	54.3	19260	PASS
95	95	100	100	100.0	35445	PASS
96	95	5	9	6.5	2303	PASS
173	174	0.00	2	1.1	296	PASS
174	95	50	100	79.5	28173	PASS
175	174	5	9	7.3	2049	PASS
176	174	95	101	96.5	27179	PASS
177	176	5	9	6.3	1715	PASS