

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110923\
 Data File : VX038710.D
 Acq On : 10 Nov 2023 07:21
 Operator : JC/MD
 Sample : 05331-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-06

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M
 Title : SW846 8260

Signal : TIC: VX038710.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.782	269	278	284	rBV2	11894	27403	1.84%	0.299%
2	3.111	324	332	344	rVB3	8720	21068	1.41%	0.230%
3	4.215	502	513	521	rBV3	8628	25912	1.74%	0.283%
4	4.574	561	572	582	rBV2	4575	16427	1.10%	0.179%
5	5.385	693	705	721	rBV2	169478	501757	33.64%	5.478%
6	5.556	722	733	762	rVB	258545	842484	56.48%	9.198%
7	5.958	787	799	810	rBV	160255	426743	28.61%	4.659%
8	6.251	826	847	857	rBV	53273	170011	11.40%	1.856%
9	6.763	921	931	951	rBV	410595	996459	66.80%	10.879%
10	7.129	985	991	1004	rVB3	6000	15096	1.01%	0.165%
11	7.982	1122	1131	1142	rBV	42614	82924	5.56%	0.905%
12	8.104	1142	1151	1162	rBV	59105	121506	8.15%	1.327%
13	8.647	1228	1240	1250	rBV	866876	1377102	92.32%	15.035%
14	10.055	1465	1471	1485	rBV	945409	1325876	88.89%	14.476%
15	10.964	1615	1620	1626	rBV	35913	45766	3.07%	0.500%
16	11.079	1634	1639	1653	rBV	852605	1107691	74.26%	12.094%
17	11.305	1667	1676	1684	rBV	52813	70218	4.71%	0.767%
18	12.024	1788	1794	1802	rBV	1116698	1491635	100.00%	16.286%
19	12.244	1824	1830	1837	rBV2	132222	168899	11.32%	1.844%
20	12.317	1837	1842	1850	rVB2	14740	23106	1.55%	0.252%
21	12.610	1885	1890	1894	rBV	21920	28241	1.89%	0.308%
22	12.701	1899	1905	1912	rVB	49011	71104	4.77%	0.776%
23	12.921	1933	1941	1947	rBV	13241	20185	1.35%	0.220%
24	13.292	1997	2002	2007	rVB3	14112	18874	1.27%	0.206%
25	13.774	2074	2081	2090	rBV	69061	91524	6.14%	0.999%
26	14.780	2242	2246	2254	rVB2	13323	19548	1.31%	0.213%
27	16.322	2493	2499	2509	rVB	28410	51639	3.46%	0.564%




Sum of corrected areas: 9159198

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110923\
Data File : VX038710.D
Acq On : 10 Nov 2023 07:21
Operator : JC/MD
Sample : 05331-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

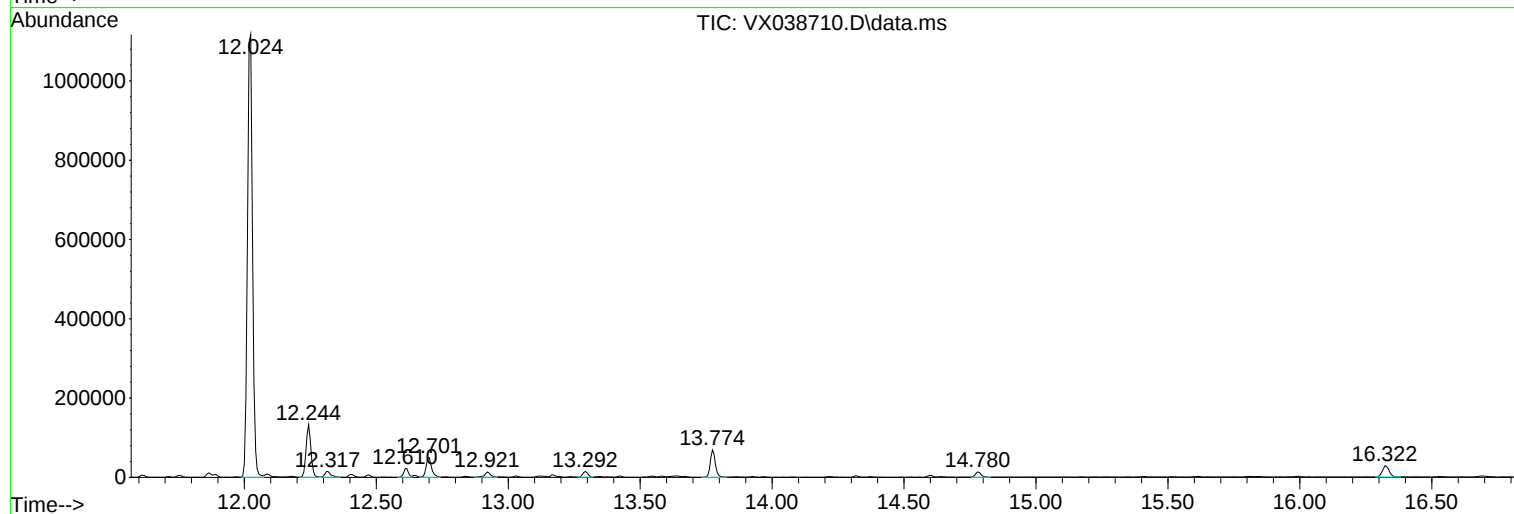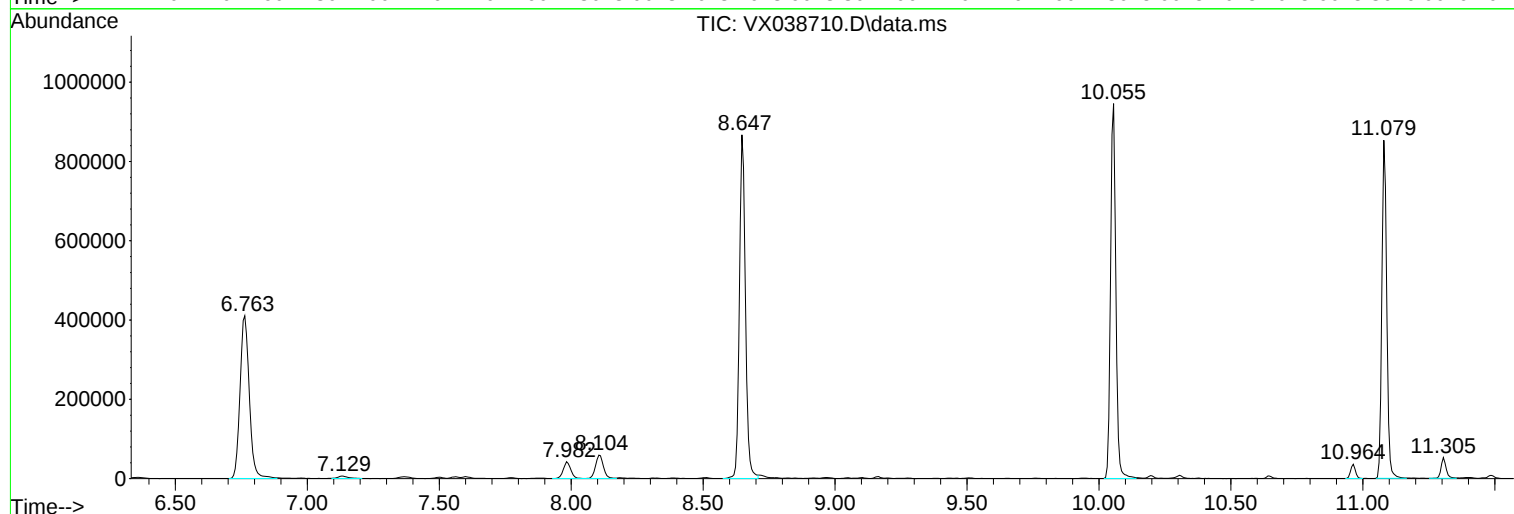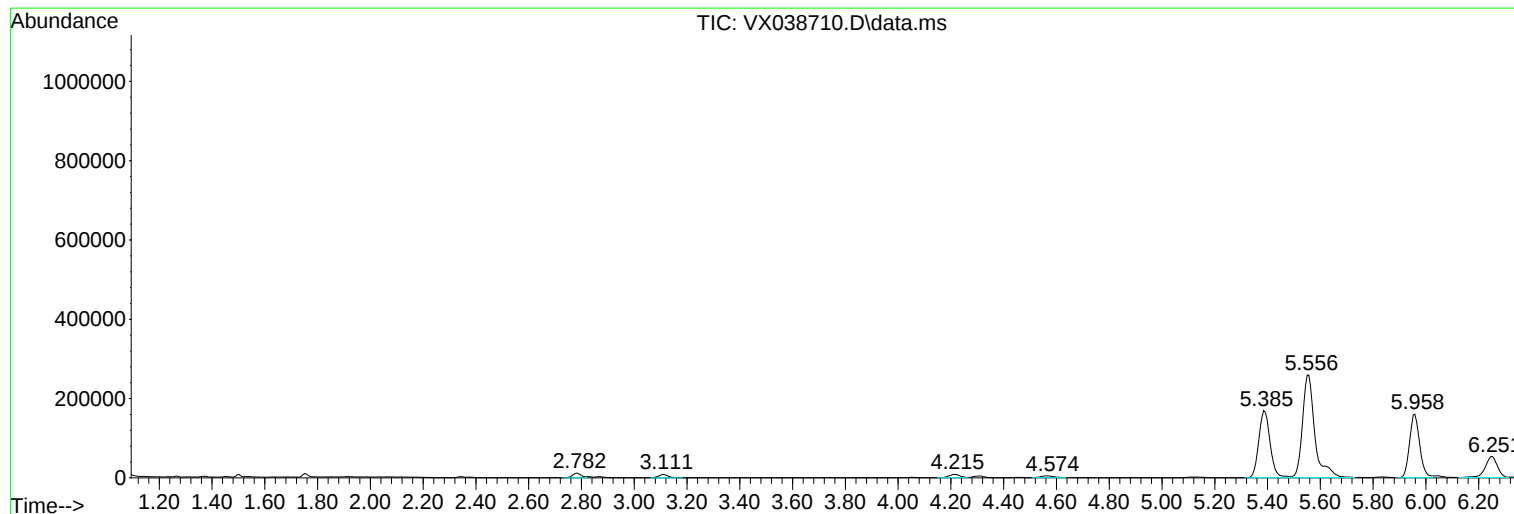

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110923\
Data File : VX038710.D
Acq On : 10 Nov 2023 07:21
Operator : JC/MD
Sample : 05331-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110923\
Data File : VX038710.D
Acq On : 10 Nov 2023 07:21
Operator : JC/MD
Sample : 05331-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------