

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111022\
 Data File : VX032733.D
 Acq On : 10 Nov 2022 17:04
 Operator : JC/MD
 Sample : N5500-01RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 NWB-1851RE

Quant Time: Nov 11 00:37:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 27 08:28:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	66904	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	74761	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	40934	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	17213	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	12821	13.792	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	27.580%#
35) Dibromofluoromethane	5.397	113	13721	25.730	ug/l	0.01
Spiked Amount	50.000	Range	75 - 124	Recovery	=	51.460%#
50) Toluene-d8	8.653	98	83428	44.991	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	89.980%#
62) 4-Bromofluorobenzene	11.079	95	18678	25.786	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	51.580%#
Target Compounds						
					Qvalue	
6) Chloroethane	1.496	64	3305	6.860	ug/l #	42
11) Tert butyl alcohol	2.959	59	134	0.990	ug/l #	72
14) Allyl chloride	2.782	41	771	0.721	ug/l #	61
16) Acetone	2.380	43	29131	86.219	ug/l	98
17) Carbon Disulfide	2.514	76	4070	2.547	ug/l	96
18) Methyl Acetate	2.715	43	260	0.237	ug/l #	51
23) Vinyl Acetate	3.459	43	1491	0.798	ug/l #	67
25) 2-Butanone	4.568	43	14034	26.810	ug/l	98
29) Tetrahydrofuran	5.019	42	375	1.123	ug/l #	70
30) Chloroform	5.184	83	387	0.265	ug/l #	18
36) 1,1-Dichloropropene	5.562	75	5105	6.874	ug/l #	51
37) Ethyl Acetate	4.568	43	14034	18.155	ug/l #	67
38) Carbon Tetrachloride	5.562	117	7006	8.506	ug/l #	16
39) Methylcyclohexane	7.391	83	1926	2.192	ug/l	94
41) Methacrylonitrile	5.032	41	462	1.173	ug/l #	33
48) Methyl methacrylate	7.665	41	360	0.587	ug/l #	77
51) 4-Methyl-2-Pentanone	8.580	43	1088	1.455	ug/l	90
52) Toluene	8.720	92	34677	25.292	ug/l	95
53) t-1,3-Dichloropropene	8.720	75	482	0.602	ug/l #	1
55) 1,1,2-Trichloroethane	9.104	97	391	0.677	ug/l #	15
59) 2-Hexanone	9.439	43	2758	4.972	ug/l	94
67) Ethyl Benzene	10.195	91	30903	18.847	ug/l	98
68) m/p-Xylenes	10.305	106	54460	85.533	ug/l	99
69) o-Xylene	10.646	106	18838	30.430	ug/l	99
70) Styrene	10.646	104	1290	1.254	ug/l #	1
73) Isopropylbenzene	10.964	105	9421	6.907	ug/l	99
74) N-amyl acetate	10.848	43	134	0.260	ug/l #	1
76) 1,2,3-Trichloropropane	11.384	75	941	2.457	ug/l #	1
78) n-propylbenzene	11.305	91	29809	18.968	ug/l	99
79) 2-Chlorotoluene	11.378	91	12287	13.055	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.451	105	37624	32.275	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.079	75	10020	83.259	ug/l #	6
82) 4-Chlorotoluene	11.451	91	4285	3.891	ug/l #	45
83) tert-Butylbenzene	11.969	119	5347	4.594	ug/l	73
84) 1,2,4-Trimethylbenzene	11.756	105	135955	117.258	ug/l	100
85) sec-Butylbenzene	11.890	105	4251	3.036	ug/l	94

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111022\
 Data File : VX032733.D
 Acq On : 10 Nov 2022 17:04
 Operator : JC/MD
 Sample : N5500-01RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 NWB-1851RE

Quant Time: Nov 11 00:37:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 27 08:28:06 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
86) p-Isopropyltoluene	12.012	119	6705	5.642	ug/l	98
89) n-Butylbenzene	12.335	91	13138	12.709	ug/l #	40
90) Hexachloroethane	12.530	117	1537	7.919	ug/l #	12
92) 1,2-Dibromo-3-Chloropr...	12.963	75	153	1.594	ug/l #	1
95) Naphthalene	13.774	128	20370	15.074	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111022\
Data File : VX032733.D
Acq On : 10 Nov 2022 17:04
Operator : JC/MD
Sample : N5500-01RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
NWB-1851RE

Quant Time: Nov 11 00:37:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 27 08:28:06 2022
Response via : Initial Calibration




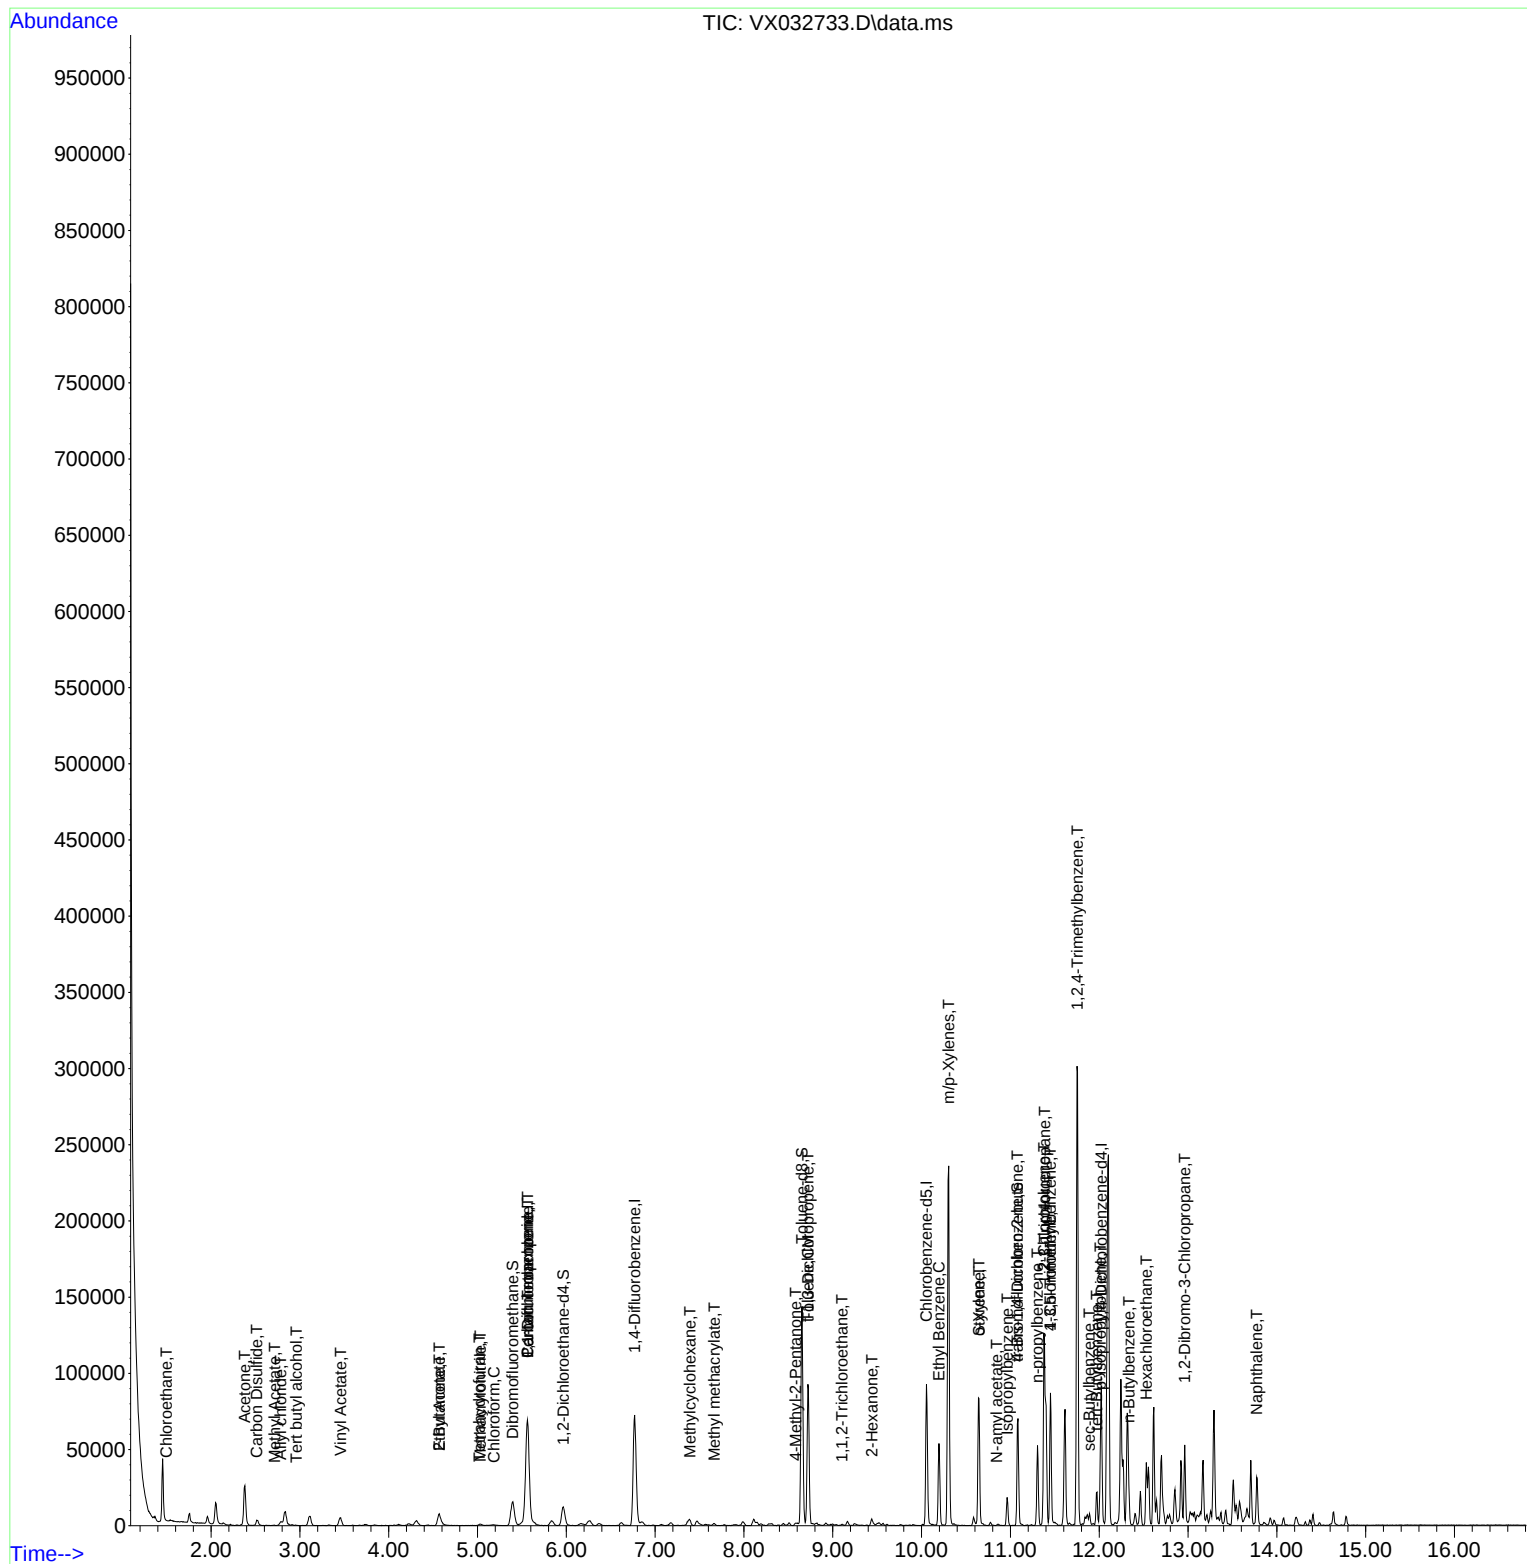


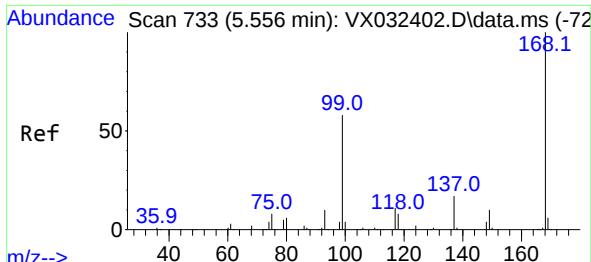

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04




Instrument :
MSVOA_X
ClientSampleId :
NWB-1851RE


Tgt Ion:168 Resp: 66904
Ion Ratio Lower Upper
168 100
99 59.6 46.1 69.1

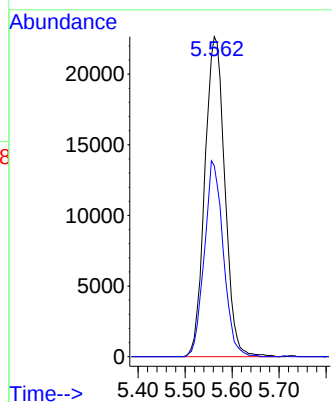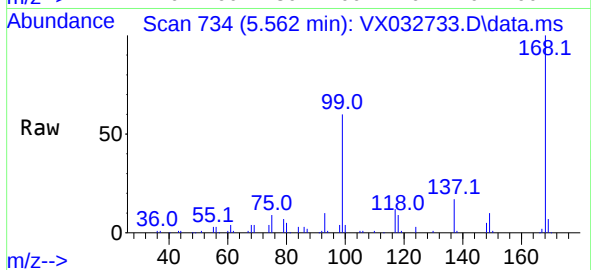

#6
Chloroethane
Concen: 6.860 ug/l
RT: 1.496 min Scan# 67
Delta R.T. -0.189 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Tgt Ion: 64 Resp: 3305
Ion Ratio Lower Upper
64 100
66 0.0 26.0 39.0#

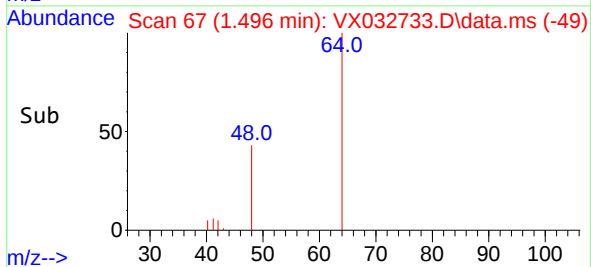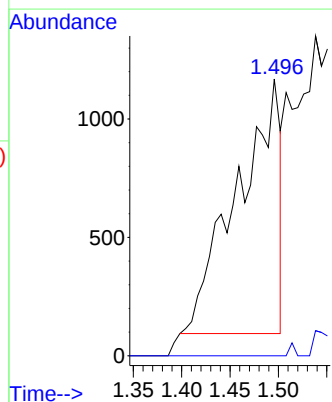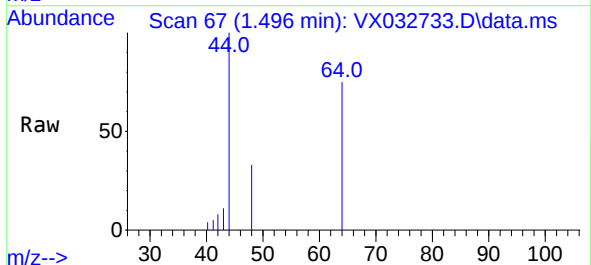

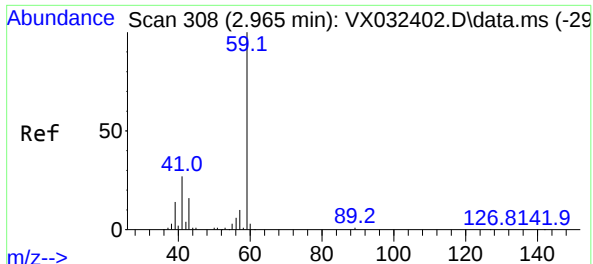

#11

Tert butyl alcohol

Concen: 0.990 ug/l

RT: 2.959 min Scan# 308

Delta R.T. -0.006 min

Lab File: VX032733.D

Acq: 10 Nov 2022 17:04

Instrument :

MSVOA_X

ClientSampleId :





NWB-1851RE

Tgt Ion: 59 Resp: 134

Ion Ratio Lower Upper

59 100

57 0.0 8.2 12.4#

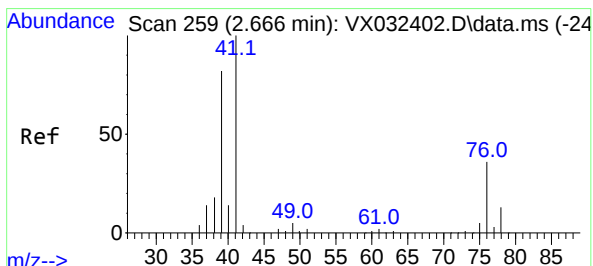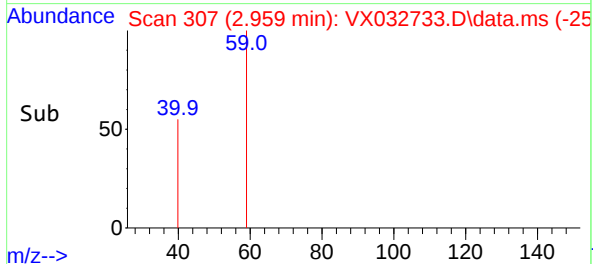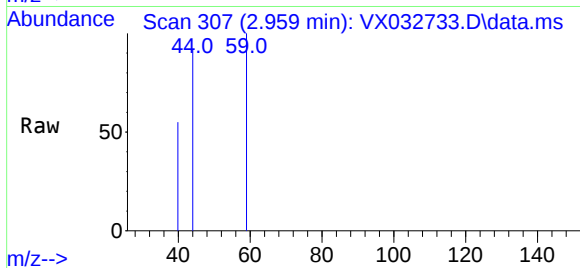

#14

Allyl chloride

Concen: 0.721 ug/l

RT: 2.782 min Scan# 278

Delta R.T. 0.116 min

Lab File: VX032733.D

Acq: 10 Nov 2022 17:04




Tgt Ion: 41 Resp: 771


Ion Ratio Lower Upper

41 100

39 52.1 61.4 92.2#

76 0.0 29.2 43.8#


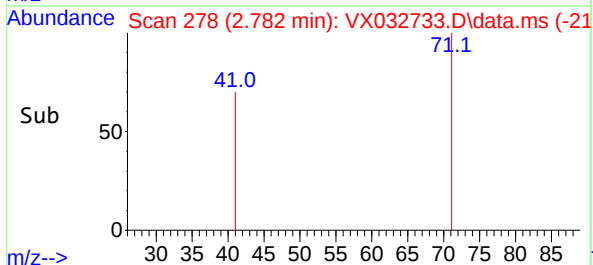
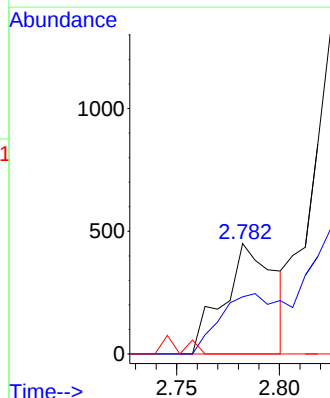
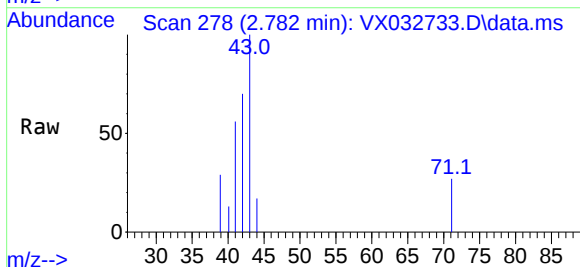




#16
Acetone
Concen: 86.219 ug/l
RT: 2.380 min Scan# 212
Delta R.T. 0.000 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04




Instrument :
MSVOA_X
ClientSampleId :
NWB-1851RE


Tgt Ion: 43 Resp: 29131
Ion Ratio Lower Upper
43 100
58 28.6 23.8 35.8



#17
Carbon Disulfide
Concen: 2.547 ug/l
RT: 2.514 min Scan# 234
Delta R.T. 0.000 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Tgt Ion: 76 Resp: 4070
Ion Ratio Lower Upper
76 100
78 10.7 7.5 11.3



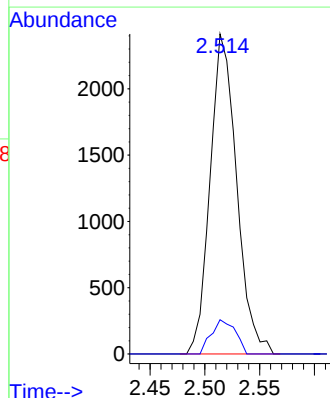





#18
Methyl Acetate
Concen: 0.237 ug/l
RT: 2.715 min Scan# 21
Delta R.T. 0.012 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04




Instrument :
MSVOA_X
ClientSampleId :
NWB-1851RE


Tgt Ion: 43 Resp: 260
Ion Ratio Lower Upper
43 100
74 0.0 19.4 29.0#



#23
Vinyl Acetate
Concen: 0.798 ug/l
RT: 3.459 min Scan# 389
Delta R.T. -0.262 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Tgt Ion: 43 Resp: 1491
Ion Ratio Lower Upper
43 100
86 23.2 8.6 12.8#


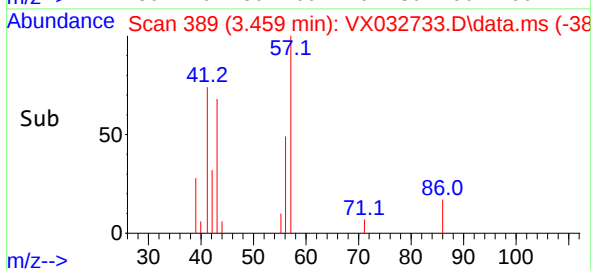






#25
2-Butanone
Concen: 26.810 ug/l
RT: 4.568 min Scan# 51
Delta R.T. 0.012 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04




Instrument :
MSVOA_X
ClientSampleId :
NWB-1851RE


Tgt Ion: 43 Resp: 14034
Ion Ratio Lower Upper
43 100
72 28.5 22.2 33.2



#29
Tetrahydrofuran
Concen: 1.123 ug/l
RT: 5.019 min Scan# 645
Delta R.T. 0.018 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Tgt Ion: 42 Resp: 375
Ion Ratio Lower Upper
42 100
72 68.5 37.6 56.4#
71 60.8 34.7 52.1#

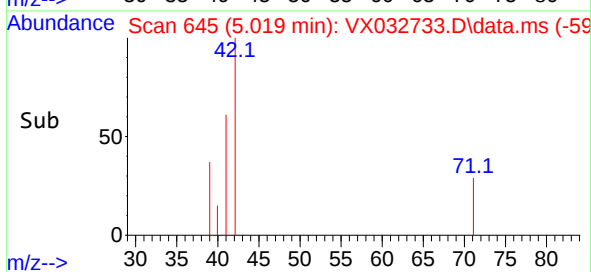

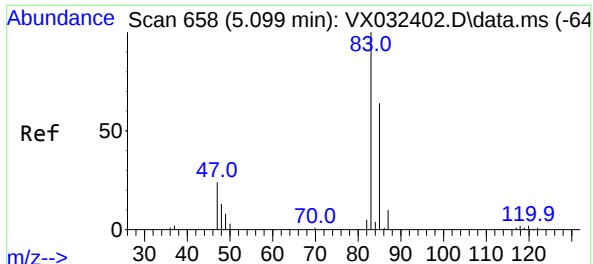

#30

Chloroform

Concen: 0.265 ug/l

RT: 5.184 min Scan# 61

Delta R.T. 0.085 min

Lab File: VX032733.D

Acq: 10 Nov 2022 17:04

Instrument :

MSVOA_X

ClientSampleId :





NWB-1851RE

Tgt Ion: 83 Resp: 387

Ion Ratio Lower Upper

83 100

85 0.0 51.1 76.7#

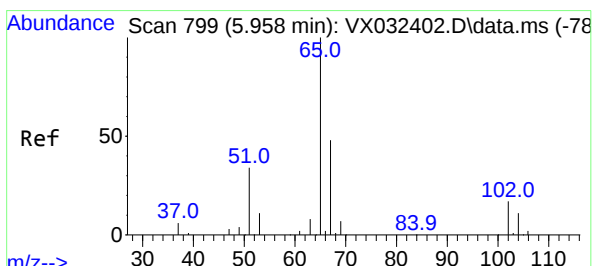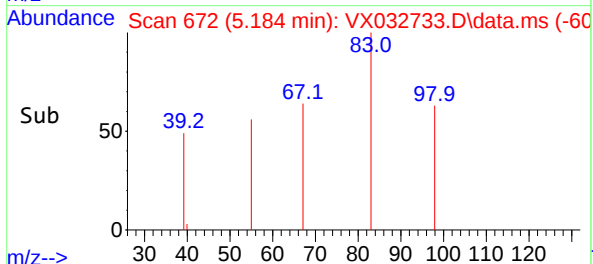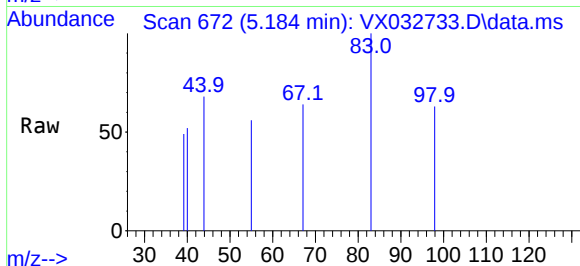

#33

1,2-Dichloroethane-d4

Concen: 13.792 ug/l

RT: 5.964 min Scan# 800

Delta R.T. 0.006 min

Lab File: VX032733.D




Acq: 10 Nov 2022 17:04


Tgt Ion: 65 Resp: 12821

Ion Ratio Lower Upper

65 100

67 50.8 0.0 101.8


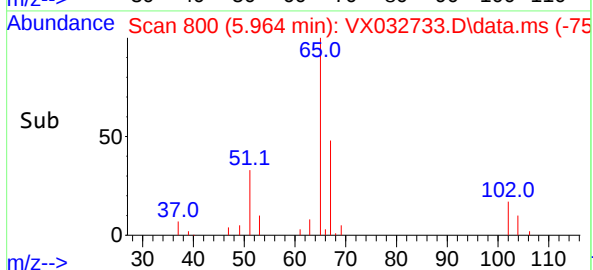

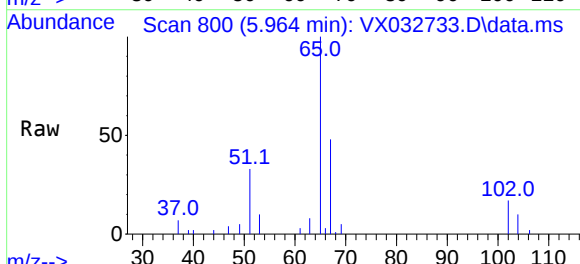




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 911
Delta R.T. 0.006 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04




Instrument :
MSVOA_X
ClientSampleId :
NWB-1851RE


Tgt Ion:114 Resp: 74761
Ion Ratio Lower Upper
114 100
63 20.3 0.0 41.6
88 15.5 0.0 33.4

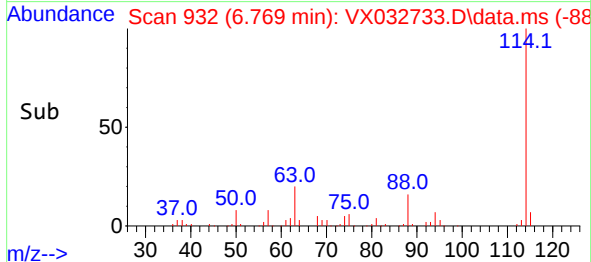

#35
Dibromofluoromethane
Concen: 25.730 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.012 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Tgt Ion:113 Resp: 13721
Ion Ratio Lower Upper
113 100
111 102.4 82.4 123.6
192 19.8 15.4 23.2


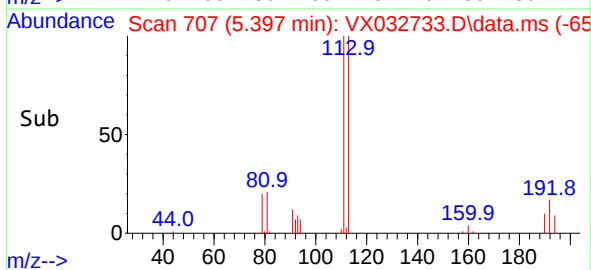






#36
1,1-Dichloropropene
Concen: 6.874 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.134 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04




Instrument :
MSVOA_X
ClientSampleId :
NWB-1851RE


Tgt Ion: 75 Resp: 5105
Ion Ratio Lower Upper
75 100
110 10.8 18.4 55.2#
77 0.0 24.5 36.7#



#37
Ethyl Acetate
Concen: 18.155 ug/l
RT: 4.568 min Scan# 571
Delta R.T. -0.146 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04


Tgt Ion: 43 Resp: 14034
Ion Ratio Lower Upper
43 100
61 0.0 11.5 17.3#
70 0.0 9.1 13.7#

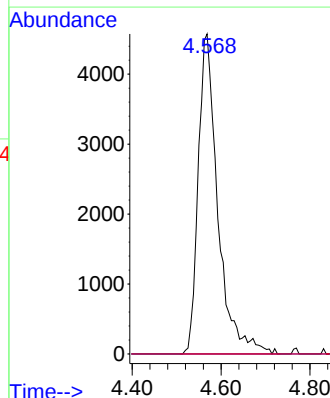



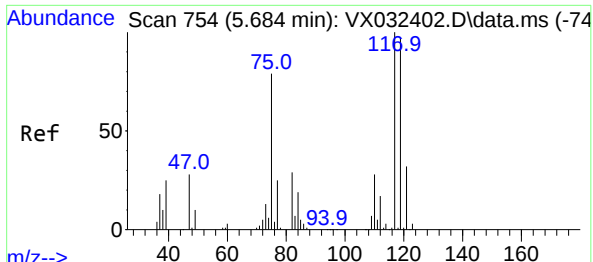


#38
Carbon Tetrachloride
Concen: 8.506 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.122 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Instrument :
MSVOA_X
ClientSampleId :
NWB-1851RE



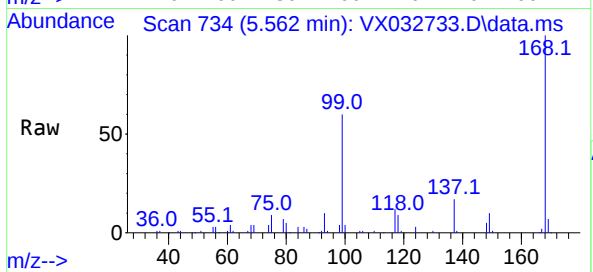



Tgt Ion:117 Resp: 7006
Ion Ratio Lower Upper
117 100
119 5.6 77.2 115.8#
121 0.0 25.8 38.6#

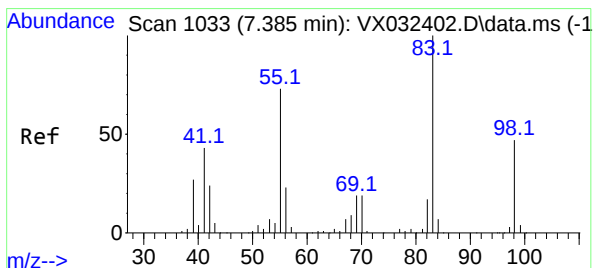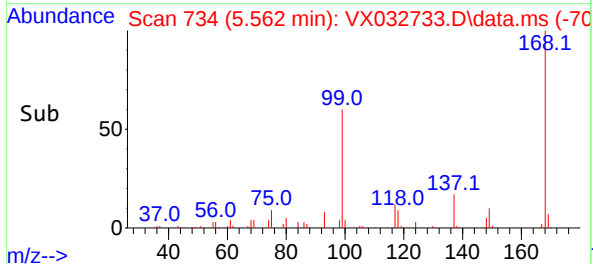

#39
Methylcyclohexane
Concen: 2.192 ug/l
RT: 7.391 min Scan# 1034
Delta R.T. 0.006 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Tgt Ion: 83 Resp: 1926
Ion Ratio Lower Upper
83 100
55 67.2 58.4 87.6
98 49.1 37.2 55.8

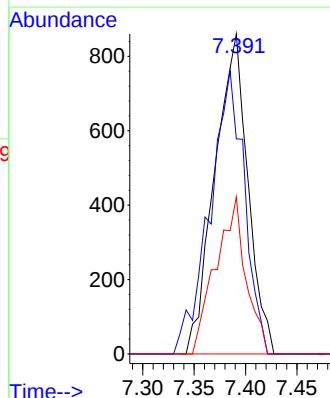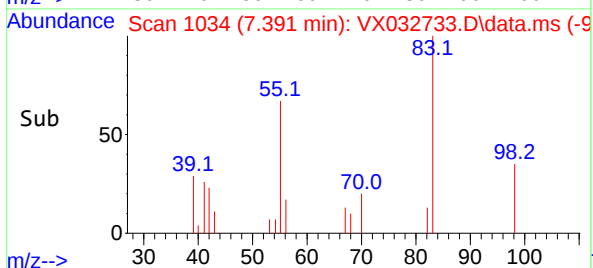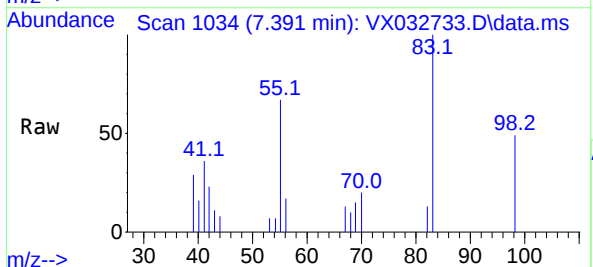




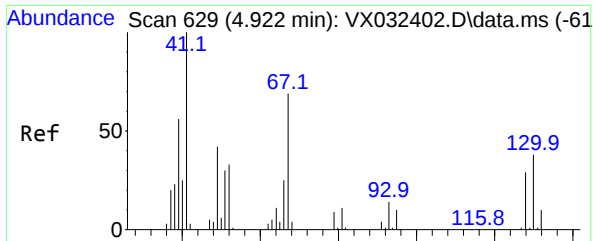


#41
Methacrylonitrile
Concen: 1.173 ug/l
RT: 5.032 min Scan# 647
Delta R.T. 0.110 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Instrument :
MSVOA_X
ClientSampleId :
NWB-1851RE

Tgt Ion: 41 Resp: 462




Ion	Ratio	Lower	Upper
41	100		
39	26.8	47.5	71.3#
67	0.0	60.5	90.7#
52	0.0	27.0	40.6#

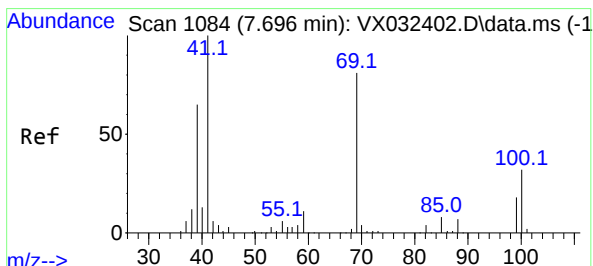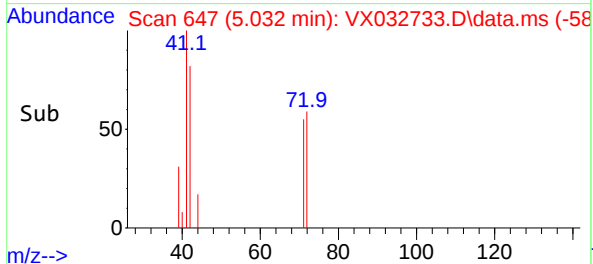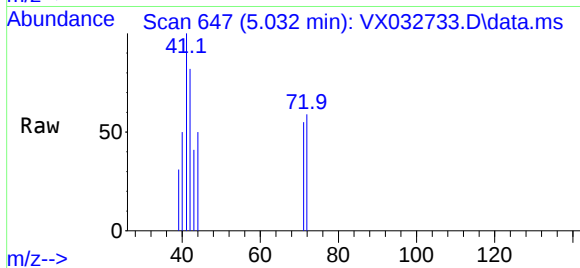


#48
Methyl methacrylate
Concen: 0.587 ug/l
RT: 7.665 min Scan# 1079
Delta R.T. -0.030 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Tgt Ion: 41 Resp: 360

Ion	Ratio	Lower	Upper
41	100		
69	107.8	65.1	97.7#
39	53.1	51.9	77.9

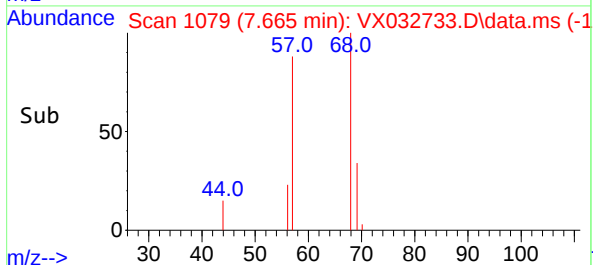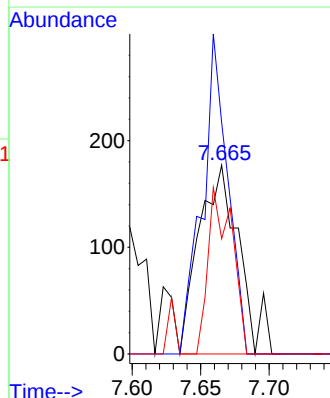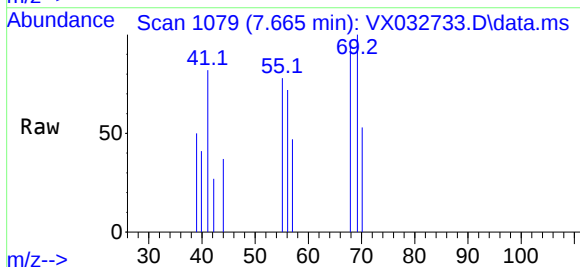

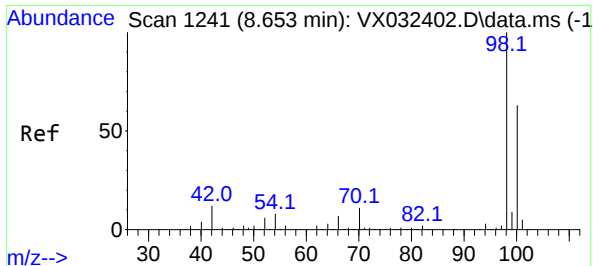

#50

Toluene-d8

Concen: 44.991 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. 0.000 min

Lab File: VX032733.D

Acq: 10 Nov 2022 17:04

Instrument :

MSVOA_X

ClientSampleId :





NWB-1851RE

Tgt Ion: 98 Resp: 83428

Ion Ratio Lower Upper

98 100

100 64.1 50.9 76.3

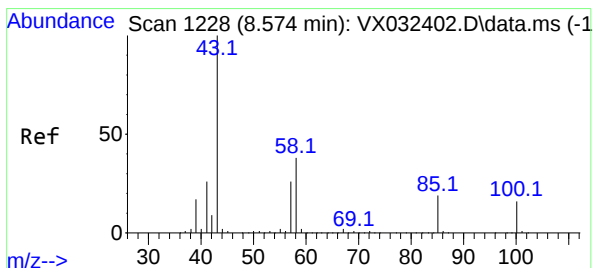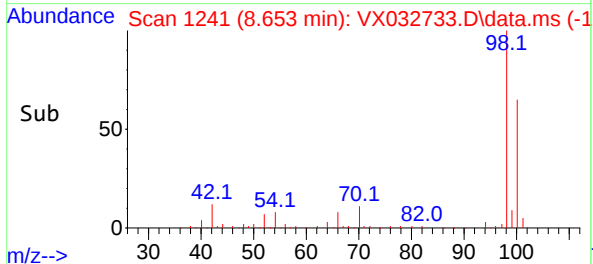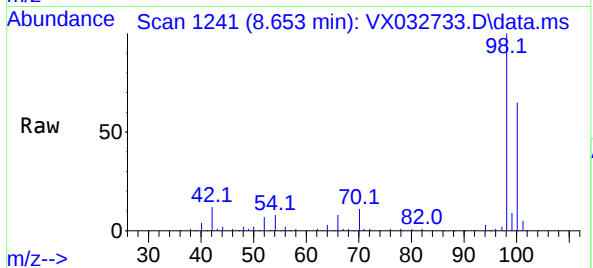

#51

4-Methyl-2-Pentanone

Concen: 1.455 ug/l

RT: 8.580 min Scan# 1229

Delta R.T. 0.006 min

Lab File: VX032733.D




Acq: 10 Nov 2022 17:04


Tgt Ion: 43 Resp: 1088

Ion Ratio Lower Upper

43 100

58 32.8 30.9 46.3

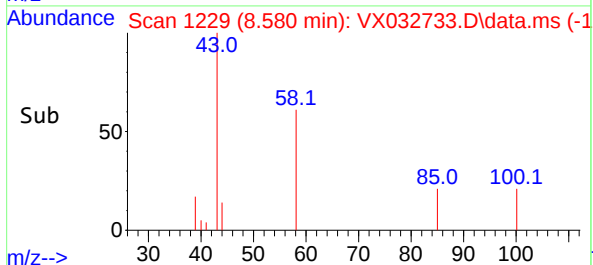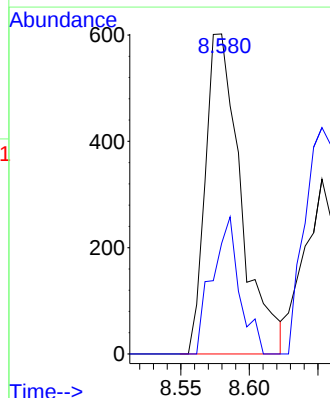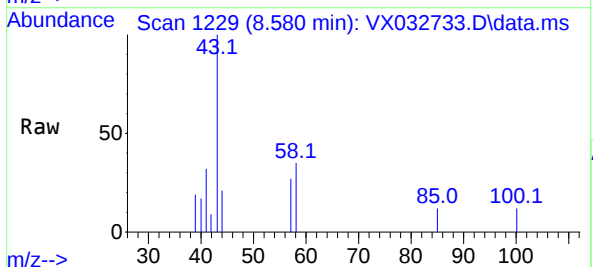

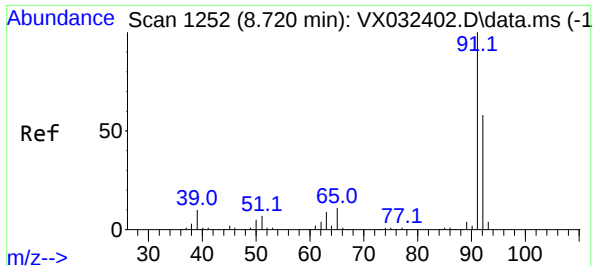

#52

Toluene

Concen: 25.292 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. 0.000 min

Lab File: VX032733.D

Acq: 10 Nov 2022 17:04

Instrument :

MSVOA_X

ClientSampleId :





NWB-1851RE

Tgt Ion: 92 Resp: 34677

Ion Ratio Lower Upper

92 100

91 180.2 138.3 207.5

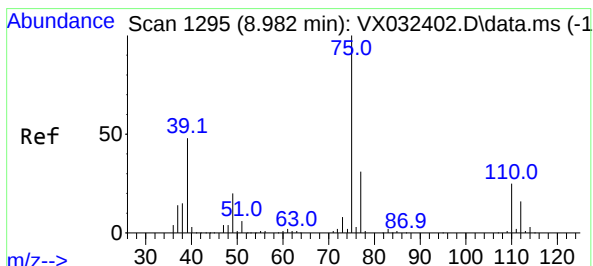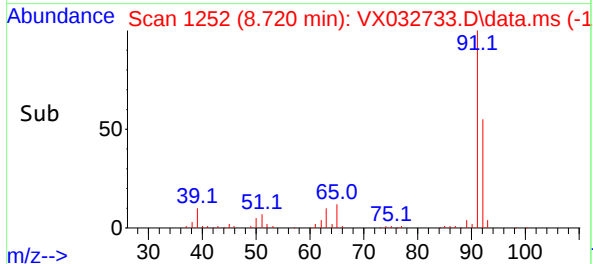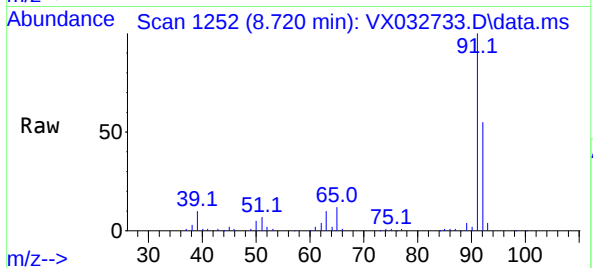

#53

t-1,3-Dichloropropene

Concen: 0.602 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.262 min

Lab File: VX032733.D




Acq: 10 Nov 2022 17:04


Tgt Ion: 75 Resp: 482

Ion Ratio Lower Upper

75 100

77 126.0 25.1 37.7#

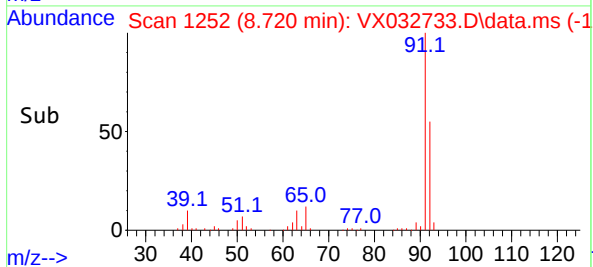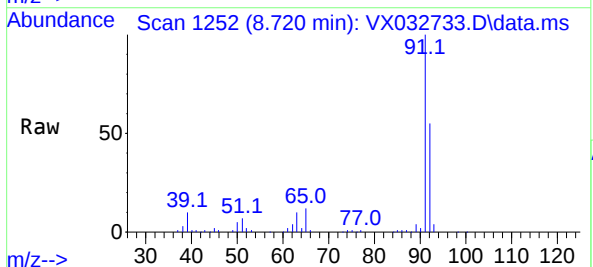




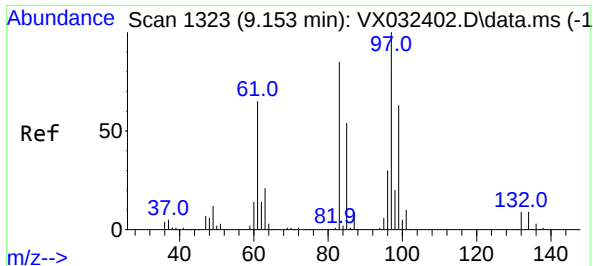


#55
1,1,2-Trichloroethane
Concen: 0.677 ug/l
RT: 9.104 min Scan# 11
Delta R.T. -0.049 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Instrument :
MSVOA_X
ClientSampleId :
NWB-1851RE

Tgt Ion: 97 Resp: 391




Ion	Ratio	Lower	Upper
97	100		
83	0.0	68.1	102.1#
85	0.0	43.3	64.9#
99	0.0	50.4	75.6#

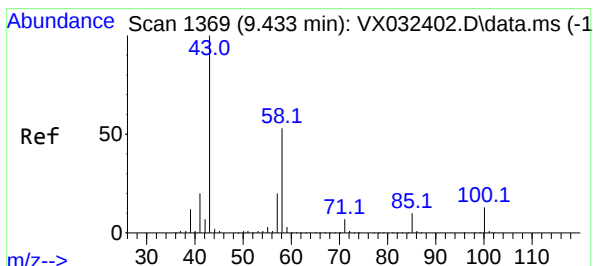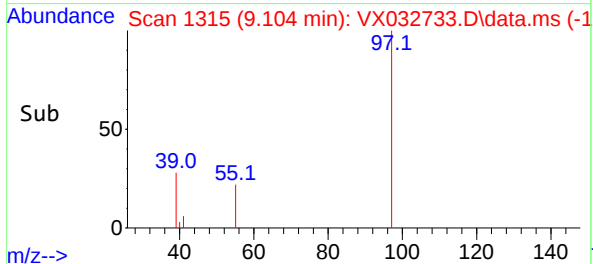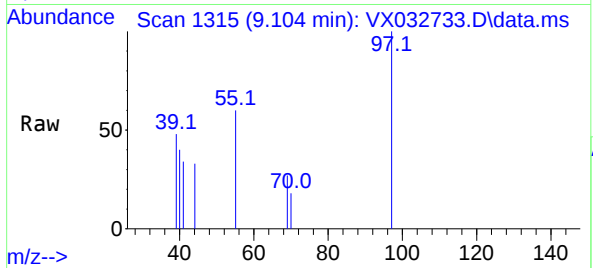


#59
2-Hexanone
Concen: 4.972 ug/l
RT: 9.439 min Scan# 1370
Delta R.T. 0.006 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Tgt Ion: 43 Resp: 2758

Ion	Ratio	Lower	Upper
43	100		
58	48.5	26.5	79.5

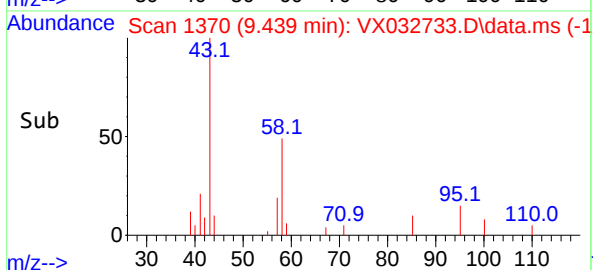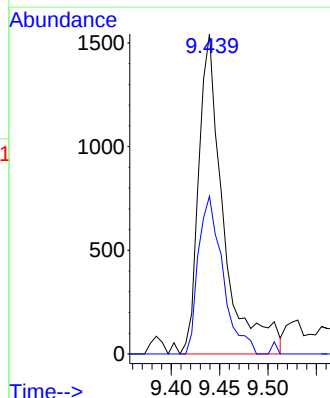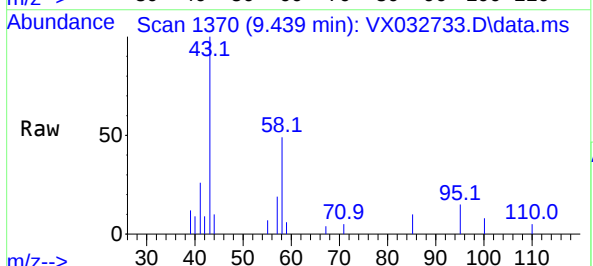



#62

4-Bromofluorobenzene

Concen: 25.786 ug/l

RT: 11.079 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX032733.D

Acq: 10 Nov 2022 17:04

Instrument :

MSVOA_X

ClientSampleId :

NWB-1851RE





Tgt Ion: 95 Resp: 18678

Ion Ratio Lower Upper

95 100

174 80.1 0.0 164.0

176 79.2 0.0 154.4

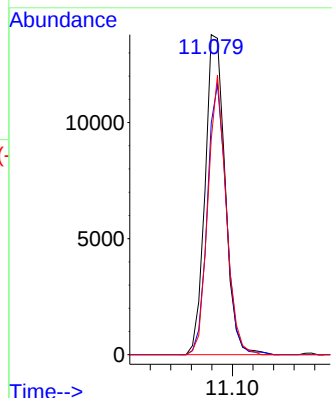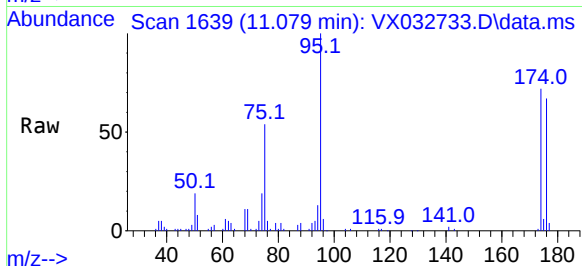

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX032733.D

Acq: 10 Nov 2022 17:04




Tgt Ion: 117 Resp: 40934


Ion Ratio Lower Upper

117 100

82 53.3 44.3 66.5

119 30.6 25.7 38.5



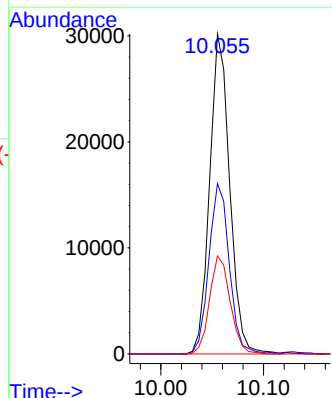
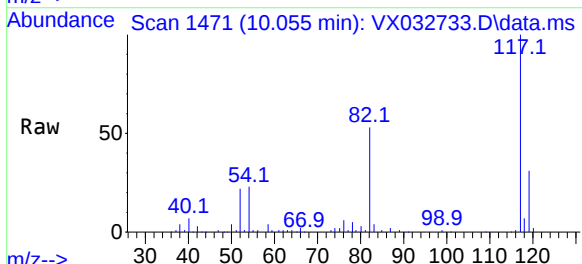




#67
Ethyl Benzene
Concen: 18.847 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04




Instrument :
MSVOA_X
ClientSampleId :
NWB-1851RE


Tgt Ion: 91 Resp: 30903
Ion Ratio Lower Upper
91 100
106 32.3 25.0 37.6

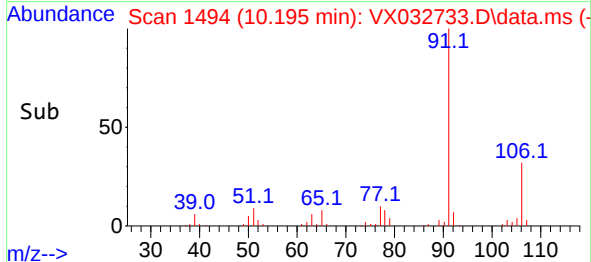

#68
m/p-Xylenes
Concen: 85.533 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Tgt Ion: 106 Resp: 54460
Ion Ratio Lower Upper
106 100
91 207.7 164.5 246.7


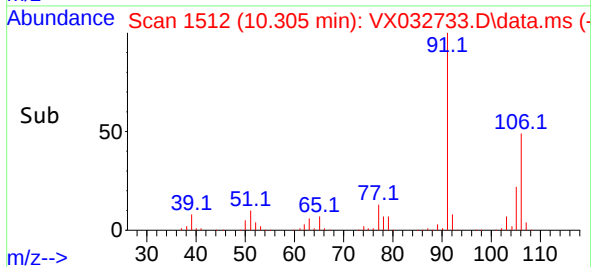

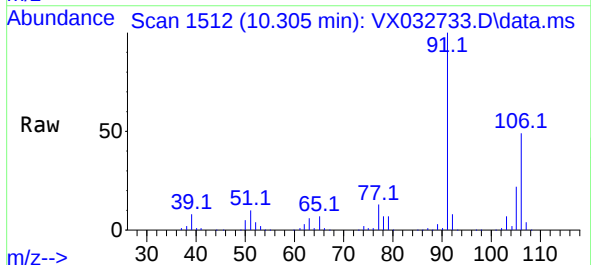




#69
o-Xylene
Concen: 30.430 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.006 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04




Instrument :
MSVOA_X
ClientSampleId :
NWB-1851RE


Tgt Ion:106 Resp: 18838
Ion Ratio Lower Upper
106 100
91 217.1 109.2 327.6



#70
Styrene
Concen: 1.254 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.012 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Tgt Ion:104 Resp: 1290
Ion Ratio Lower Upper
104 100
78 248.5 41.8 62.8#
103 203.5 44.5 66.7#



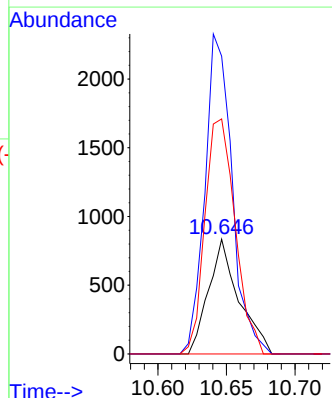





#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04




Instrument :
MSVOA_X
ClientSampleId :
NWB-1851RE


Tgt Ion:152 Resp: 17213
Ion Ratio Lower Upper
152 100
115 64.6 44.0 132.0
150 156.9 0.0 351.8

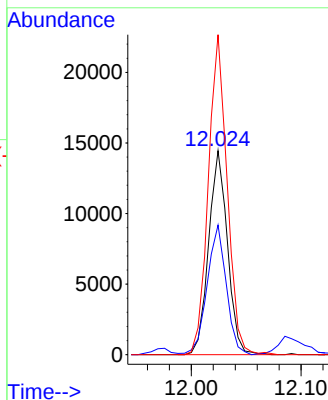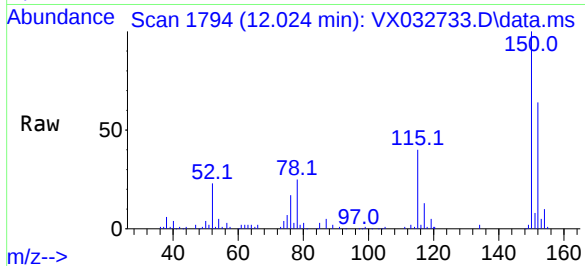

#73
Isopropylbenzene
Concen: 6.907 ug/l
RT: 10.964 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Tgt Ion:105 Resp: 9421
Ion Ratio Lower Upper
105 100
120 25.6 13.1 39.3


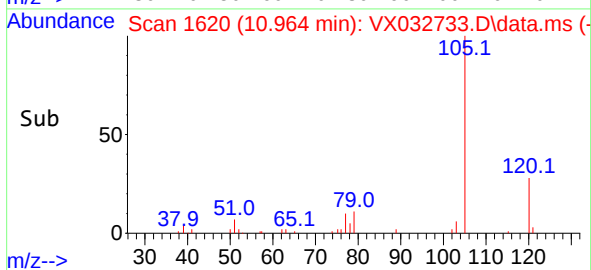
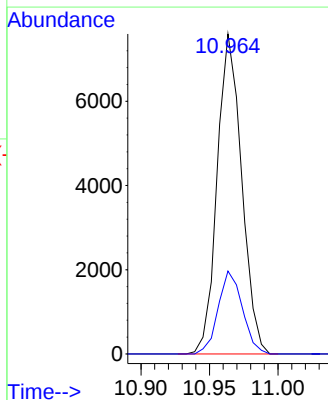
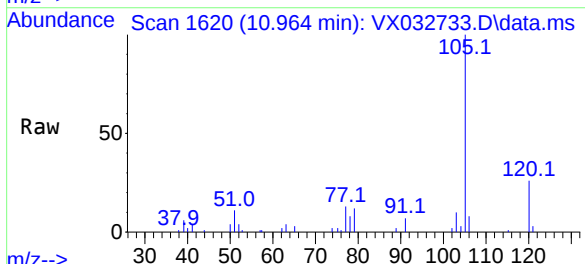




#74
N-amy1 acetate
Concen: 0.260 ug/l
RT: 10.848 min Scan# 1600
Delta R.T. 0.006 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04




Instrument :
MSVOA_X
ClientSampleId :
NWB-1851RE


Tgt Ion: 43	Resp:	134
Ion	Ratio	Lower Upper
43	100	
70	0.0	33.6 50.4#
55	173.1	19.4 29.2#
61	0.0	18.8 28.2#

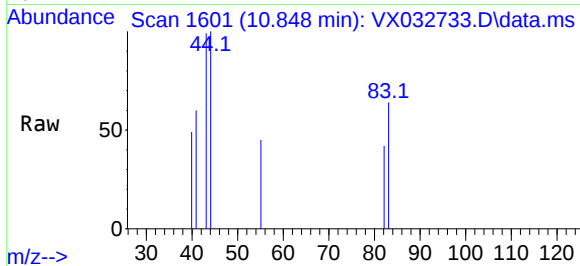

#76
1,2,3-Trichloropropane
Concen: 2.457 ug/l
RT: 11.384 min Scan# 1689
Delta R.T. 0.140 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Tgt Ion: 75	Resp:	941
Ion	Ratio	Lower Upper
75	100	
77	1188.7	20.0 60.0#


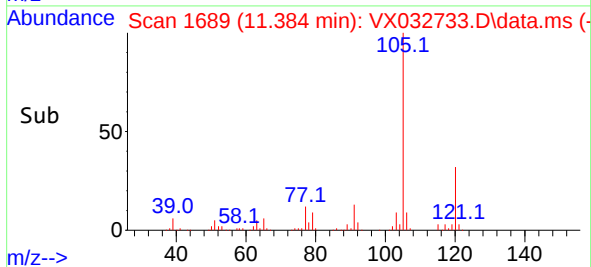

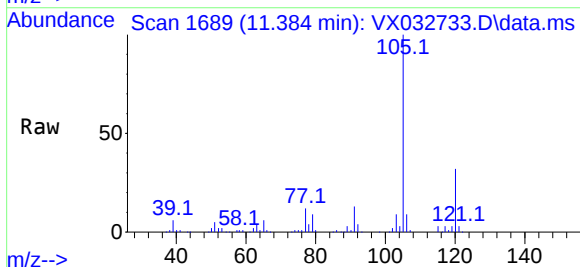




#78
n-propylbenzene
Concen: 18.968 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.000 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04




Instrument :
MSVOA_X
ClientSampleId :
NWB-1851RE


Tgt Ion: 91 Resp: 29809
Ion Ratio Lower Upper
91 100
120 22.7 11.6 34.8

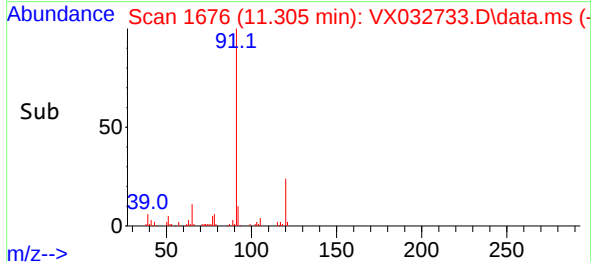

#79
2-Chlorotoluene
Concen: 13.055 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Tgt Ion: 91 Resp: 12287
Ion Ratio Lower Upper
91 100
126 0.0 17.1 51.2#


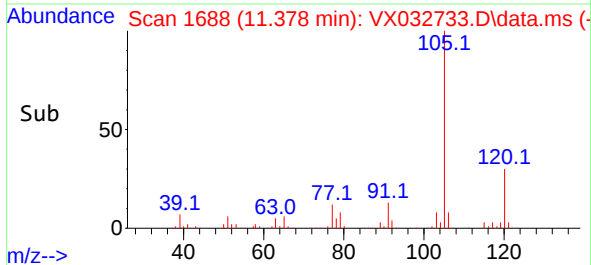

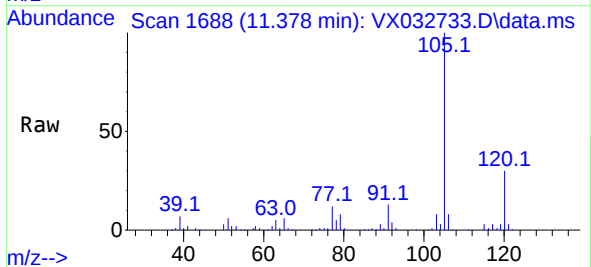




#80
1,3,5-Trimethylbenzene
Concen: 32.275 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04




Instrument :
MSVOA_X
ClientSampleId :
NWB-1851RE


Tgt Ion:105 Resp: 37624
Ion Ratio Lower Upper
105 100
120 47.5 23.6 71.0

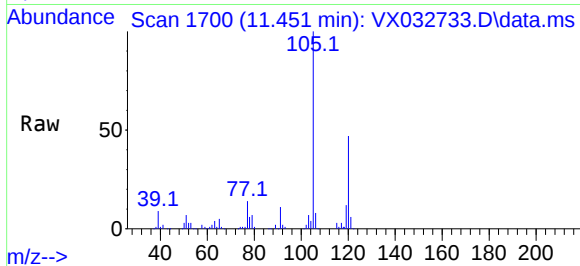

#81
trans-1,4-Dichloro-2-butene
Concen: 83.259 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Tgt Ion: 75 Resp: 10020
Ion Ratio Lower Upper
75 100
53 0.0 86.9 130.3#
89 0.0 38.3 57.5#


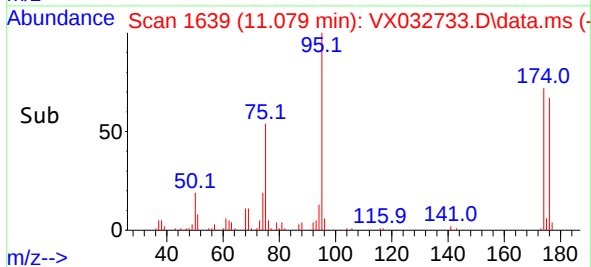

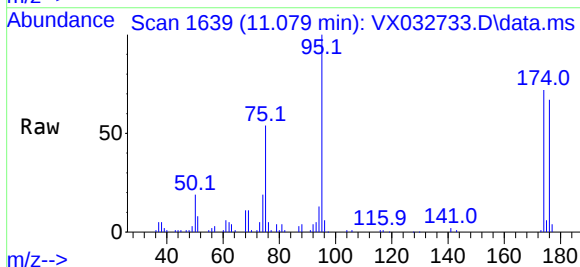




#82
4-Chlorotoluene
Concen: 3.891 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04




Instrument :
MSVOA_X
ClientSampleId :
NWB-1851RE


Tgt Ion: 91 Resp: 4285
Ion Ratio Lower Upper
91 100
126 0.0 14.8 44.4#

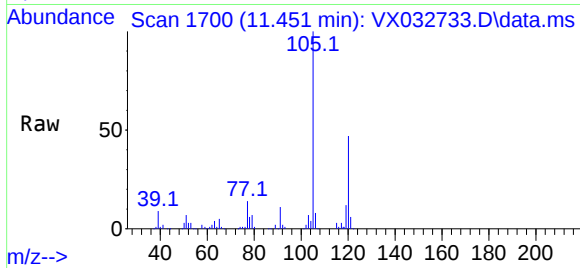

#83
tert-Butylbenzene
Concen: 4.594 ug/l
RT: 11.969 min Scan# 1785
Delta R.T. 0.256 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Tgt Ion: 119 Resp: 5347
Ion Ratio Lower Upper
119 100
91 36.9 29.4 88.2
134 31.4 11.0 33.0


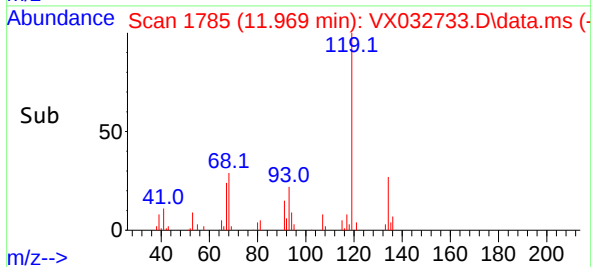

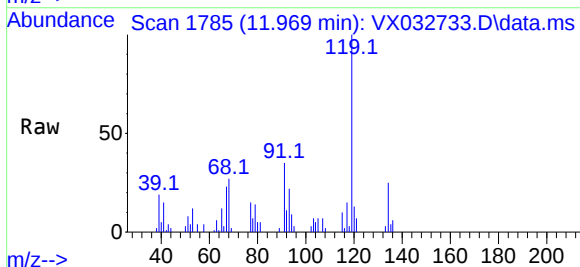




#84
1,2,4-Trimethylbenzene
Concen: 117.258 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04




Instrument :
MSVOA_X
ClientSampleId :
NWB-1851RE


Tgt Ion:105 Resp: 135955
Ion Ratio Lower Upper
105 100
120 43.7 21.9 65.5

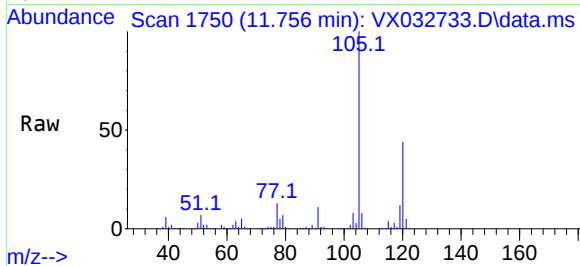

#85
sec-Butylbenzene
Concen: 3.036 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. 0.000 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Tgt Ion:105 Resp: 4251
Ion Ratio Lower Upper
105 100
134 17.0 9.9 29.7


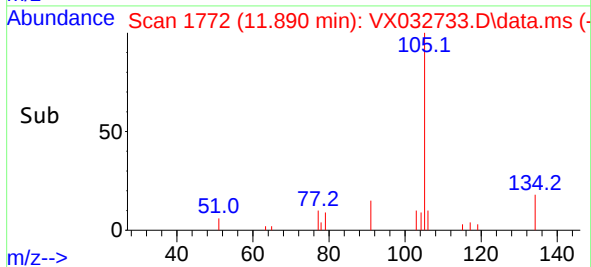

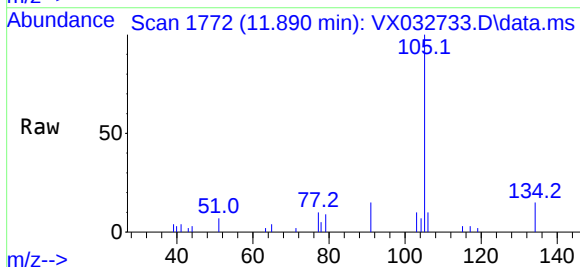




#86
p-Isopropyltoluene
Concen: 5.642 ug/l
RT: 12.012 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04




Instrument :
MSVOA_X
ClientSampleId :
NWB-1851RE


Tgt Ion:119 Resp: 6705
Ion Ratio Lower Upper
119 100
134 26.8 12.9 38.7
91 25.8 12.5 37.5

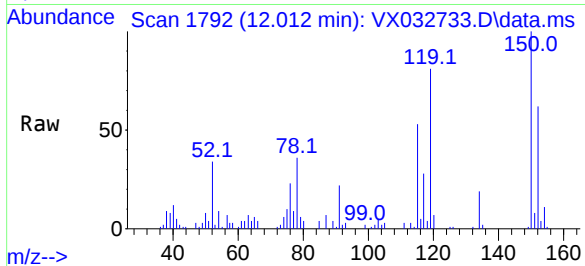

#89
n-Butylbenzene
Concen: 12.709 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Tgt Ion: 91 Resp: 13138
Ion Ratio Lower Upper
91 100
92 34.0 26.2 78.6
134 90.6 12.9 38.6#


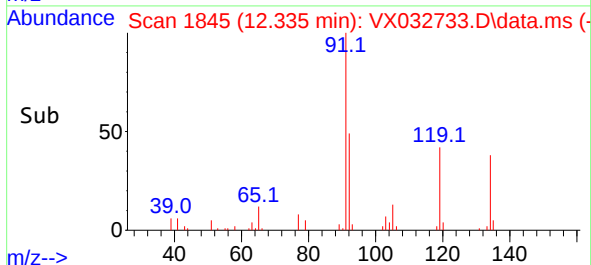
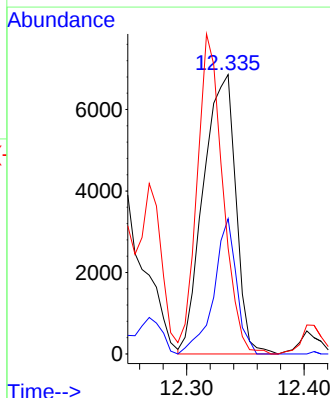
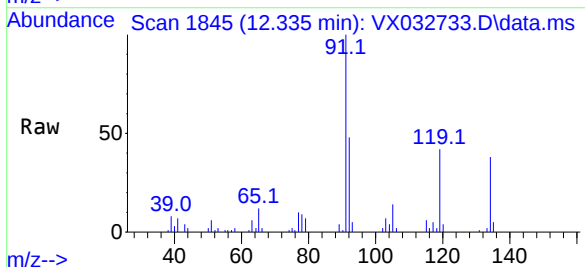




#90
Hexachloroethane
Concen: 7.919 ug/l
RT: 12.530 min Scan# 117
Delta R.T. -0.012 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04




Instrument : MSVOA_X
ClientSampleId : NWB-1851RE


Tgt Ion:117 Resp: 1537
Ion Ratio Lower Upper
117 100
201 0.0 37.6 112.9#

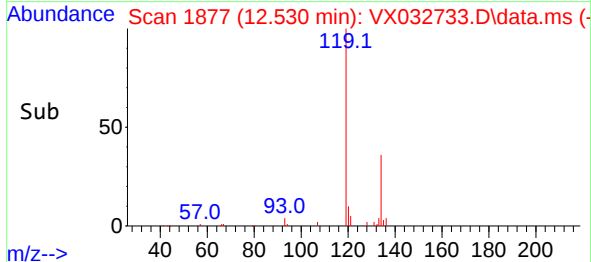

#92
1,2-Dibromo-3-Chloropropane
Concen: 1.594 ug/l
RT: 12.963 min Scan# 1948
Delta R.T. 0.018 min
Lab File: VX032733.D
Acq: 10 Nov 2022 17:04

Tgt Ion: 75 Resp: 153
Ion Ratio Lower Upper
75 100
155 0.0 41.6 124.8#
157 0.0 54.1 162.4#

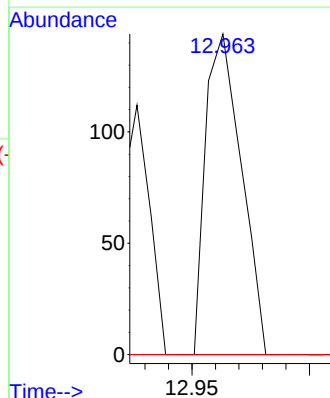



#95

Naphthalene

Concen: 15.074 ug/l

RT: 13.774 min Scan# 20

Delta R.T. -0.006 min

Lab File: VX032733.D


Acq: 10 Nov 2022 17:04

Instrument :

MSVOA_X

ClientSampleId :

NWB-1851RE

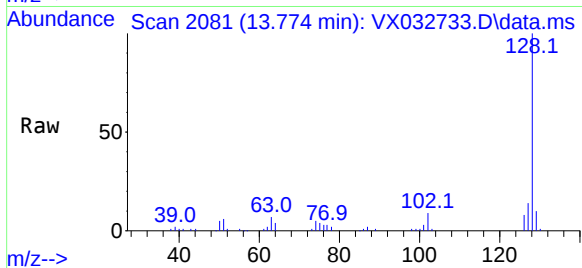

Tgt Ion:128 Resp: 20370

Ion Ratio Lower Upper

128 100

127 12.7 10.2 15.4

129 11.1 8.9 13.3

