



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111022\
Data File : VX032717.D
Acq On : 10 Nov 2022 10:14
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Title : SW846 8260
Last Update : Thu Oct 27 08:28:06 2022

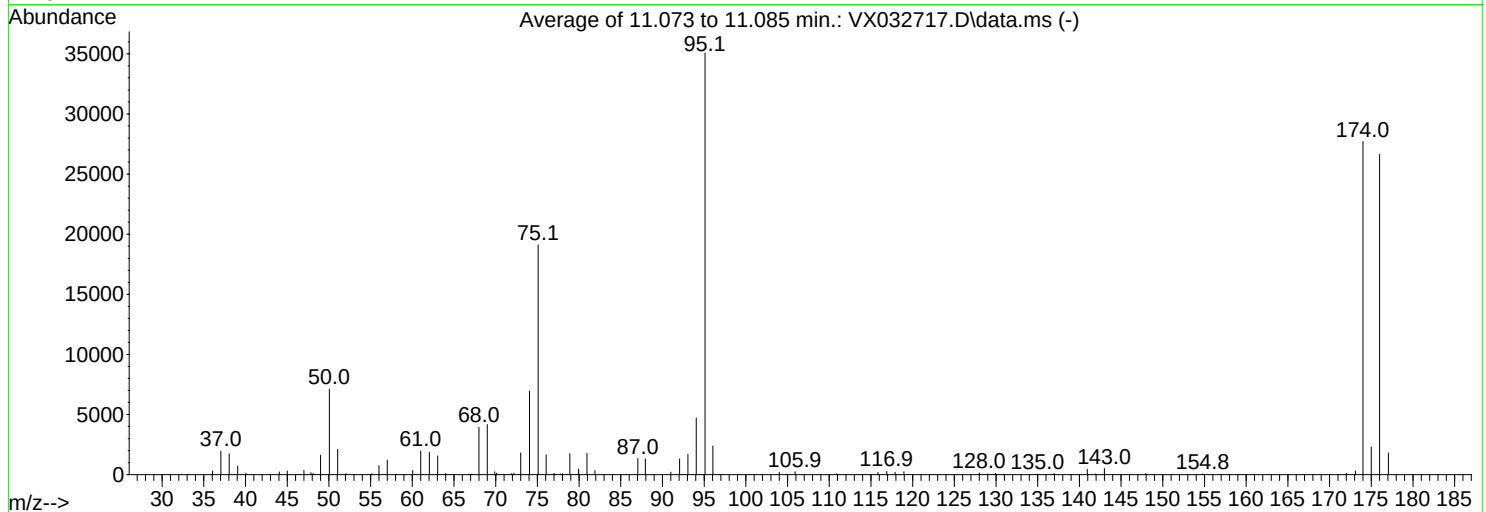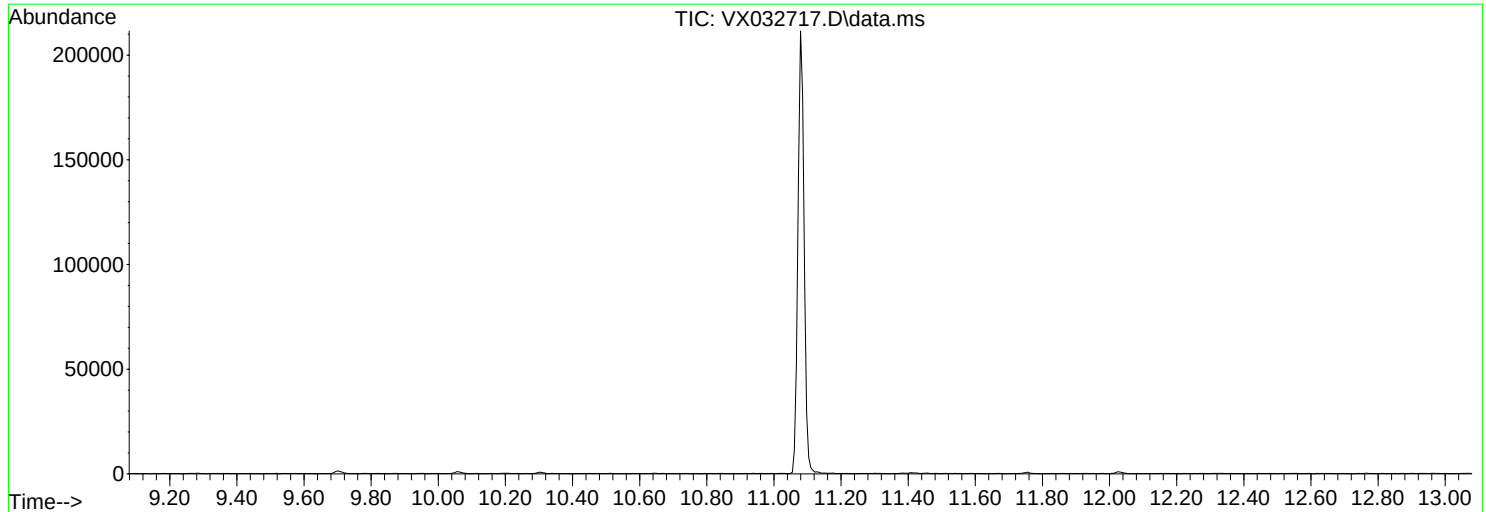

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.3	7115	PASS
75	95	30	60	54.5	19107	PASS
95	95	100	100	100.0	35085	PASS
96	95	5	9	6.8	2382	PASS
173	174	0.00	2	1.1	311	PASS
174	95	50	100	79.0	27709	PASS
175	174	5	9	8.3	2300	PASS
176	174	95	101	96.1	26629	PASS
177	176	5	9	6.8	1808	PASS