

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111023\
 Data File : VX038743.D
 Acq On : 10 Nov 2023 20:47
 Operator : JC/MD
 Sample : 05316-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 NWB-1979

Quant Time: Nov 11 02:00:48 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 08 03:19:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	256122	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	423085	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	445439	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	259883	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	147780	46.346	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	92.700%		
35) Dibromofluoromethane	5.385	113	136872	44.918	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	89.840%		
50) Toluene-d8	8.647	98	505647	46.372	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	92.740%		
62) 4-Bromofluorobenzene	11.079	95	221711	52.443	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	104.880%		
Target Compounds						Qvalue
11) Tert butyl alcohol	2.953	59	24583	37.713	ug/l	# 91
13) Acrolein	2.233	56	495	1.002	ug/l	# 41
14) Allyl chloride	2.648	41	1110	0.324	ug/l	# 24
16) Acetone	2.373	43	288395	214.757	ug/l	90
20) Methylene Chloride	2.794	84	3207	1.185	ug/l	# 74
25) 2-Butanone	4.556	43	42247	21.717	ug/l	# 85
36) 1,1-Dichloropropene	5.550	75	16477	4.353	ug/l	# 52
37) Ethyl Acetate	4.556	43	42202	10.920	ug/l	# 69
38) Carbon Tetrachloride	5.550	117	24363	5.757	ug/l	# 14
39) Methylcyclohexane	7.391	83	1680	0.355	ug/l	# 76
40) Benzene	6.044	78	57511	5.275	ug/l	99
43) Isopropyl Acetate	6.342	43	2101	0.354	ug/l	# 62
44) Trichloroethene	7.129	130	2806	0.827	ug/l	91
48) Methyl methacrylate	7.677	41	1566	0.547	ug/l	# 49
49) 1,4-Dioxane	7.671	88	1382	21.202	ug/l	# 85
51) 4-Methyl-2-Pentanone	8.580	43	1865	0.482	ug/l	# 78
52) Toluene	8.720	92	63171	8.845	ug/l	96
58) 2-Chloroethyl Vinyl ether	8.214	63	740	0.355	ug/l	# 47
59) 2-Hexanone	9.439	43	2064	0.659	ug/l	94
67) Ethyl Benzene	10.195	91	21125	1.377	ug/l	92
68) m/p-Xylenes	10.299	106	54454	8.945	ug/l	95
69) o-Xylene	10.640	106	22205	3.751	ug/l	99
70) Styrene	10.659	104	39035	3.995	ug/l	94
73) Isopropylbenzene	10.963	105	3217	0.202	ug/l	95
76) 1,2,3-Trichloropropane	11.079	75	107829	20.950	ug/l	# 39
78) n-propylbenzene	11.311	91	7431	0.401	ug/l	79
79) 2-Chlorotoluene	11.384	91	2981	0.268	ug/l	# 42
80) 1,3,5-Trimethylbenzene	11.451	105	15551	1.133	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.079	75	107829	63.699	ug/l	# 5
84) 1,2,4-Trimethylbenzene	11.750	105	56936	4.183	ug/l	74
85) sec-Butylbenzene	11.750	105	56936	3.282	ug/l	# 57
90) Hexachloroethane	12.530	117	577	0.230	ug/l	# 17
95) Naphthalene	13.774	128	88176	5.002	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
NWB-1979

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111023\
Data File : VX038743.D
Acq On : 10 Nov 2023 20:47
Operator : JC/MD
Sample : 05316-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
NWB-1979

Quant Time: Nov 11 02:00:48 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 08 03:19:07 2023
Response via : Initial Calibration




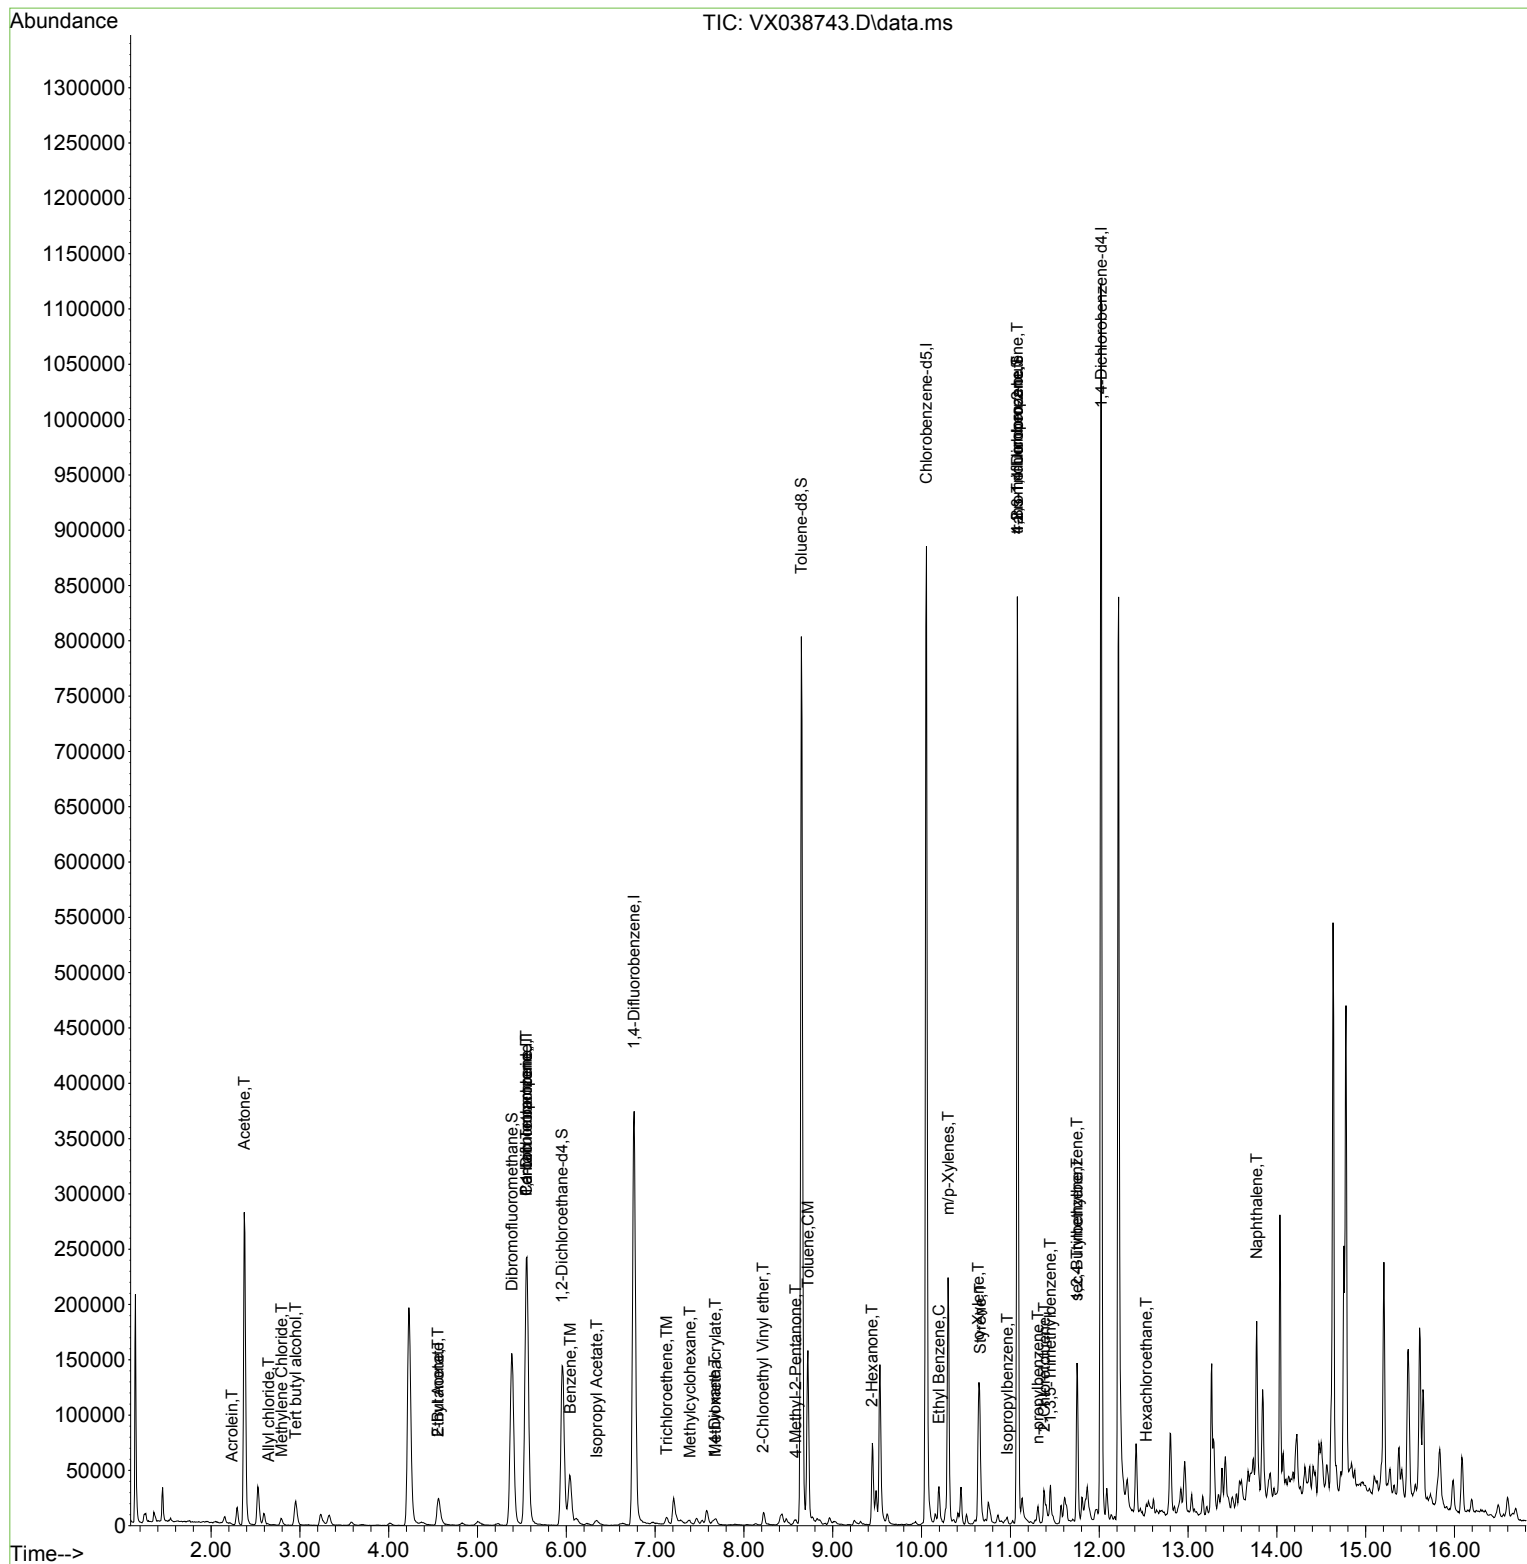


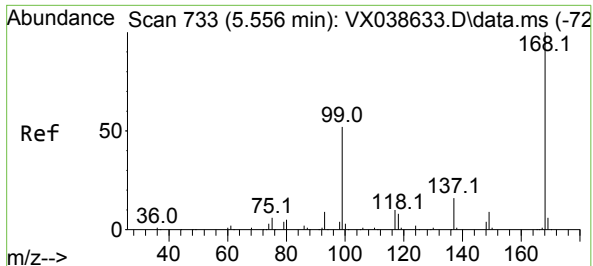

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47




Instrument :
MSVOA_X
ClientSampleId :
NWB-1979


Tgt Ion:168 Resp: 256122
Ion Ratio Lower Upper
168 100
99 52.7 56.6 85.0#

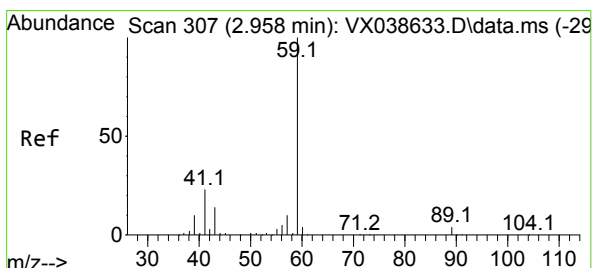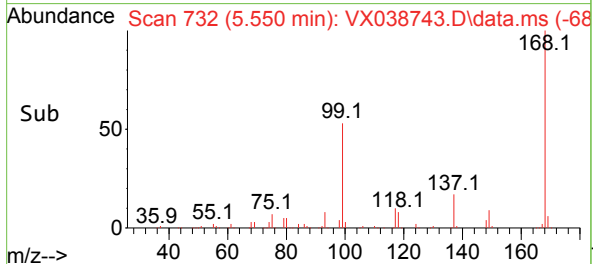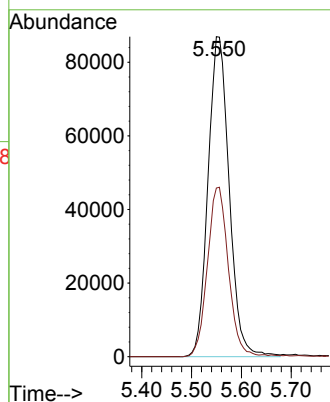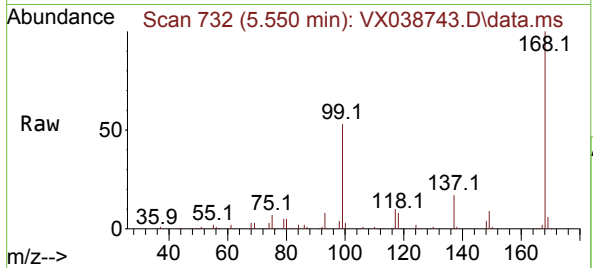

#11
Tert butyl alcohol
Concen: 37.713 ug/l
RT: 2.953 min Scan# 306
Delta R.T. -0.006 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47

Tgt Ion: 59 Resp: 24583
Ion Ratio Lower Upper
59 100
57 10.8 6.0 9.0#

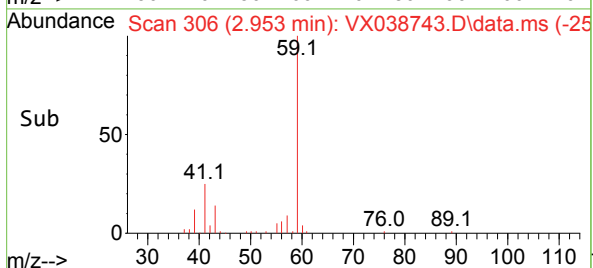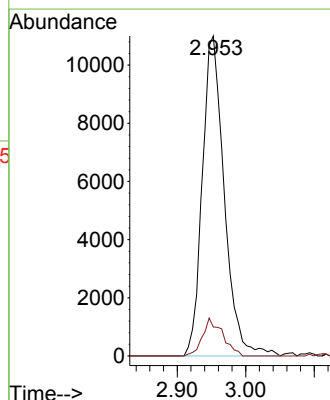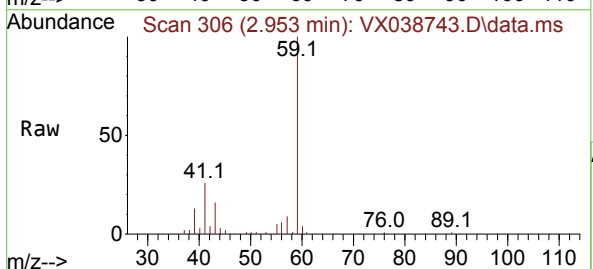



#13

Acrolein

Concen: 1.002 ug/l

RT: 2.233 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX038743.D

Acq: 10 Nov 2023 20:47

Instrument :

MSVOA_X

ClientSampleId :





NWB-1979

Tgt Ion: 56 Resp: 495

Ion Ratio Lower Upper

56 100

55 120.4 57.1 85.7#

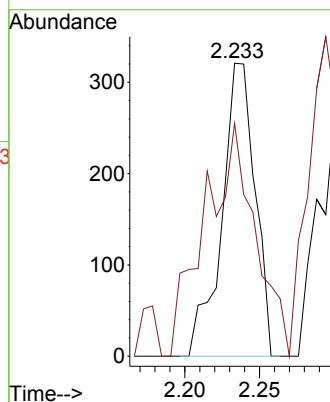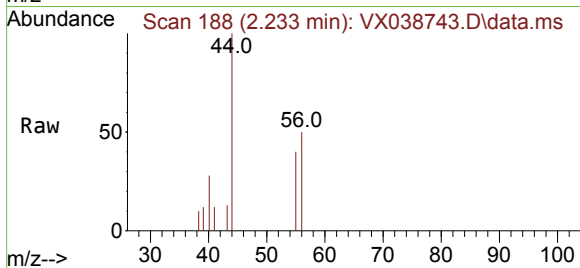

#14

Allyl chloride

Concen: 0.324 ug/l

RT: 2.648 min Scan# 256

Delta R.T. -0.018 min

Lab File: VX038743.D

Acq: 10 Nov 2023 20:47




Tgt Ion: 41 Resp: 1110


Ion Ratio Lower Upper

41 100

39 0.0 55.8 83.6#

76 0.0 24.3 36.5#



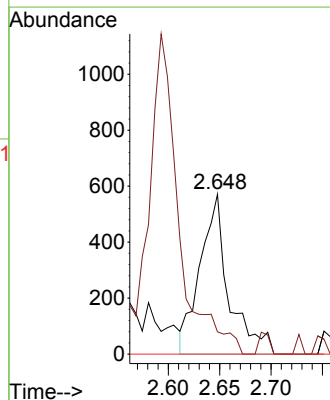
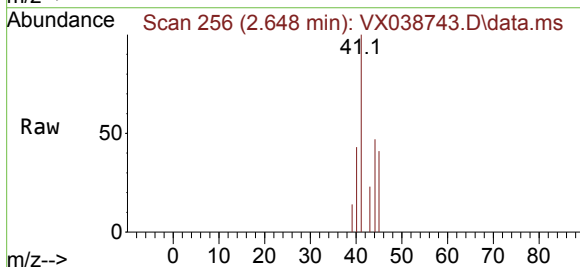




#16
Acetone
Concen: 214.757 ug/l
RT: 2.373 min Scan# 211
Delta R.T. -0.006 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47




Instrument :
MSVOA_X
ClientSampleId :
NWB-1979


Tgt Ion: 43 Resp: 288395
Ion Ratio Lower Upper
43 100
58 32.6 21.9 32.9

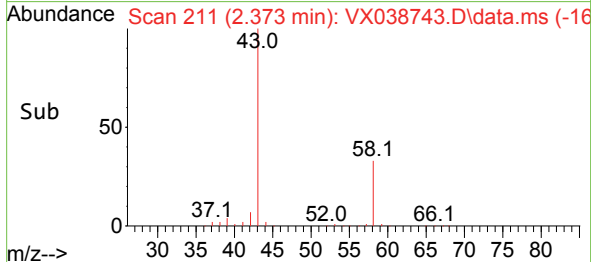

#20
Methylene Chloride
Concen: 1.185 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.006 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47

Tgt Ion: 84 Resp: 3207
Ion Ratio Lower Upper
84 100
49 87.1 103.6 155.4#
51 27.7 33.8 50.6#
86 55.6 49.4 74.0

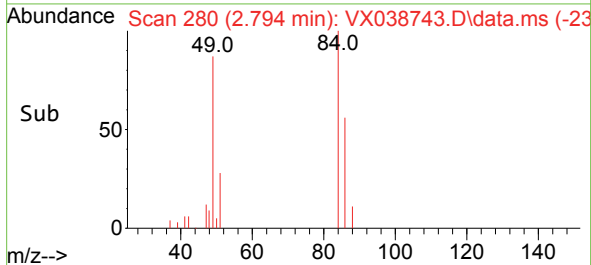



#25

2-Butanone

Concen: 21.717 ug/l

RT: 4.556 min Scan# 5

Delta R.T. 0.000 min

Lab File: VX038743.D

Acq: 10 Nov 2023 20:47

Instrument :

MSVOA_X

ClientSampleId :





NWB-1979

Tgt Ion: 43 Resp: 42247

Ion Ratio Lower Upper

43 100

72 31.5 19.4 29.2#

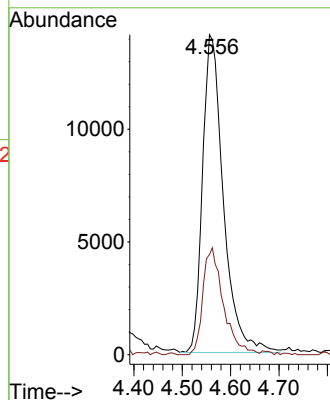

#33

1,2-Dichloroethane-d4

Concen: 46.346 ug/l

RT: 5.952 min Scan# 798

Delta R.T. -0.006 min

Lab File: VX038743.D




Acq: 10 Nov 2023 20:47


Tgt Ion: 65 Resp: 147780

Ion Ratio Lower Upper

65 100

67 51.3 0.0 100.2


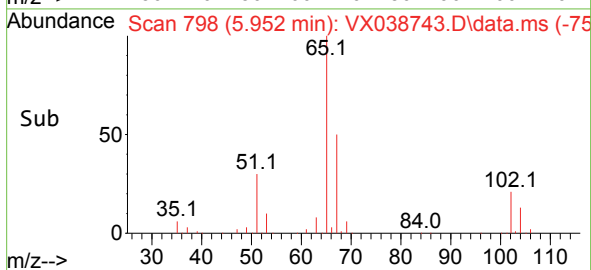
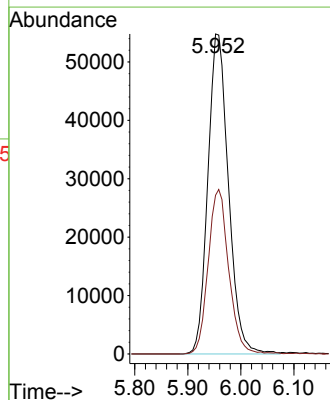





#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47




Instrument :
MSVOA_X
ClientSampleId :
NWB-1979


Tgt Ion:114 Resp: 423085
Ion Ratio Lower Upper
114 100
63 17.1 0.0 45.0
88 15.1 0.0 36.6

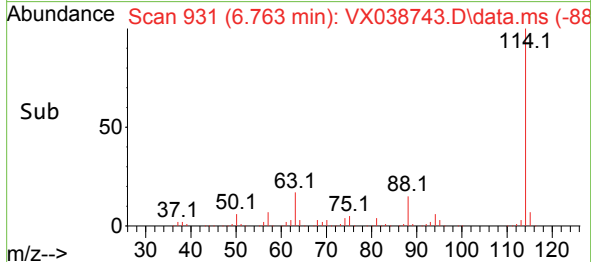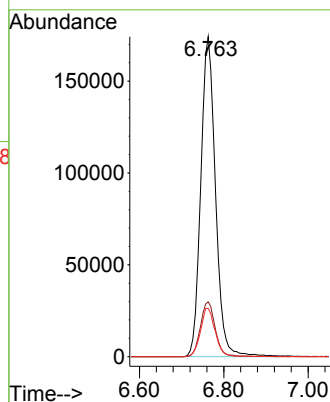

#35
Dibromofluoromethane
Concen: 44.918 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47

Tgt Ion:113 Resp: 136872
Ion Ratio Lower Upper
113 100
111 103.6 82.9 124.3
192 21.5 13.3 19.9#



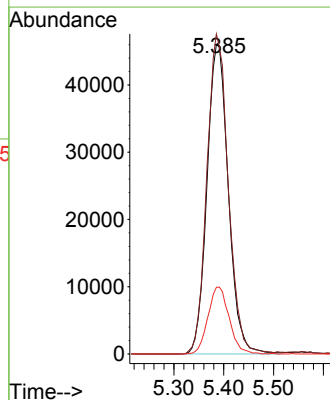
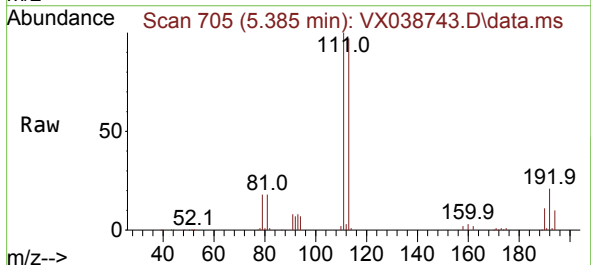




#36
1,1-Dichloropropene
Concen: 4.353 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.146 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47




Instrument :
MSVOA_X
ClientSampleId :
NWB-1979


Tgt Ion: 75 Resp: 16477
Ion Ratio Lower Upper
75 100
110 10.8 17.0 50.9#
77 0.0 24.7 37.1#

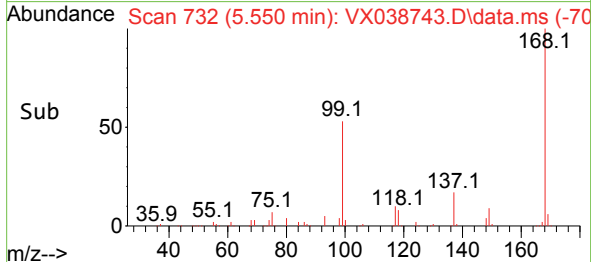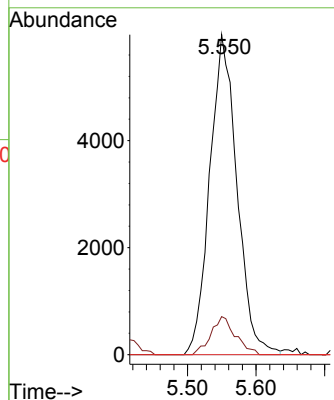

#37
Ethyl Acetate
Concen: 10.920 ug/l
RT: 4.556 min Scan# 569
Delta R.T. -0.158 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47

Tgt Ion: 43 Resp: 42202
Ion Ratio Lower Upper
43 100
61 0.0 10.6 16.0#
70 0.0 8.3 12.5#


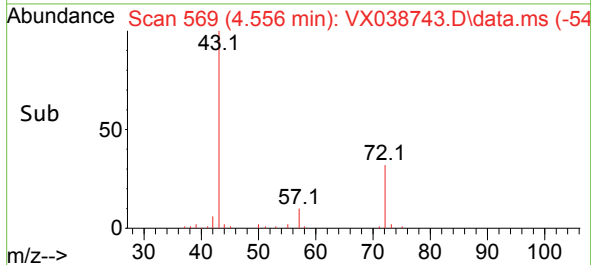
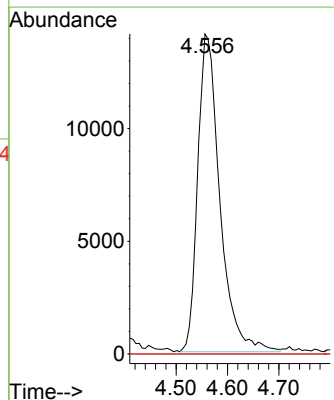





#38
Carbon Tetrachloride
Concen: 5.757 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47




Instrument :
MSVOA_X
ClientSampleId :
NWB-1979


Tgt Ion:117 Resp: 24363
Ion Ratio Lower Upper
117 100
119 3.8 78.2 117.2#
121 0.0 24.4 36.6#

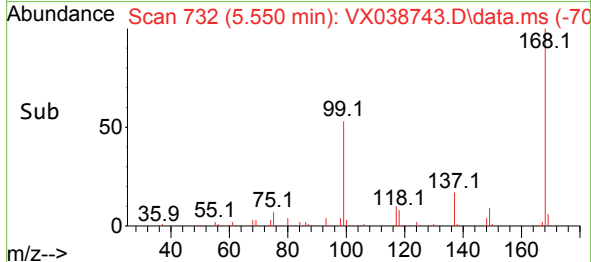

#39
Methylcyclohexane
Concen: 0.355 ug/l
RT: 7.391 min Scan# 1034
Delta R.T. 0.006 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47

Tgt Ion: 83 Resp: 1680
Ion Ratio Lower Upper
83 100
55 55.8 64.6 97.0#
98 34.0 36.7 55.1#

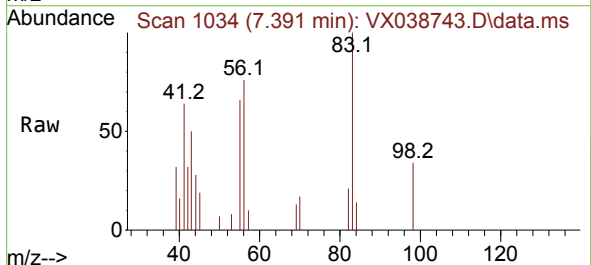



#40

Benzene

Concen: 5.275 ug/l

RT: 6.044 min Scan# 812

Delta R.T. 0.006 min

Lab File: VX038743.D

Acq: 10 Nov 2023 20:47

Instrument :

MSVOA_X

ClientSampleId :





NWB-1979

Tgt Ion: 78 Resp: 57511

Ion Ratio Lower Upper

78 100

77 23.5 19.3 28.9

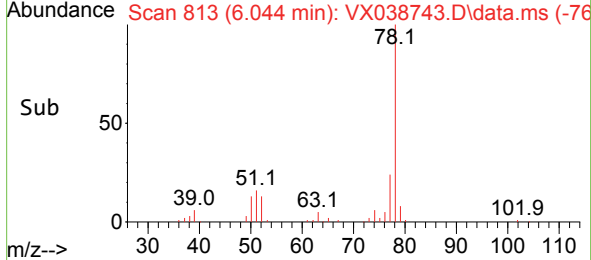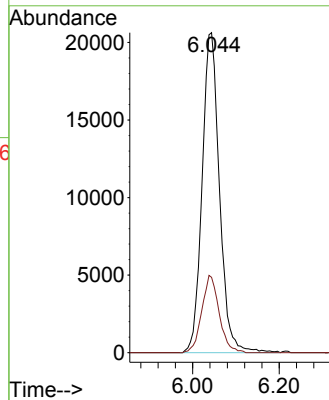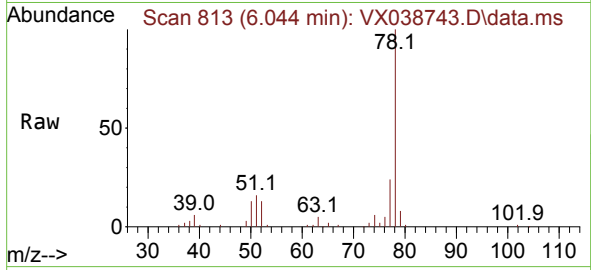

#43

Isopropyl Acetate

Concen: 0.354 ug/l

RT: 6.342 min Scan# 862

Delta R.T. 0.000 min

Lab File: VX038743.D

Acq: 10 Nov 2023 20:47




Tgt Ion: 43 Resp: 2101


Ion Ratio Lower Upper

43 100

61 0.0 15.2 22.8#

87 0.0 9.8 14.6#


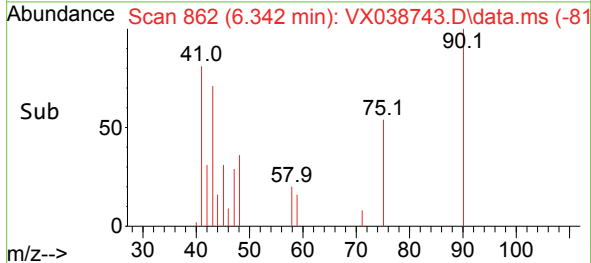
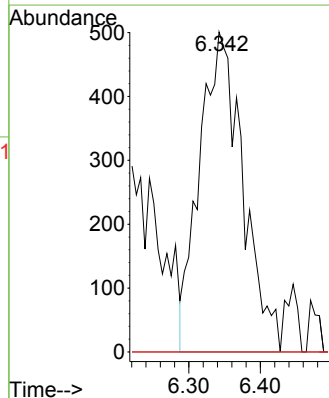



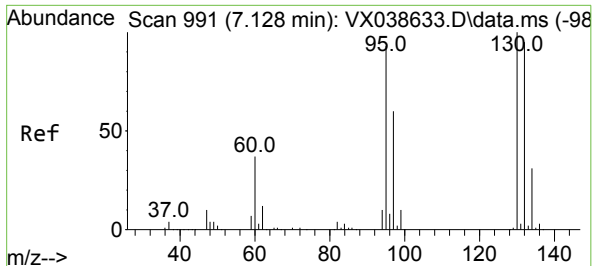

#44
Trichloroethene
Concen: 0.827 ug/l
RT: 7.129 min Scan# 991
Delta R.T. 0.000 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47




Instrument :
MSVOA_X
ClientSampleId :
NWB-1979


Tgt Ion:130 Resp: 2806
Ion Ratio Lower Upper
130 100
95 92.7 0.0 204.4

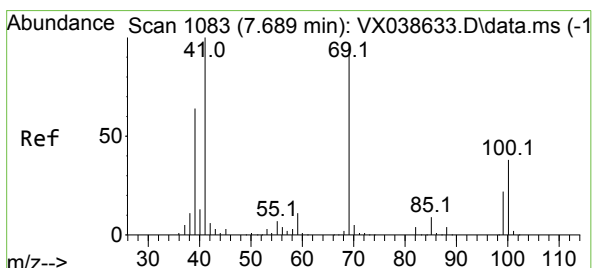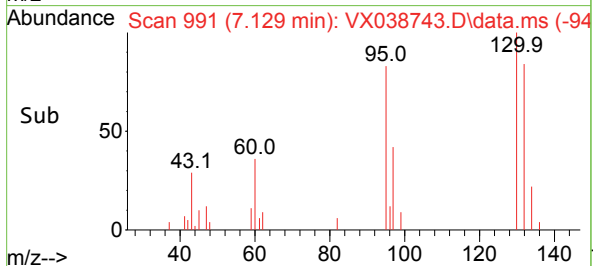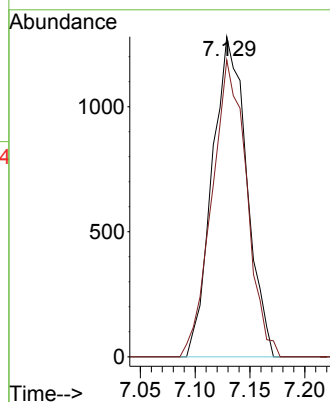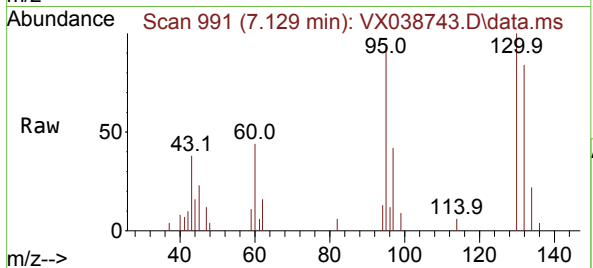

#48
Methyl methacrylate
Concen: 0.547 ug/l
RT: 7.677 min Scan# 1081
Delta R.T. -0.012 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47

Tgt Ion: 41 Resp: 1566
Ion Ratio Lower Upper
41 100
69 0.0 59.2 88.8#
39 64.2 47.7 71.5


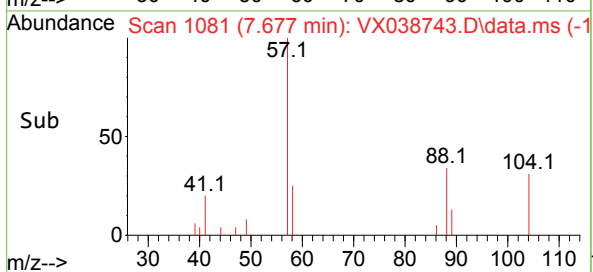
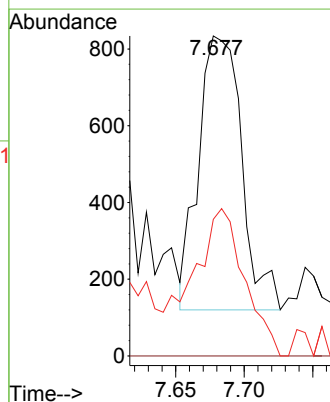
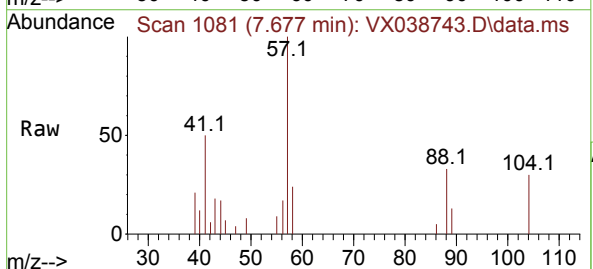




#49
1,4-Dioxane
Concen: 21.202 ug/l
RT: 7.671 min Scan# 1078
Delta R.T. 0.013 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47




Instrument :
MSVOA_X
ClientSampleId :
NWB-1979


Tgt Ion: 88 Resp: 1382
Ion Ratio Lower Upper
88 100
43 24.1 0.0 0.0#
58 87.9 60.1 90.1



#50
Toluene-d8
Concen: 46.372 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47

Tgt Ion: 98 Resp: 505647
Ion Ratio Lower Upper
98 100
100 65.7 53.1 79.7


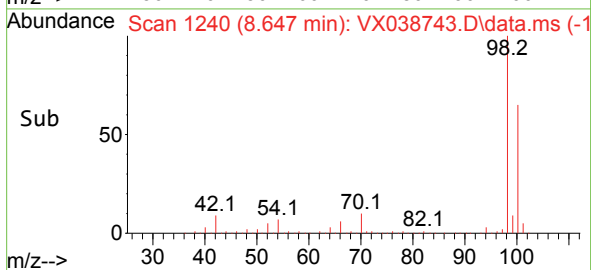






#51
4-Methyl-2-Pentanone
Concen: 0.482 ug/l
RT: 8.580 min Scan# 1229
Delta R.T. 0.006 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47




Instrument :
MSVOA_X
ClientSampleId :
NWB-1979


Tgt Ion: 43 Resp: 1865
Ion Ratio Lower Upper
43 100
58 51.2 30.4 45.6#

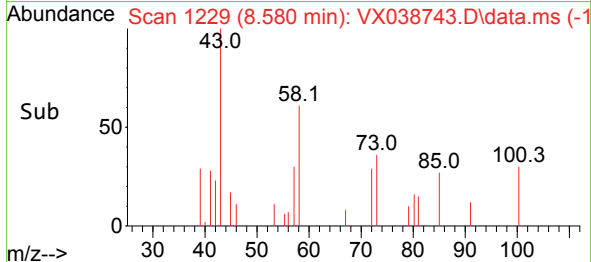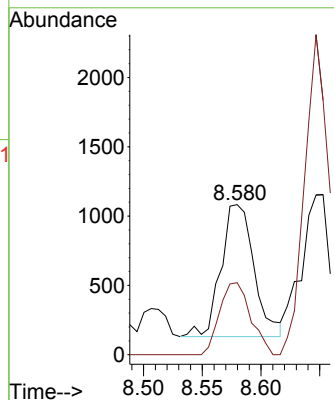

#52
Toluene
Concen: 8.845 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.000 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47

Tgt Ion: 92 Resp: 63171
Ion Ratio Lower Upper
92 100
91 173.3 134.2 201.2


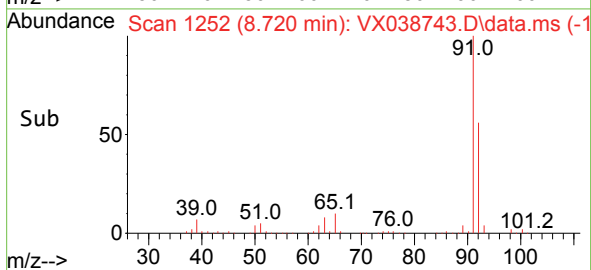
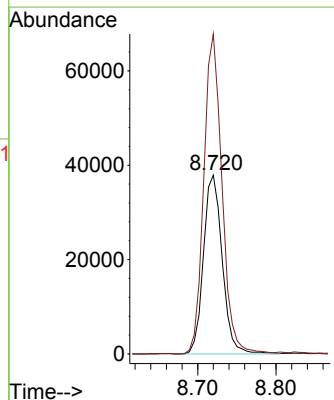





#58
2-Chloroethyl Vinyl ether
Concen: 0.355 ug/l
RT: 8.214 min Scan# 1174
Delta R.T. -0.030 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47




Instrument :
MSVOA_X
ClientSampleId :
NWB-1979


Tgt Ion: 63 Resp: 740
Ion Ratio Lower Upper
63 100
106 0.0 22.5 33.7#

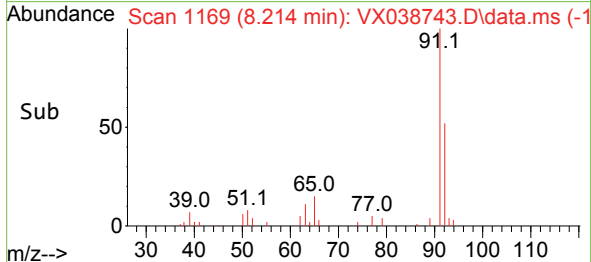

#59
2-Hexanone
Concen: 0.659 ug/l
RT: 9.439 min Scan# 1370
Delta R.T. 0.013 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47

Tgt Ion: 43 Resp: 2064
Ion Ratio Lower Upper
43 100
58 56.7 26.2 78.5

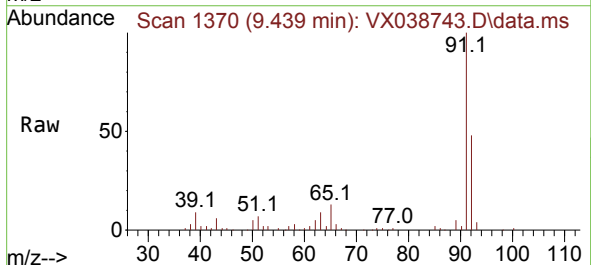



#62

4-Bromofluorobenzene

Concen: 52.443 ug/l

RT: 11.079 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX038743.D

Acq: 10 Nov 2023 20:47

Instrument :

MSVOA_X

ClientSampleId :

NWB-1979





Tgt Ion: 95 Resp: 221711

Ion Ratio Lower Upper

95 100

174 87.8 0.0 135.6

176 84.7 0.0 131.0

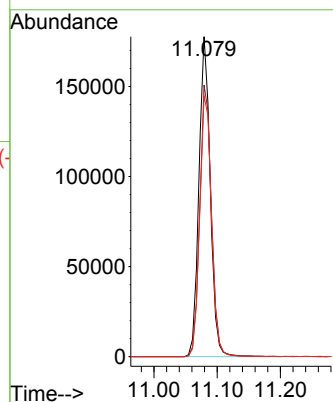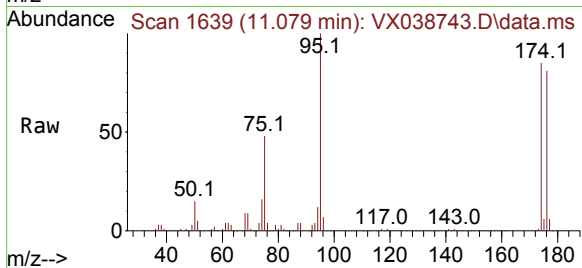

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX038743.D

Acq: 10 Nov 2023 20:47




Tgt Ion: 117 Resp: 445439


Ion Ratio Lower Upper

117 100

82 49.8 46.2 69.4

119 31.9 25.5 38.3


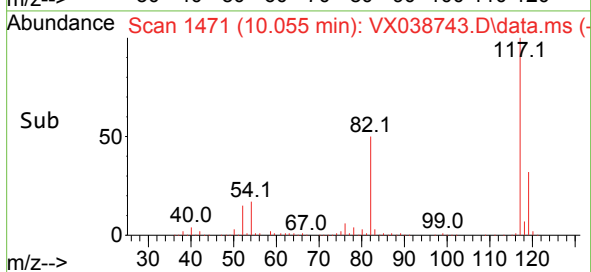
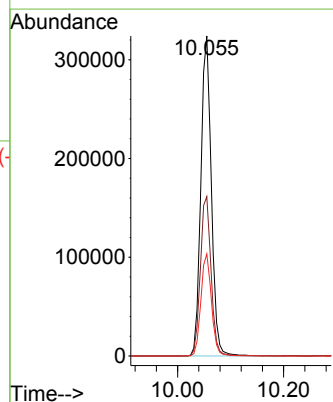
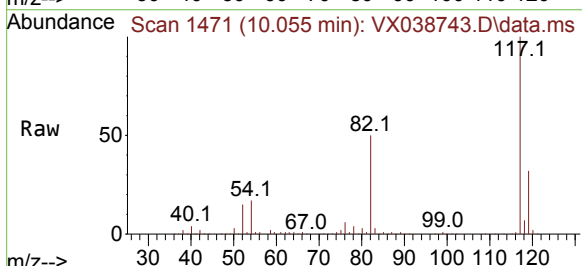




#67
Ethyl Benzene
Concen: 1.377 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47




Instrument :
MSVOA_X
ClientSampleId :
NWB-1979


Tgt Ion: 91 Resp: 21125
Ion Ratio Lower Upper
91 100
106 35.3 24.9 37.3



#68
m/p-Xylenes
Concen: 8.945 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. 0.000 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47

Tgt Ion: 106 Resp: 54454
Ion Ratio Lower Upper
106 100
91 199.9 165.5 248.3


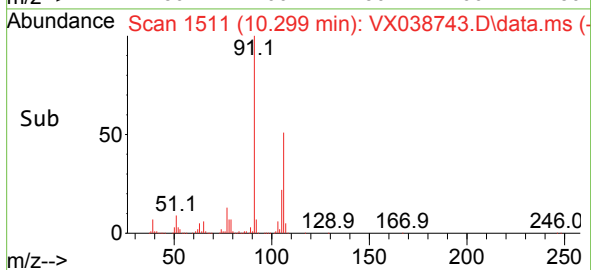






#69
o-Xylene
Concen: 3.751 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47




Instrument :
MSVOA_X
ClientSampleId :
NWB-1979


Tgt Ion:106 Resp: 22205
Ion Ratio Lower Upper
106 100
91 215.5 108.9 326.8

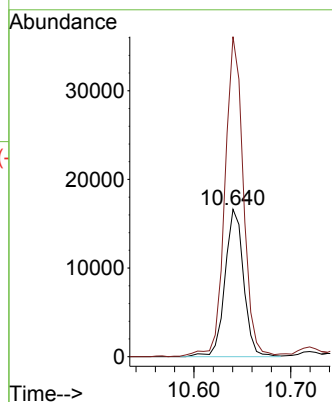

#70
Styrene
Concen: 3.995 ug/l
RT: 10.659 min Scan# 1570
Delta R.T. 0.006 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47

Tgt Ion:104 Resp: 39035
Ion Ratio Lower Upper
104 100
78 45.8 43.6 65.4
103 54.9 43.6 65.4


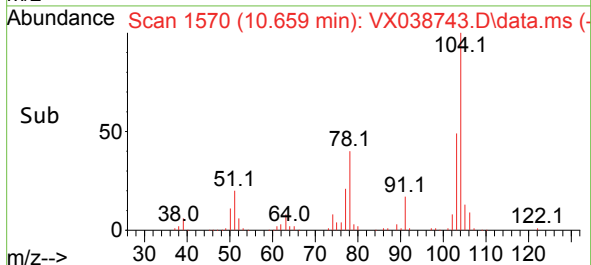






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47




Instrument :
MSVOA_X
ClientSampleId :
NWB-1979


Tgt Ion:152 Resp: 259883
Ion Ratio Lower Upper
152 100
115 57.5 43.3 129.9
150 154.8 0.0 345.0

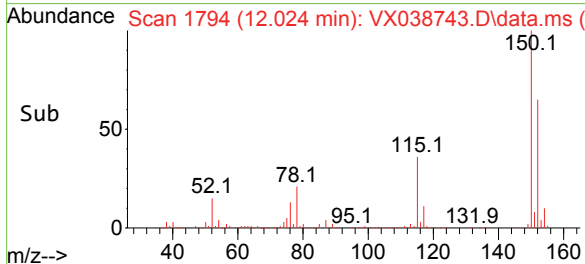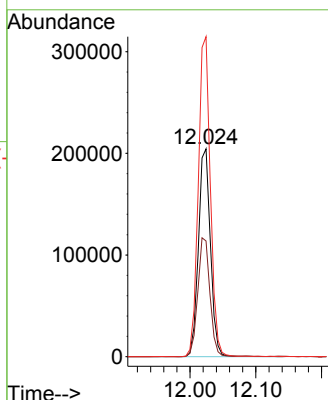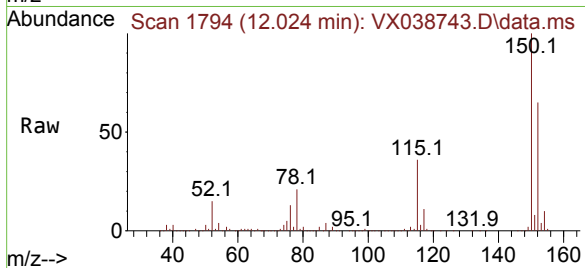

#73
Isopropylbenzene
Concen: 0.202 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47

Tgt Ion:105 Resp: 3217
Ion Ratio Lower Upper
105 100
120 23.4 12.9 38.6

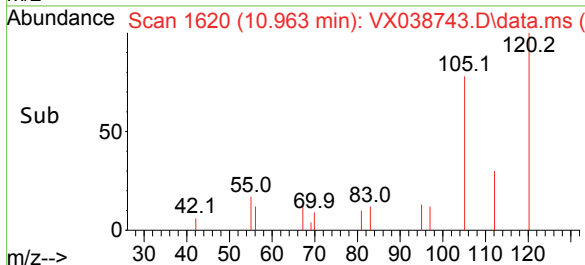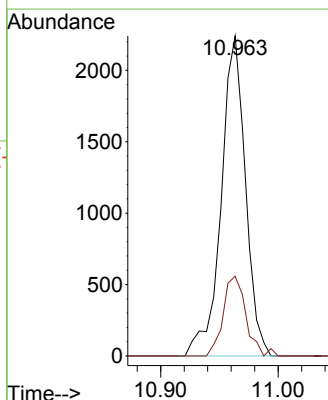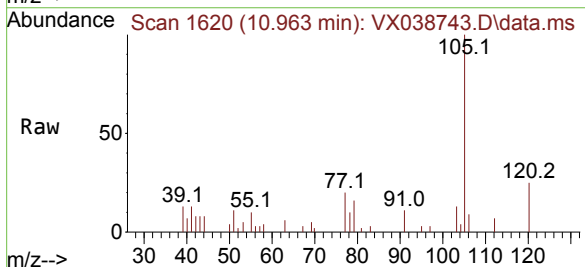



#76

1,2,3-Trichloropropane

Concen: 20.950 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.158 min

Lab File: VX038743.D

Acq: 10 Nov 2023 20:47

Instrument :

MSVOA_X

ClientSampleId :





NWB-1979

Tgt Ion: 75 Resp: 107829

Ion Ratio Lower Upper

75 100

77 1.2 19.1 57.5#

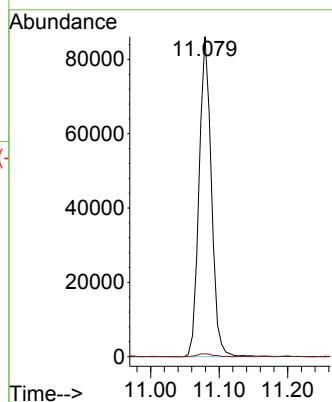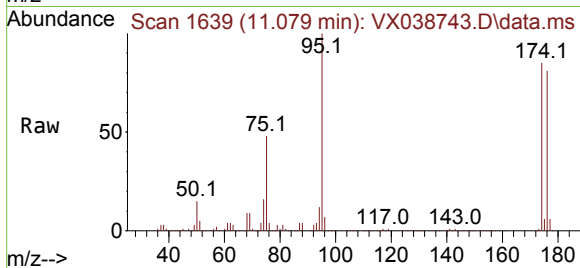

#78

n-propylbenzene

Concen: 0.401 ug/l

RT: 11.311 min Scan# 1677

Delta R.T. 0.006 min

Lab File: VX038743.D




Acq: 10 Nov 2023 20:47


Tgt Ion: 91 Resp: 7431

Ion Ratio Lower Upper

91 100

120 12.9 11.5 34.4


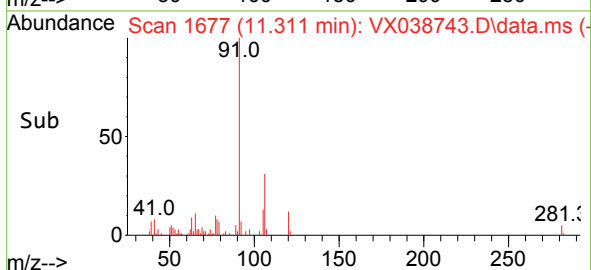

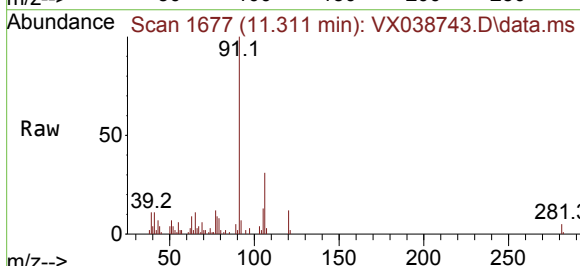




#79
2-Chlorotoluene
Concen: 0.268 ug/l
RT: 11.384 min Scan# 1
Delta R.T. 0.019 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47




Instrument :
MSVOA_X
ClientSampleId :
NWB-1979


Tgt Ion: 91 Resp: 2981
Ion Ratio Lower Upper
91 100
126 0.0 16.3 48.8#

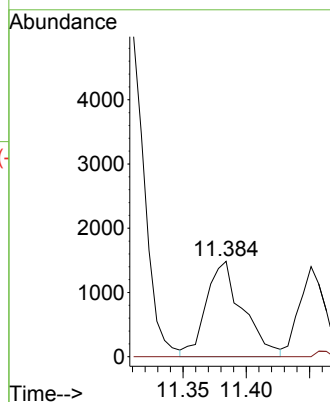

#80
1,3,5-Trimethylbenzene
Concen: 1.133 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47

Tgt Ion: 105 Resp: 15551
Ion Ratio Lower Upper
105 100
120 48.5 24.1 72.3


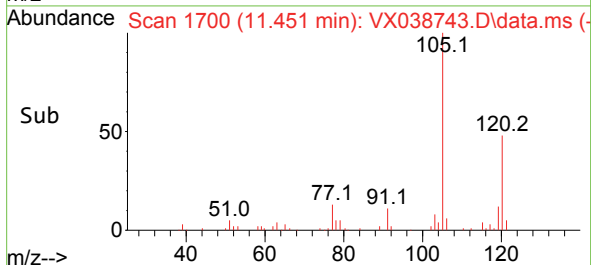
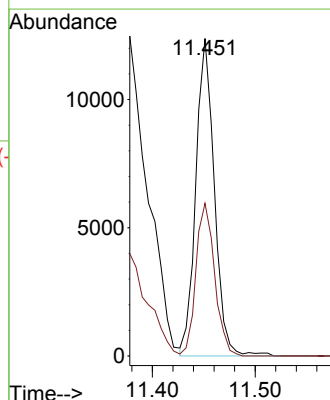





#81
trans-1,4-Dichloro-2-butene
Concen: 63.699 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47




Instrument :
MSVOA_X
ClientSampleId :
NWB-1979


Tgt Ion: 75 Resp: 107829
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 36.9 55.3#

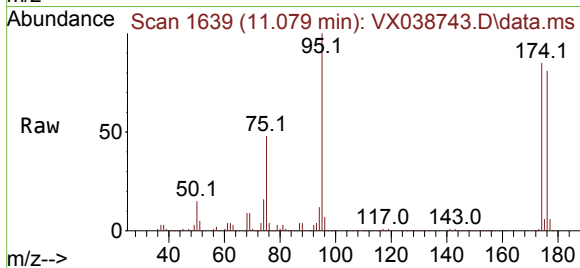

#84
1,2,4-Trimethylbenzene
Concen: 4.183 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VX038743.D
Acq: 10 Nov 2023 20:47

Tgt Ion: 105 Resp: 56936
Ion Ratio Lower Upper
105 100
120 25.7 21.2 63.6




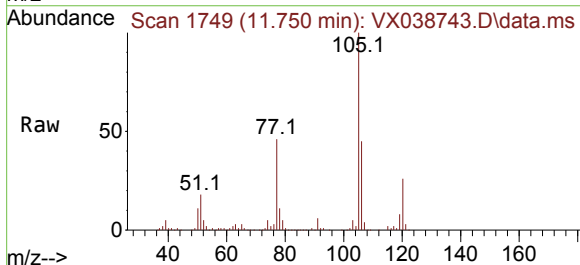


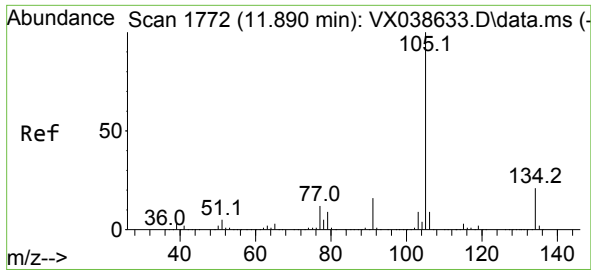

#85
 sec-Butylbenzene
 Concen: 3.282 ug/l
 RT: 11.750 min Scan# 11749
 Delta R.T. -0.140 min
 Lab File: VX038743.D
 Acq: 10 Nov 2023 20:47




Instrument :
 MSVOA_X
 ClientSampleId :
 NWB-1979


Tgt Ion:105 Resp: 56936
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.8 29.4#

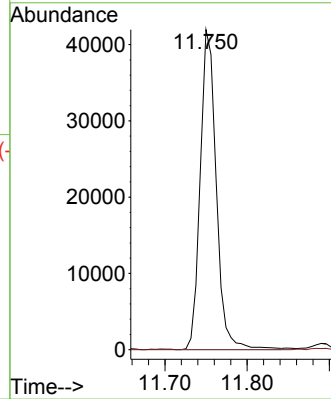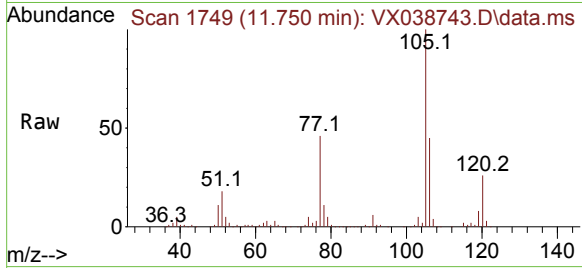

#90
 Hexachloroethane
 Concen: 0.230 ug/l
 RT: 12.530 min Scan# 1877
 Delta R.T. -0.006 min
 Lab File: VX038743.D
 Acq: 10 Nov 2023 20:47

Tgt Ion:117 Resp: 577
 Ion Ratio Lower Upper
 117 100
 201 0.0 32.9 98.6#

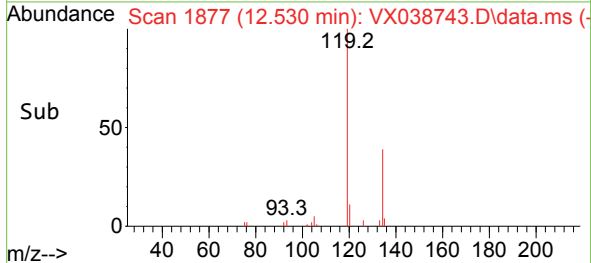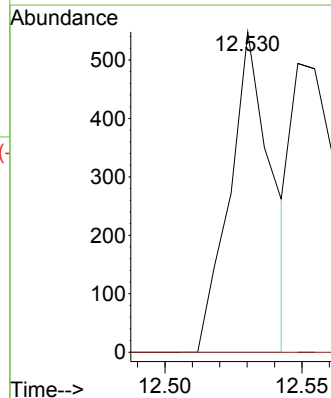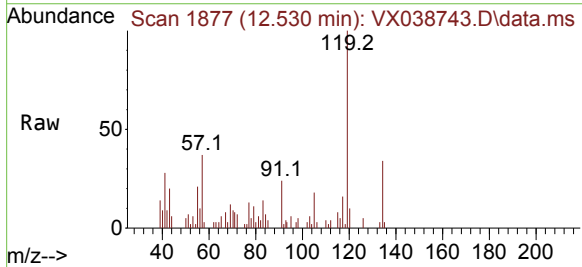

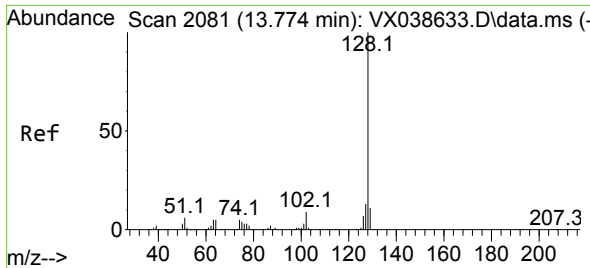

#95

Naphthalene

Concen: 5.002 ug/l

RT: 13.774 min Scan# 2081

Delta R.T. 0.000 min

Lab File: VX038743.D


Acq: 10 Nov 2023 20:47

Instrument :

MSVOA_X

ClientSampleId :

NWB-1979

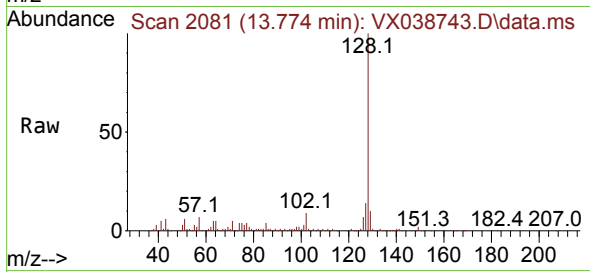

Tgt Ion:128 Resp: 88176

Ion Ratio Lower Upper

128 100

127 13.4 10.3 15.5

129 11.4 8.8 13.2

