

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111023\
 Data File : VX038734.D
 Acq On : 10 Nov 2023 17:20
 Operator : JC/MD
 Sample : 05348-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BPOW5-3-20231108

Quant Time: Nov 11 01:57:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 08 03:19:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	271842	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	449104	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	461950	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	263113	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	156097	46.123	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	92.240%
35) Dibromofluoromethane	5.391	113	145606	45.015	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	90.040%
50) Toluene-d8	8.646	98	529458	45.743	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	91.480%#
62) 4-Bromofluorobenzene	11.079	95	224063	49.929	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.860%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111023\
Data File : VX038734.D
Acq On : 10 Nov 2023 17:20
Operator : JC/MD
Sample : 05348-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPOW5-3-20231108

Quant Time: Nov 11 01:57:05 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 08 03:19:07 2023
Response via : Initial Calibration




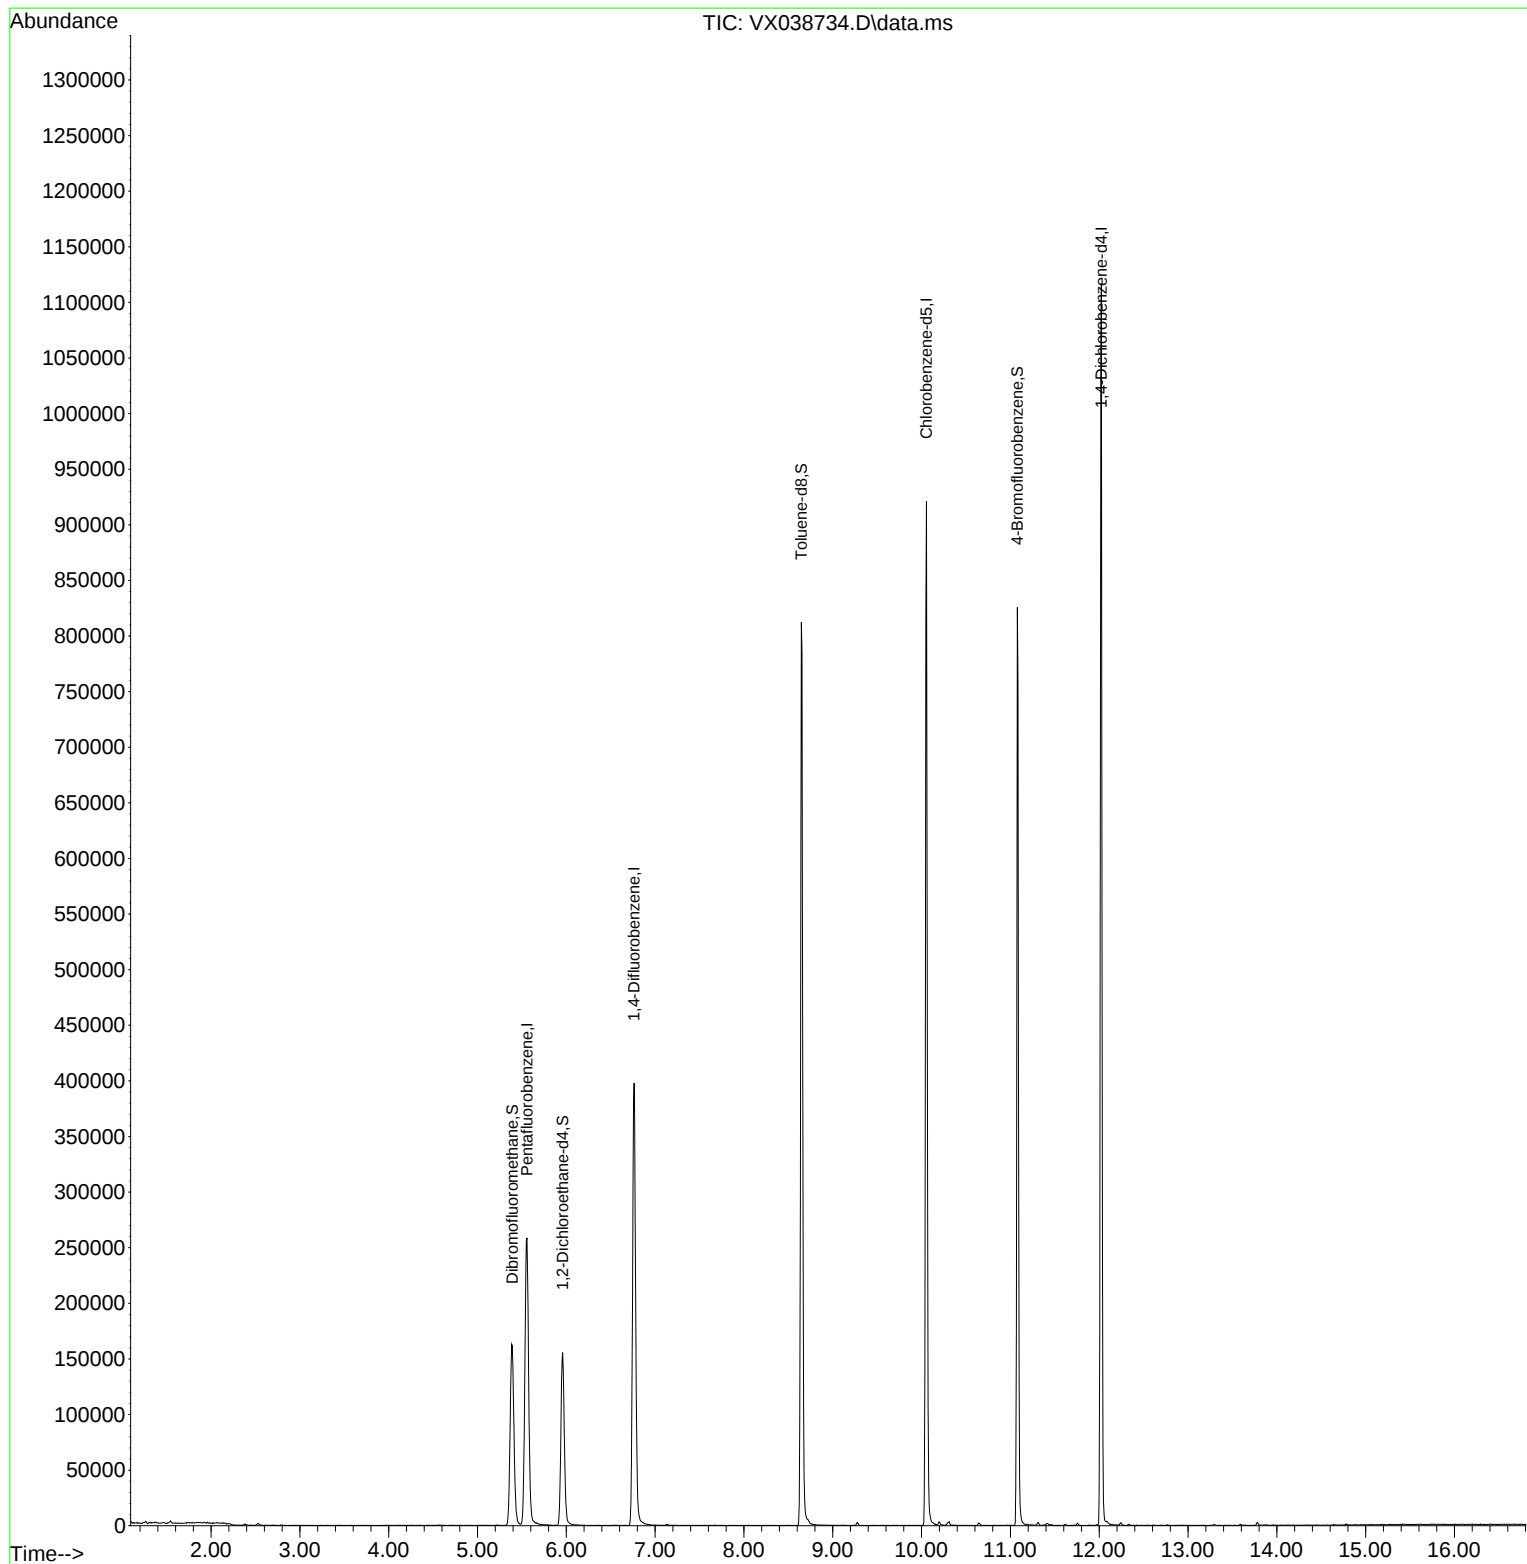


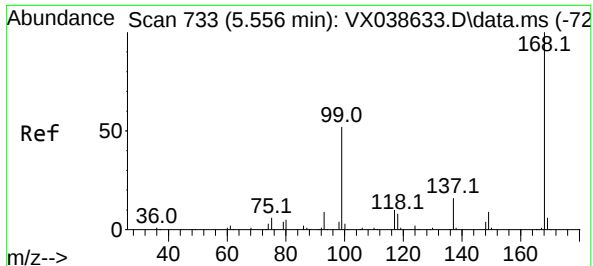

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.000 min
Lab File: VX038734.D
Acq: 10 Nov 2023 17:20




Instrument :
MSVOA_X
ClientSampleId :
BPOW5-3-20231108


Tgt Ion:168 Resp: 271842
Ion Ratio Lower Upper
168 100
99 50.3 56.6 85.0#

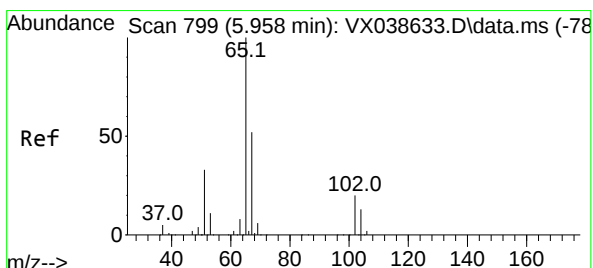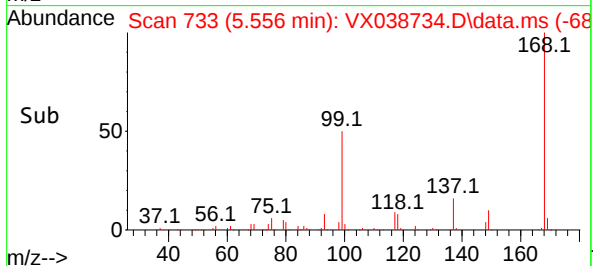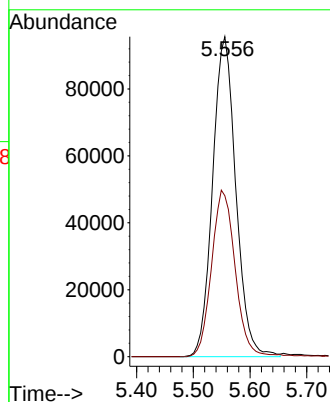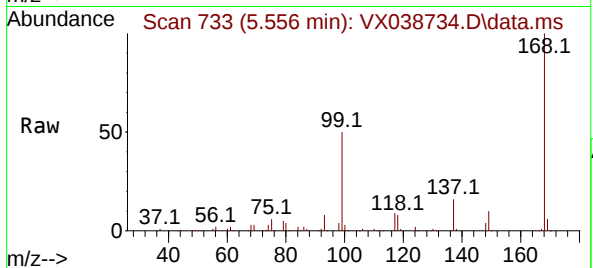

#33
1,2-Dichloroethane-d4
Concen: 46.123 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX038734.D
Acq: 10 Nov 2023 17:20

Tgt Ion: 65 Resp: 156097
Ion Ratio Lower Upper
65 100
67 51.9 0.0 100.2


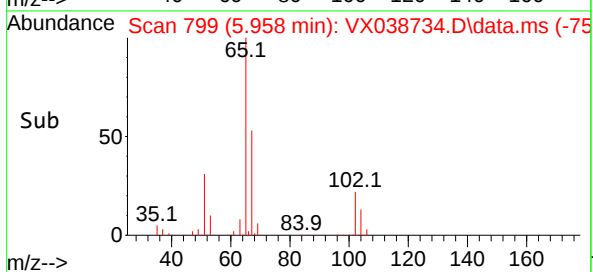
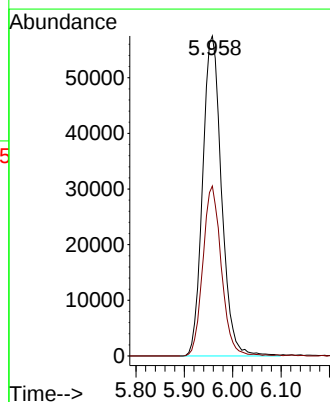
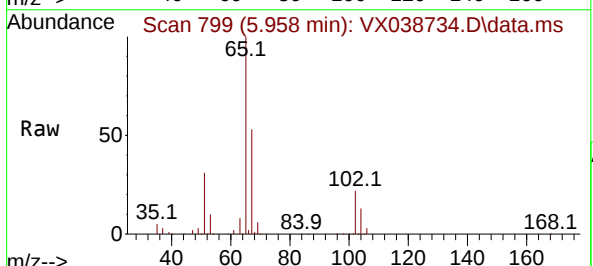


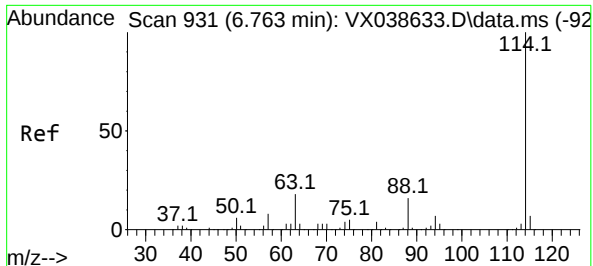

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX038734.D
Acq: 10 Nov 2023 17:20




Instrument :
MSVOA_X
ClientSampleId :
BPOW5-3-20231108


Tgt Ion:114 Resp: 449104
Ion Ratio Lower Upper
114 100
63 17.4 0.0 45.0
88 15.1 0.0 36.6

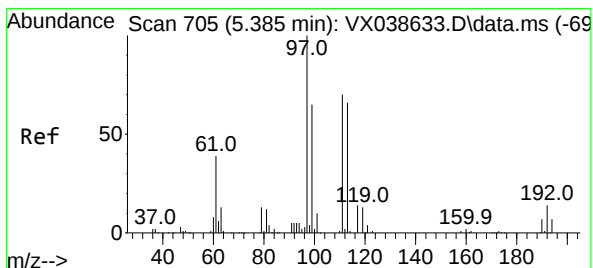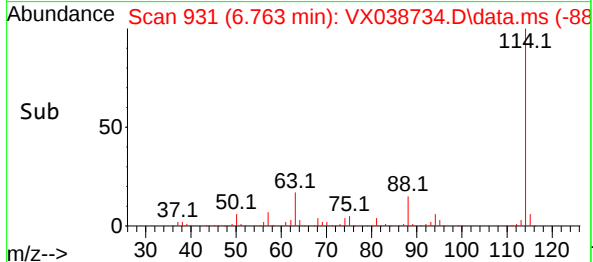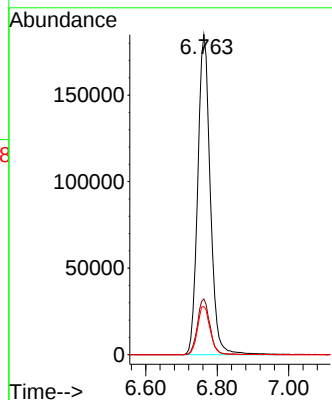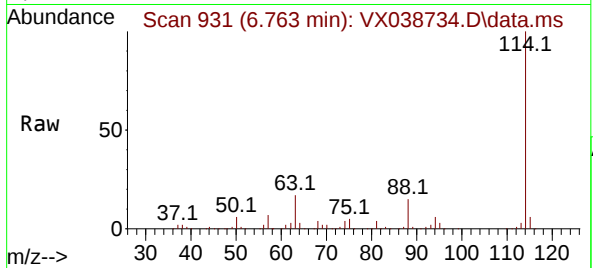

#35
Dibromofluoromethane
Concen: 45.015 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX038734.D
Acq: 10 Nov 2023 17:20

Tgt Ion:113 Resp: 145606
Ion Ratio Lower Upper
113 100
111 103.7 82.9 124.3
192 21.3 13.3 19.9#


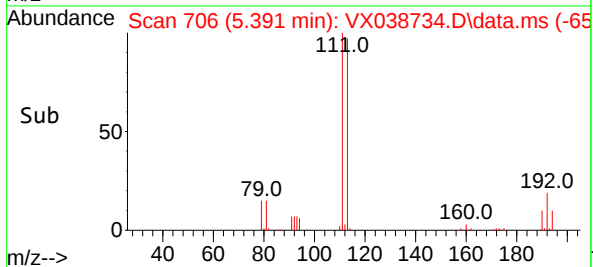
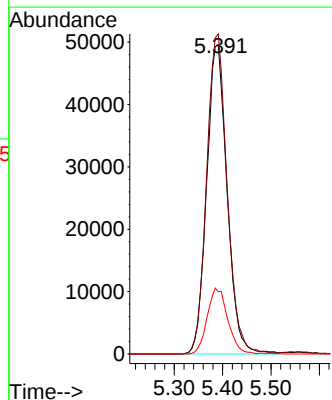
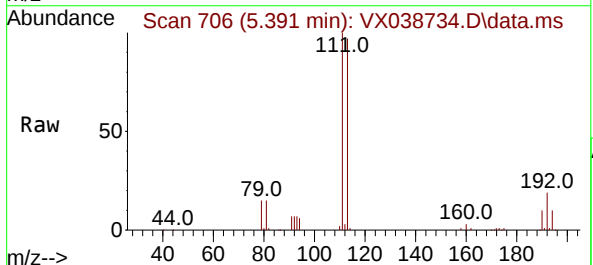


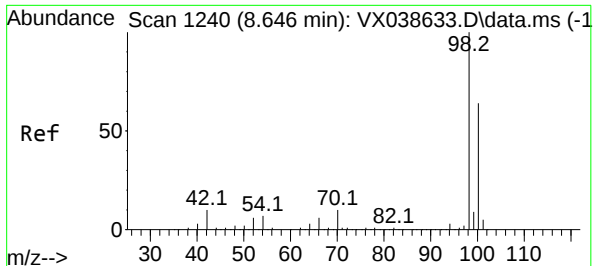

#50
Toluene-d8
Concen: 45.743 ug/l
RT: 8.646 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX038734.D
Acq: 10 Nov 2023 17:20




Instrument :
MSVOA_X
ClientSampleId :
BPOW5-3-20231108


Tgt Ion: 98 Resp: 529458
Ion Ratio Lower Upper
98 100
100 65.3 53.1 79.7

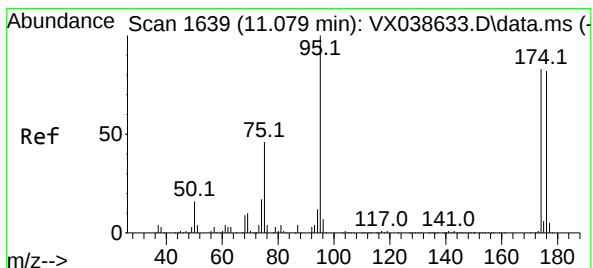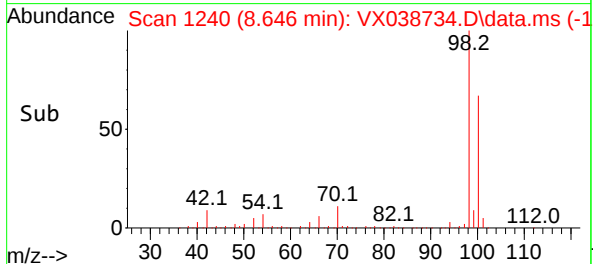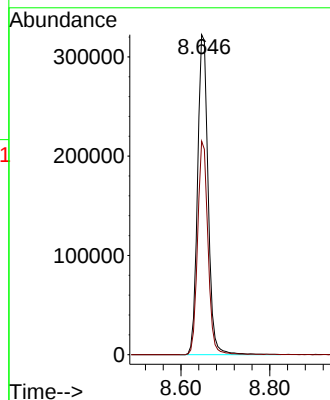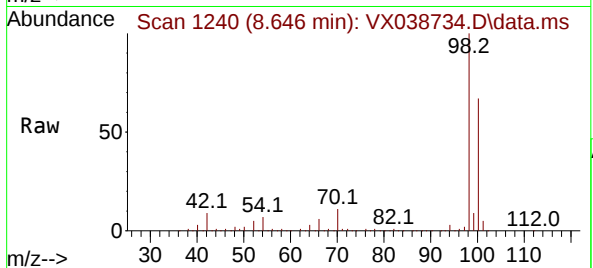

#62
4-Bromofluorobenzene
Concen: 49.929 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX038734.D
Acq: 10 Nov 2023 17:20

Tgt Ion: 95 Resp: 224063
Ion Ratio Lower Upper
95 100
174 88.1 0.0 135.6
176 84.0 0.0 131.0

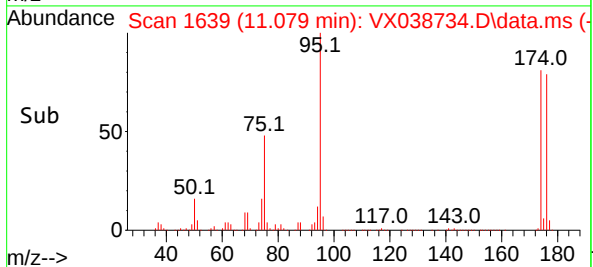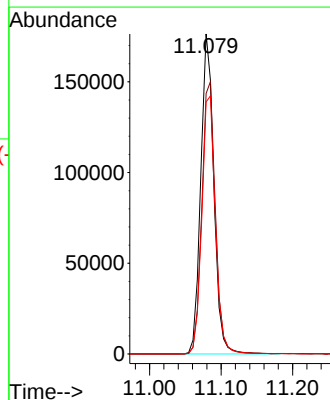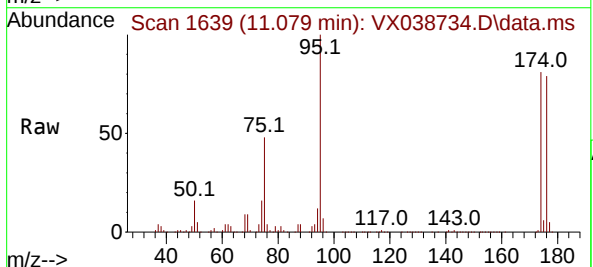

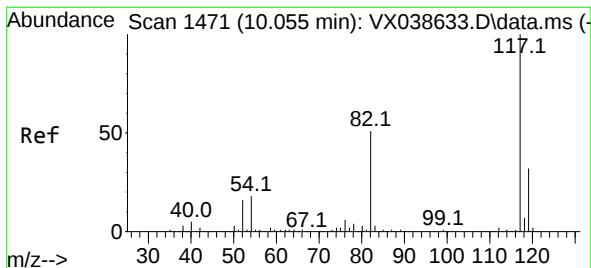

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX038734.D

Acq: 10 Nov 2023 17:20

Instrument :

MSVOA_X

ClientSampleId :

BPOW5-3-20231108





Tgt Ion:117 Resp: 461950

Ion Ratio Lower Upper

117 100

82 49.9 46.2 69.4

119 32.5 25.5 38.3

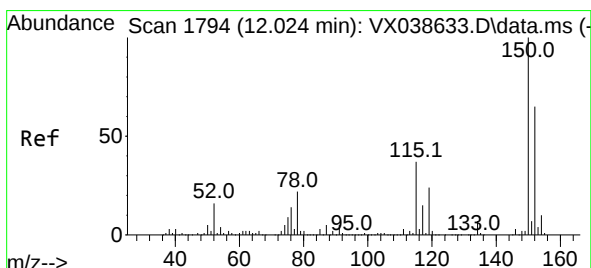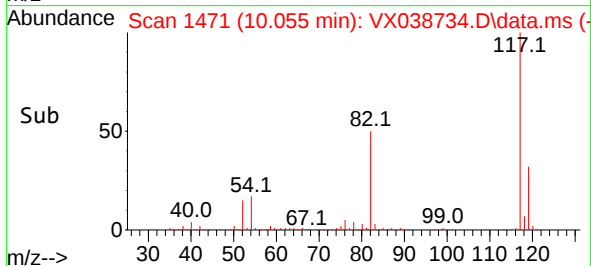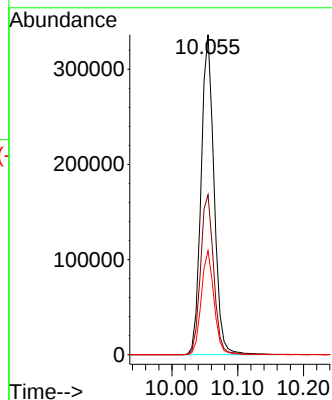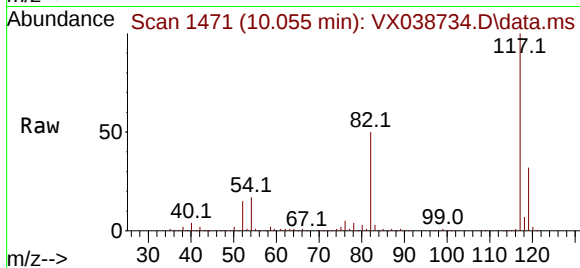

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX038734.D

Acq: 10 Nov 2023 17:20

Tgt Ion:152 Resp: 263113

Ion Ratio Lower Upper

152 100

115 58.0 43.3 129.9

150 154.8 0.0 345.0

