

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111023\
 Data File : VX038751.D
 Acq On : 11 Nov 2023 02:05
 Operator : JC/MD
 Sample : 05241-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FSND-RB-4-20231102

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M

Title : SW846 8260

Signal : TIC: VX038751.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.526	229	236	244	rBV2	12048	22783	1.56%	0.299%
2	5.385	693	705	722	rBV	159761	465472	31.78%	6.101%
3	5.550	722	732	748	rBV	249189	712269	48.62%	9.336%
4	5.958	788	799	812	rBV	146148	394988	26.96%	5.177%
5	6.763	921	931	957	rBV	383227	933279	63.71%	12.233%
6	8.647	1234	1240	1249	rBV	804107	1272995	86.90%	16.686%
7	8.720	1249	1252	1267	rVB	12497	25657	1.75%	0.336%
8	10.055	1465	1471	1487	rBV	902727	1254964	85.67%	16.450%
9	11.079	1634	1639	1655	rBV	834255	1066874	72.83%	13.984%
10	11.311	1670	1677	1683	rVB2	10489	14990	1.02%	0.196%
11	12.018	1788	1793	1814	rBV	1103507	1464848	100.00%	19.201%




Sum of corrected areas: 7629119

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111023\
Data File : VX038751.D
Acq On : 11 Nov 2023 02:05
Operator : JC/MD
Sample : 05241-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-RB-4-20231102

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

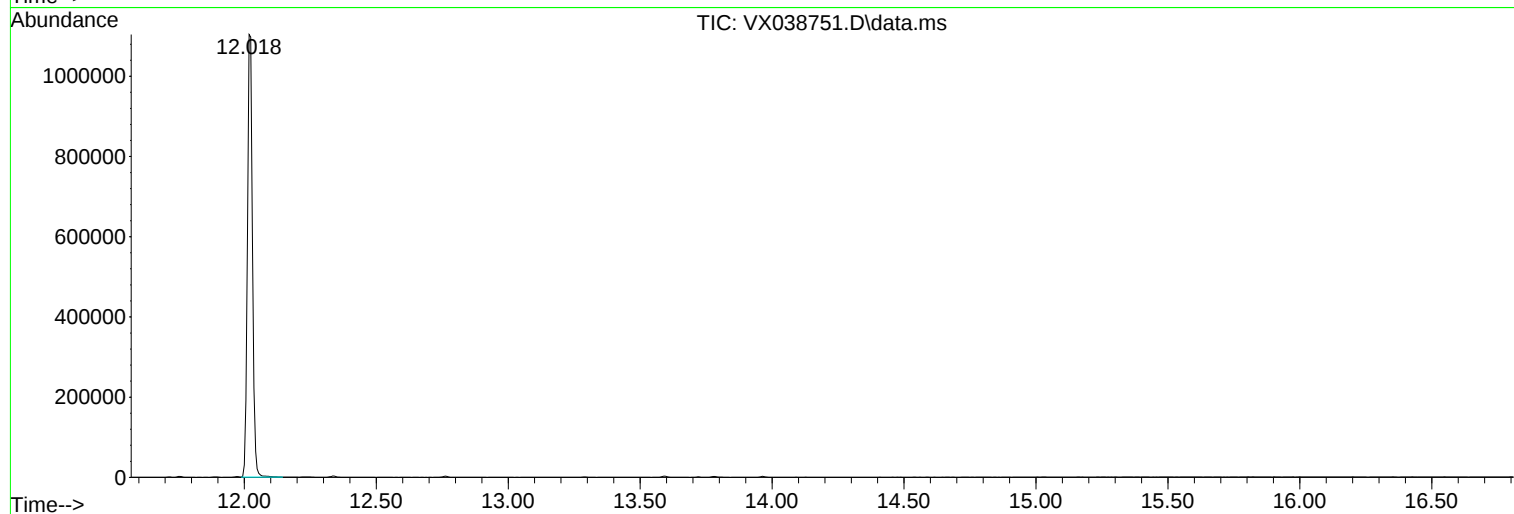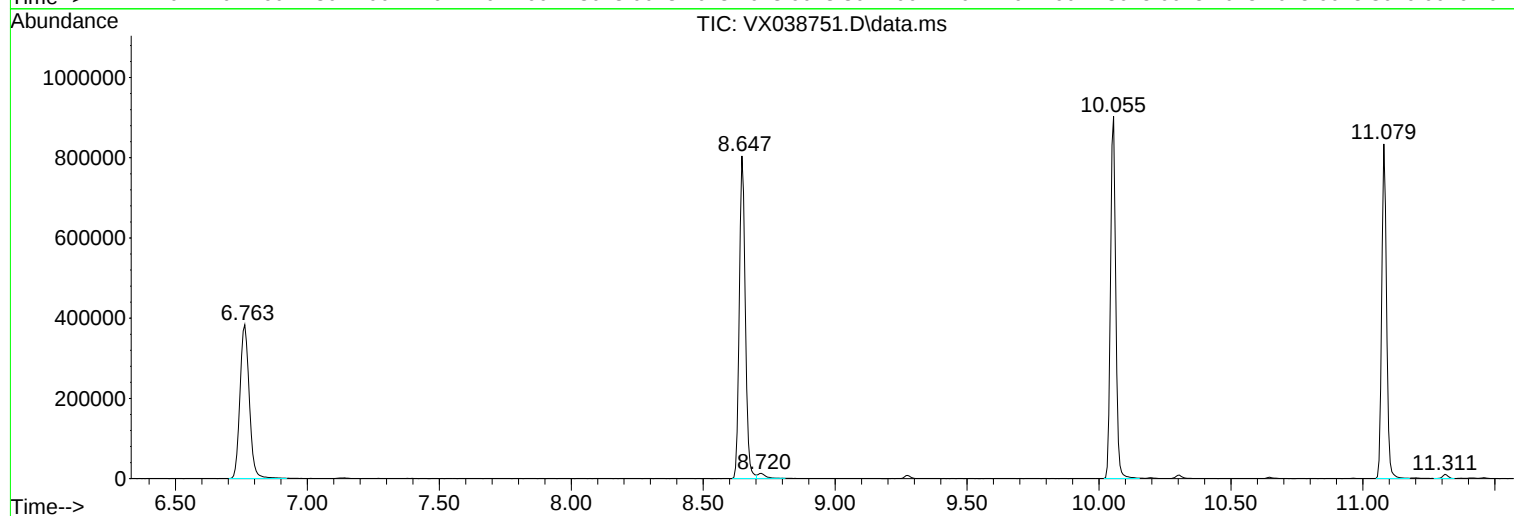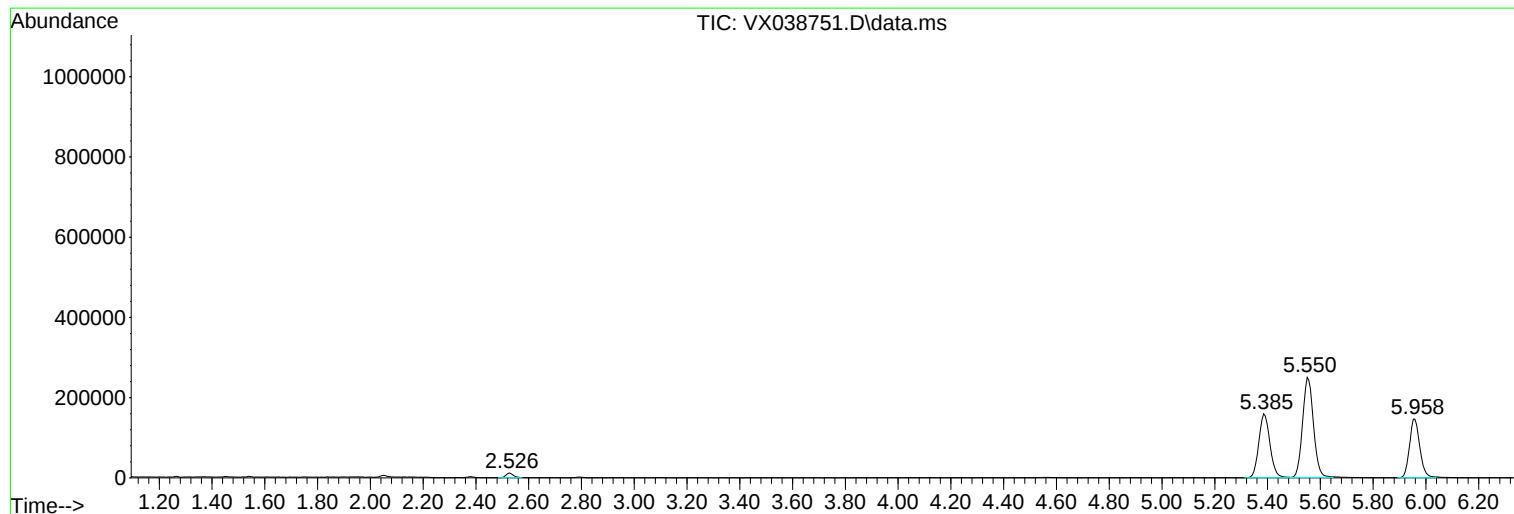

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111023\
Data File : VX038751.D
Acq On : 11 Nov 2023 02:05
Operator : JC/MD
Sample : 05241-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-RB-4-20231102

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111023\
Data File : VX038751.D
Acq On : 11 Nov 2023 02:05
Operator : JC/MD
Sample : 05241-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-RB-4-20231102

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------