
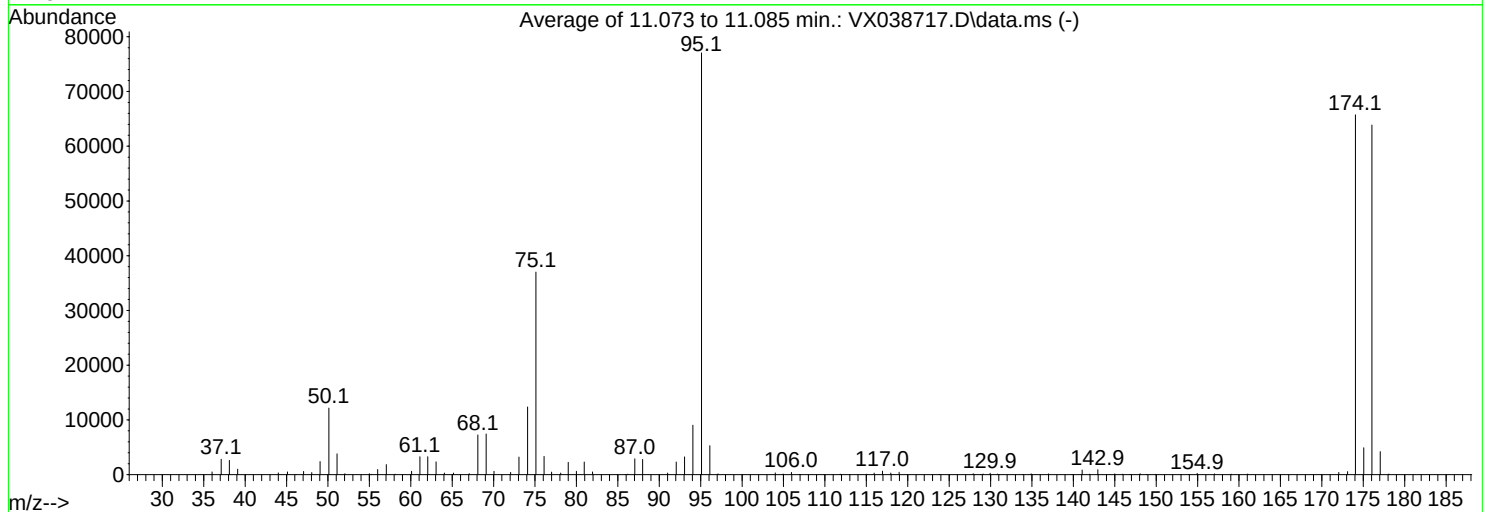


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111023\
Data File : VX038717.D
Acq On : 10 Nov 2023 10:05
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M
Title : SW846 8260
Last Update : Wed Nov 08 03:19:07 2023

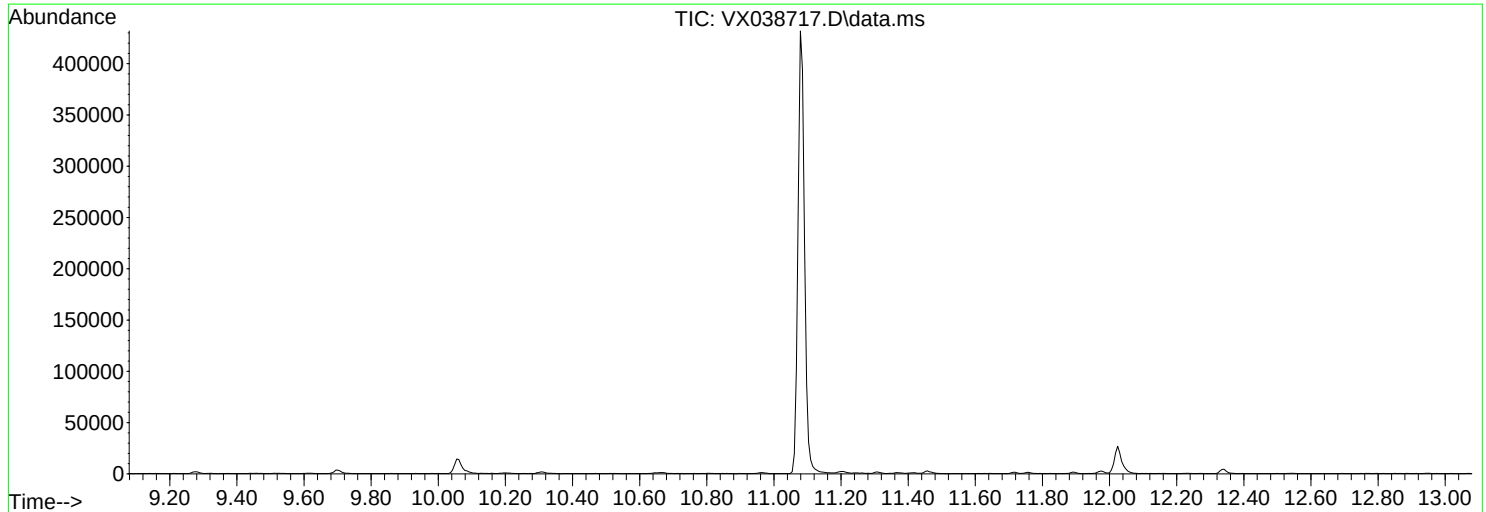

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	12153	PASS
75	95	30	60	48.0	37003	PASS
95	95	100	100	100.0	77059	PASS
96	95	5	9	6.9	5302	PASS
173	174	0.00	2	0.8	551	PASS
174	95	50	100	85.3	65741	PASS
175	174	5	9	7.5	4913	PASS
176	174	95	101	97.2	63877	PASS
177	176	5	9	6.6	4216	PASS