

(QT Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\ VX111121\  
Data File : VX025134.D  
Acq On : 11 Nov 2021 16:42  
Operator : JC/MD  
Sample : VSTDCCC050  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 10 Sample Multiplier: 1

**Instrument :**  
MSVOA\_X  
**LabSampleId :**  
VSTDCCC050

Quant Time: Nov 12 05:05:21 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXLM111121WMA.M  
Quant Title : VOC Analysis  
QLast Update : Thu Nov 11 16:29:23 2021  
Response via : Initial Calibration

## Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/12/2021  
Supervised By :Mahesh Dadoda 11/12/2021

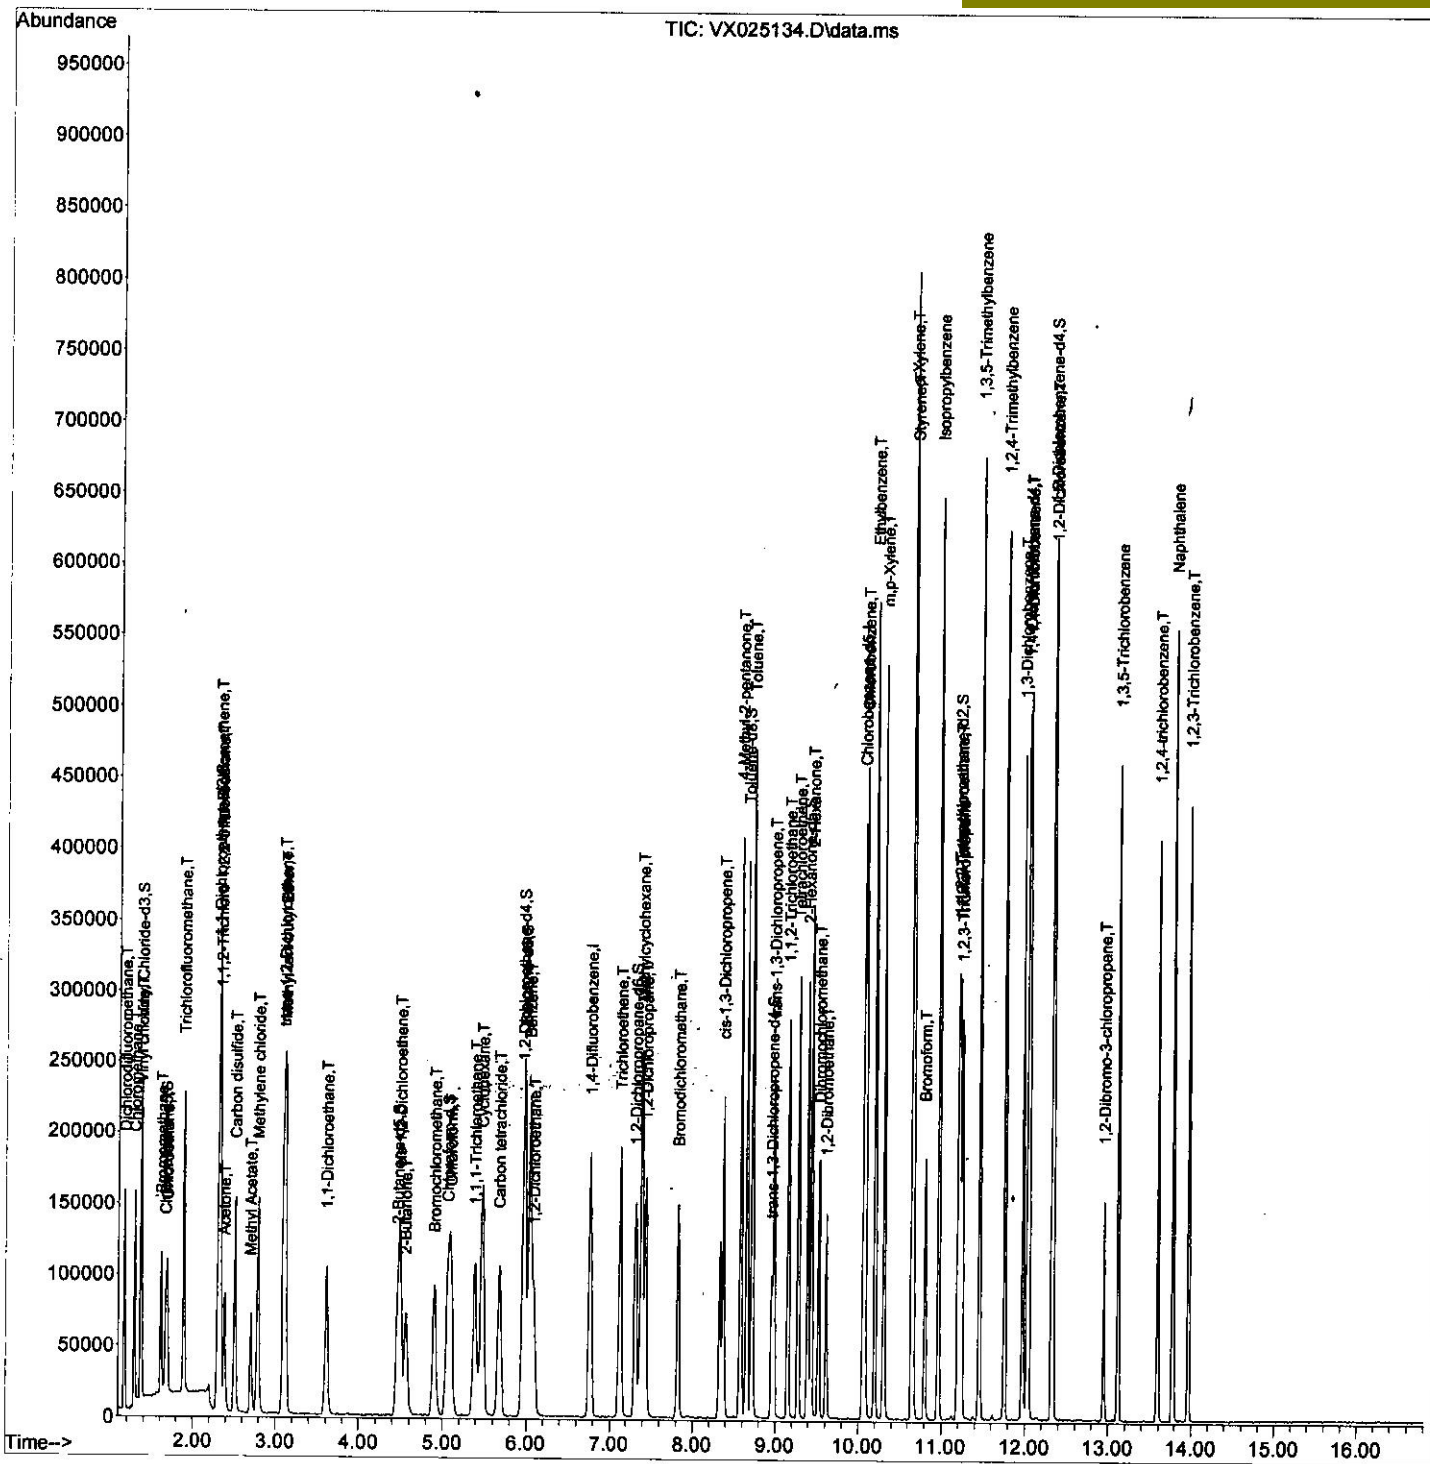

## Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX111121\  
Data File : VX025134.D  
Acq On : 11 Nov 2021 16:42  
Operator : JC/MD  
Sample : VSTDCCC050  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
LabSampleId :  
VSTDCCC050

Quant Time: Nov 12 05:05:21 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXLM111121WMA.M  
Quant Title : VOC Analysis  
QLast Update : Thu Nov 11 16:29:23 2021  
Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/12/2021  
Supervised By :Mahesh Dadoda 11/12/2021

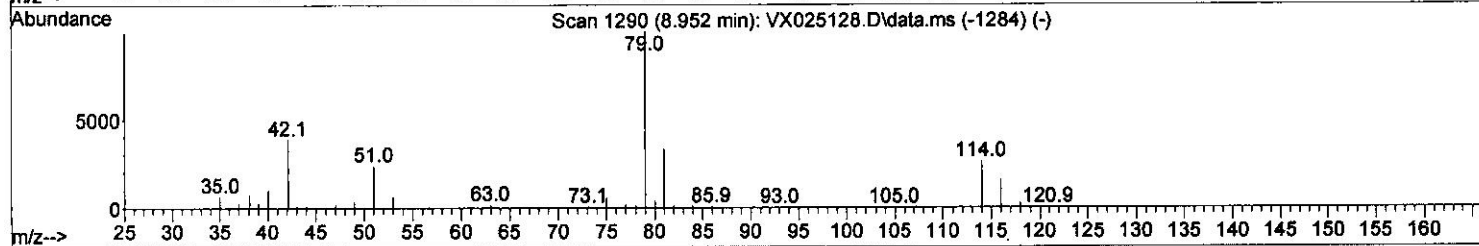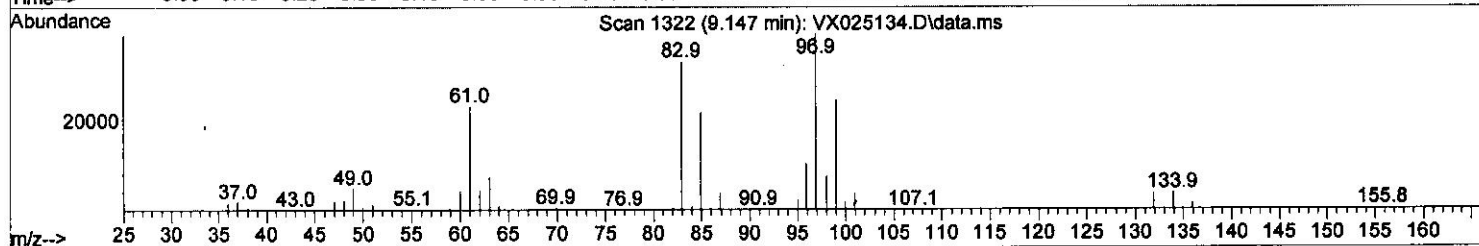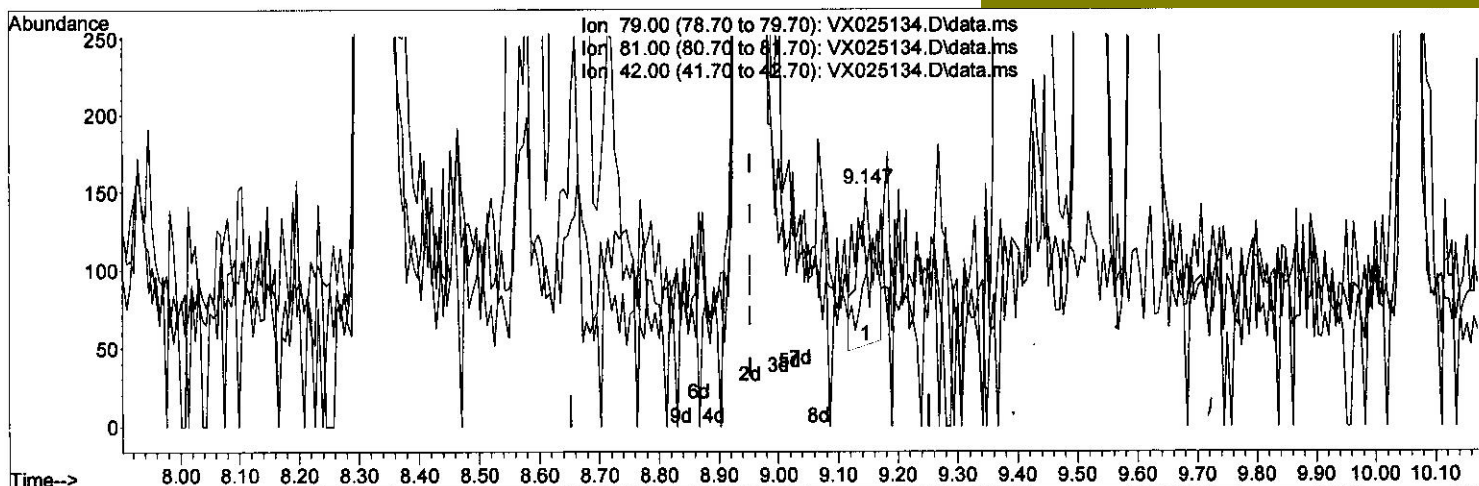

TIC: VX025134.D\data.ms

(43) trans-1,3-Dichloropropene-d4 (S)

9.147min (+ 0.195) 0.25 ug/L

response 214

Ion	Exp%	Act%
79.00	100.00	100.00
81.00	33.30	33.64
42.00	28.20	27.10
0.00	0.00	0.00

# Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX111121\  
 Data File : VX025134.D  
 Acq On : 11 Nov 2021 16:42  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 LabSampleId :  
 VSTDCCC050

Quant Time: Nov 12 05:05:21 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXLM111121WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Thu Nov 11 16:29:23 2021  
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/12/2021  
 Supervised By :Mahesh Dadoda 11/12/2021

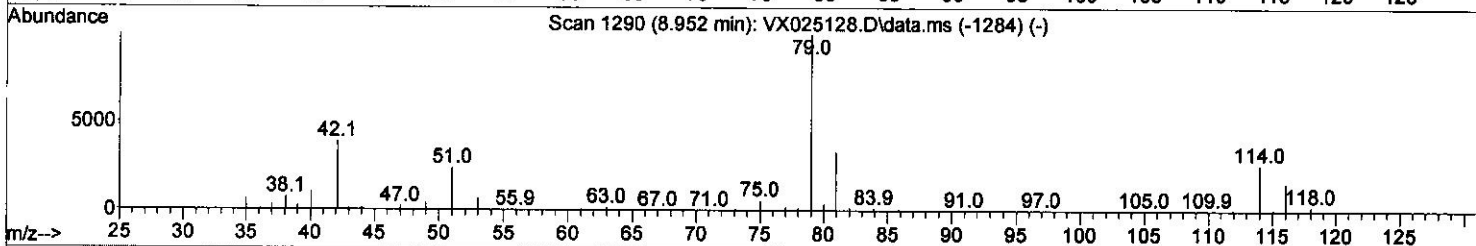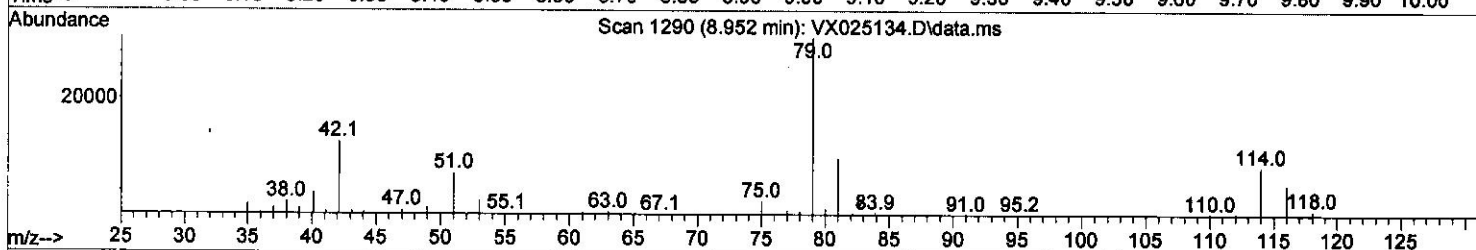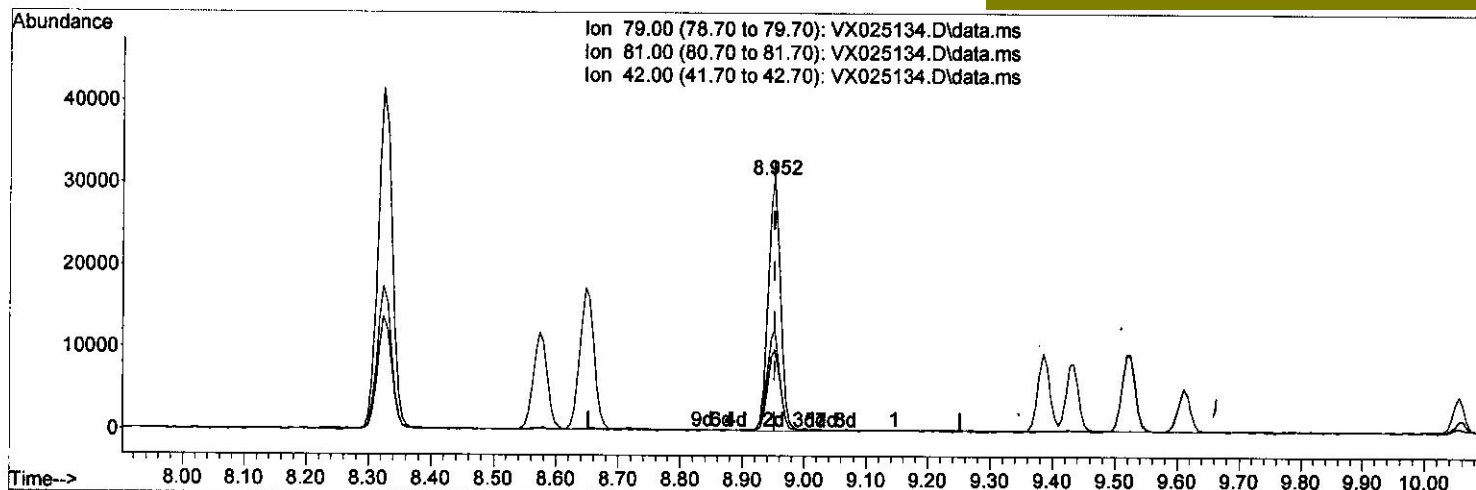

TIC: VX025134.D\data.ms

(43) trans-1,3-Dichloropropene-d4 (S)

8.952min (-0.000) 52.10 ug/L m

response 43823

Ion	Exp%	Act%
79.00	100.00	100.00
81.00	33.30	0.16#
42.00	28.20	0.13#
0.00	0.00	0.00

# Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX111121\  
 Data File : VX025134.D  
 Acq On : 11 Nov 2021 16:42  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 LabSampleId :  
 VSTDCCC050

Quant Time: Nov 12 05:05:21 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXLM111121WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Thu Nov 11 16:29:23 2021  
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/12/2021  
 Supervised By :Mahesh Dadoda 11/12/2021

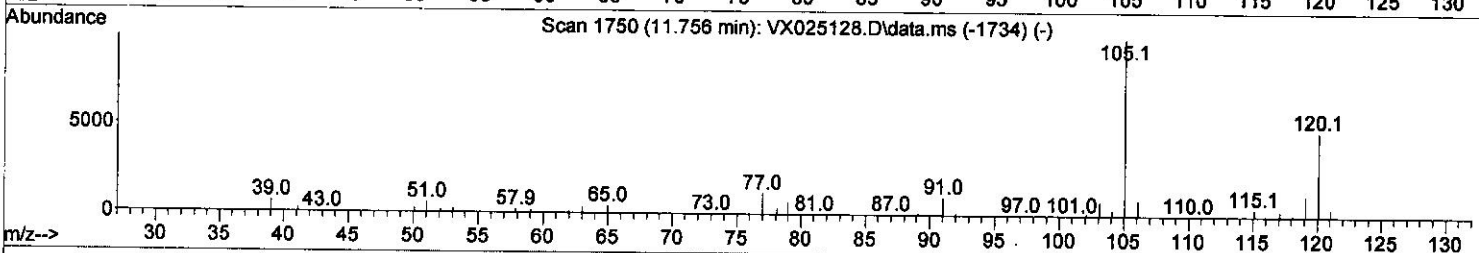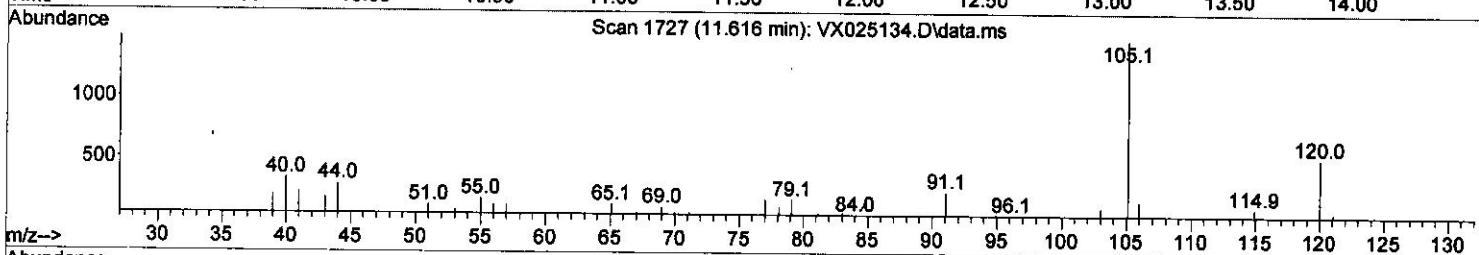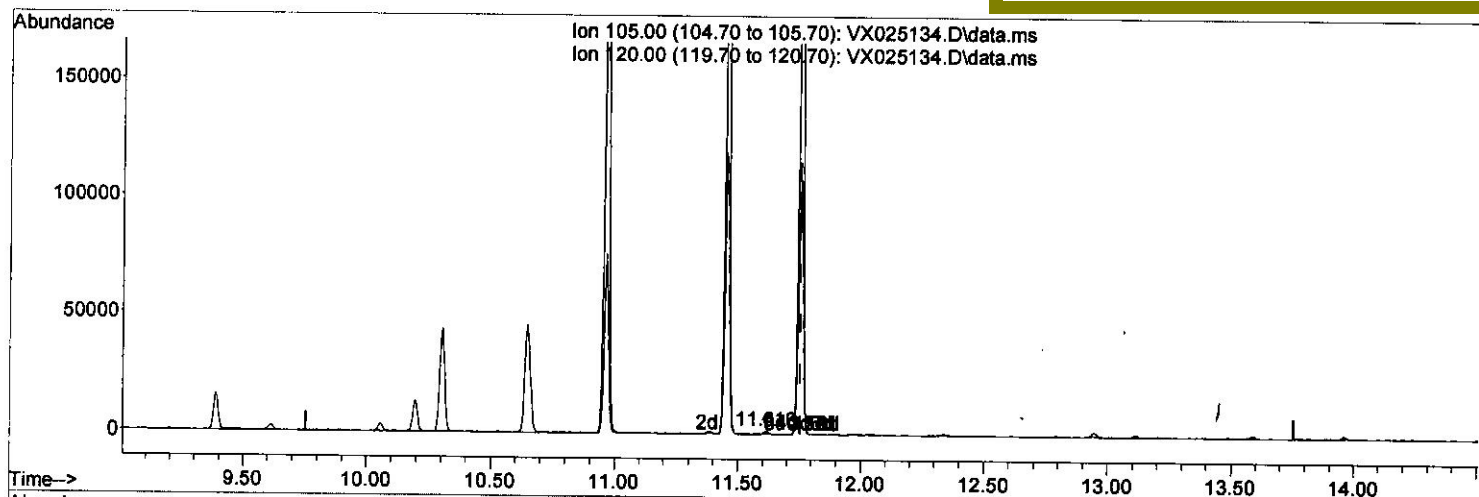

TIC: VX025134.D\data.ms

(63) 1,2,4-Trimethylbenzene

11.616min (-0.140) 0.32 ug/L

response 1891

Ion	Exp%	Act%
105.00	100.00	100.00
120.00	38.80	34.58
0.00	0.00	0.00
0.00	0.00	0.00



# Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX111121\  
 Data File : VX025134.D  
 Acq On : 11 Nov 2021 16:42  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 LabSampleId :  
 VSTDCCC050

Quant Time: Nov 12 05:05:21 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXLM111121WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Thu Nov 11 16:29:23 2021  
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/12/2021  
 Supervised By :Mahesh Dadoda 11/12/2021

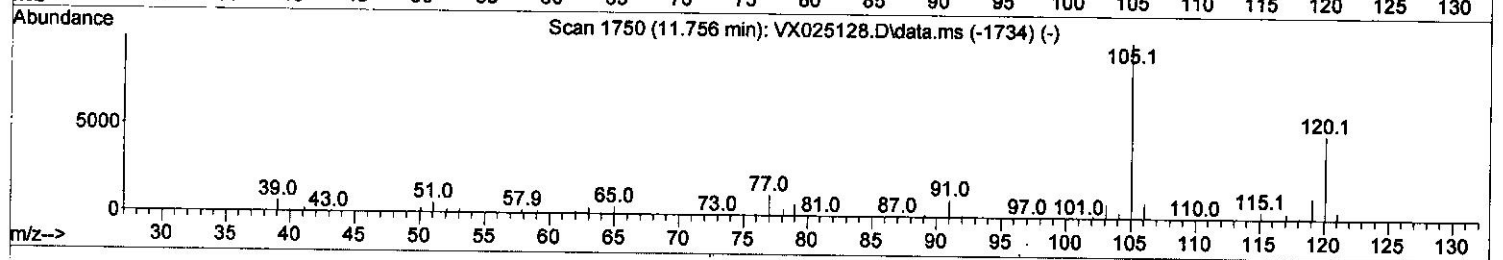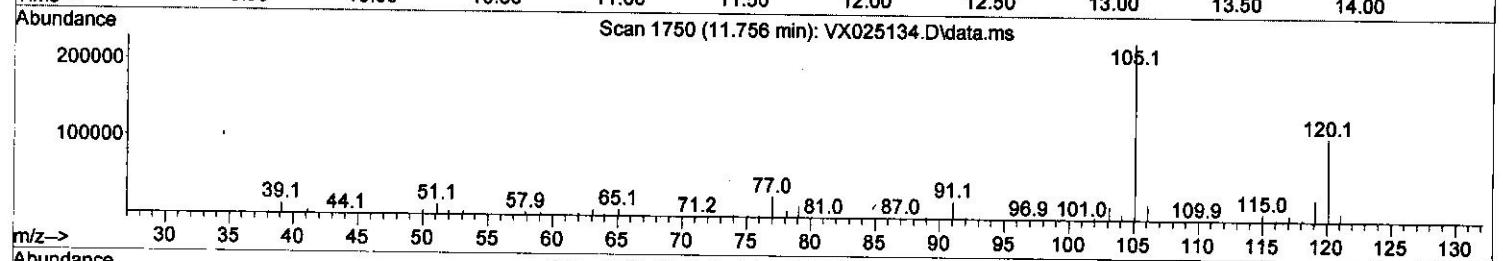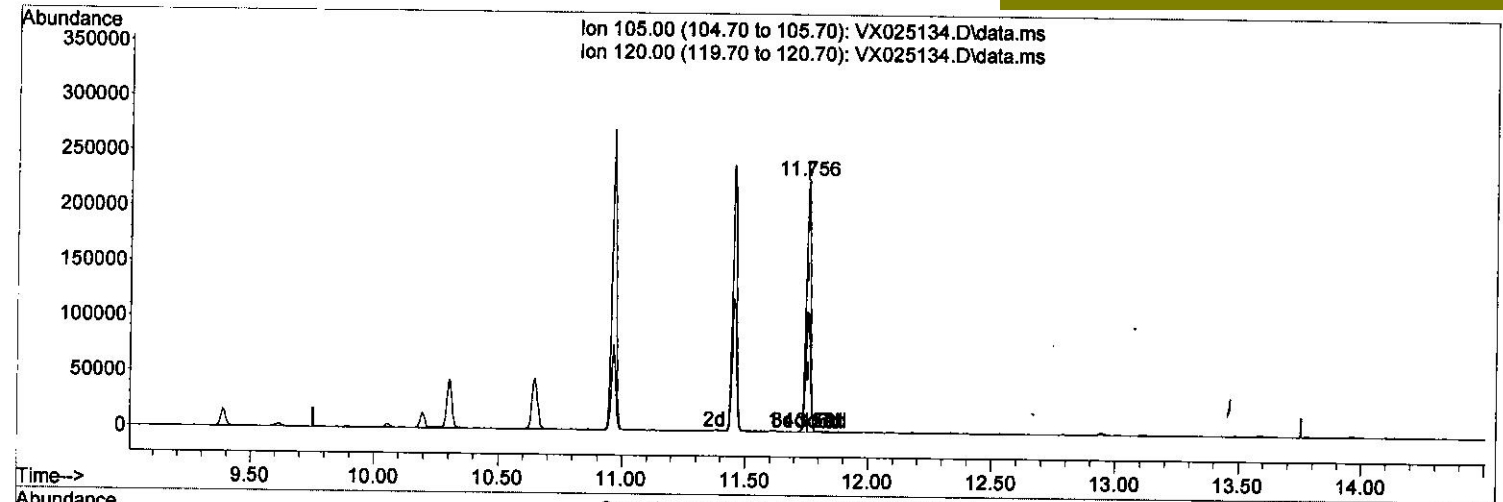

TIC: VX025134.D\data.ms

(63) 1,2,4-Trimethylbenzene

11.756min (+ 0.000) 48.61 ug/L m

response 285888

Ion	Exp%	Act%
105.00	100.00	100.00
120.00	38.80	0.23#
0.00	0.00	0.00
0.00	0.00	0.00

## Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX111121\  
 Data File : VX025134.D  
 Acq On : 11 Nov 2021 16:42  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 LabSampleId :  
 VSTDCCC050

Quant Time: Nov 12 05:05:21 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXLM111121WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Thu Nov 11 16:29:23 2021  
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/12/2021  
 Supervised By : Mahesh Dadoda 11/12/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	200997	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	185942	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	96615	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	67052	49.379	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 98.760%			
7) Chloroethane-d5	1.666	69	47784	61.744	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 123.480%			
11) 1,1-Dichloroethene-d2	2.307	63	114298	48.940	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 97.880%			
21) 2-Butanone-d5	4.459	46	114297	111.384	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 111.380%			
24) Chloroform-d	5.056	84	122203	51.156	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 102.320%			
26) 1,2-Dichloroethane-d4	5.958	65	74622	51.536	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 103.080%			
32) Benzene-d6	5.977	84	255557	50.357	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 100.720%			
36) 1,2-Dichloropropane-d6	7.312	67	78120	50.414	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 100.820%			
41) Toluene-d8	8.653	98	239652	49.449	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 98.900%			
43) trans-1,3-Dichloroprop...	8.952	79	43823m	52.097	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 104.200%			
47) 2-Hexanone-d5	9.385	63	89083	107.057	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 107.060%			
56) 1,1,2,2-Tetrachloroeth...	11.195	84	115166	51.601	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 103.200%			
66) 1,2-Dichlorobenzene-d4	12.323	152	95409	49.816	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 99.640%			
Target Compounds						
2) Dichlorodifluoromethane	1.167	85	78102	49.718	ug/L	99
3) Chloromethane	1.288	50	82198	48.333	ug/L	89
5) Vinyl chloride	1.374	62	85140	48.547	ug/L	99
6) Bromomethane	1.612	94	35547	52.821	ug/L	96
8) Chloroethane	1.685	64	49565	56.281	ug/L	98
9) Trichlorofluoromethane	1.886	101	125943	49.199	ug/L	100
10) 1,1,2-Trichloro-1,2,2-...	2.331	101	65552	49.417	ug/L	96
12) 1,1-Dichloroethene	2.319	96	63177	49.298	ug/L	83
13) Acetone	2.386	43	88739	92.189	ug/L	98
14) Carbon disulfide	2.514	76	187013	47.362	ug/L	100
15) Methyl Acetate	2.703	43	79502	50.730	ug/L #	82
16) Methylene chloride	2.788	84	70213	49.528	ug/L	84
17) trans-1,2-Dichloroethene	3.093	96	67144	48.243	ug/L	89
18) Methyl tert-butyl Ether	3.111	73	222954	51.251	ug/L #	90
19) 1,1-Dichloroethane	3.611	63	116426	49.453	ug/L	96
20) cis-1,2-Dichloroethene	4.489	96	75953	49.322	ug/L	99
22) 2-Butanone	4.556	43	127551	99.546	ug/L	85
23) Bromochloromethane	4.904	128	39628	49.984	ug/L #	76

m  
 11/12/21

## Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX111121\  
 Data File : VX025134.D  
 Acq On : 11 Nov 2021 16:42  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 LabSampleId :  
 VSTDCCC050

Quant Time: Nov 12 05:05:21 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXLM111121WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Thu Nov 11 16:29:23 2021  
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/12/2021  
 Supervised By : Mahesh Dadoda 11/12/2021

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
25) Chloroform	5.093	83	121387	50.305 ug/L	97
27) 1,2-Dichloroethane	6.086	62	90462	51.130 ug/L #	86
29) Cyclohexane	5.471	56	113433	47.750 ug/L	87
30) 1,1,1-Trichloroethane	5.385	97	109618	47.975 ug/L #	94
31) Carbon tetrachloride	5.678	117	97770	48.459 ug/L	98
33) Benzene	6.038	78	279822	48.982 ug/L	100
34) Trichloroethene	7.129	95	71766	48.073 ug/L	82
35) Methylcyclohexane	7.385	83	123248	48.822 ug/L	93
37) 1,2-Dichloropropane	7.434	63	69781	48.761 ug/L	100
38) Bromodichloromethane	7.824	83	95196	49.155 ug/L	97
39) cis-1,3-Dichloropropene	8.366	75	115553	49.175 ug/L	98
40) 4-Methyl-2-pentanone	8.574	43	232027	102.017 ug/L #	84
42) Toluene	8.720	91	302062	48.680 ug/L	96
44) trans-1,3-Dichloropropene	8.976	75	113871	49.793 ug/L	97
45) 1,1,2-Trichloroethane	9.153	97	71485	49.468 ug/L	99
46) Tetrachloroethene	9.275	164	60510	48.582 ug/L	89
48) 2-Hexanone	9.433	43	185227	99.356 ug/L #	84
49) Dibromochloromethane	9.525	129	82654	50.105 ug/L	100
50) 1,2-Dibromoethane	9.610	107	78524	50.774 ug/L #	100
51) Chlorobenzene	10.080	112	197032	49.419 ug/L	96
52) Ethylbenzene	10.195	91	328554	49.260 ug/L	94
53) m,p-Xylene	10.305	106	130243	48.298 ug/L	81
54) o-Xylene	10.647	106	130302	48.967 ug/L	79
55) Styrene	10.659	104	222433	49.227 ug/L	81
57) 1,1,2,2-Tetrachloroethane	11.213	83	113799	49.600 ug/L	98
59) Bromoform	10.799	173	63931	48.963 ug/L #	95
60) Isopropylbenzene	10.964	105	330633	47.859 ug/L	95
61) 1,2,3-Trichloropropane	11.238	75	89844	49.385 ug/L	95
62) 1,3,5-Trimethylbenzene	11.451	105	287792	49.099 ug/L	89
63) 1,2,4-Trimethylbenzene	11.756	105	285888m	48.615 ug/L	93
64) 1,3-Dichlorobenzene	11.969	146	154073	48.923 ug/L	95
65) 1,4-Dichlorobenzene	12.043	146	153635	48.828 ug/L	95
67) 1,2-Dichlorobenzene	12.335	146	152575	48.779 ug/L	95
68) 1,2-Dibromo-3-chloropr...	12.945	75	26450	50.269 ug/L #	58
69) 1,3,5-Trimethylbenzene	13.116	180	112994	49.594 ug/L	96
70) 1,2,4-trichlorobenzene	13.591	180	101853	51.250 ug/L	97
71) Naphthalene	13.780	128	360513	53.494 ug/L	99
72) 1,2,3-Trichlorobenzene	13.963	180	102559	52.054 ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed