

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111121\
 Data File : VX025135.D
 Acq On : 11 Nov 2021 17:54
 Operator : JC/MD
 Sample : VX1111WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK635

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

Signal : TIC: VX025135.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rBV	109433	111771	15.21%	1.938%
2	1.666	92	95	107	rVB	65409	83174	11.32%	1.442%
3	2.306	194	200	215	rVB	158913	255888	34.83%	4.437%
4	2.947	300	305	313	rVB	4396	10074	1.37%	0.175%
5	3.105	329	331	334	rBV4	767	729	0.10%	0.013%
6	3.556	403	405	407	rVB3	527	374	0.05%	0.006%
7	4.404	541	544	545	rBV2	673	716	0.10%	0.012%
8	4.465	545	554	566	rVV	61092	177270	24.13%	3.074%
9	4.696	589	592	593	rBV3	455	518	0.07%	0.009%
10	4.806	608	610	612	rBV3	488	565	0.08%	0.010%
11	5.062	641	652	667	rVB	91971	283195	38.55%	4.910%
12	5.312	692	693	696	rVB3	396	341	0.05%	0.006%
13	5.361	699	701	702	rBV2	726	415	0.06%	0.007%
14	5.458	714	717	718	rBV3	569	684	0.09%	0.012%
15	5.556	730	733	735	rVB4	547	651	0.09%	0.011%
16	5.659	748	750	751	rBV2	600	363	0.05%	0.006%
17	5.977	789	802	820	rBV2	246460	734710	100.00%	12.739%
18	6.495	884	887	888	rBV3	600	581	0.08%	0.010%
19	6.672	914	916	918	rVV2	563	449	0.06%	0.008%
20	6.769	922	932	949	rVB	184842	451653	61.47%	7.831%
21	7.037	974	976	977	rBV2	469	437	0.06%	0.008%
22	7.110	982	988	998	rVB7	2953	7339	1.00%	0.127%
23	7.312	1013	1021	1037	rVB	152304	328716	44.74%	5.700%
24	7.635	1073	1074	1077	rBV3	336	376	0.05%	0.007%
25	7.696	1083	1084	1086	rBV2	724	367	0.05%	0.006%
26	7.714	1086	1087	1092	rVV4	375	425	0.06%	0.007%
27	7.805	1099	1102	1105	rBV4	544	718	0.10%	0.012%
28	8.049	1141	1142	1145	rBV3	485	455	0.06%	0.008%
29	8.074	1145	1146	1149	rVB3	662	510	0.07%	0.009%
30	8.098	1149	1150	1155	rBV4	409	610	0.08%	0.011%
31	8.141	1155	1157	1159	rBV3	412	361	0.05%	0.006%
32	8.330	1181	1188	1197	rBV	117620	193953	26.40%	3.363%
33	8.653	1234	1241	1248	rBV	400282	621239	84.56%	10.772%
34	8.720	1249	1252	1258	rVB	5733	8524	1.16%	0.148%
35	8.952	1283	1290	1304	rBV	87089	129537	17.63%	2.246%
36	9.275	1340	1343	1349	rVB7	957	1736	0.24%	0.030%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111121\
 Data File : VX025135.D
 Acq On : 11 Nov 2021 17:54
 Operator : JC/MD
 Sample : VX1111WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK635

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

37	9.384	1356	1361	1373	rVV	288457	401533	54.65%	6.962%
38	9.616	1396	1399	1400	rBV3	696	680	0.09%	0.012%
39	9.708	1409	1414	1418	rBV	2932	4635	0.63%	0.080%
40	9.805	1426	1430	1432	rBV4	318	382	0.05%	0.007%
41	9.842	1434	1436	1440	rVV3	607	669	0.09%	0.012%
42	9.903	1444	1446	1449	rVB4	400	439	0.06%	0.008%
43	9.976	1456	1458	1461	rBV4	454	558	0.08%	0.010%
44	10.055	1465	1471	1479	rBV	394547	521993	71.05%	9.051%
45	10.305	1509	1512	1515	rBV3	1139	1381	0.19%	0.024%
46	10.378	1523	1524	1527	rVB2	780	497	0.07%	0.009%
47	10.421	1529	1531	1534	rBV4	591	631	0.09%	0.011%
48	10.470	1537	1539	1541	rBV3	528	498	0.07%	0.009%
49	10.506	1543	1545	1547	rVB2	801	506	0.07%	0.009%
50	10.531	1547	1549	1550	rBV	786	681	0.09%	0.012%
51	10.653	1565	1569	1573	rBV6	1084	1856	0.25%	0.032%
52	10.841	1598	1600	1602	rVV3	555	452	0.06%	0.008%
53	10.921	1608	1613	1614	rBV4	303	439	0.06%	0.008%
54	11.037	1631	1632	1635	rBV3	416	354	0.05%	0.006%
55	11.091	1637	1641	1642	rBV4	499	593	0.08%	0.010%
56	11.122	1642	1646	1650	rVB2	2305	3422	0.47%	0.059%
57	11.195	1652	1658	1665	rBV	286339	362511	49.34%	6.286%
58	11.372	1686	1687	1689	rBV2	498	400	0.05%	0.007%
59	11.451	1695	1700	1702	rBV4	1070	1446	0.20%	0.025%
60	11.634	1728	1730	1732	rVB3	699	432	0.06%	0.007%
61	11.707	1739	1742	1744	rBV4	454	453	0.06%	0.008%
62	11.750	1745	1749	1752	rVV3	2614	3675	0.50%	0.064%
63	11.817	1758	1760	1762	rBV3	393	491	0.07%	0.009%
64	11.841	1762	1764	1769	rVV6	629	832	0.11%	0.014%
65	11.933	1776	1779	1783	rBV3	1720	2474	0.34%	0.043%
66	11.975	1783	1786	1789	rBV4	1252	1841	0.25%	0.032%
67	12.024	1789	1794	1801	rBV	402432	496904	67.63%	8.616%
68	12.128	1809	1811	1813	rBV3	1129	1232	0.17%	0.021%
69	12.152	1813	1815	1820	rVB3	2414	2756	0.38%	0.048%
70	12.207	1822	1824	1826	rBV3	505	419	0.06%	0.007%
71	12.323	1835	1843	1851	rBV	411134	522117	71.06%	9.053%
72	12.433	1857	1861	1865	rVB4	1356	2097	0.29%	0.036%
73	12.469	1865	1867	1868	rBV2	602	512	0.07%	0.009%
74	12.762	1913	1915	1917	rBV2	686	432	0.06%	0.007%
75	13.006	1953	1955	1958	rVB4	392	425	0.06%	0.007%
76	13.152	1978	1979	1983	rVB4	633	702	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111121\
 Data File : VX025135.D
 Acq On : 11 Nov 2021 17:54
 Operator : JC/MD
 Sample : VX1111WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK635

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
 Title : VOC Analysis

77	13.250	1993	1995	1998	rVB3	604	637	0.09%	0.011%
78	13.286	1998	2001	2003	rBV3	462	529	0.07%	0.009%
79	13.439	2022	2026	2029	rVB4	397	441	0.06%	0.008%
80	13.463	2029	2030	2032	rBV2	498	425	0.06%	0.007%
81	13.512	2035	2038	2039	rBV3	394	410	0.06%	0.007%
82	13.591	2048	2051	2054	rVB5	979	1174	0.16%	0.020%
83	13.640	2057	2059	2062	rBV4	495	707	0.10%	0.012%
84	13.682	2062	2066	2068	rBV4	470	609	0.08%	0.011%
85	13.932	2106	2107	2109	rBV2	532	369	0.05%	0.006%
86	14.012	2118	2120	2123	rVB4	594	706	0.10%	0.012%
87	14.036	2123	2124	2126	rBV2	560	416	0.06%	0.007%
88	14.134	2137	2140	2142	rBV4	515	594	0.08%	0.010%
89	14.170	2144	2146	2147	rBV2	596	548	0.07%	0.010%
90	14.286	2162	2165	2168	rVB3	715	789	0.11%	0.014%
91	14.329	2168	2172	2175	rBV5	549	857	0.12%	0.015%
92	14.457	2191	2193	2194	rBV2	588	368	0.05%	0.006%
93	14.883	2261	2263	2265	rBV2	515	465	0.06%	0.008%
94	15.121	2300	2302	2303	rBV2	478	389	0.05%	0.007%
95	15.188	2311	2313	2317	rBV4	430	428	0.06%	0.007%
96	15.249	2321	2323	2324	rBV	527	402	0.05%	0.007%
97	15.322	2333	2335	2336	rBV2	501	353	0.05%	0.006%
98	15.457	2353	2357	2360	rBV5	514	976	0.13%	0.017%
99	15.731	2400	2402	2404	rBV3	608	468	0.06%	0.008%
100	16.499	2527	2528	2531	rVB4	787	358	0.05%	0.006%



Sum of corrected areas: 5767192

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111121\
Data File : VX025135.D
Acq On : 11 Nov 2021 17:54
Operator : JC/MD
Sample : VX1111WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK635

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

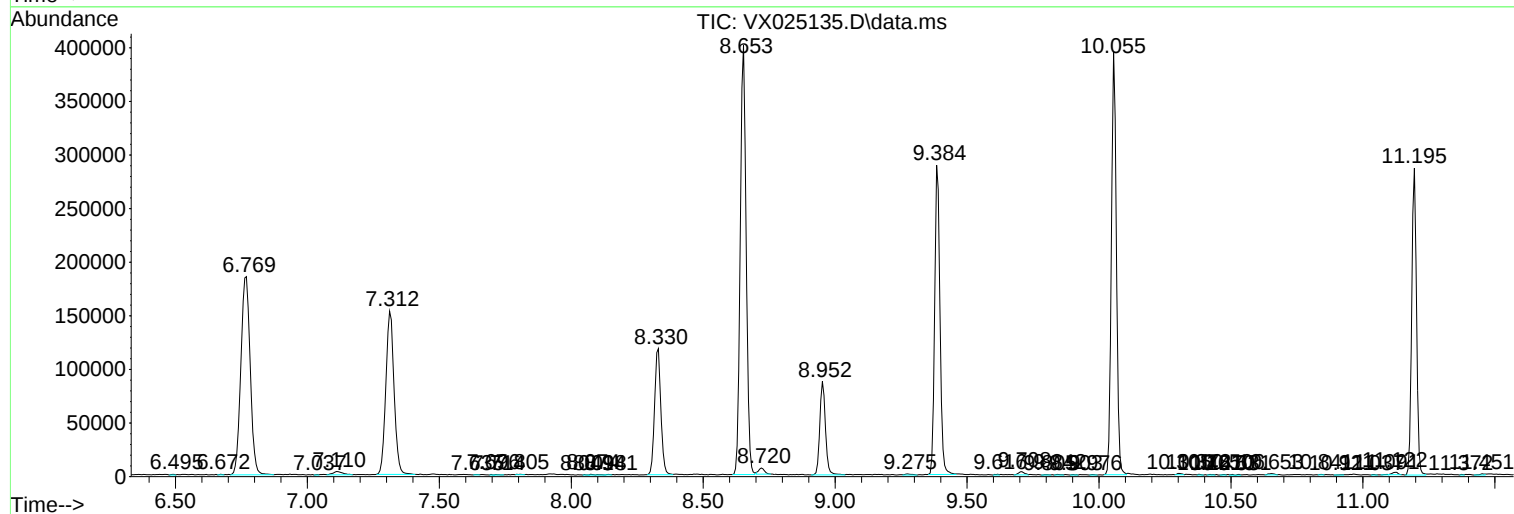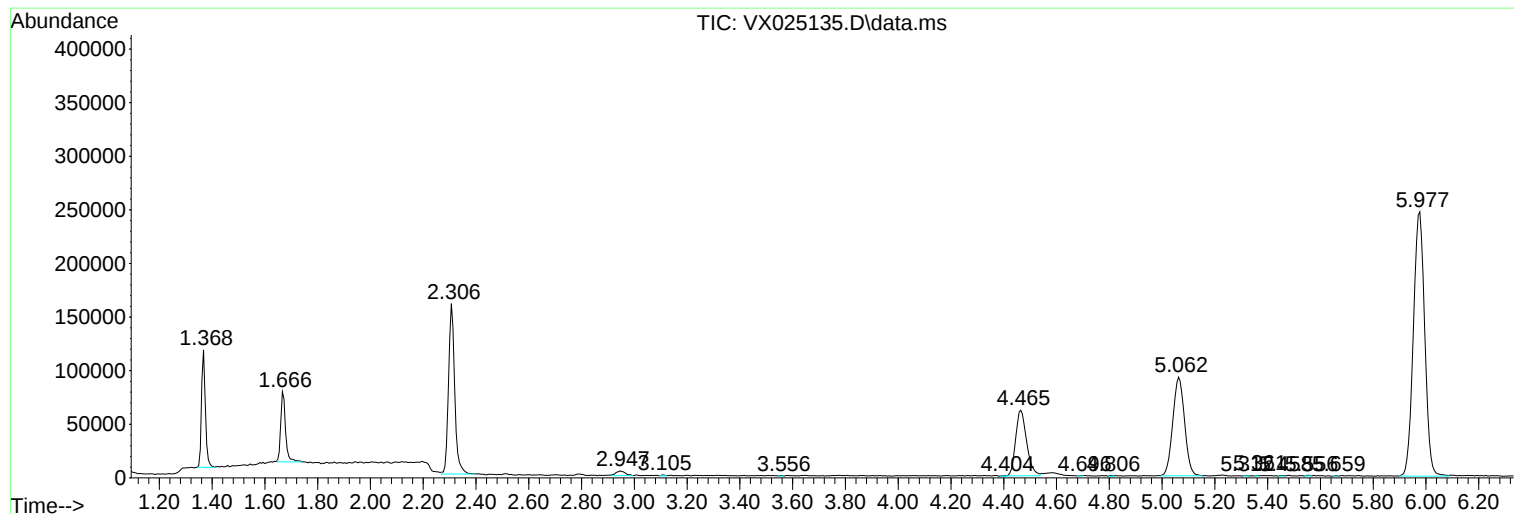

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111121\
Data File : VX025135.D
Acq On : 11 Nov 2021 17:54
Operator : JC/MD
Sample : VX1111WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK635

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111121\
Data File : VX025135.D
Acq On : 11 Nov 2021 17:54
Operator : JC/MD
Sample : VX1111WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK635

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc