

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111121\
 Data File : VX025138.D
 Acq On : 11 Nov 2021 19:04
 Operator : JC/MD
 Sample : M4645-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CON00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M

Title : VOC Analysis

Signal : TIC: VX025138.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rVB	101549	102044	14.74%	1.884%
2	1.666	92	95	102	rVB	81303	96463	13.93%	1.781%
3	2.306	194	200	213	rVB	148679	240985	34.80%	4.450%
4	3.050	320	322	327	rVB6	481	453	0.07%	0.008%
5	3.087	327	328	331	rBV3	643	546	0.08%	0.010%
6	3.148	336	338	340	rVB2	606	395	0.06%	0.007%
7	3.178	340	343	344	rBV3	458	454	0.07%	0.008%
8	3.233	350	352	355	rBV3	450	581	0.08%	0.011%
9	3.550	401	404	405	rBV3	282	328	0.05%	0.006%
10	3.635	417	418	421	rVB3	803	476	0.07%	0.009%
11	3.678	421	425	428	rBV5	452	954	0.14%	0.018%
12	3.952	465	470	472	rBV4	814	1317	0.19%	0.024%
13	4.007	477	479	482	rVV4	564	629	0.09%	0.012%
14	4.056	485	487	488	rBV2	422	294	0.04%	0.005%
15	4.324	529	531	533	rBV2	335	300	0.04%	0.006%
16	4.465	545	554	567	rBV	54170	157636	22.76%	2.911%
17	4.788	602	607	608	rBV5	652	990	0.14%	0.018%
18	5.062	641	652	666	rVB	88294	266209	38.44%	4.916%
19	5.214	676	677	681	rBV4	374	497	0.07%	0.009%
20	5.495	722	723	726	rBV2	407	501	0.07%	0.009%
21	5.861	780	783	785	rBV4	296	414	0.06%	0.008%
22	5.977	788	802	819	rBV2	232917	692522	100.00%	12.789%
23	6.604	904	905	909	rVB3	532	631	0.09%	0.012%
24	6.653	909	913	915	rBV3	475	517	0.07%	0.010%
25	6.678	915	917	919	rBV2	369	371	0.05%	0.007%
26	6.769	922	932	943	rBV	176689	423934	61.22%	7.829%
27	7.110	983	988	995	rBV7	2358	5657	0.82%	0.104%
28	7.312	1010	1021	1034	rBV	141941	312821	45.17%	5.777%
29	7.482	1045	1049	1054	rBV6	786	1378	0.20%	0.025%
30	7.793	1098	1100	1102	rBV2	443	412	0.06%	0.008%
31	7.848	1107	1109	1114	rBV3	393	553	0.08%	0.010%
32	7.921	1118	1121	1122	rBV3	573	573	0.08%	0.011%
33	8.055	1141	1143	1145	rVB3	598	451	0.07%	0.008%
34	8.086	1145	1148	1150	rBV4	451	489	0.07%	0.009%
35	8.122	1150	1154	1156	rBV3	787	698	0.10%	0.013%
36	8.159	1158	1160	1164	rVB4	395	392	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111121\
 Data File : VX025138.D
 Acq On : 11 Nov 2021 19:04
 Operator : JC/MD
 Sample : M4645-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CON00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

37	8.190	1164	1165	1172	rVB5	581	961	0.14%	0.018%
38	8.250	1172	1175	1176	rBV2	421	339	0.05%	0.006%
39	8.330	1181	1188	1196	rBV	109243	180764	26.10%	3.338%
40	8.531	1218	1221	1224	rBV4	571	942	0.14%	0.017%
41	8.653	1234	1241	1248	rBV	375781	583357	84.24%	10.773%
42	8.720	1248	1252	1258	rVB	5407	8427	1.22%	0.156%
43	8.952	1283	1290	1299	rBV	82667	119777	17.30%	2.212%
44	9.110	1314	1316	1318	rBV3	616	622	0.09%	0.011%
45	9.165	1321	1325	1326	rVV3	631	584	0.08%	0.011%
46	9.189	1326	1329	1332	rVV4	538	613	0.09%	0.011%
47	9.220	1332	1334	1336	rVB3	411	313	0.05%	0.006%
48	9.281	1339	1344	1349	rBV4	1349	2080	0.30%	0.038%
49	9.384	1356	1361	1375	rBV	257506	366429	52.91%	6.767%
50	9.616	1397	1399	1401	rBV3	509	581	0.08%	0.011%
51	9.714	1414	1415	1420	rVB4	391	454	0.07%	0.008%
52	9.769	1420	1424	1425	rVB4	496	509	0.07%	0.009%
53	9.854	1433	1438	1442	rBV4	561	1148	0.17%	0.021%
54	10.055	1465	1471	1481	rVV	366755	492571	71.13%	9.096%
55	10.305	1509	1512	1516	rVB5	1350	1936	0.28%	0.036%
56	10.360	1520	1521	1523	rBV	336	288	0.04%	0.005%
57	10.457	1534	1537	1538	rBV3	520	559	0.08%	0.010%
58	10.573	1553	1556	1557	rBV3	313	279	0.04%	0.005%
59	10.854	1600	1602	1606	rVB5	265	309	0.04%	0.006%
60	11.091	1637	1641	1642	rBV3	347	486	0.07%	0.009%
61	11.122	1642	1646	1650	rVB3	2821	3693	0.53%	0.068%
62	11.195	1652	1658	1667	rBV	269180	341531	49.32%	6.307%
63	11.384	1688	1689	1693	rBV3	707	694	0.10%	0.013%
64	11.463	1697	1702	1703	rBV4	657	1191	0.17%	0.022%
65	11.549	1714	1716	1718	rVB3	438	333	0.05%	0.006%
66	11.591	1721	1723	1724	rBV	500	321	0.05%	0.006%
67	11.750	1745	1749	1754	rVB3	3413	4612	0.67%	0.085%
68	11.835	1760	1763	1768	rBV5	744	1259	0.18%	0.023%
69	11.933	1776	1779	1784	rBV3	1391	1850	0.27%	0.034%
70	12.024	1789	1794	1803	rBV	374344	465766	67.26%	8.601%
71	12.225	1823	1827	1832	rBV	9194	12979	1.87%	0.240%
72	12.323	1837	1843	1851	rVV	386163	486840	70.30%	8.991%
73	12.427	1857	1860	1864	rBV6	918	1202	0.17%	0.022%
74	12.805	1920	1922	1923	rBV2	427	281	0.04%	0.005%
75	12.853	1928	1930	1934	rVB3	429	451	0.07%	0.008%
76	12.963	1946	1948	1952	rBV4	502	352	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111121\
 Data File : VX025138.D
 Acq On : 11 Nov 2021 19:04
 Operator : JC/MD
 Sample : M4645-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CON00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

77	13.048	1958	1962	1963	rBV3	732	927	0.13%	0.017%
78	13.146	1977	1978	1980	rBV2	373	284	0.04%	0.005%
79	13.292	2000	2002	2004	rBV3	519	488	0.07%	0.009%
80	13.359	2008	2013	2014	rBV4	474	629	0.09%	0.012%
81	13.420	2019	2023	2024	rBV3	422	511	0.07%	0.009%
82	13.597	2049	2052	2053	rBV2	555	553	0.08%	0.010%
83	13.634	2057	2058	2061	rVB2	485	323	0.05%	0.006%
84	13.768	2077	2080	2081	rBV2	520	437	0.06%	0.008%
85	13.786	2081	2083	2086	rVB4	846	892	0.13%	0.016%
86	13.817	2086	2088	2091	rBV3	323	502	0.07%	0.009%
87	13.902	2097	2102	2107	rBV6	324	501	0.07%	0.009%
88	14.097	2132	2134	2136	rVB2	466	396	0.06%	0.007%
89	14.121	2136	2138	2140	rBV3	418	415	0.06%	0.008%
90	14.158	2140	2144	2147	rVV5	470	741	0.11%	0.014%
91	14.231	2154	2156	2157	rBV2	415	330	0.05%	0.006%
92	14.286	2163	2165	2167	rBV3	630	640	0.09%	0.012%
93	14.304	2167	2168	2171	rVV3	557	505	0.07%	0.009%
94	14.725	2231	2237	2238	rBV5	511	1027	0.15%	0.019%
95	14.774	2242	2245	2249	rBV6	478	890	0.13%	0.016%
96	14.883	2260	2263	2264	rBV3	542	628	0.09%	0.012%
97	15.420	2349	2351	2353	rBV3	555	481	0.07%	0.009%
98	15.536	2368	2370	2372	rVB3	571	423	0.06%	0.008%
99	15.676	2391	2393	2397	rBV5	631	545	0.08%	0.010%
100	16.164	2471	2473	2475	rBV3	501	406	0.06%	0.007%

Sum of corrected areas: 5415022




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111121\
Data File : VX025138.D
Acq On : 11 Nov 2021 19:04
Operator : JC/MD
Sample : M4645-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CON00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

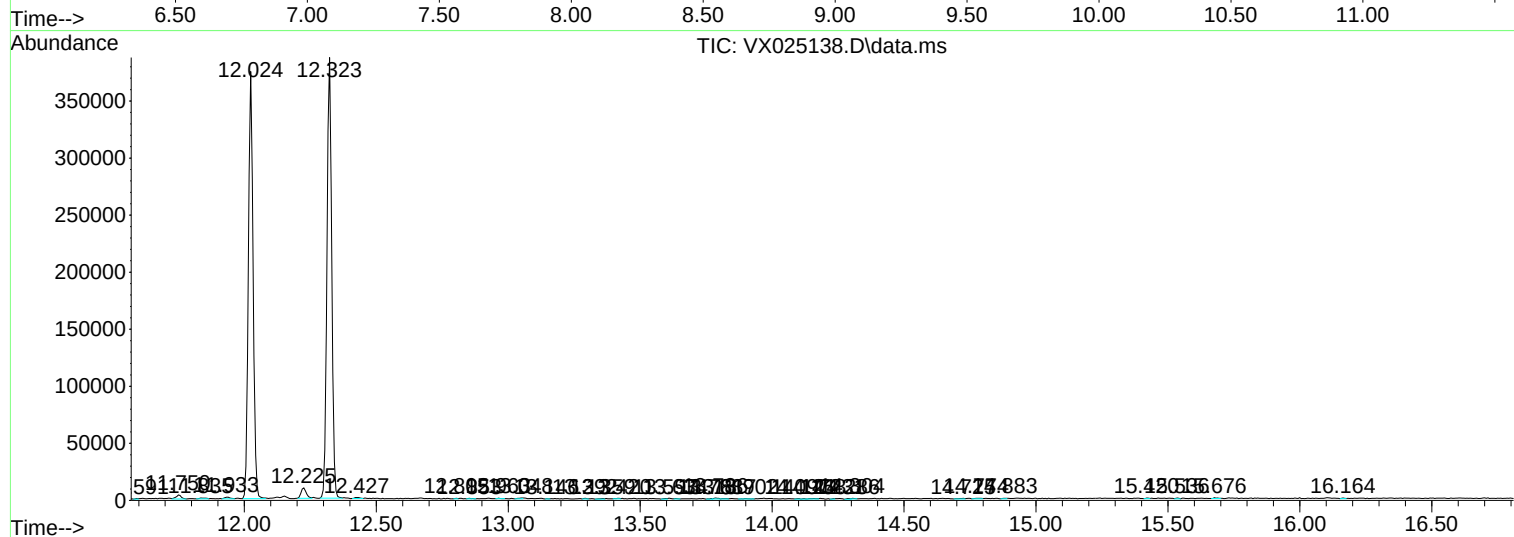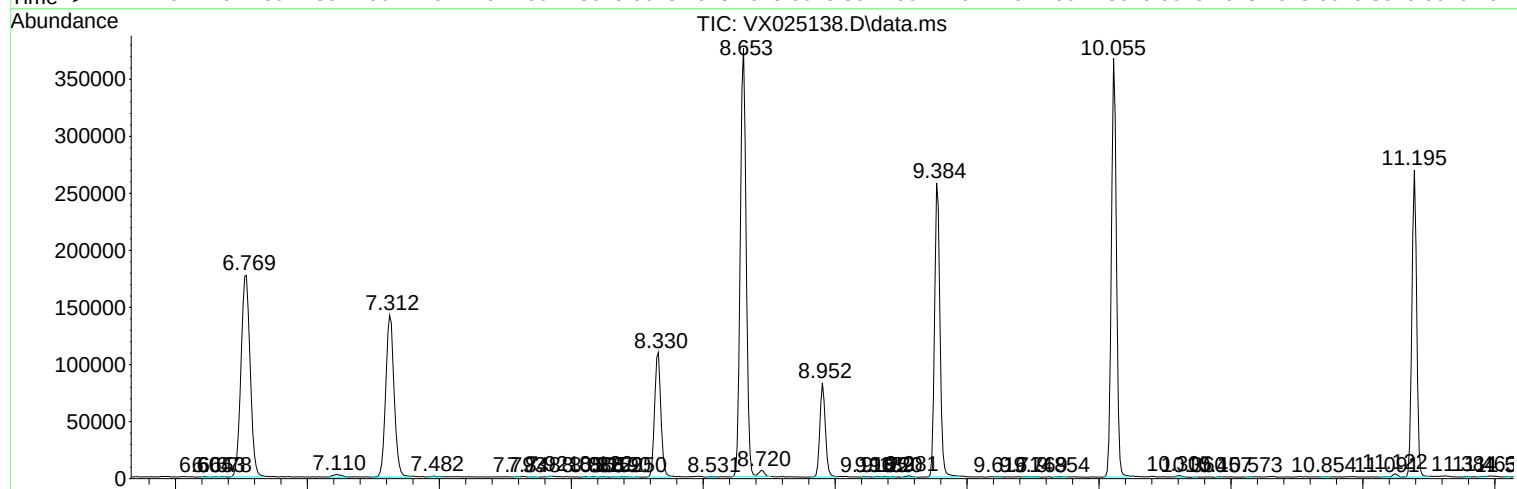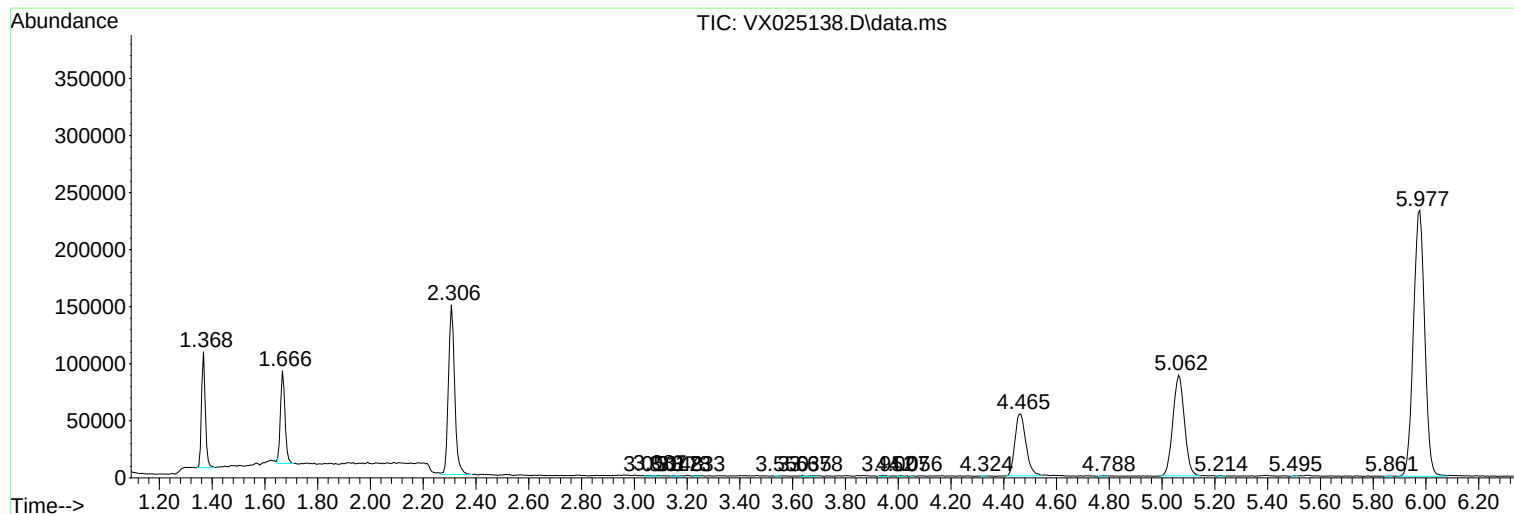

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111121\
Data File : VX025138.D
Acq On : 11 Nov 2021 19:04
Operator : JC/MD
Sample : M4645-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CON00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111121\
Data File : VX025138.D
Acq On : 11 Nov 2021 19:04
Operator : JC/MD
Sample : M4645-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CON00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc