

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111122\
 Data File : VX032775.D
 Acq On : 11 Nov 2022 15:24
 Operator : JC/MD
 Sample : N5559-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 001-WILLETS-PT-BLVD(NOV)

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X111022W.M

Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VX032775.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.550	73	76	78	rBV3	2243	2916	1.21%	0.209%
2	2.386	206	213	227	rBV	85751	158863	65.85%	11.377%
3	2.575	234	244	272	rVV2	28384	131680	54.58%	9.430%
4	2.940	298	304	312	rBV2	3779	9107	3.77%	0.652%
5	4.013	474	480	486	rBV3	1131	2554	1.06%	0.183%
6	4.568	563	571	584	rBV2	7372	21882	9.07%	1.567%
7	4.903	616	626	643	rBV3	24525	71493	29.63%	5.120%
8	5.038	643	648	650	rBV2	1745	3126	1.30%	0.224%
9	5.958	790	799	812	rBV2	29955	80834	33.51%	5.789%
10	6.763	922	931	943	rBV	71550	170353	70.61%	12.200%
11	7.476	1043	1048	1055	rBV3	1235	2939	1.22%	0.210%
12	8.580	1224	1229	1234	rBV2	4146	6573	2.72%	0.471%
13	8.653	1234	1241	1247	rVV	132794	207428	85.98%	14.855%
14	8.720	1247	1252	1265	rVB	22253	35522	14.72%	2.544%
15	8.848	1269	1273	1280	rBV	3461	5261	2.18%	0.377%
16	10.055	1465	1471	1486	rBV	183985	241256	100.00%	17.278%
17	10.860	1598	1603	1608	rBV2	1802	2424	1.00%	0.174%
18	11.085	1632	1640	1651	rBV	157978	210781	87.37%	15.095%
19	11.762	1746	1751	1756	rBV5	2235	3449	1.43%	0.247%
20	11.890	1768	1772	1774	rBV4	2011	2484	1.03%	0.178%
21	12.012	1786	1792	1795	rBV	10016	11739	4.87%	0.841%
22	12.219	1822	1826	1835	rBV3	2837	4993	2.07%	0.358%
23	12.579	1880	1885	1889	rBV3	4747	5574	2.31%	0.399%
24	13.335	2006	2009	2016	rVB2	2428	3121	1.29%	0.224%




Sum of corrected areas: 1396352

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111122\
Data File : VX032775.D
Acq On : 11 Nov 2022 15:24
Operator : JC/MD
Sample : N5559-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
001-WILLETS-PT-BLVD(NOV)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X111022W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

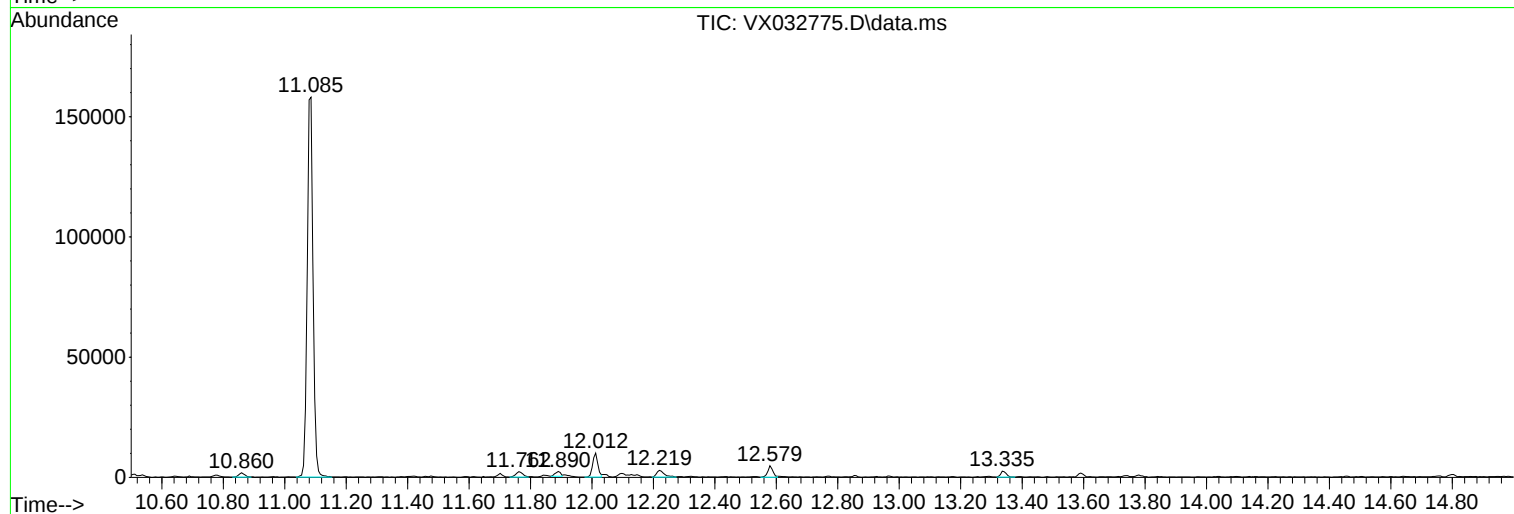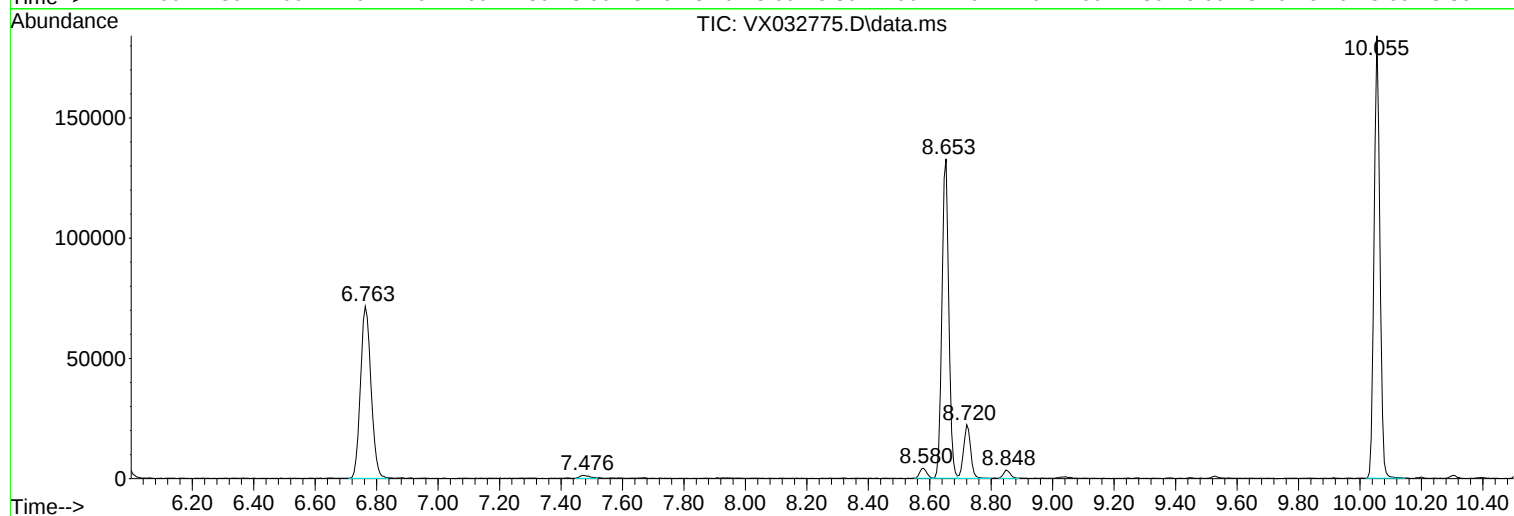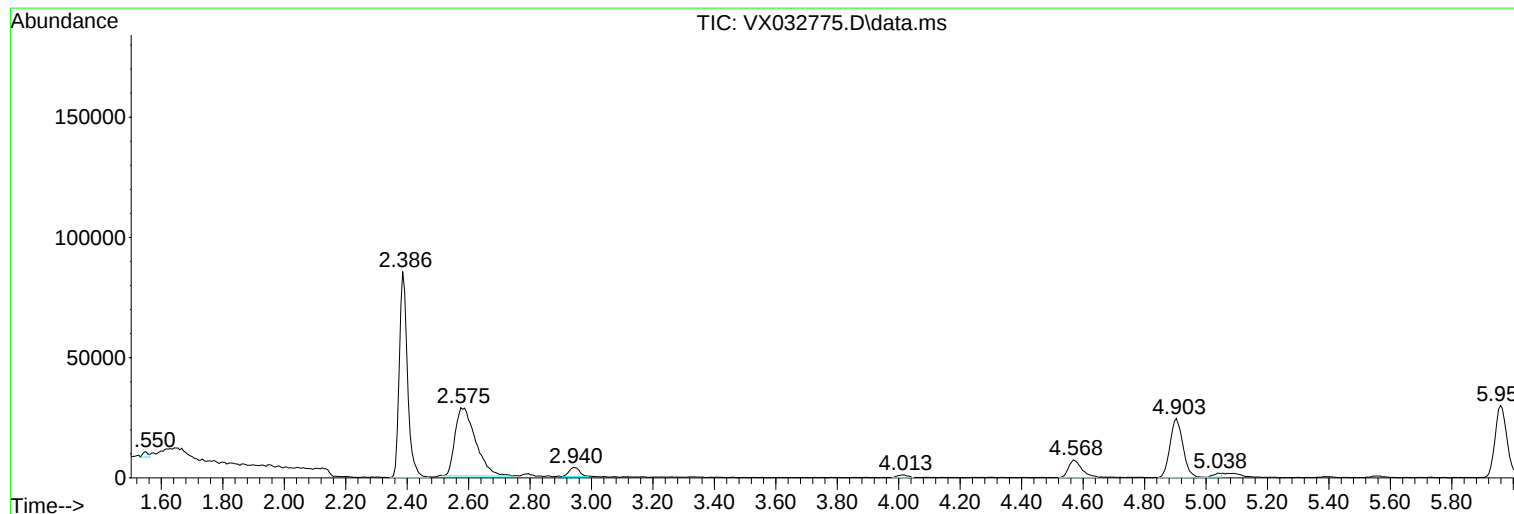

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111122\
Data File : VX032775.D
Acq On : 11 Nov 2022 15:24
Operator : JC/MD
Sample : N5559-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
001-WILLETS-PT-BLVD(NOV)










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X111022W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.575	55.26 ug/l	131680	Bromochloromethane	4.903

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	83
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
3			Hydrazine, ethyl-	60	C2H8N2	000624-80-6	43
4			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
5			4-Penten-2-ol	86	C5H10O	000625-31-0	9

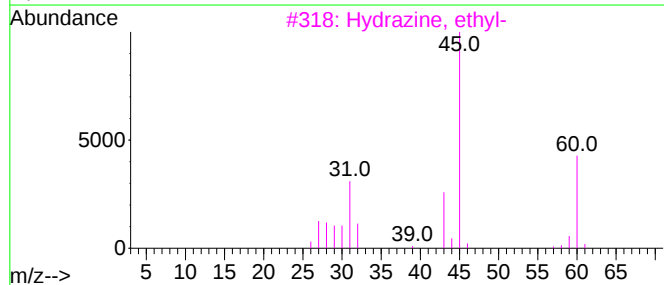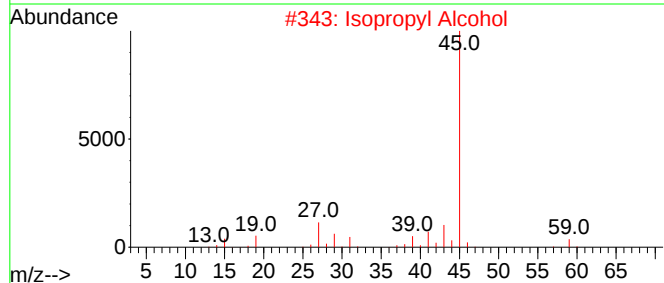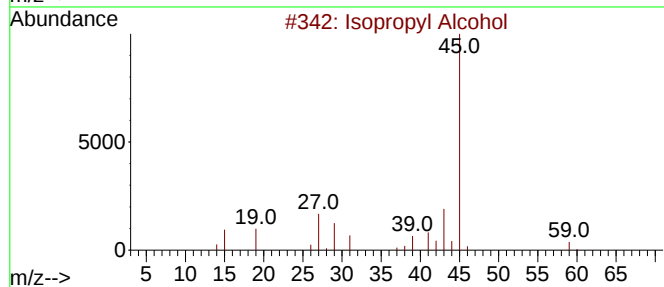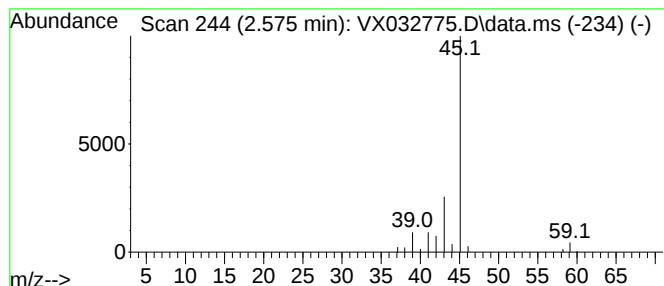

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111122\
Data File : VX032775.D
Acq On : 11 Nov 2022 15:24
Operator : JC/MD
Sample : N5559-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
001-WILLETS-PT-BLVD(NOV)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X111022W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.575	55.3	ug/l	131680	1	4.903	71493	30.0