

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111122\
 Data File : VX032776.D
 Acq On : 11 Nov 2022 15:47
 Operator : JC/MD
 Sample : N5559-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 002-35TH-AVE(NOV)

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X111022W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VX032776.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.550	73	76	78	rBV	3059	3081	1.31%	0.222%
2	2.385	205	213	228	rBV	88579	161371	68.51%	11.605%
3	2.581	229	245	268	rBV2	31444	137490	58.37%	9.888%
4	2.946	298	305	316	rVB3	2661	6258	2.66%	0.450%
5	4.568	564	571	582	rBV	6741	19374	8.22%	1.393%
6	4.903	615	626	640	rVB3	23457	70602	29.97%	5.078%
7	5.050	640	650	653	rBV6	2072	6439	2.73%	0.463%
8	5.958	790	799	815	rBV2	30462	80001	33.96%	5.753%
9	6.763	921	931	947	rBV	69193	166285	70.59%	11.959%
10	7.470	1042	1047	1057	rBV	1287	2685	1.14%	0.193%
11	8.579	1223	1229	1234	rBV3	4334	7467	3.17%	0.537%
12	8.653	1234	1241	1247	rVV	127338	202899	86.14%	14.592%
13	8.720	1247	1252	1261	rVB	22617	36387	15.45%	2.617%
14	8.848	1268	1273	1279	rBV	3217	4943	2.10%	0.355%
15	10.055	1466	1471	1480	rBV	180187	235557	100.00%	16.941%
16	10.860	1599	1603	1608	rBV3	1616	2357	1.00%	0.170%
17	11.085	1632	1640	1652	rBV	160933	211678	89.86%	15.223%
18	11.762	1747	1751	1759	rBV5	2222	3918	1.66%	0.282%
19	11.890	1768	1772	1784	rVB6	2235	4590	1.95%	0.330%
20	12.012	1788	1792	1796	rBV	10023	12346	5.24%	0.888%
21	12.097	1801	1806	1809	rBV5	1622	2387	1.01%	0.172%
22	12.219	1821	1826	1832	rBV2	3554	5028	2.13%	0.362%
23	12.579	1881	1885	1889	rVB2	3646	4378	1.86%	0.315%
24	13.335	2005	2009	2014	rVB3	2334	2962	1.26%	0.213%




Sum of corrected areas: 1390483

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111122\
Data File : VX032776.D
Acq On : 11 Nov 2022 15:47
Operator : JC/MD
Sample : N5559-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
002-35TH-AVE(NOV)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X111022W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

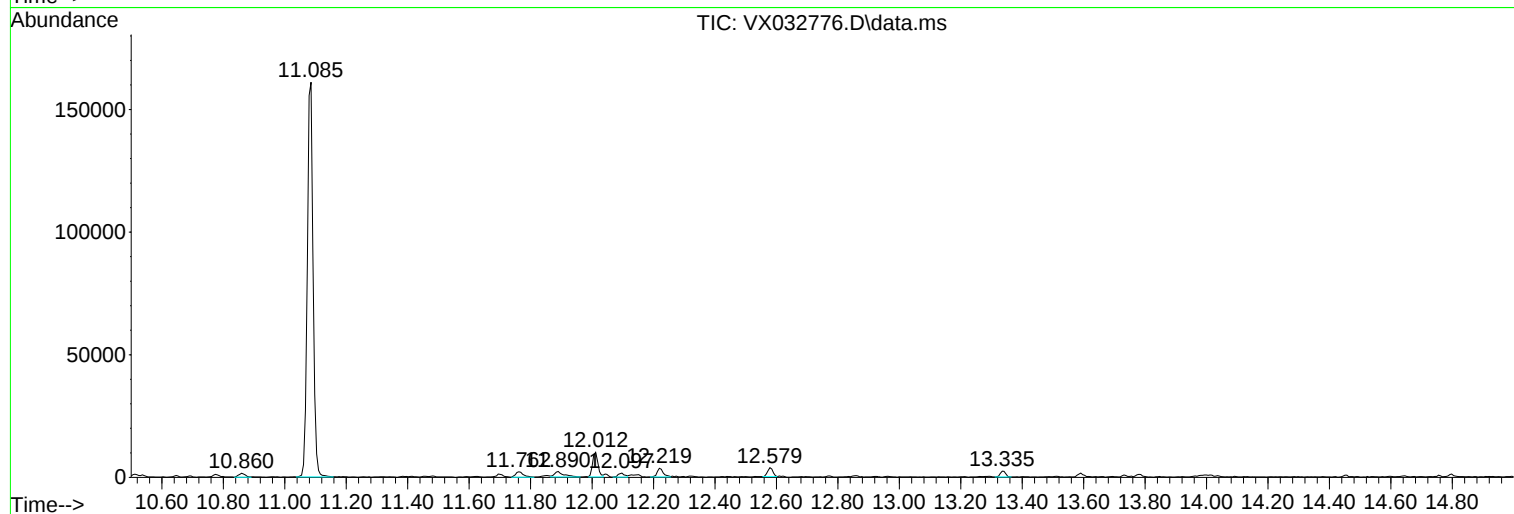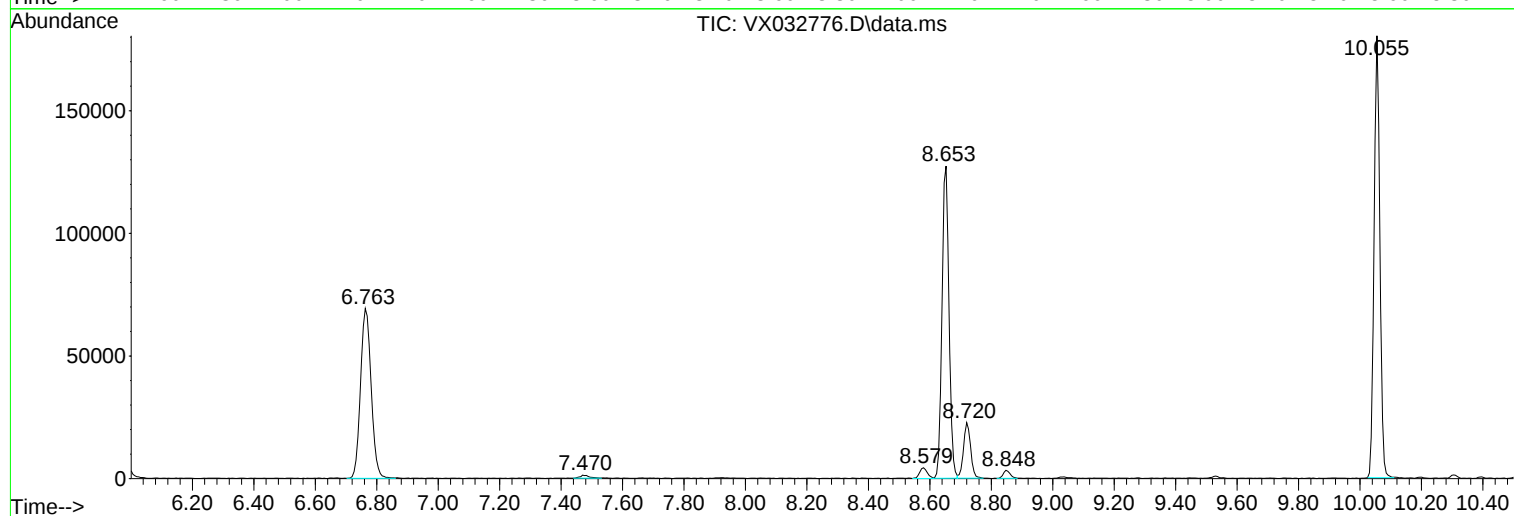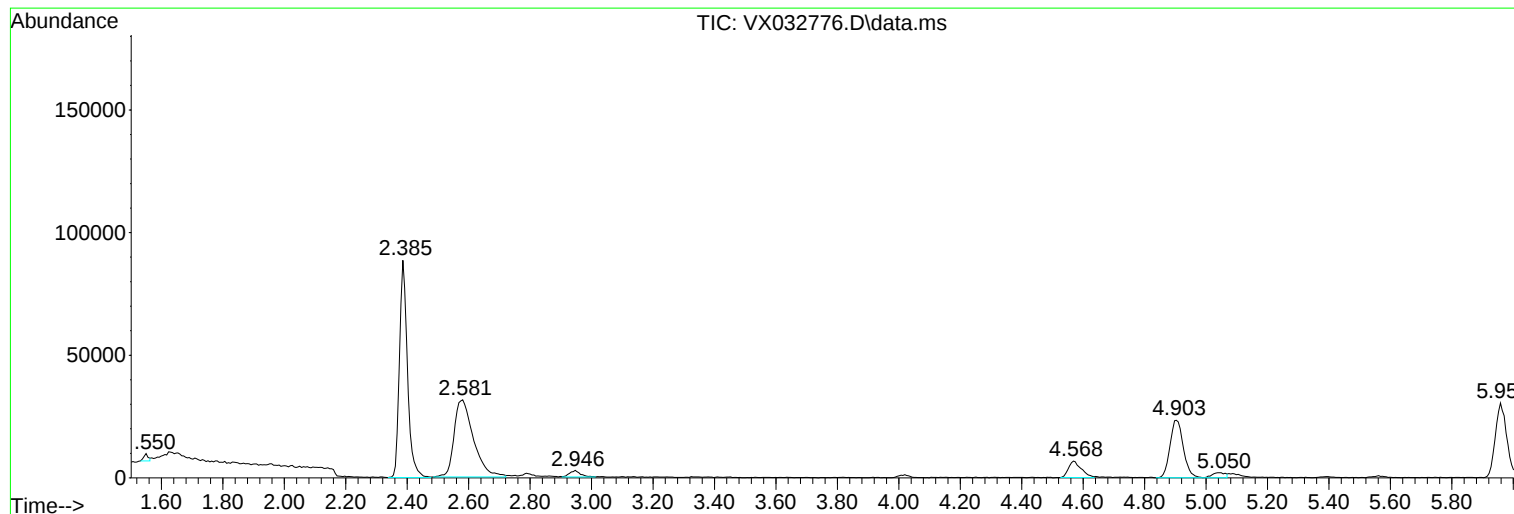

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111122\
Data File : VX032776.D
Acq On : 11 Nov 2022 15:47
Operator : JC/MD
Sample : N5559-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
002-35TH-AVE(NOV)










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X111022W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.581	58.42 ug/l	137490	Bromochloromethane	4.903

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
4			Hydrazine, ethyl-	60	C2H8N2	000624-80-6	40
5			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9

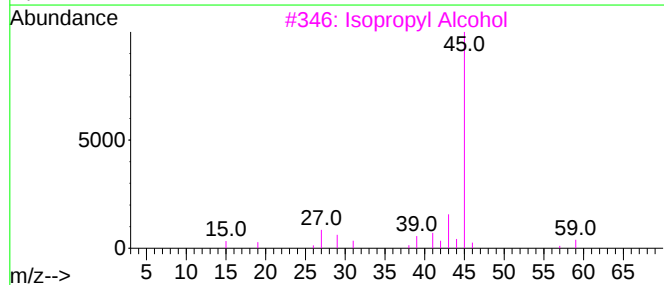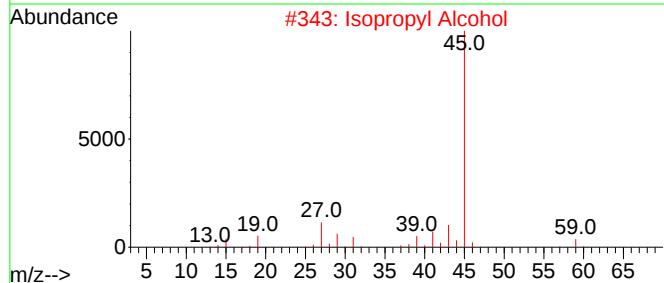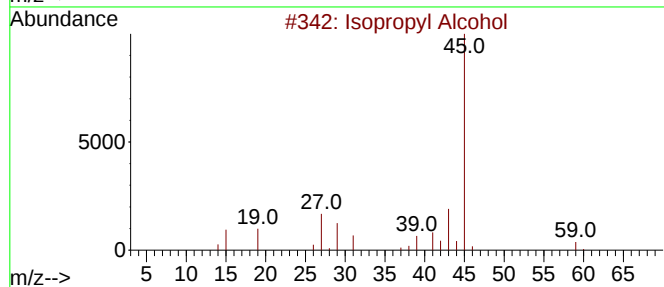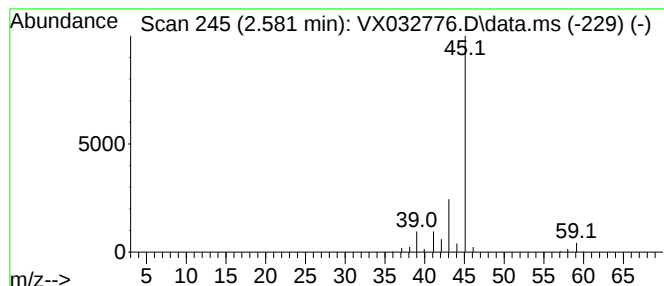

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111122\
Data File : VX032776.D
Acq On : 11 Nov 2022 15:47
Operator : JC/MD
Sample : N5559-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
002-35TH-AVE(NOV)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X111022W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.581	58.4	ug/l	137490	1	4.903	70602	30.0