
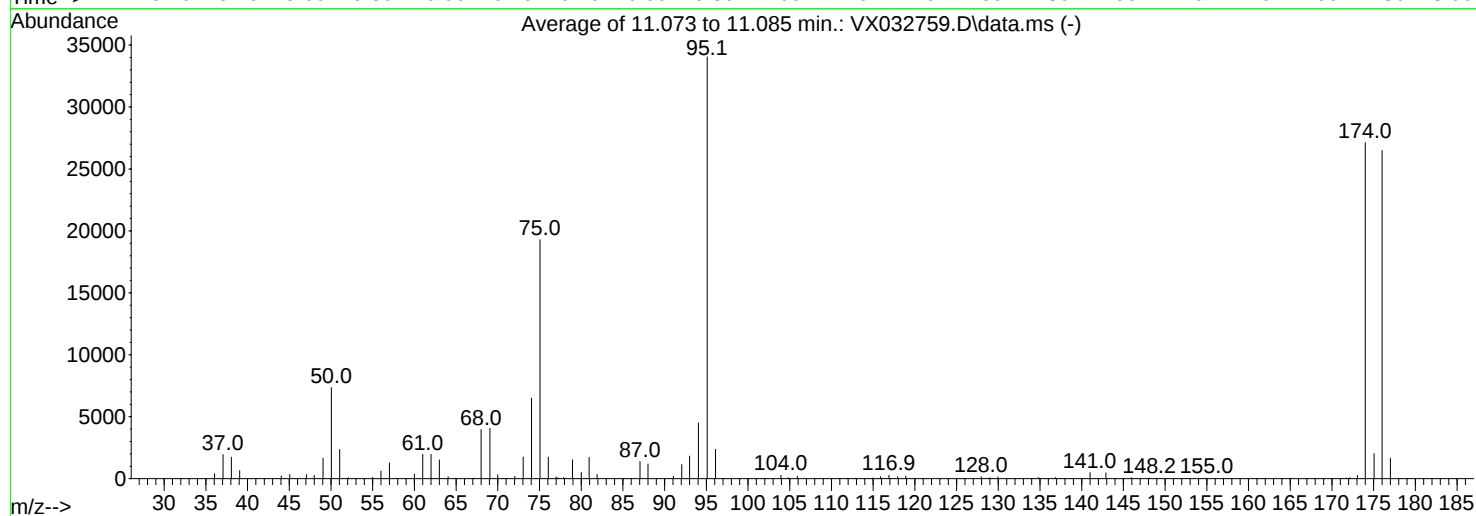


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111122\
 Data File : VX032759.D
 Acq On : 11 Nov 2022 08:44
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X111022W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Nov 11 05:24:06 2022

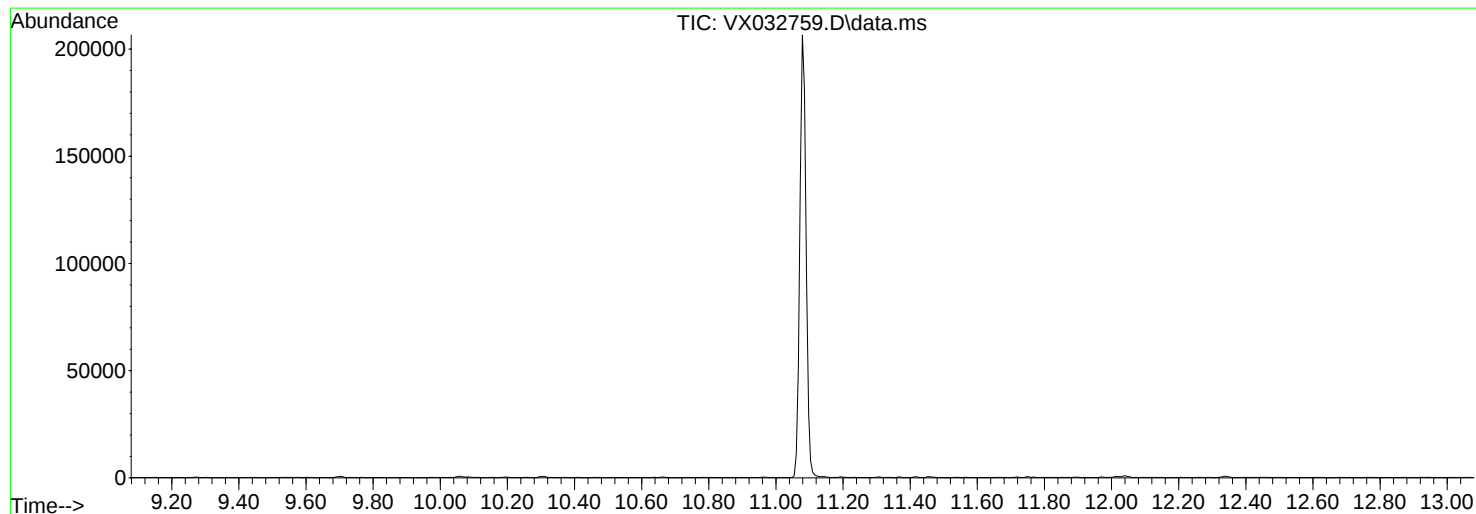

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	7353	PASS
75	95	30	60	56.6	19284	PASS
95	95	100	100	100.0	34051	PASS
96	95	5	9	7.0	2383	PASS
173	174	0.00	2	0.9	255	PASS
174	95	50	100	79.7	27141	PASS
175	174	5	9	7.5	2026	PASS
176	174	95	101	97.6	26499	PASS
177	176	5	9	6.2	1646	PASS