

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043780.D
 Acq On : 11 Nov 2024 10:40
 Operator : JC/MD
 Sample : P4751-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 12 00:51:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 12 00:51:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	298559	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.049	117	268104	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	122106	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	69828	43.902	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	87.800%		
7) Chloroethane-d5	1.642	69	37902	55.439	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	110.880%		
11) 1,1-Dichloroethene-d2	2.294	65	33418	45.513	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	91.020%		
21) 2-Butanone-d5	4.459	46	96481	92.645	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	92.650%		
24) Chloroform-d	5.050	84	153909	44.887	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.780%		
26) 1,2-Dichloroethane-d4	5.952	65	95748	43.957	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.920%		
32) Benzene-d6	5.964	84	322685	46.553	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.100%		
36) 1,2-Dichloropropane-d6	7.300	67	95955	45.501	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	91.000%		
41) Toluene-d8	8.647	98	293267	46.575	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.140%		
43) trans-1,3-Dichloroprop...	8.952	79	42080	41.725	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.440%		
47) 2-Hexanone-d5	9.385	63	83177	99.663	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	99.660%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	135144	49.947	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	99.900%		
66) 1,2-Dichlorobenzene-d4	12.317	152	114411	54.079	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	108.160%		
Target Compounds					Qvalue	
13) Acetone	2.386	43	28640	29.569	ug/L	96
37) 1,2-Dichloropropane	7.300	63	10912	5.361	ug/L #	85
61) 1,2,3-Trichloropropane	12.018	75	13516	5.703	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043780.D
Acq On : 11 Nov 2024 10:40
Operator : JC/MD
Sample : P4751-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 12 00:51:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 12 00:51:02 2024
Response via : Initial Calibration




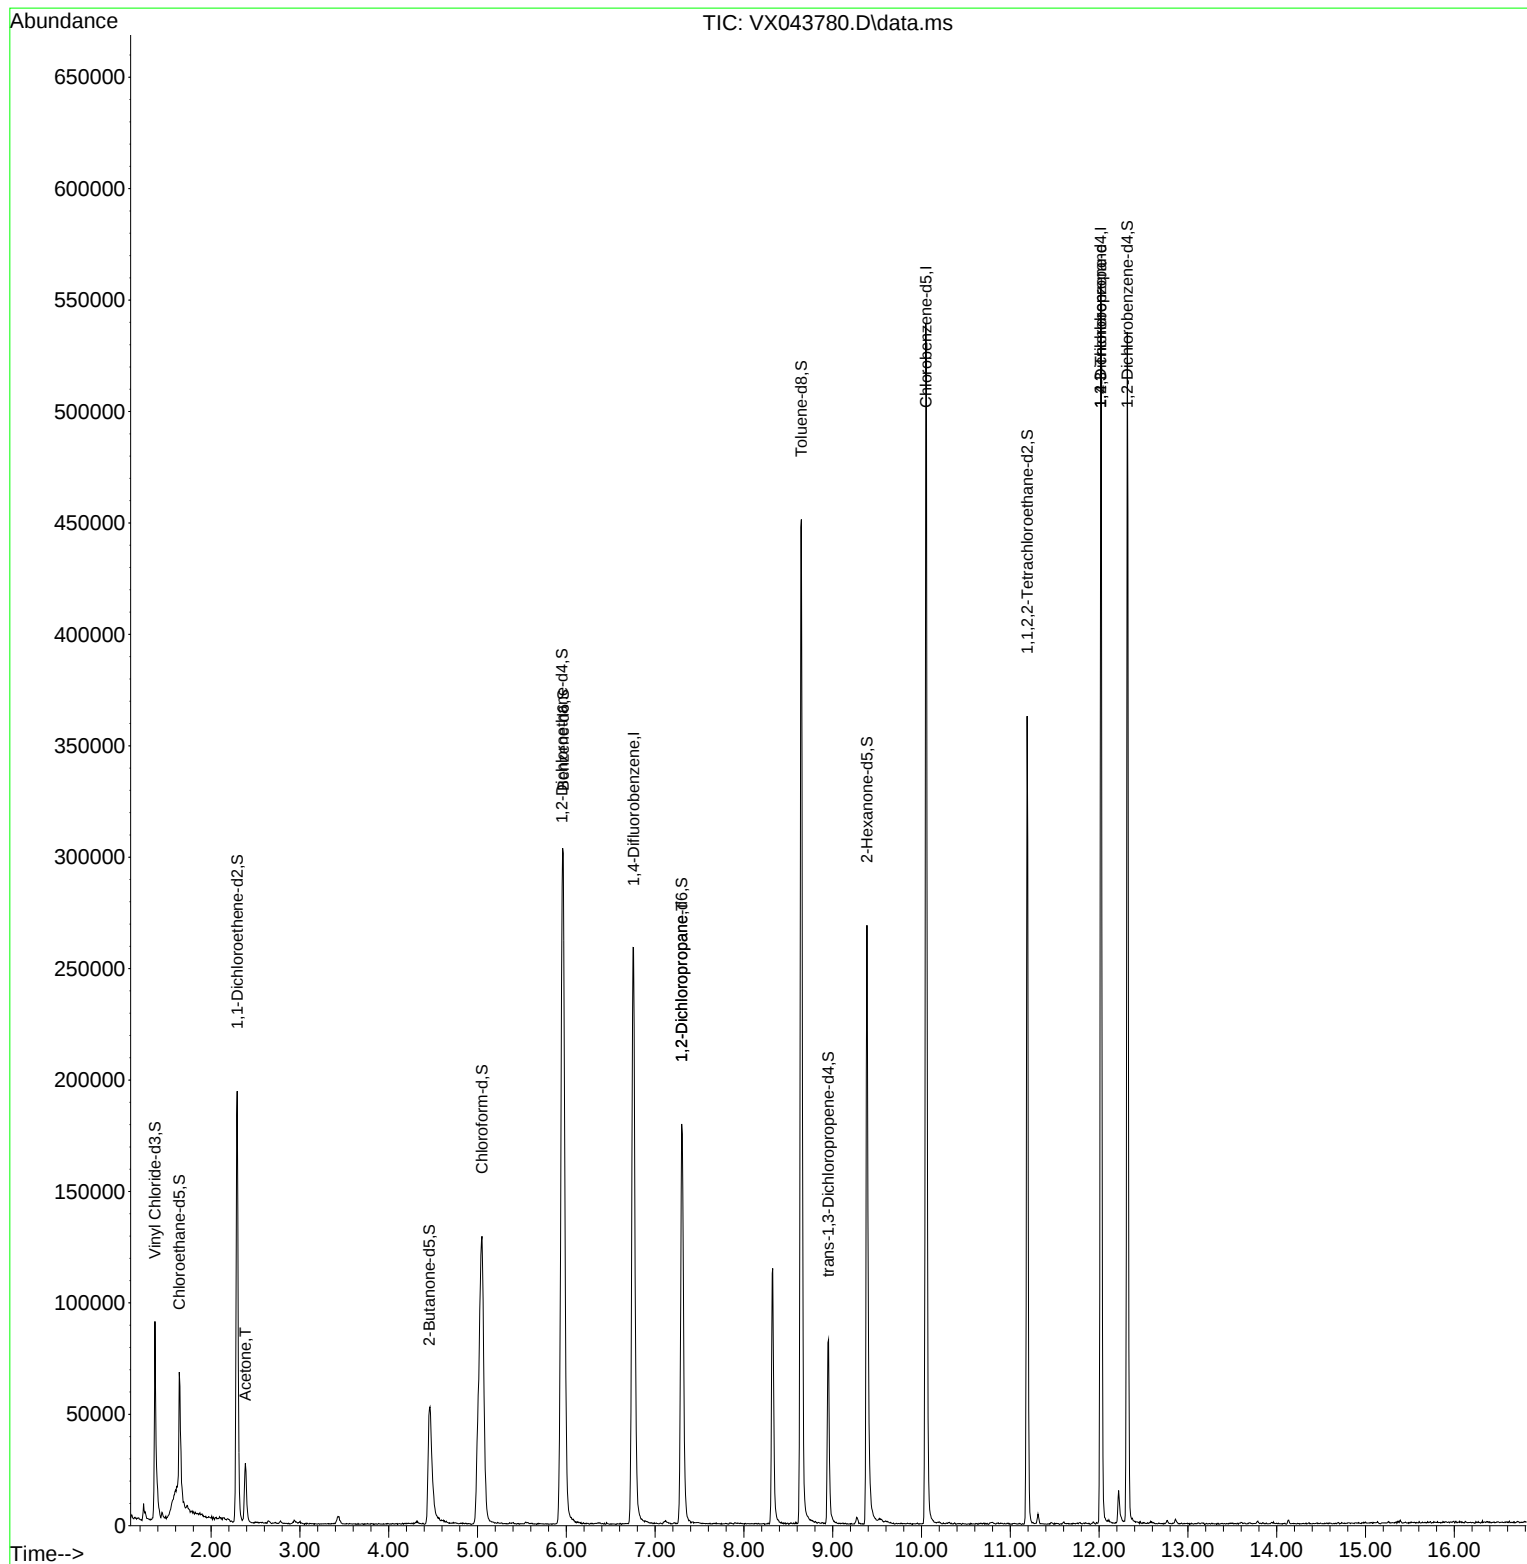


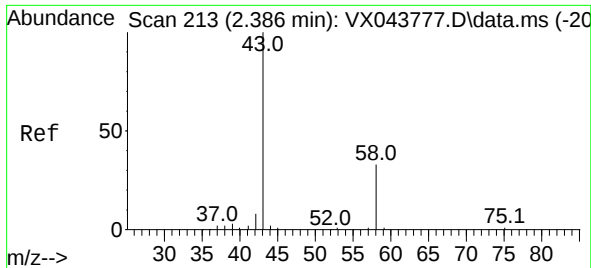

#13
Acetone
Concen: 29.569 ug/L
RT: 2.386 min Scan# 213
Delta R.T. 0.000 min
Lab File: VX043780.D
Acq: 11 Nov 2024 10:40




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 28640
Ion Ratio Lower Upper
43 100
58 34.1 0.0 63.6

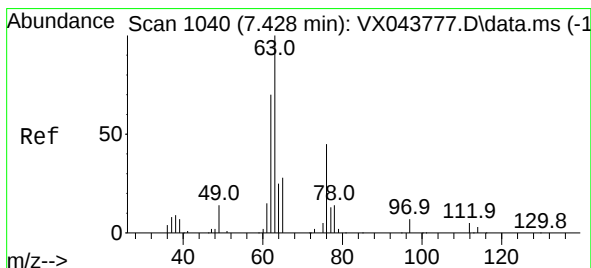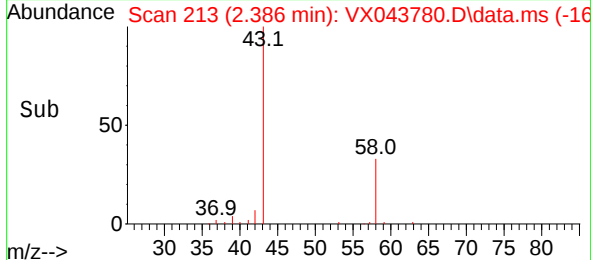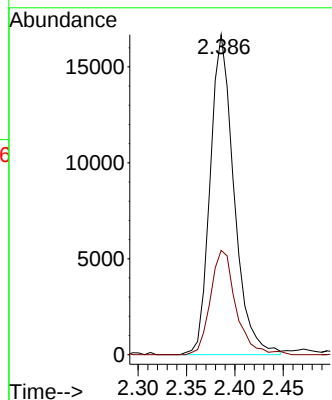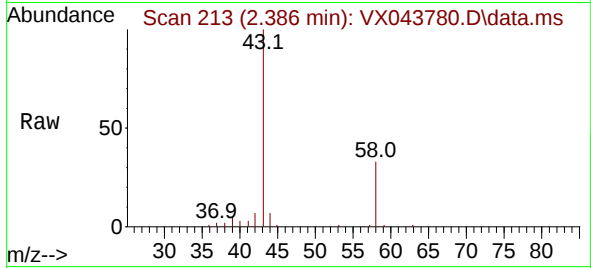

#37
1,2-Dichloropropane
Concen: 5.361 ug/L
RT: 7.300 min Scan# 1019
Delta R.T. -0.128 min
Lab File: VX043780.D
Acq: 11 Nov 2024 10:40

Tgt Ion: 63 Resp: 10912
Ion Ratio Lower Upper
63 100
112 0.0 3.8 5.8#

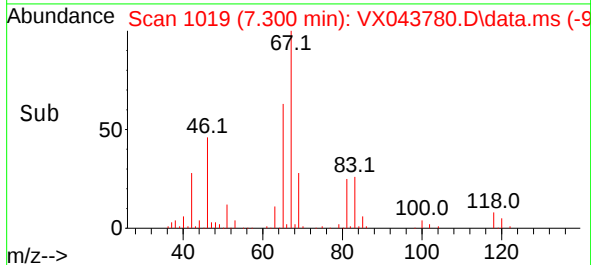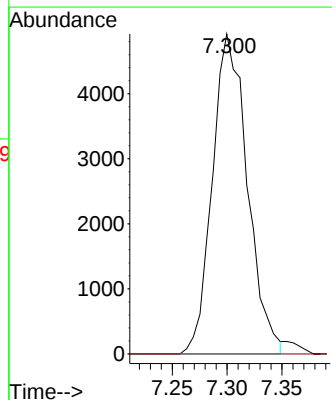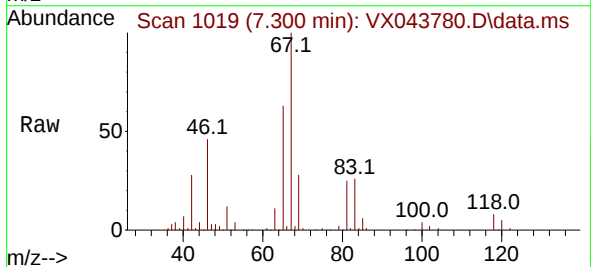

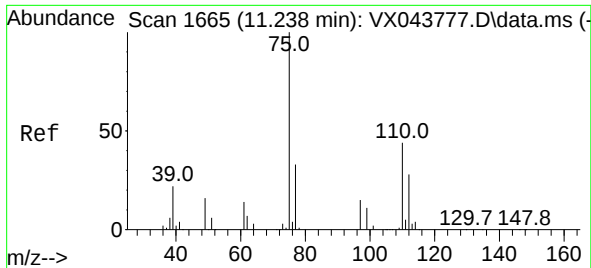

#61

1,2,3-Trichloropropane

Concen: 5.703 ug/L

RT: 12.018 min Scan# 11

Delta R.T. 0.780 min


Lab File: VX043780.D

Acq: 11 Nov 2024 10:40

Instrument :

MSVOA_X

ClientSampleId :

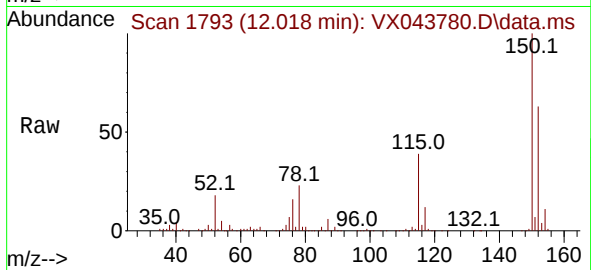

Tgt Ion: 75 Resp: 13516

Ion Ratio Lower Upper

75 100

77 31.8 25.4 38.0

110 3.2 33.6 50.4#

