

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043788.D
 Acq On : 11 Nov 2024 13:45
 Operator : JC/MD
 Sample : P4786-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 12 00:54:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 12 00:51:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	324120	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	285644	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	125656	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	69970	40.522	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	81.040%
7) Chloroethane-d5	1.648	69	39833	53.668	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	107.340%
11) 1,1-Dichloroethene-d2	2.294	65	34063	42.733	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.460%
21) 2-Butanone-d5	4.464	46	94323	83.430	ug/L	0.01
Spiked Amount	100.000	Range	40 - 130	Recovery	=	83.430%
24) Chloroform-d	5.050	84	159244	42.780	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.560%
26) 1,2-Dichloroethane-d4	5.952	65	101461	42.906	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.820%
32) Benzene-d6	5.970	84	335103	45.376	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.760%
36) 1,2-Dichloropropane-d6	7.305	67	99818	44.427	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	88.860%
41) Toluene-d8	8.647	98	299585	44.656	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.320%
43) trans-1,3-Dichloroprop...	8.951	79	42324	39.390	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.780%
47) 2-Hexanone-d5	9.384	63	80570	90.612	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.610%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	132719	46.038	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.080%
66) 1,2-Dichlorobenzene-d4	12.323	152	108125	49.664	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.320%
Target Compounds						
13) Acetone	2.386	43	19222	18.281	ug/L	Qvalue 94
61) 1,2,3-Trichloropropane	12.018	75	13515	5.541	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043788.D
Acq On : 11 Nov 2024 13:45
Operator : JC/MD
Sample : P4786-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 12 00:54:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 12 00:51:02 2024
Response via : Initial Calibration

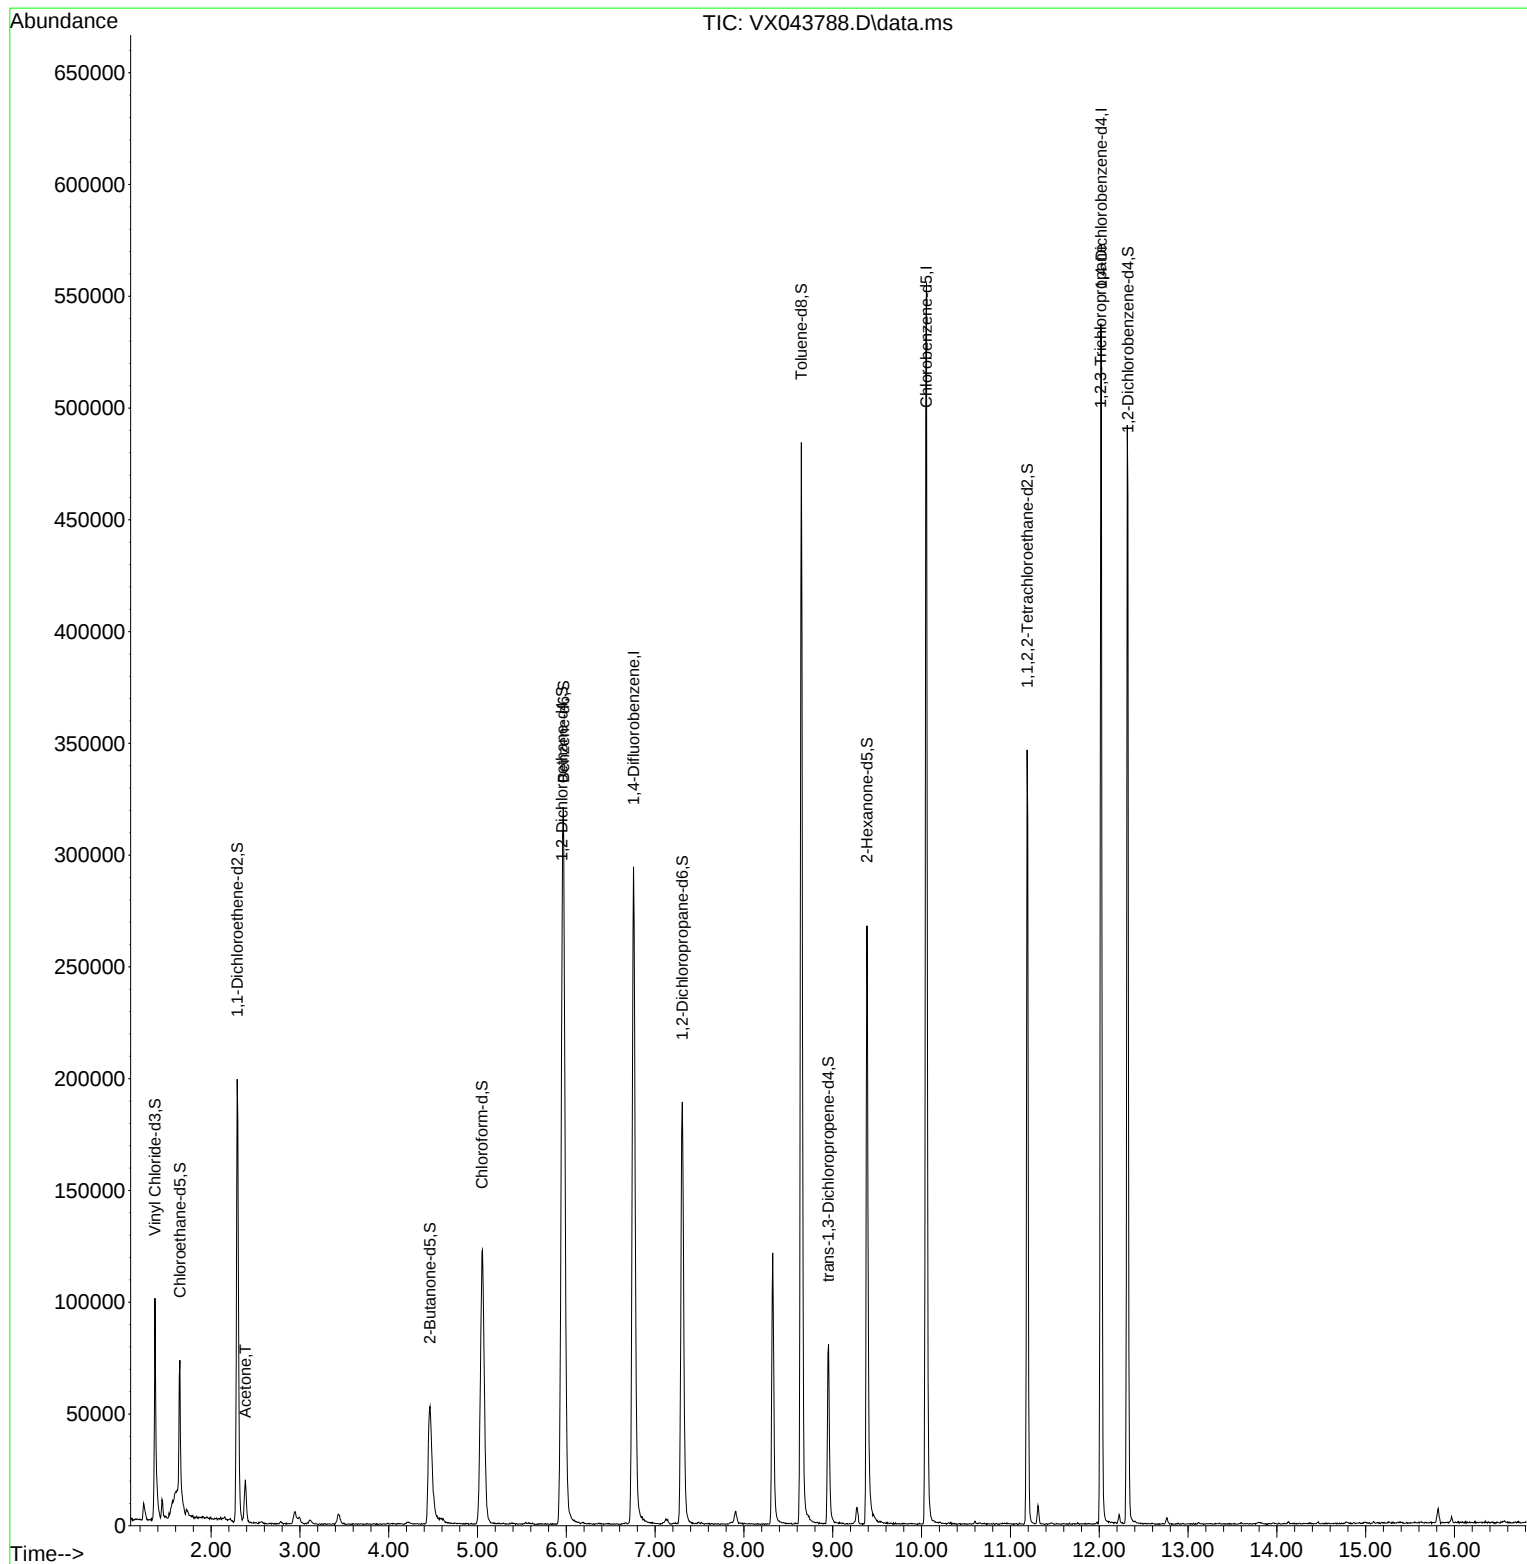

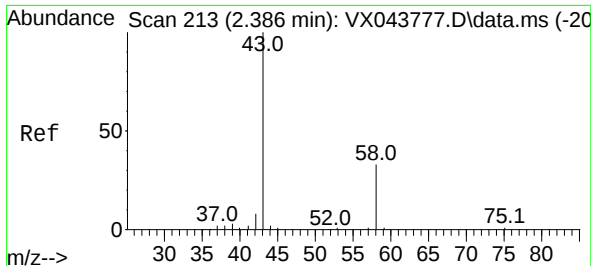

#13

Acetone

Concen: 18.281 ug/L

RT: 2.386 min Scan# 21

Delta R.T. -0.000 min

Lab File: VX043788.D

Acq: 11 Nov 2024 13:45

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 19222

Ion Ratio Lower Upper

43 100

58 35.4 0.0 63.6

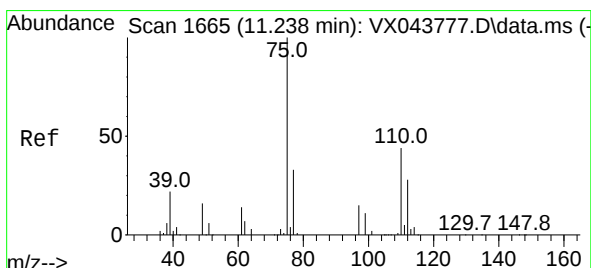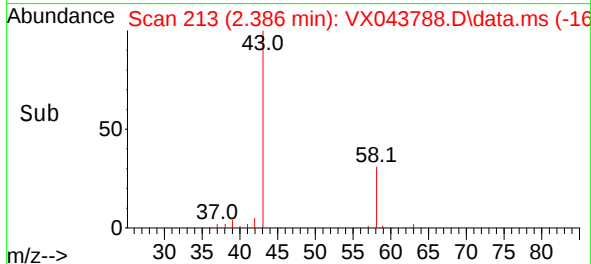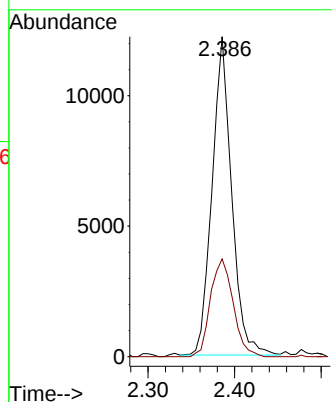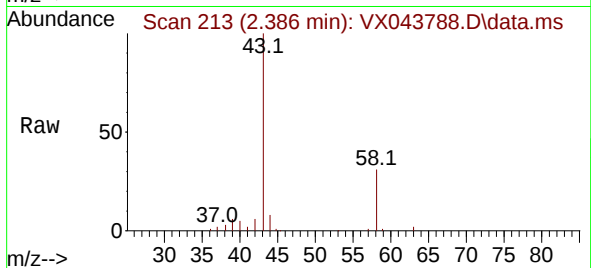

#61

1,2,3-Trichloropropane

Concen: 5.541 ug/L

RT: 12.018 min Scan# 1793

Delta R.T. 0.780 min

Lab File: VX043788.D

Acq: 11 Nov 2024 13:45

Tgt Ion: 75 Resp: 13515

Ion Ratio Lower Upper

75 100

77 32.7 25.4 38.0

110 3.9 33.6 50.4#

