

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043790.D
 Acq On : 11 Nov 2024 14:31
 Operator : JC/MD
 Sample : P4786-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 12 00:54:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 12 00:51:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	170099	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	160868	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	70955	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	37021	40.854	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	81.700%		
7) Chloroethane-d5	1.648	69	24435	62.732	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	125.460%		
11) 1,1-Dichloroethene-d2	2.294	65	17098	40.873	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	81.740%		
21) 2-Butanone-d5	4.459	46	58376	98.388	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	98.390%		
24) Chloroform-d	5.056	84	93813	48.023	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.040%		
26) 1,2-Dichloroethane-d4	5.952	65	60509	48.758	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.520%		
32) Benzene-d6	5.970	84	192567	46.300	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.600%		
36) 1,2-Dichloropropane-d6	7.306	67	60397	47.732	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.460%		
41) Toluene-d8	8.647	98	168635	44.634	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.260%		
43) trans-1,3-Dichloroprop...	8.952	79	25195	41.636	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.280%		
47) 2-Hexanone-d5	9.384	63	48305	96.462	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	96.460%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	80515	49.593	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	99.180%		
66) 1,2-Dichlorobenzene-d4	12.317	152	66386	54.000	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	108.000%		
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	12.018	75	7898	5.734	ug/L	# 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043790.D
Acq On : 11 Nov 2024 14:31
Operator : JC/MD
Sample : P4786-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Nov 12 00:54:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 12 00:51:02 2024
Response via : Initial Calibration

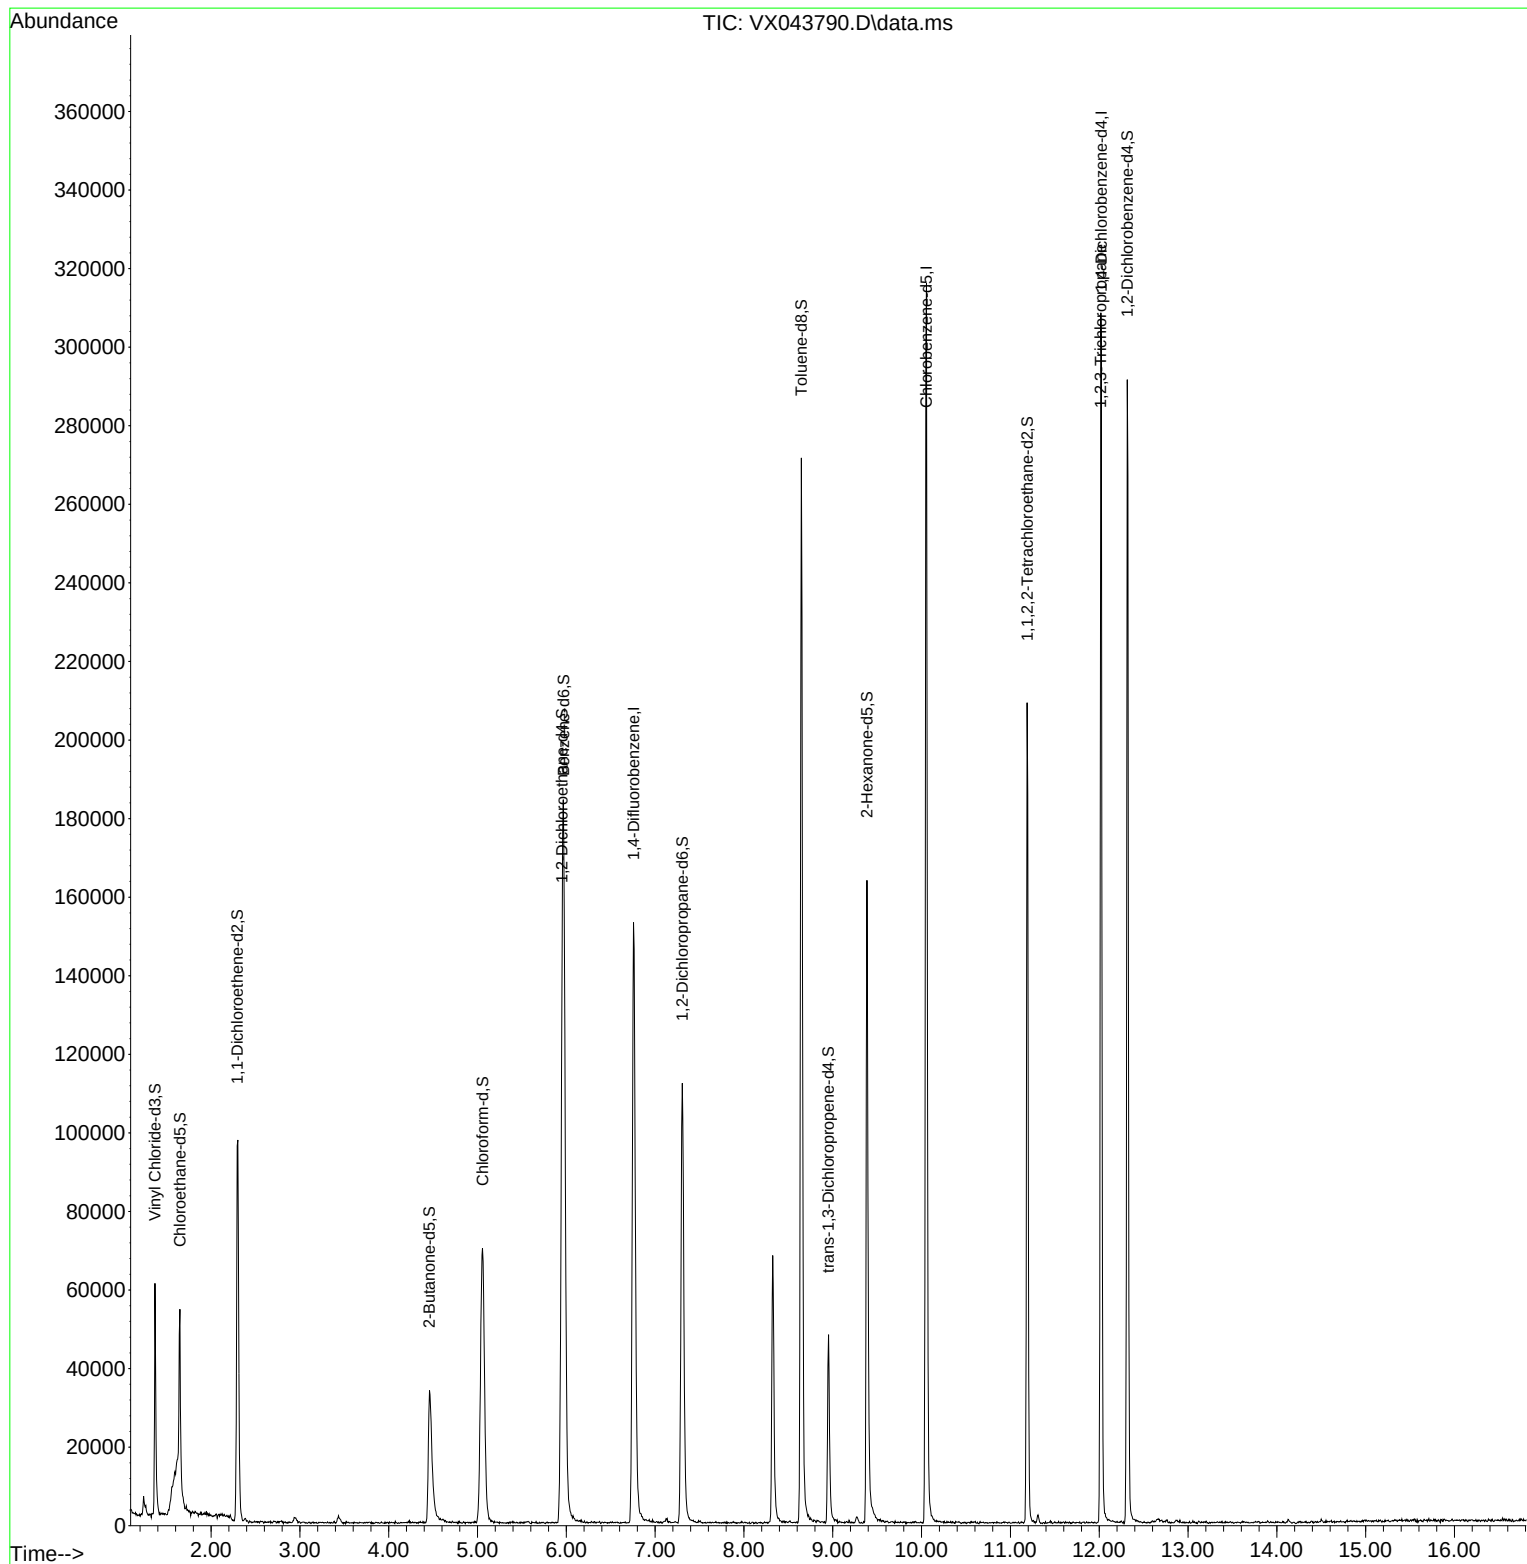

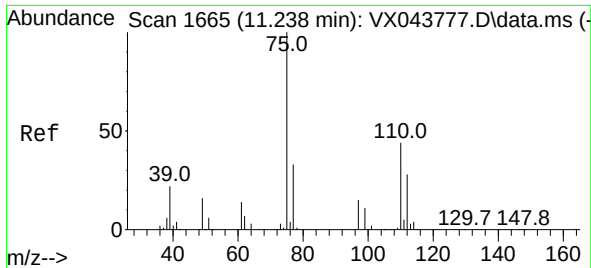

#61
 1,2,3-Trichloropropane
 Concen: 5.734 ug/L
 RT: 12.018 min Scan# 11
 Delta R.T. 0.780 min
 Lab File: VX043790.D
 Acq: 11 Nov 2024 14:31

Instrument :
 MSVOA_X
 ClientSampleId :

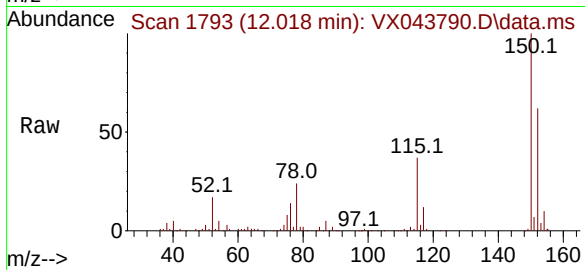

Tgt Ion: 75 Resp: 7898
 Ion Ratio Lower Upper
 75 100
 77 31.3 25.4 38.0
 110 3.7 33.6 50.4#

