

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043791.D
 Acq On : 11 Nov 2024 14:54
 Operator : JC/MD
 Sample : P4786-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 12 00:54:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 12 00:51:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	186174	50.000	ug/L	0.01
28) Chlorobenzene-d5	10.055	117	169425	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	72379	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	37909	38.222	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	76.440%		
7) Chloroethane-d5	1.648	69	26178	61.404	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	122.800%		
11) 1,1-Dichloroethene-d2	2.300	65	18294	39.956	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	79.920%		
21) 2-Butanone-d5	4.465	46	56437	86.907	ug/L	0.01
Spiked Amount 100.000	Range 40 - 130		Recovery =	86.910%		
24) Chloroform-d	5.056	84	96138	44.964	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.920%		
26) 1,2-Dichloroethane-d4	5.952	65	58146	42.808	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.620%		
32) Benzene-d6	5.970	84	196668	44.898	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.800%		
36) 1,2-Dichloropropane-d6	7.305	67	60284	45.236	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	90.480%		
41) Toluene-d8	8.647	98	175034	43.988	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.980%		
43) trans-1,3-Dichloroprop...	8.952	79	23340	36.622	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	73.240%		
47) 2-Hexanone-d5	9.384	63	46685	88.519	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	88.520%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	77607	45.388	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	90.780%		
66) 1,2-Dichlorobenzene-d4	12.317	152	64164	51.165	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.340%		
Target Compounds					Qvalue	
48) 2-Hexanone	9.384	43	5207	3.979	ug/L #	73
61) 1,2,3-Trichloropropane	12.018	75	8396	5.976	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043791.D
Acq On : 11 Nov 2024 14:54
Operator : JC/MD
Sample : P4786-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 12 00:54:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 12 00:51:02 2024
Response via : Initial Calibration

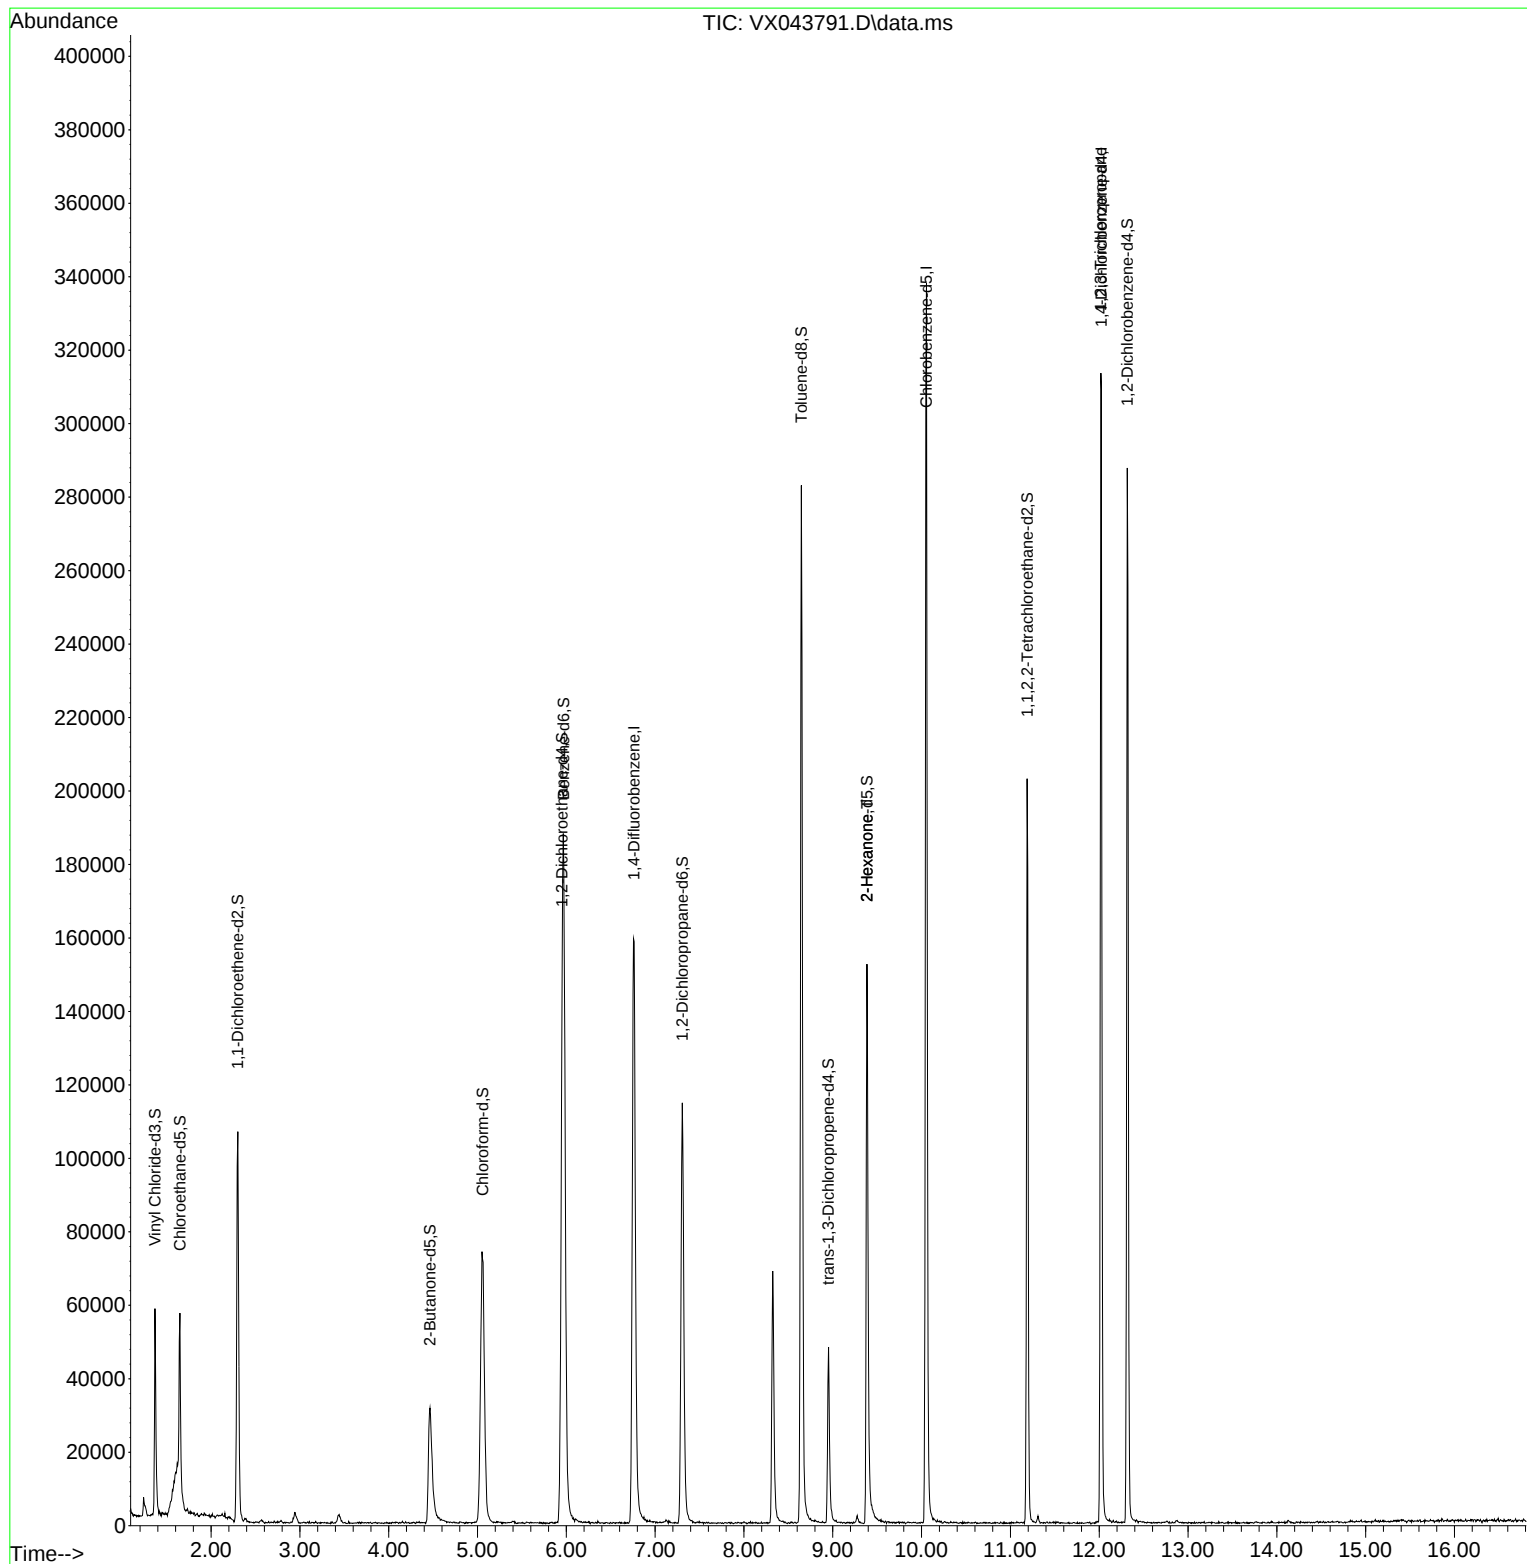

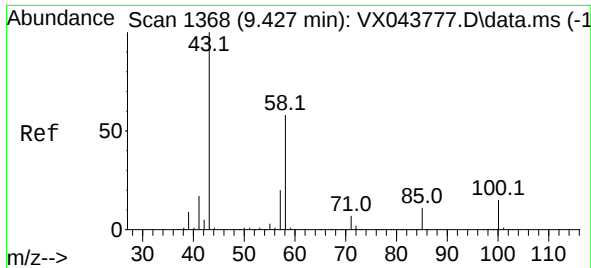

#48

2-Hexanone

Concen: 3.979 ug/L

RT: 9.384 min Scan# 14

Delta R.T. -0.043 min

Lab File: VX043791.D





Acq: 11 Nov 2024 14:54

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion: 43	Resp: 5207
Ion Ratio	Lower Upper
43	100
58	32.7 44.6 67.0#
57	24.1 15.7 23.5#
100	0.0 11.0 16.4#

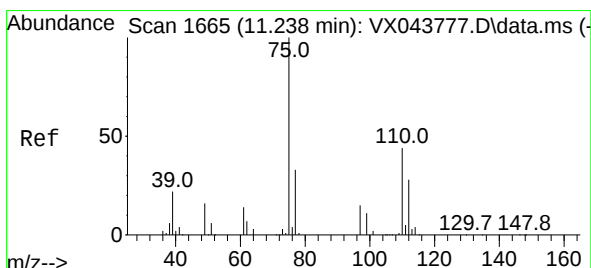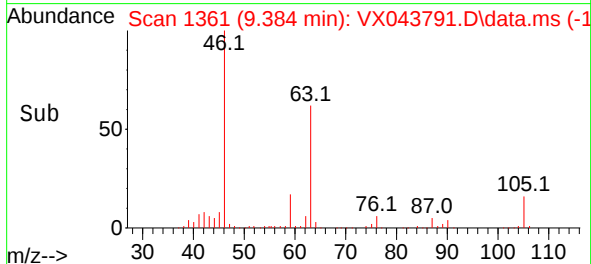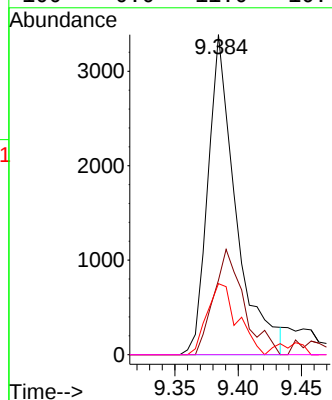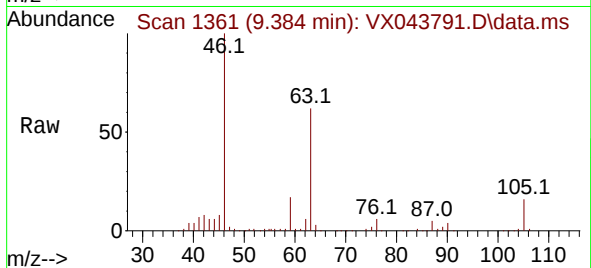

#61

1,2,3-Trichloropropane

Concen: 5.976 ug/L

RT: 12.018 min Scan# 1793

Delta R.T. 0.780 min

Lab File: VX043791.D

Acq: 11 Nov 2024 14:54

Tgt Ion: 75	Resp: 8396
Ion Ratio	Lower Upper
75	100
77	28.5 25.4 38.0
110	3.3 33.6 50.4#

