

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043795.D
 Acq On : 11 Nov 2024 16:27
 Operator : JC/MD
 Sample : P4786-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 12 00:55:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 12 00:51:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	281081	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	253210	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	110392	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	57203	38.201	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	76.400%		
7) Chloroethane-d5	1.648	69	35176	54.651	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	109.300%		
11) 1,1-Dichloroethene-d2	2.294	65	28983	41.928	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.860%		
21) 2-Butanone-d5	4.465	46	85260	86.961	ug/L	0.01
Spiked Amount 100.000	Range 40 - 130		Recovery =	86.960%		
24) Chloroform-d	5.056	84	140794	43.615	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.240%		
26) 1,2-Dichloroethane-d4	5.952	65	89016	43.408	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.820%		
32) Benzene-d6	5.964	84	288296	44.038	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.080%		
36) 1,2-Dichloropropane-d6	7.306	67	88192	44.280	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	88.560%		
41) Toluene-d8	8.647	98	260809	43.856	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.720%		
43) trans-1,3-Dichloroprop...	8.952	79	36305	38.116	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	76.240%		
47) 2-Hexanone-d5	9.384	63	73391	93.110	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	93.110%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	121977	47.732	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	95.460%		
66) 1,2-Dichlorobenzene-d4	12.317	152	97958	51.215	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.440%		
Target Compounds			Qvalue			
37) 1,2-Dichloropropane	7.306	63	9786	5.090	ug/L #	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043795.D
Acq On : 11 Nov 2024 16:27
Operator : JC/MD
Sample : P4786-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 12 00:55:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 12 00:51:02 2024
Response via : Initial Calibration

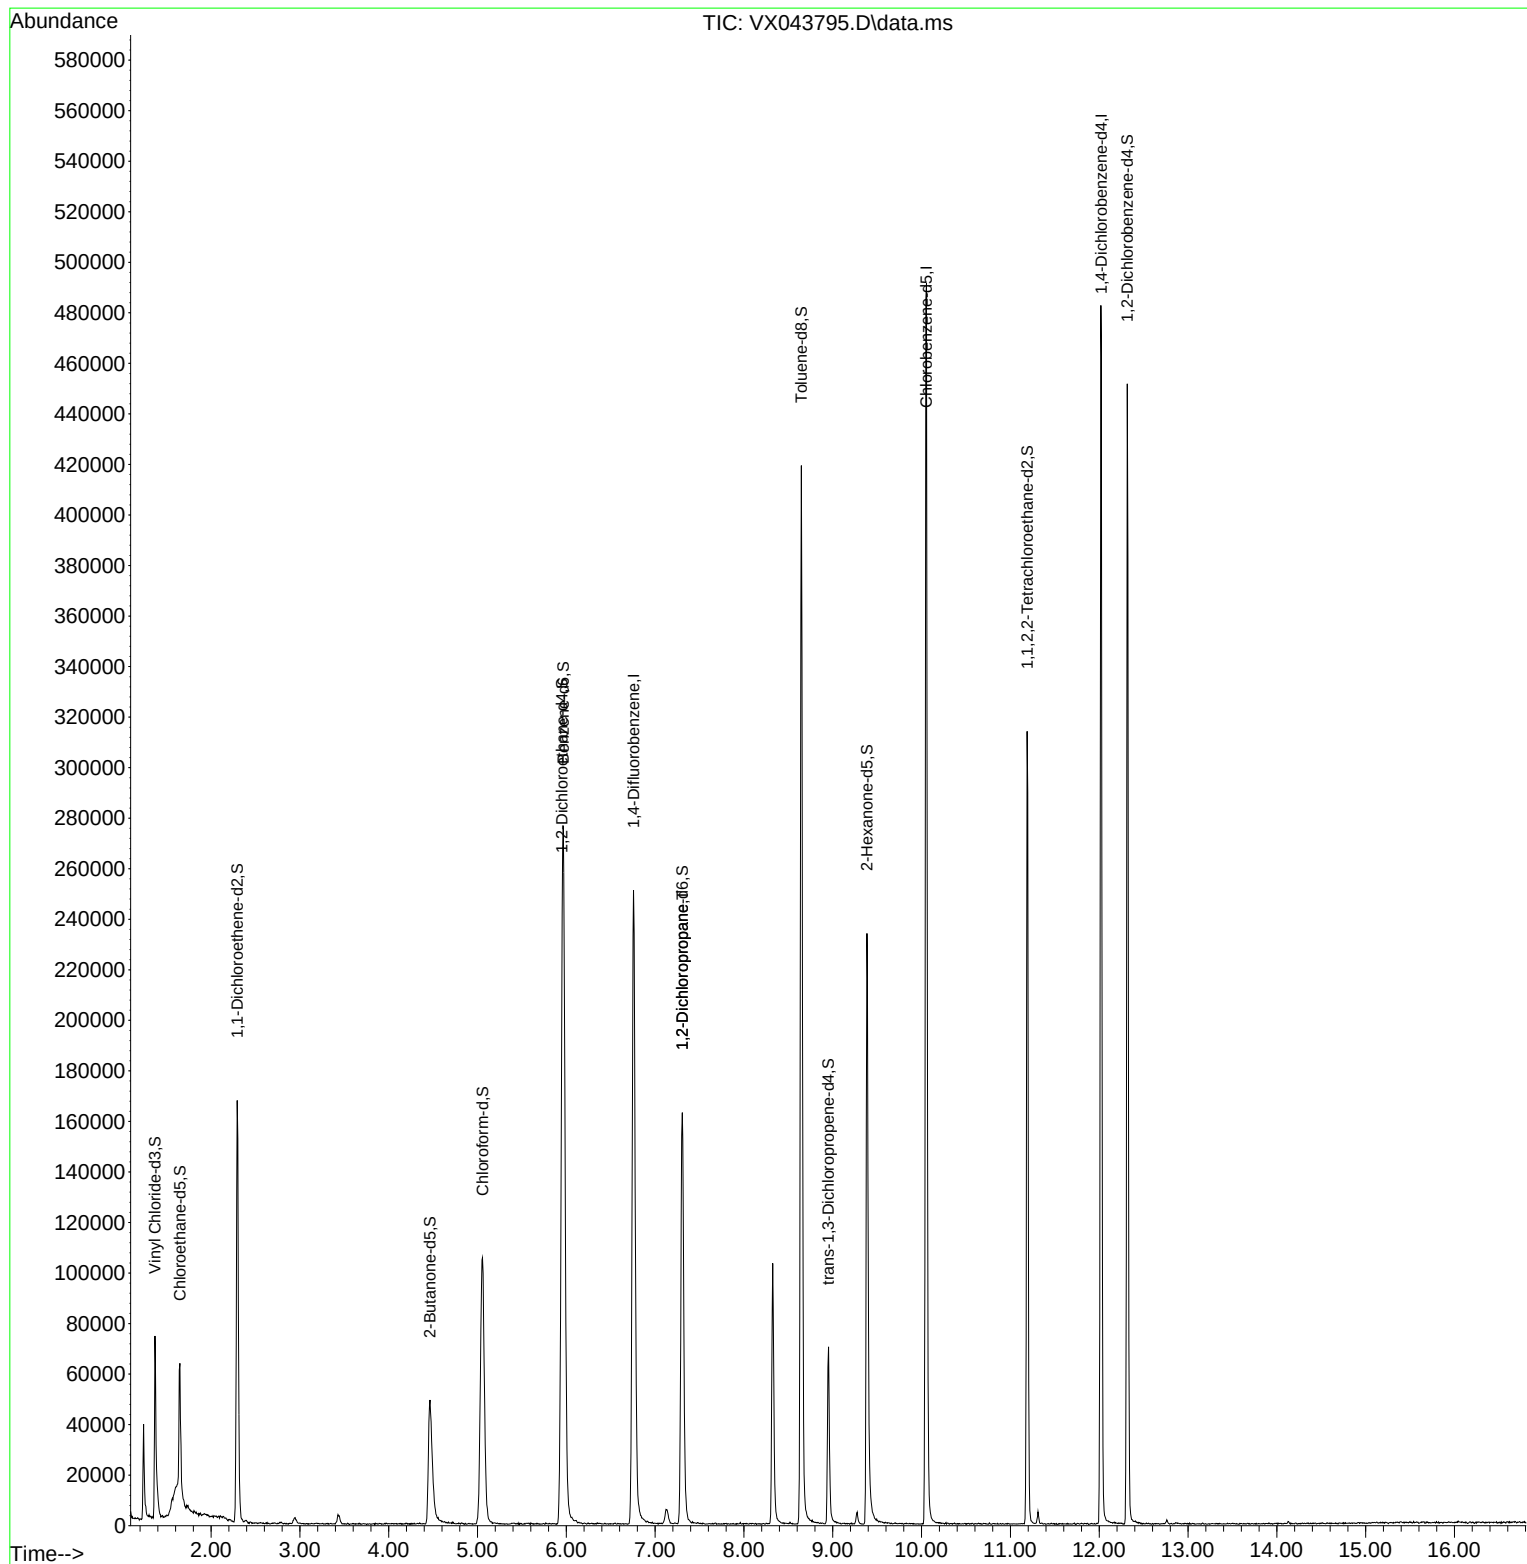

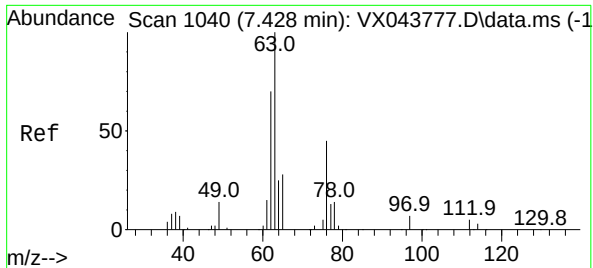

#37
1,2-Dichloropropane
Concen: 5.090 ug/L
RT: 7.306 min Scan# 10
Delta R.T. -0.122 min
Lab File: VX043795.D
Acq: 11 Nov 2024 16:27

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 63 Resp: 9786
Ion Ratio Lower Upper
63 100
112 0.0 3.8 5.8#

