

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043780.D
 Acq On : 11 Nov 2024 10:40
 Operator : JC/MD
 Sample : P4751-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH9H0

Quant Time: Nov 12 00:51:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 12 00:51:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	298559	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.049	117	268104	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	122106	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	69828	43.902	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.800%
7) Chloroethane-d5	1.642	69	37902	55.439	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	110.880%
11) 1,1-Dichloroethene-d2	2.294	65	33418	45.513	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.020%
21) 2-Butanone-d5	4.459	46	96481	92.645	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	92.650%
24) Chloroform-d	5.050	84	153909	44.887	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.780%
26) 1,2-Dichloroethane-d4	5.952	65	95748	43.957	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.920%
32) Benzene-d6	5.964	84	322685	46.553	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.100%
36) 1,2-Dichloropropane-d6	7.300	67	95955	45.501	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.000%
41) Toluene-d8	8.647	98	293267	46.575	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.140%
43) trans-1,3-Dichloroprop...	8.952	79	42080	41.725	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.440%
47) 2-Hexanone-d5	9.385	63	83177	99.663	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.660%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	135144	49.947	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.900%
66) 1,2-Dichlorobenzene-d4	12.317	152	114411	54.079	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	108.160%
Target Compounds					Qvalue	
13) Acetone	2.386	43	28640	29.569	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043780.D
Acq On : 11 Nov 2024 10:40
Operator : JC/MD
Sample : P4751-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH9H0

Quant Time: Nov 12 00:51:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 12 00:51:02 2024
Response via : Initial Calibration

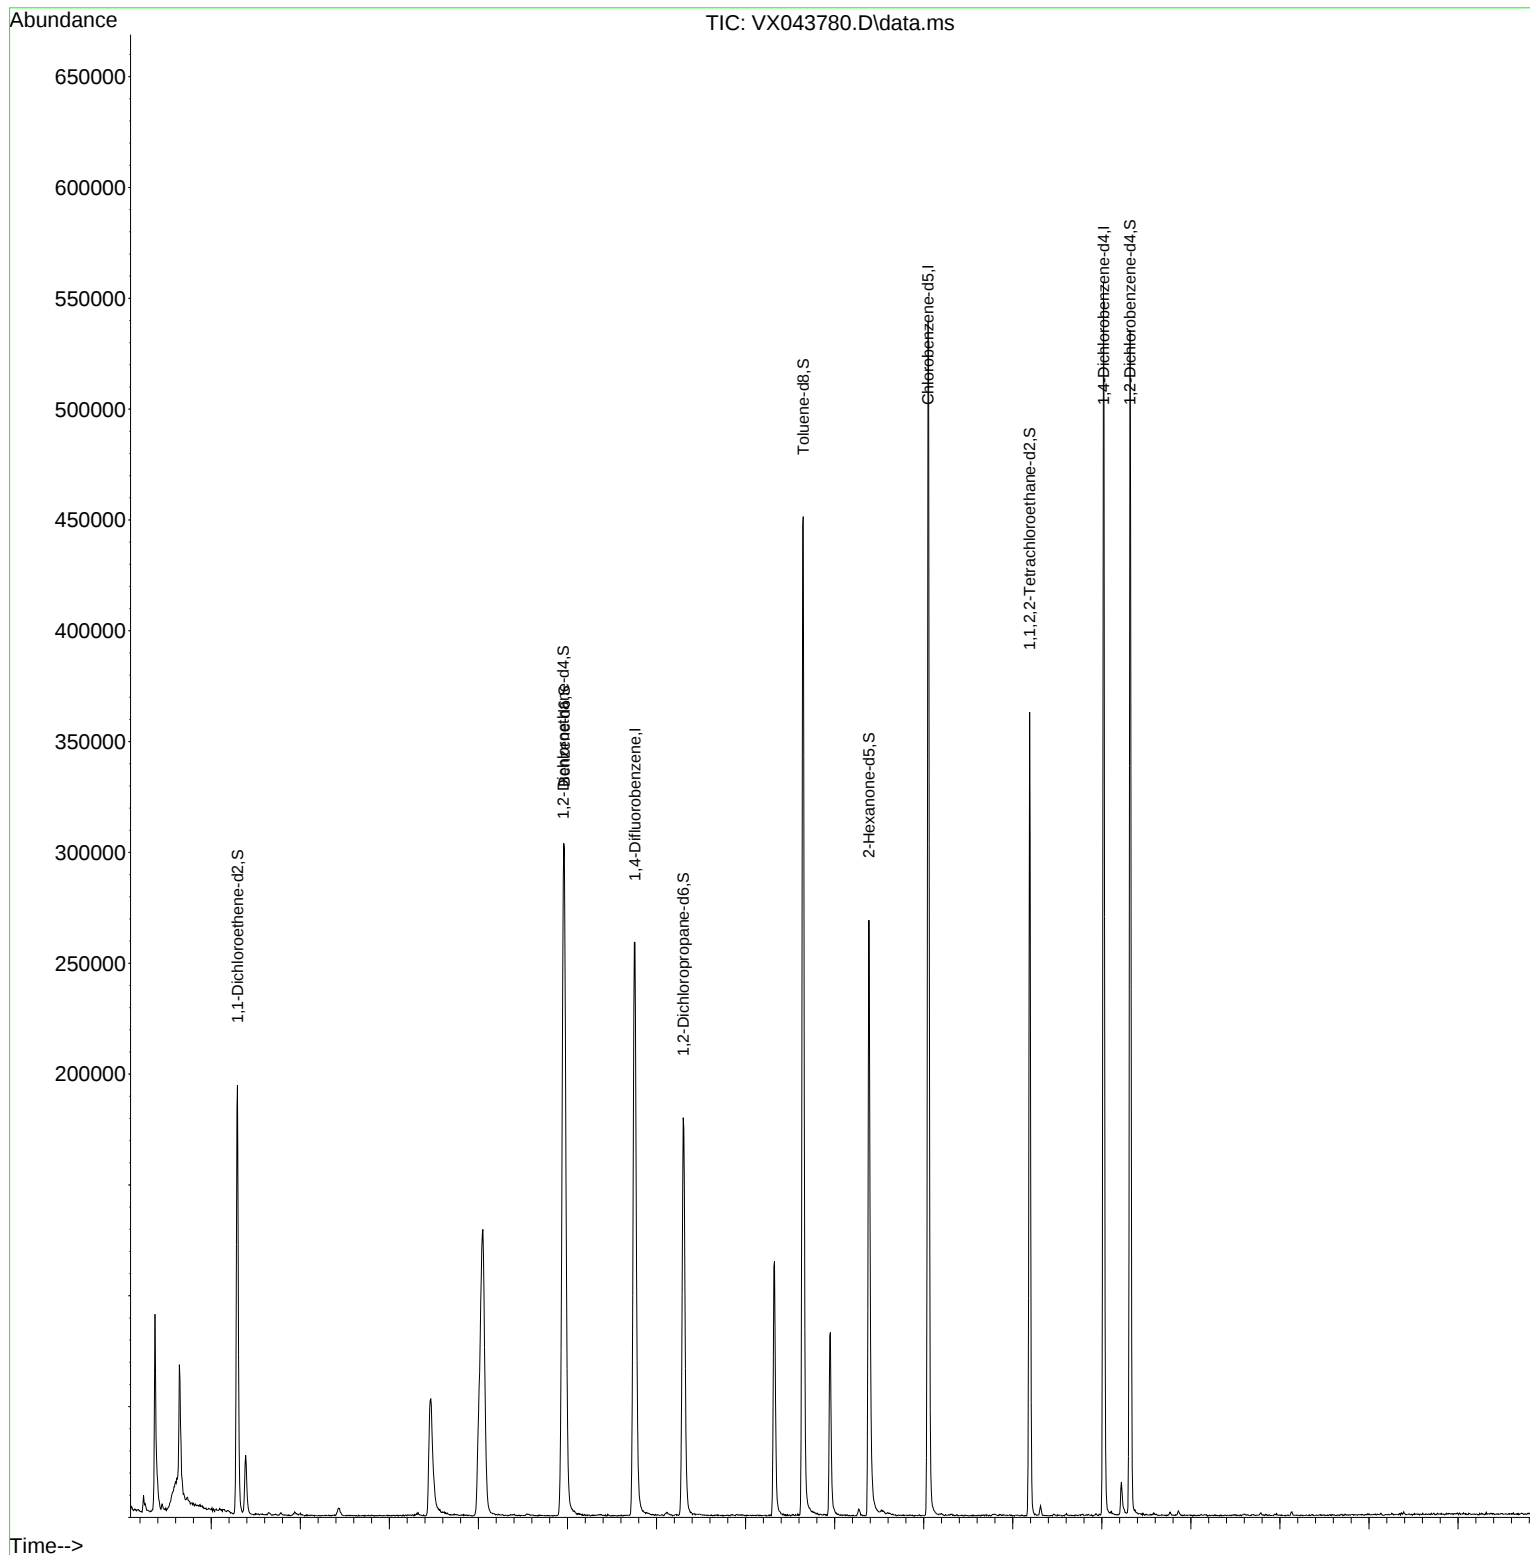

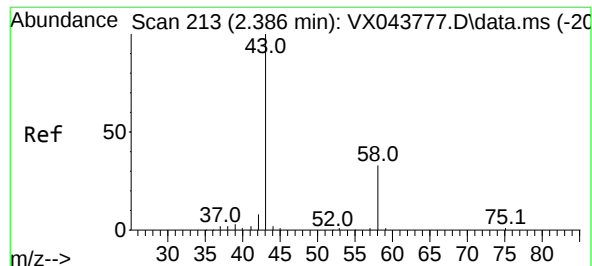

#13
 Acetone
 Concen: 29.569 ug/L
 RT: 2.386 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VX043780.D
 Acq: 11 Nov 2024 10:40

Instrument :
 MSVOA_X
 ClientSampleId :
 BH9H0

Tgt Ion: 43 Resp: 28640
 Ion Ratio Lower Upper
 43 100
 58 34.1 0.0 63.6

