

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043780.D
 Acq On : 11 Nov 2024 10:40
 Operator : JC/MD
 Sample : P4751-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH9H0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043780.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	31	rBV2	7543	10794	1.18%	0.145%
2	1.368	41	46	57	rBV	88266	116195	12.75%	1.562%
3	1.642	88	91	102	rVB	60967	94402	10.36%	1.269%
4	2.294	191	198	207	rBV	193281	304910	33.45%	4.098%
5	2.386	208	213	225	rVB	26661	46351	5.08%	0.623%
6	2.648	253	256	262	rVB4	1224	2142	0.23%	0.029%
7	2.782	274	278	284	rVB4	1137	1517	0.17%	0.020%
8	2.935	295	303	306	rBV3	1758	3192	0.35%	0.043%
9	3.069	322	325	326	rBV	559	444	0.05%	0.006%
10	3.111	330	332	335	rBV2	288	322	0.04%	0.004%
11	3.166	340	341	346	rBV2	310	478	0.05%	0.006%
12	3.428	378	384	393	rVB5	3363	7921	0.87%	0.106%
13	3.733	431	434	436	rBV2	352	380	0.04%	0.005%
14	3.800	444	445	449	rVV3	404	431	0.05%	0.006%
15	3.886	457	459	462	rVV2	358	349	0.04%	0.005%
16	4.044	482	485	486	rBV2	366	366	0.04%	0.005%
17	4.123	494	498	502	rBV2	333	603	0.07%	0.008%
18	4.312	525	529	533	rVV4	1182	1868	0.20%	0.025%
19	4.465	544	554	574	rBV2	52675	174219	19.11%	2.342%
20	5.050	633	650	665	rBV3	129082	505837	55.49%	6.799%
21	5.227	677	679	682	rVB3	451	347	0.04%	0.005%
22	5.361	699	701	704	rVV	467	487	0.05%	0.007%
23	5.483	719	721	723	rBV	277	327	0.04%	0.004%
24	5.544	727	731	733	rBV3	795	1074	0.12%	0.014%
25	5.684	751	754	755	rBV	461	468	0.05%	0.006%
26	5.849	779	781	784	rBV2	353	384	0.04%	0.005%
27	5.958	788	799	818	rBV3	303101	911613	100.00%	12.253%
28	6.190	836	837	839	rVB2	516	331	0.04%	0.004%
29	6.452	878	880	886	rBV2	795	775	0.09%	0.010%
30	6.751	920	929	944	rBV	258587	647259	71.00%	8.700%
31	7.117	983	989	992	rBV6	1544	3145	0.34%	0.042%
32	7.220	1002	1006	1007	rBV3	489	573	0.06%	0.008%
33	7.300	1011	1019	1032	rBV2	179316	404327	44.35%	5.435%
34	7.617	1068	1071	1073	rVB2	434	426	0.05%	0.006%
35	7.836	1105	1107	1109	rBV	551	534	0.06%	0.007%
36	7.897	1115	1117	1121	rBV2	599	955	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043780.D
 Acq On : 11 Nov 2024 10:40
 Operator : JC/MD
 Sample : P4751-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH9H0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	8.013	1135	1136	1138	rBV	453	353	0.04%	0.005%
38	8.159	1158	1160	1163	rVB3	347	334	0.04%	0.004%
39	8.263	1172	1177	1178	rBV	489	483	0.05%	0.006%
40	8.324	1181	1187	1199	rBV	114703	198961	21.83%	2.674%
41	8.488	1212	1214	1217	rVB	599	641	0.07%	0.009%
42	8.525	1217	1220	1224	rBV3	737	1274	0.14%	0.017%
43	8.647	1233	1240	1256	rBV	450560	760989	83.48%	10.229%
44	8.952	1285	1290	1303	rVB	82457	130323	14.30%	1.752%
45	9.269	1338	1342	1346	rBV	3013	4699	0.52%	0.063%
46	9.385	1356	1361	1381	rBV	268633	431091	47.29%	5.795%
47	10.049	1465	1470	1486	rBV	538374	760162	83.39%	10.218%
48	10.244	1500	1502	1506	rBV2	442	402	0.04%	0.005%
49	10.299	1510	1511	1512	rVV	671	455	0.05%	0.006%
50	10.372	1519	1523	1525	rVB2	626	687	0.08%	0.009%
51	10.464	1536	1538	1541	rBV	492	601	0.07%	0.008%
52	10.549	1551	1552	1555	rBV	511	481	0.05%	0.006%
53	10.665	1569	1571	1574	rVV3	503	566	0.06%	0.008%
54	10.701	1574	1577	1578	rVV2	593	545	0.06%	0.007%
55	10.738	1581	1583	1585	rVB2	454	342	0.04%	0.005%
56	10.848	1599	1601	1602	rBV2	549	377	0.04%	0.005%
57	11.031	1629	1631	1633	rBV2	369	493	0.05%	0.007%
58	11.189	1652	1657	1666	rBV	362340	464319	50.93%	6.241%
59	11.311	1673	1677	1681	rVB2	4317	5281	0.58%	0.071%
60	11.457	1699	1701	1707	rVB5	806	1170	0.13%	0.016%
61	11.604	1721	1725	1727	rBV3	1054	1292	0.14%	0.017%
62	11.707	1740	1742	1743	rBV2	451	429	0.05%	0.006%
63	11.787	1751	1755	1758	rVB4	666	924	0.10%	0.012%
64	11.829	1758	1762	1763	rBV2	460	421	0.05%	0.006%
65	11.933	1773	1779	1783	rBV5	1150	2012	0.22%	0.027%
66	11.969	1783	1785	1788	rBV	738	764	0.08%	0.010%
67	12.018	1788	1793	1805	rBV	556309	704307	77.26%	9.467%
68	12.219	1822	1826	1837	rBV2	14350	22753	2.50%	0.306%
69	12.317	1837	1842	1857	rVB	534141	670991	73.60%	9.019%
70	12.579	1883	1885	1886	rBV	763	450	0.05%	0.006%
71	12.671	1898	1900	1904	rBV2	359	351	0.04%	0.005%
72	12.768	1911	1916	1919	rBV2	1503	1880	0.21%	0.025%
73	12.860	1928	1931	1938	rVB3	2204	3252	0.36%	0.044%
74	12.927	1940	1942	1945	rVB3	451	322	0.04%	0.004%
75	13.122	1970	1974	1977	rVV4	465	680	0.07%	0.009%
76	13.207	1985	1988	1990	rBV2	568	684	0.08%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043780.D
 Acq On : 11 Nov 2024 10:40
 Operator : JC/MD
 Sample : P4751-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH9H0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	13.268	1996	1998	2003	rBV	472	573	0.06%	0.008%
78	13.329	2007	2008	2011	rBV2	507	496	0.05%	0.007%
79	13.579	2047	2049	2050	rBV	532	549	0.06%	0.007%
80	13.701	2063	2069	2071	rBV3	524	972	0.11%	0.013%
81	13.786	2079	2083	2087	rVV3	1139	1454	0.16%	0.020%
82	13.841	2090	2092	2095	rBV2	532	514	0.06%	0.007%
83	13.945	2106	2109	2111	rBV4	679	843	0.09%	0.011%
84	13.963	2111	2112	2115	rVB	762	445	0.05%	0.006%
85	14.134	2136	2140	2144	rBV2	1771	2446	0.27%	0.033%
86	14.560	2207	2210	2211	rBV2	387	389	0.04%	0.005%
87	14.695	2228	2232	2234	rVB3	652	833	0.09%	0.011%
88	14.731	2236	2238	2241	rVV	539	443	0.05%	0.006%
89	14.957	2274	2275	2278	rBV3	372	449	0.05%	0.006%
90	14.999	2281	2282	2285	rVB	560	334	0.04%	0.004%
91	15.091	2296	2297	2299	rBV	487	430	0.05%	0.006%
92	15.255	2322	2324	2327	rVB3	787	754	0.08%	0.010%
93	15.365	2340	2342	2344	rBV2	1031	951	0.10%	0.013%
94	15.390	2344	2346	2350	rVB4	1380	1391	0.15%	0.019%
95	15.499	2362	2364	2365	rBV	509	424	0.05%	0.006%
96	15.603	2379	2381	2383	rBV2	679	394	0.04%	0.005%
97	15.701	2395	2397	2398	rBV2	649	381	0.04%	0.005%
98	16.018	2447	2449	2451	rBV2	779	623	0.07%	0.008%
99	16.121	2464	2466	2471	rBV4	698	842	0.09%	0.011%
100	16.243	2485	2486	2488	rBV2	681	412	0.05%	0.006%

Sum of corrected areas: 7439629




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043780.D
Acq On : 11 Nov 2024 10:40
Operator : JC/MD
Sample : P4751-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH9H0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

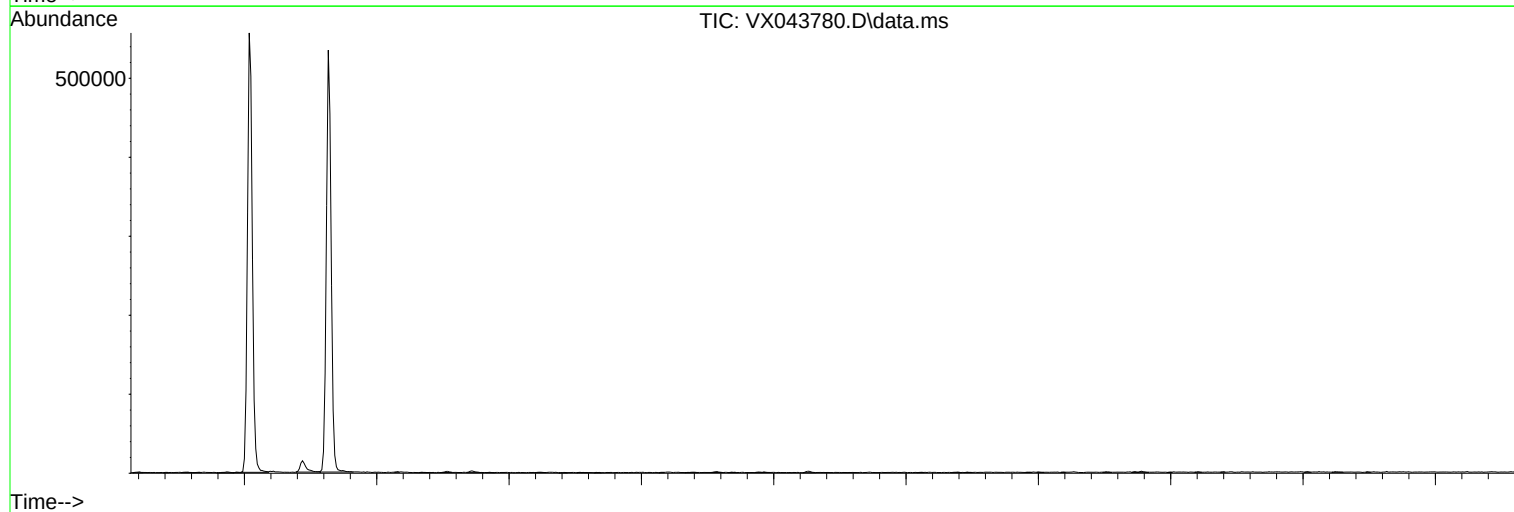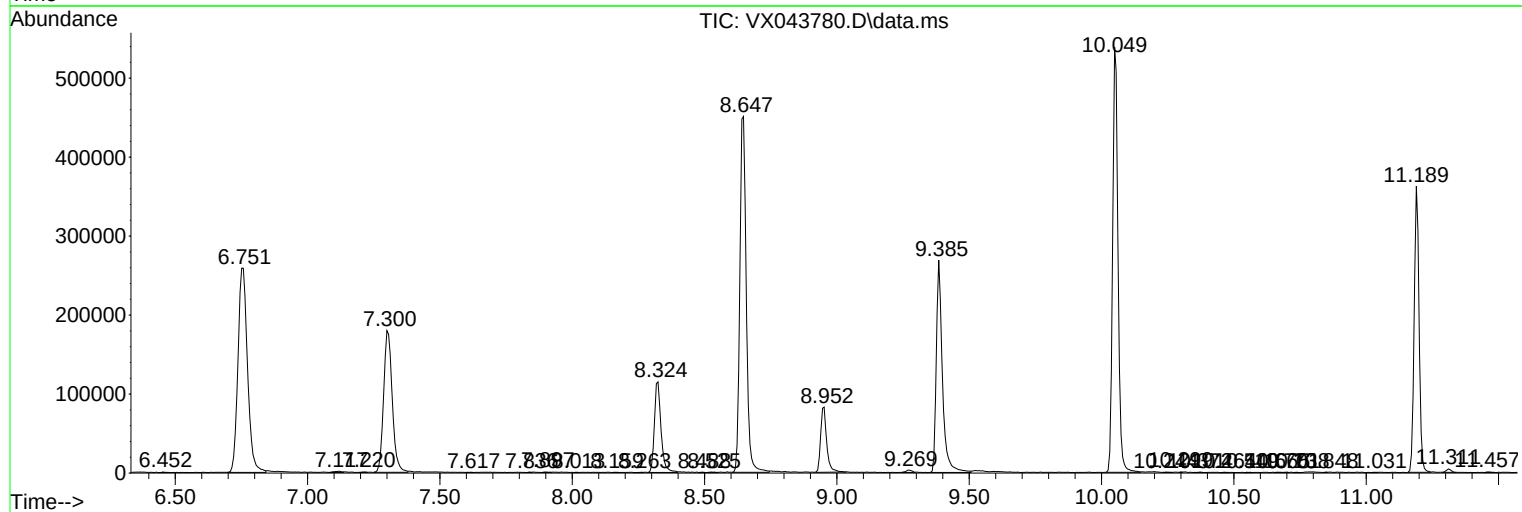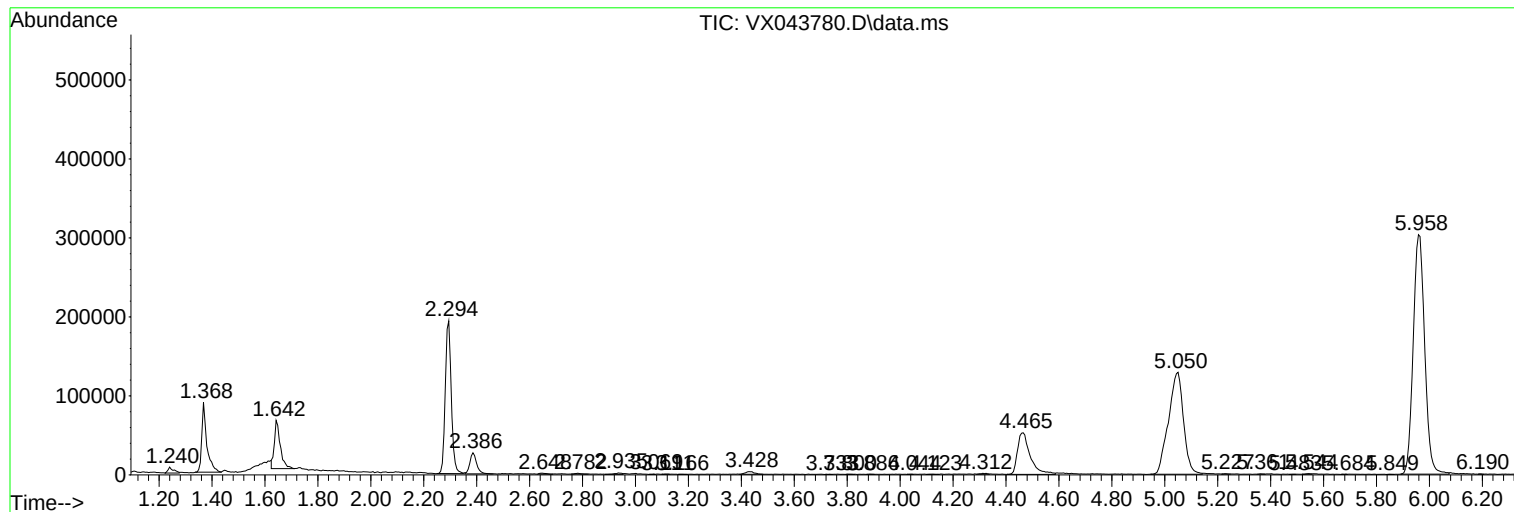

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043780.D
Acq On : 11 Nov 2024 10:40
Operator : JC/MD
Sample : P4751-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH9H0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043780.D
Acq On : 11 Nov 2024 10:40
Operator : JC/MD
Sample : P4751-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH9H0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------