

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043786.D
 Acq On : 11 Nov 2024 12:59
 Operator : JC/MD
 Sample : VIBLK677
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK677

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043786.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	31	rBV2	6359	10210	1.10%	0.149%
2	1.368	43	46	60	rVB	73063	101409	10.97%	1.479%
3	1.648	89	92	105	rVB	51004	92981	10.06%	1.356%
4	2.294	192	198	211	rVB	167565	264683	28.62%	3.861%
5	2.788	273	279	283	rBV4	1223	2311	0.25%	0.034%
6	2.941	297	304	311	rBV	5203	10854	1.17%	0.158%
7	3.069	321	325	326	rBV2	907	930	0.10%	0.014%
8	3.209	344	348	350	rBV3	315	466	0.05%	0.007%
9	3.434	376	385	395	rBV4	3923	9690	1.05%	0.141%
10	3.599	410	412	415	rBV3	335	388	0.04%	0.006%
11	3.739	432	435	437	rBV2	368	438	0.05%	0.006%
12	3.794	440	444	446	rBV	281	315	0.03%	0.005%
13	4.001	474	478	481	rBV2	245	419	0.05%	0.006%
14	4.032	481	483	487	rVB2	407	462	0.05%	0.007%
15	4.093	487	493	494	rBV2	276	471	0.05%	0.007%
16	4.349	533	535	537	rBV2	342	384	0.04%	0.006%
17	4.410	542	545	546	rBV2	421	312	0.03%	0.005%
18	4.471	546	555	576	rBV	55831	191010	20.66%	2.786%
19	4.757	600	602	606	rVB2	656	491	0.05%	0.007%
20	4.849	615	617	620	rVB2	485	382	0.04%	0.006%
21	4.879	620	622	624	rBV3	410	314	0.03%	0.005%
22	4.904	624	626	628	rVB2	753	599	0.06%	0.009%
23	5.056	637	651	670	rBV	115793	368426	39.84%	5.374%
24	5.208	673	676	677	rVB3	391	308	0.03%	0.004%
25	5.385	701	705	711	rBV4	621	1478	0.16%	0.022%
26	5.556	727	733	735	rBV3	634	1194	0.13%	0.017%
27	5.605	740	741	744	rBV2	280	296	0.03%	0.004%
28	5.635	744	746	749	rBV2	268	310	0.03%	0.005%
29	5.788	766	771	772	rBV2	525	715	0.08%	0.010%
30	5.964	787	800	820	rBV2	309893	924670	100.00%	13.487%
31	6.251	845	847	849	rBV2	308	309	0.03%	0.005%
32	6.757	921	930	945	rBV	235801	578969	62.61%	8.445%
33	7.129	984	991	996	rBV8	3147	8433	0.91%	0.123%
34	7.306	1011	1020	1037	rBV	186991	424001	45.85%	6.184%
35	7.446	1041	1043	1045	rBV2	510	313	0.03%	0.005%
36	7.623	1068	1072	1074	rVV2	277	348	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043786.D
 Acq On : 11 Nov 2024 12:59
 Operator : JC/MD
 Sample : VIBLK677
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK677

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.714	1085	1087	1091	rBV2	458	536	0.06%	0.008%
38	7.763	1091	1095	1098	rBV3	255	452	0.05%	0.007%
39	7.824	1103	1105	1108	rVB2	661	735	0.08%	0.011%
40	7.903	1116	1118	1120	rBB2	390	321	0.03%	0.005%
41	7.952	1123	1126	1127	rBV2	365	335	0.04%	0.005%
42	8.049	1141	1142	1145	rVB	430	347	0.04%	0.005%
43	8.165	1158	1161	1164	rBV2	302	438	0.05%	0.006%
44	8.269	1177	1178	1181	rBV	534	351	0.04%	0.005%
45	8.324	1181	1187	1199	rBV	124323	208296	22.53%	3.038%
46	8.580	1227	1229	1232	rBV3	485	627	0.07%	0.009%
47	8.647	1233	1240	1250	rBV	432714	701605	75.88%	10.234%
48	8.952	1284	1290	1305	rVV	86790	136271	14.74%	1.988%
49	9.135	1318	1320	1322	rVB	358	296	0.03%	0.004%
50	9.196	1328	1330	1333	rVB2	555	432	0.05%	0.006%
51	9.275	1338	1343	1347	rVB5	2711	4269	0.46%	0.062%
52	9.330	1348	1352	1353	rBV2	337	309	0.03%	0.005%
53	9.385	1356	1361	1374	rBV	256967	429840	46.49%	6.270%
54	9.647	1402	1404	1407	rVB3	491	555	0.06%	0.008%
55	9.702	1410	1413	1418	rVB2	2562	3167	0.34%	0.046%
56	9.781	1425	1426	1430	rBV4	290	380	0.04%	0.006%
57	9.830	1433	1434	1436	rVB2	481	308	0.03%	0.004%
58	10.055	1465	1471	1487	rBV	454530	664017	71.81%	9.685%
59	10.195	1491	1494	1499	rVB4	1607	2708	0.29%	0.039%
60	10.305	1507	1512	1517	rBV5	1918	3396	0.37%	0.050%
61	10.531	1546	1549	1551	rVB	406	526	0.06%	0.008%
62	10.647	1564	1568	1576	rBV5	2146	4836	0.52%	0.071%
63	10.860	1601	1603	1606	rVB	437	359	0.04%	0.005%
64	10.945	1615	1617	1618	rVV	492	322	0.03%	0.005%
65	10.964	1618	1620	1625	rVB4	1684	2436	0.26%	0.036%
66	11.122	1645	1646	1649	rBV2	364	294	0.03%	0.004%
67	11.189	1652	1657	1665	rBV	386934	488965	52.88%	7.132%
68	11.457	1697	1701	1706	rBV4	2197	3241	0.35%	0.047%
69	11.591	1719	1723	1728	rVB3	306	391	0.04%	0.006%
70	11.652	1732	1733	1737	rVB2	396	532	0.06%	0.008%
71	11.683	1737	1738	1741	rBV2	515	526	0.06%	0.008%
72	11.756	1746	1750	1754	rBV3	2260	3036	0.33%	0.044%
73	11.976	1779	1786	1788	rBV3	3855	5064	0.55%	0.074%
74	12.018	1788	1793	1808	rVB	428043	559647	60.52%	8.163%
75	12.238	1827	1829	1831	rVB2	456	307	0.03%	0.004%
76	12.317	1837	1842	1852	rBV	475100	593804	64.22%	8.661%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043786.D
 Acq On : 11 Nov 2024 12:59
 Operator : JC/MD
 Sample : VIBLK677
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK677

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	12.646	1894	1896	1898	rBV	560	507	0.05%	0.007%
78	12.713	1906	1907	1910	rVB2	503	375	0.04%	0.005%
79	12.841	1925	1928	1929	rBV	439	424	0.05%	0.006%
80	12.951	1943	1946	1948	rBV2	619	472	0.05%	0.007%
81	13.018	1954	1957	1958	rBV	352	421	0.05%	0.006%
82	13.116	1969	1973	1977	rBV5	2560	4066	0.44%	0.059%
83	13.280	1997	2000	2002	rVB	547	491	0.05%	0.007%
84	13.329	2005	2008	2011	rBV3	562	930	0.10%	0.014%
85	13.463	2028	2030	2031	rBV2	379	296	0.03%	0.004%
86	13.536	2039	2042	2043	rVB2	476	341	0.04%	0.005%
87	13.597	2047	2052	2056	rVB3	3048	4609	0.50%	0.067%
88	13.780	2078	2082	2090	rBV	5990	8503	0.92%	0.124%
89	13.908	2102	2103	2106	rVB	439	360	0.04%	0.005%
90	13.963	2107	2112	2116	rBV3	3692	5242	0.57%	0.076%
91	14.097	2130	2134	2135	rBV2	296	371	0.04%	0.005%
92	14.317	2168	2170	2173	rBV	446	412	0.04%	0.006%
93	14.530	2201	2205	2208	rBV5	351	523	0.06%	0.008%
94	14.579	2211	2213	2216	rBV3	538	656	0.07%	0.010%
95	15.012	2282	2284	2288	rVB3	579	486	0.05%	0.007%
96	15.073	2292	2294	2297	rVB	599	390	0.04%	0.006%
97	15.383	2343	2345	2348	rBV2	791	1058	0.11%	0.015%
98	15.731	2400	2402	2404	rBV2	514	361	0.04%	0.005%
99	15.786	2407	2411	2412	rBV3	576	580	0.06%	0.008%
100	16.347	2501	2503	2505	rBV2	757	474	0.05%	0.007%

Sum of corrected areas: 6855914




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043786.D
Acq On : 11 Nov 2024 12:59
Operator : JC/MD
Sample : VIBLK677
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK677

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

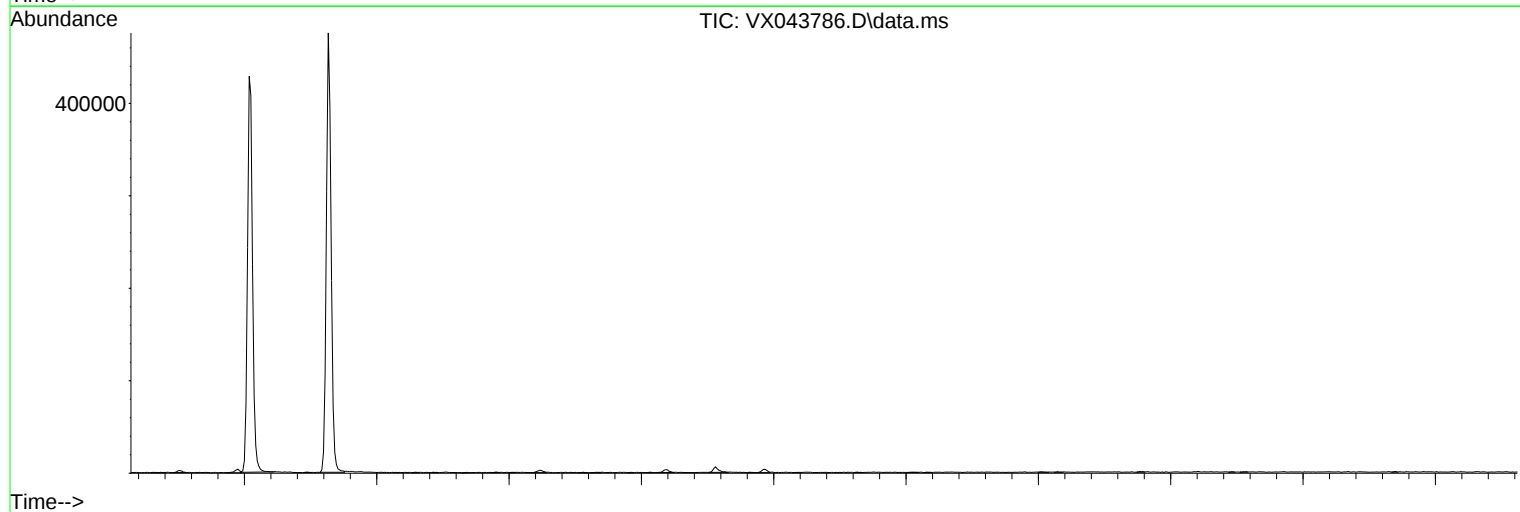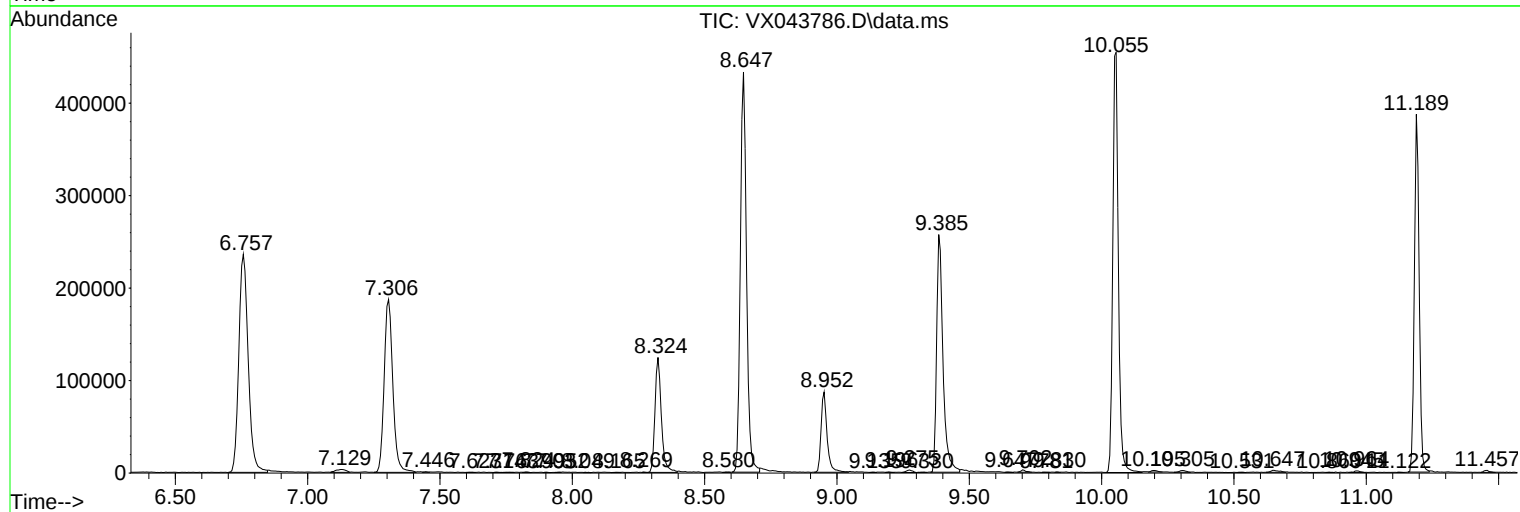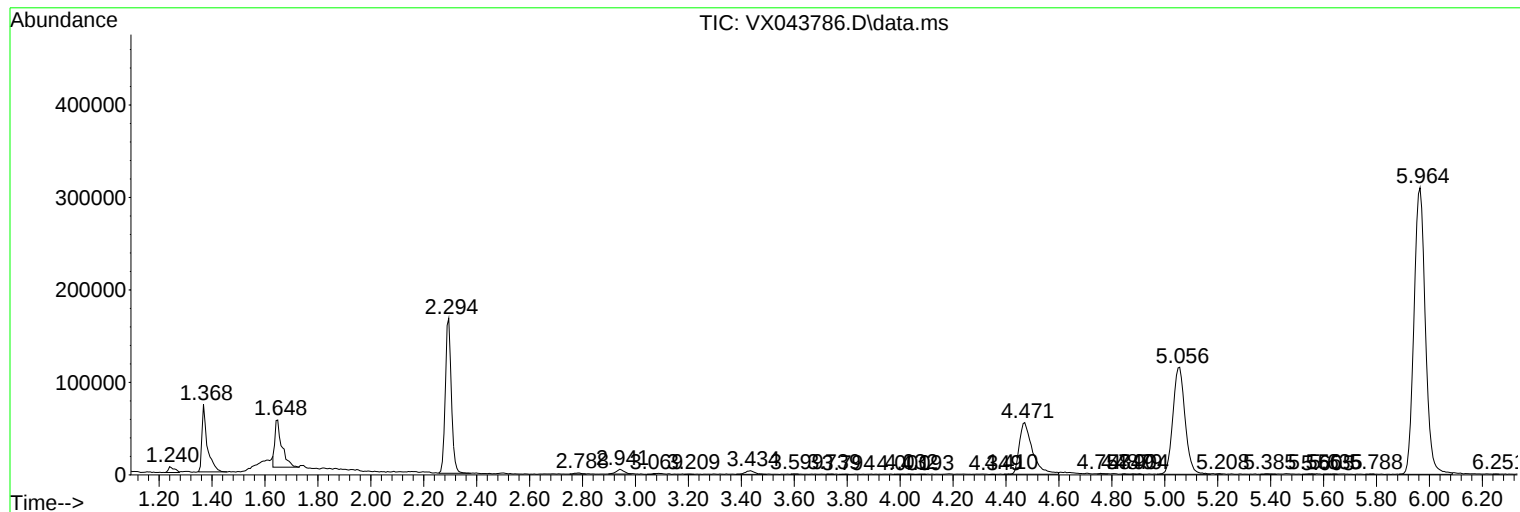

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043786.D
Acq On : 11 Nov 2024 12:59
Operator : JC/MD
Sample : VIBLK677
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK677

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043786.D
Acq On : 11 Nov 2024 12:59
Operator : JC/MD
Sample : VIBLK677
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK677

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
