

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043788.D
 Acq On : 11 Nov 2024 13:45
 Operator : JC/MD
 Sample : P4786-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27M3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043788.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	33	rVB3	7674	12307	1.29%	0.165%
2	1.367	41	46	56	rBV	99005	121917	12.81%	1.632%
3	1.447	56	59	64	rVV	8231	9528	1.00%	0.128%
4	1.526	70	72	73	rBV2	2263	1516	0.16%	0.020%
5	1.648	88	92	102	rVB	68910	97979	10.29%	1.311%
6	2.294	192	198	207	rBV	197890	310753	32.65%	4.160%
7	2.386	208	213	220	rVB	19187	31386	3.30%	0.420%
8	2.538	237	238	239	rBV	692	370	0.04%	0.005%
9	2.782	275	278	283	rVB4	1190	1969	0.21%	0.026%
10	2.825	283	285	288	rVB3	422	486	0.05%	0.007%
11	2.946	298	305	310	rBV2	5354	13154	1.38%	0.176%
12	3.087	326	328	329	rVV2	609	572	0.06%	0.008%
13	3.111	329	332	341	rVB4	1742	3891	0.41%	0.052%
14	3.276	357	359	363	rBV2	383	487	0.05%	0.007%
15	3.367	371	374	376	rVV2	261	330	0.03%	0.004%
16	3.434	378	385	393	rBV6	4511	11282	1.19%	0.151%
17	3.495	393	395	397	rVB2	595	329	0.03%	0.004%
18	3.550	400	404	406	rVB2	284	344	0.04%	0.005%
19	3.757	436	438	441	rBV	479	482	0.05%	0.006%
20	3.904	458	462	464	rVB	386	466	0.05%	0.006%
21	3.928	464	466	468	rBV	334	386	0.04%	0.005%
22	3.989	472	476	479	rBV2	501	592	0.06%	0.008%
23	4.123	497	498	506	rVB3	380	593	0.06%	0.008%
24	4.208	506	512	513	rBV	973	1526	0.16%	0.020%
25	4.464	546	554	568	rBV	52393	166212	17.46%	2.225%
26	4.739	598	599	604	rVB3	454	515	0.05%	0.007%
27	5.056	639	651	668	rBV	122560	373661	39.26%	5.002%
28	5.385	702	705	706	rBV	494	421	0.04%	0.006%
29	5.434	712	713	716	rBV2	390	375	0.04%	0.005%
30	5.544	725	731	733	rBV2	871	1086	0.11%	0.015%
31	5.964	788	800	819	rBV2	320886	951721	100.00%	12.739%
32	6.452	877	880	882	rBV2	269	364	0.04%	0.005%
33	6.665	913	915	918	rVB3	524	544	0.06%	0.007%
34	6.757	921	930	944	rBV	293555	703845	73.95%	9.421%
35	7.092	983	985	986	rBV2	623	659	0.07%	0.009%
36	7.202	1001	1003	1006	rBV	487	722	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043788.D
 Acq On : 11 Nov 2024 13:45
 Operator : JC/MD
 Sample : P4786-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27M3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.305	1012	1020	1038	rVB	188684	420760	44.21%	5.632%
38	7.488	1047	1050	1053	rVB4	692	919	0.10%	0.012%
39	7.519	1053	1055	1061	rVB3	867	1151	0.12%	0.015%
40	7.561	1061	1062	1067	rBV3	322	548	0.06%	0.007%
41	7.598	1067	1068	1072	rVB2	558	556	0.06%	0.007%
42	7.635	1072	1074	1076	rBV	477	528	0.06%	0.007%
43	7.708	1084	1086	1090	rVB3	378	340	0.04%	0.005%
44	7.860	1104	1111	1112	rBV2	904	1625	0.17%	0.022%
45	7.903	1112	1118	1124	rVB4	5456	11050	1.16%	0.148%
46	8.000	1132	1134	1136	rBV	519	526	0.06%	0.007%
47	8.324	1181	1187	1198	rBV	121250	203459	21.38%	2.723%
48	8.531	1219	1221	1224	rVB2	492	371	0.04%	0.005%
49	8.580	1224	1229	1230	rBV3	618	709	0.07%	0.009%
50	8.647	1233	1240	1251	rBV	483720	772940	81.21%	10.346%
51	8.951	1284	1290	1301	rBV	80188	130085	13.67%	1.741%
52	9.153	1320	1323	1326	rBV3	364	436	0.05%	0.006%
53	9.275	1336	1343	1349	rVB2	7397	12765	1.34%	0.171%
54	9.384	1356	1361	1372	rBV	267636	405770	42.64%	5.431%
55	9.646	1403	1404	1409	rVB2	521	690	0.07%	0.009%
56	9.793	1427	1428	1431	rBV3	384	335	0.04%	0.004%
57	9.872	1437	1441	1443	rBV3	366	520	0.05%	0.007%
58	10.055	1465	1471	1482	rBV	554807	814384	85.57%	10.901%
59	10.305	1508	1512	1514	rBV3	686	982	0.10%	0.013%
60	10.329	1514	1516	1517	rVB	847	499	0.05%	0.007%
61	10.372	1522	1523	1526	rVB	479	404	0.04%	0.005%
62	10.604	1557	1561	1565	rVV3	1205	1434	0.15%	0.019%
63	10.811	1593	1595	1597	rVB	491	360	0.04%	0.005%
64	10.841	1597	1600	1603	rVB2	530	583	0.06%	0.008%
65	11.104	1641	1643	1644	rBV	716	478	0.05%	0.006%
66	11.189	1652	1657	1669	rBV	346143	450902	47.38%	6.035%
67	11.311	1672	1677	1683	rVB2	8178	11139	1.17%	0.149%
68	11.664	1732	1735	1737	rBV	616	454	0.05%	0.006%
69	11.713	1741	1743	1745	rVV	323	346	0.04%	0.005%
70	11.756	1748	1750	1753	rVB2	783	785	0.08%	0.011%
71	11.799	1753	1757	1758	rBV3	381	474	0.05%	0.006%
72	11.975	1782	1786	1788	rBV3	940	961	0.10%	0.013%
73	12.018	1788	1793	1807	rBV	536873	720924	75.75%	9.650%
74	12.225	1823	1827	1832	rBV3	3846	4837	0.51%	0.065%
75	12.317	1837	1842	1854	rBV	491107	638700	67.11%	8.549%
76	12.554	1878	1881	1884	rBV2	327	431	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043788.D
 Acq On : 11 Nov 2024 13:45
 Operator : JC/MD
 Sample : P4786-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27M3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	12.719	1906	1908	1909	rVV	430	354	0.04%	0.005%
78	12.762	1910	1915	1920	rVV	2994	4523	0.48%	0.061%
79	12.890	1934	1936	1939	rVB	542	402	0.04%	0.005%
80	12.945	1939	1945	1947	rBV3	383	550	0.06%	0.007%
81	13.115	1971	1973	1977	rBV2	710	952	0.10%	0.013%
82	13.310	2004	2005	2010	rVV3	368	486	0.05%	0.007%
83	13.353	2010	2012	2014	rVV2	548	501	0.05%	0.007%
84	13.597	2051	2052	2054	rBV2	567	437	0.05%	0.006%
85	13.792	2079	2084	2087	rBV2	855	1858	0.20%	0.025%
86	14.024	2119	2122	2125	rBV2	488	578	0.06%	0.008%
87	14.133	2136	2140	2142	rBV3	929	982	0.10%	0.013%
88	14.426	2185	2188	2191	rBV3	254	414	0.04%	0.006%
89	14.469	2191	2195	2199	rVB2	996	1140	0.12%	0.015%
90	15.066	2291	2293	2295	rBV2	314	373	0.04%	0.005%
91	15.091	2295	2297	2300	rVB2	841	847	0.09%	0.011%
92	15.182	2309	2312	2314	rBV2	682	710	0.07%	0.010%
93	15.298	2330	2331	2333	rBV2	594	353	0.04%	0.005%
94	15.816	2411	2416	2421	rVB5	6716	11140	1.17%	0.149%
95	15.968	2436	2441	2445	rBV7	2937	3925	0.41%	0.053%
96	16.231	2482	2484	2485	rBV2	778	417	0.04%	0.006%
97	16.322	2497	2499	2502	rBV3	507	466	0.05%	0.006%
98	16.346	2502	2503	2505	rVV	908	625	0.07%	0.008%
99	16.383	2507	2509	2512	rVB2	703	585	0.06%	0.008%
100	16.523	2531	2532	2534	rBV	523	346	0.04%	0.005%

Sum of corrected areas: 7470894




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043788.D
Acq On : 11 Nov 2024 13:45
Operator : JC/MD
Sample : P4786-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27M3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

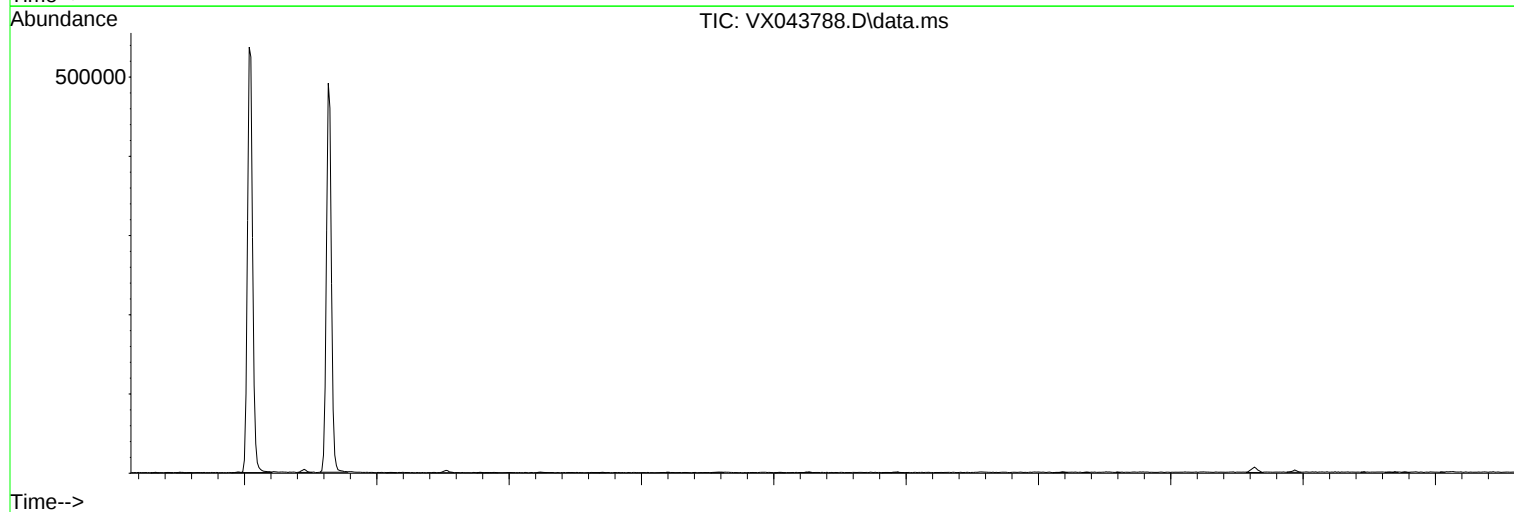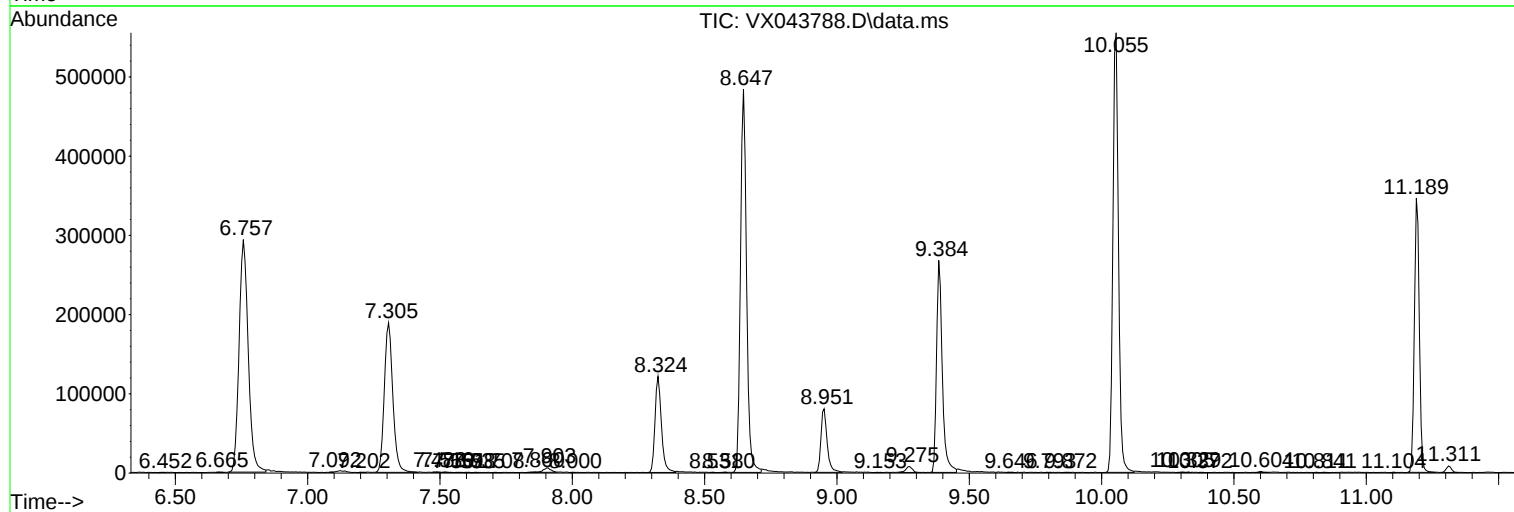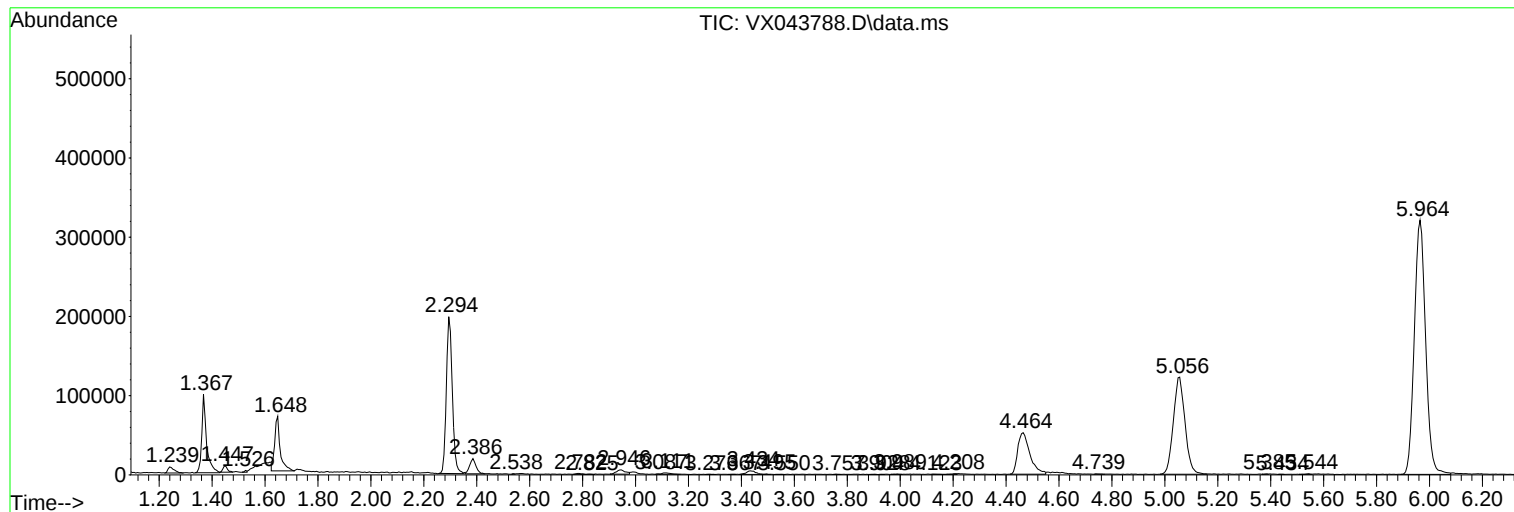

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043788.D
Acq On : 11 Nov 2024 13:45
Operator : JC/MD
Sample : P4786-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27M3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043788.D
Acq On : 11 Nov 2024 13:45
Operator : JC/MD
Sample : P4786-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27M3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
