

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043789.D
 Acq On : 11 Nov 2024 14:08
 Operator : JC/MD
 Sample : P4786-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27M4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043789.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	27	rBV	6880	6934	0.80%	0.102%
2	1.368	43	46	58	rBV	82347	103463	11.97%	1.529%
3	1.648	88	92	102	rVB	58161	88964	10.30%	1.314%
4	2.294	191	198	208	rBV	178078	278000	32.17%	4.107%
5	2.502	228	232	238	rBV	3641	5982	0.69%	0.088%
6	2.599	247	248	251	rVB2	568	385	0.04%	0.006%
7	2.709	261	266	267	rBV2	1016	1293	0.15%	0.019%
8	2.746	270	272	273	rVB	658	373	0.04%	0.006%
9	2.935	297	303	304	rBV4	2187	2894	0.33%	0.043%
10	3.428	378	384	392	rBV4	3799	9257	1.07%	0.137%
11	3.648	418	420	422	rVB2	405	309	0.04%	0.005%
12	3.690	422	427	428	rBV2	290	346	0.04%	0.005%
13	3.819	446	448	450	rBV2	327	404	0.05%	0.006%
14	4.001	477	478	479	rVV	518	286	0.03%	0.004%
15	4.123	497	498	501	rBV2	500	352	0.04%	0.005%
16	4.154	501	503	506	rBV2	309	323	0.04%	0.005%
17	4.288	522	525	527	rBV3	316	428	0.05%	0.006%
18	4.367	536	538	541	rVB2	430	299	0.03%	0.004%
19	4.465	546	554	566	rBV	50504	150390	17.40%	2.222%
20	5.056	638	651	667	rVV	113683	369774	42.79%	5.463%
21	5.318	692	694	695	rBV	443	328	0.04%	0.005%
22	5.385	700	705	707	rBV4	645	1132	0.13%	0.017%
23	5.446	713	715	720	rBV2	475	394	0.05%	0.006%
24	5.532	727	729	731	rBV2	385	406	0.05%	0.006%
25	5.708	756	758	761	rVV2	377	297	0.03%	0.004%
26	5.964	789	800	822	rBV3	293002	864144	100.00%	12.767%
27	6.196	837	838	842	rBV	443	477	0.06%	0.007%
28	6.629	906	909	911	rBV2	438	432	0.05%	0.006%
29	6.757	921	930	950	rBV2	249292	616239	71.31%	9.105%
30	7.098	984	986	987	rBV2	834	567	0.07%	0.008%
31	7.306	1012	1020	1032	rBV	172830	385315	44.59%	5.693%
32	7.556	1059	1061	1063	rVB	371	340	0.04%	0.005%
33	7.629	1072	1073	1075	rVV2	709	294	0.03%	0.004%
34	7.665	1076	1079	1081	rVB2	344	357	0.04%	0.005%
35	7.751	1091	1093	1097	rVB2	253	284	0.03%	0.004%
36	7.860	1107	1111	1113	rBV2	479	552	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043789.D
Acq On : 11 Nov 2024 14:08
Operator : JC/MD
Sample : P4786-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27M4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Title : VOC Analysis

37	7.958	1125	1127	1131	rVB3	519	541	0.06%	0.008%
38	8.068	1143	1145	1149	rVB2	328	459	0.05%	0.007%
39	8.324	1181	1187	1198	rBV	108772	182012	21.06%	2.689%
40	8.574	1226	1228	1229	rBV2	389	407	0.05%	0.006%
41	8.647	1233	1240	1258	rBV	447631	710407	82.21%	10.496%
42	8.872	1273	1277	1278	rBV3	339	408	0.05%	0.006%
43	8.952	1285	1290	1299	rBV	74202	116163	13.44%	1.716%
44	9.104	1313	1315	1318	rVB2	530	400	0.05%	0.006%
45	9.275	1338	1343	1349	rVB2	4056	6483	0.75%	0.096%
46	9.385	1356	1361	1375	rBV	244314	392118	45.38%	5.793%
47	9.586	1392	1394	1405	rVB5	2822	5809	0.67%	0.086%
48	9.714	1413	1415	1418	rBV4	303	394	0.05%	0.006%
49	9.805	1428	1430	1434	rVB	542	687	0.08%	0.010%
50	9.848	1434	1437	1438	rBV2	432	541	0.06%	0.008%
51	10.055	1465	1471	1488	rBV	503181	732935	84.82%	10.829%
52	10.305	1509	1512	1513	rBV3	556	519	0.06%	0.008%
53	10.348	1517	1519	1523	rBV3	452	754	0.09%	0.011%
54	10.476	1537	1540	1543	rBV3	466	547	0.06%	0.008%
55	10.653	1564	1569	1570	rBV2	528	595	0.07%	0.009%
56	10.775	1587	1589	1591	rBV2	393	389	0.05%	0.006%
57	10.829	1595	1598	1599	rVB2	369	372	0.04%	0.005%
58	10.848	1599	1601	1602	rBV2	420	289	0.03%	0.004%
59	10.866	1602	1604	1606	rBV	589	396	0.05%	0.006%
60	10.964	1618	1620	1624	rVB2	389	376	0.04%	0.006%
61	11.006	1624	1627	1628	rVB2	453	329	0.04%	0.005%
62	11.189	1652	1657	1671	rVB	326245	427540	49.48%	6.317%
63	11.311	1673	1677	1680	rVV4	3554	4750	0.55%	0.070%
64	11.451	1696	1700	1701	rVV3	383	485	0.06%	0.007%
65	11.494	1704	1707	1709	rVB2	333	326	0.04%	0.005%
66	11.573	1716	1720	1726	rVB3	1751	2554	0.30%	0.038%
67	11.762	1747	1751	1753	rBV3	437	646	0.07%	0.010%
68	11.829	1760	1762	1767	rVV4	1330	1578	0.18%	0.023%
69	11.866	1767	1768	1771	rVB	486	331	0.04%	0.005%
70	11.933	1778	1779	1781	rVB3	604	295	0.03%	0.004%
71	11.976	1784	1786	1788	rBV2	788	791	0.09%	0.012%
72	12.018	1788	1793	1807	rVV	492801	644487	74.58%	9.522%
73	12.219	1822	1826	1835	rBV	9423	15114	1.75%	0.223%
74	12.317	1837	1842	1857	rVB	477563	598886	69.30%	8.848%
75	12.457	1864	1865	1868	rBV2	702	633	0.07%	0.009%
76	12.585	1881	1886	1888	rBV3	771	1464	0.17%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043789.D
 Acq On : 11 Nov 2024 14:08
 Operator : JC/MD
 Sample : P4786-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27M4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	12.762	1911	1915	1920	rVB4	1469	2453	0.28%	0.036%
78	12.860	1926	1931	1935	rBV3	2935	4832	0.56%	0.071%
79	13.122	1972	1974	1980	rVV3	634	761	0.09%	0.011%
80	13.189	1983	1985	1986	rBV	529	347	0.04%	0.005%
81	13.439	2023	2026	2028	rBV2	483	448	0.05%	0.007%
82	13.591	2048	2051	2055	rBV4	1218	1628	0.19%	0.024%
83	13.835	2089	2091	2094	rVB4	417	370	0.04%	0.005%
84	13.969	2111	2113	2118	rVB2	588	559	0.06%	0.008%
85	14.006	2118	2119	2122	rBV2	440	490	0.06%	0.007%
86	14.128	2135	2139	2144	rVV6	991	1497	0.17%	0.022%
87	14.207	2149	2152	2155	rBV3	583	744	0.09%	0.011%
88	14.237	2155	2157	2160	rVB3	322	313	0.04%	0.005%
89	14.347	2173	2175	2180	rBV3	418	544	0.06%	0.008%
90	14.426	2186	2188	2189	rBV2	453	280	0.03%	0.004%
91	14.853	2255	2258	2261	rBV4	443	691	0.08%	0.010%
92	15.438	2352	2354	2356	rBV3	508	578	0.07%	0.009%
93	15.566	2373	2375	2380	rVB3	1308	1437	0.17%	0.021%
94	15.603	2380	2381	2382	rBV	663	397	0.05%	0.006%
95	15.707	2396	2398	2401	rBV2	708	720	0.08%	0.011%
96	16.097	2460	2462	2463	rBV	520	325	0.04%	0.005%
97	16.225	2481	2483	2486	rBV3	646	725	0.08%	0.011%
98	16.353	2503	2504	2508	rVB2	934	575	0.07%	0.008%
99	16.481	2522	2525	2527	rBV4	798	951	0.11%	0.014%
100	16.652	2551	2553	2555	rBV2	669	585	0.07%	0.009%

Sum of corrected areas: 6768474




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043789.D
Acq On : 11 Nov 2024 14:08
Operator : JC/MD
Sample : P4786-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27M4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

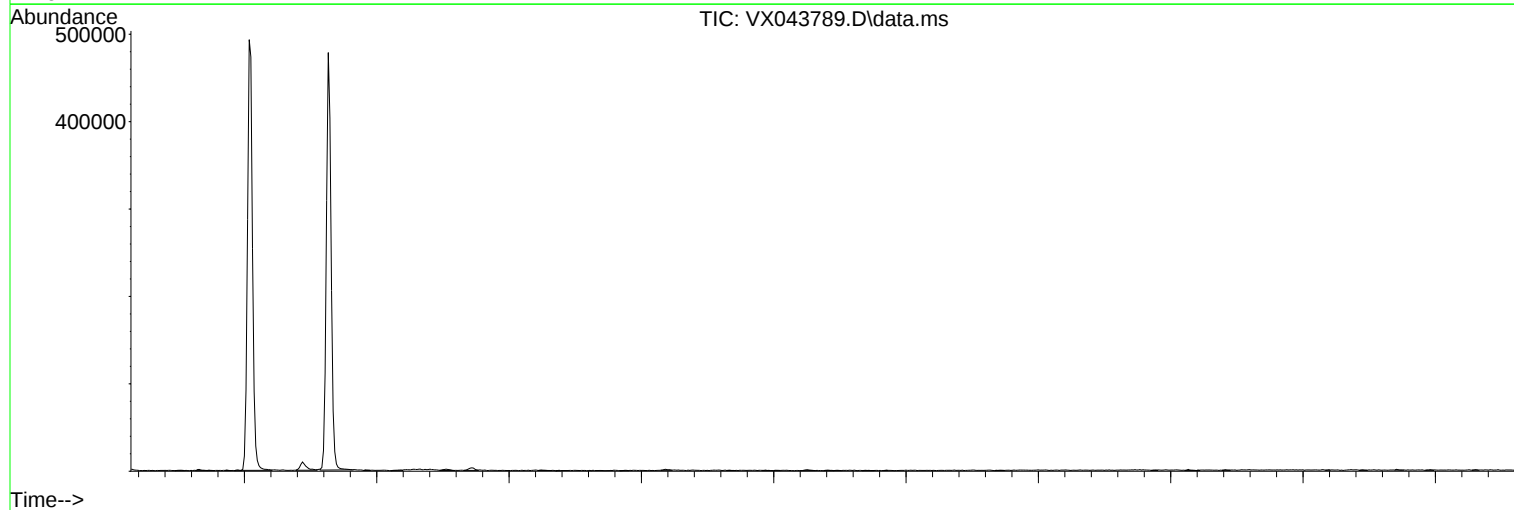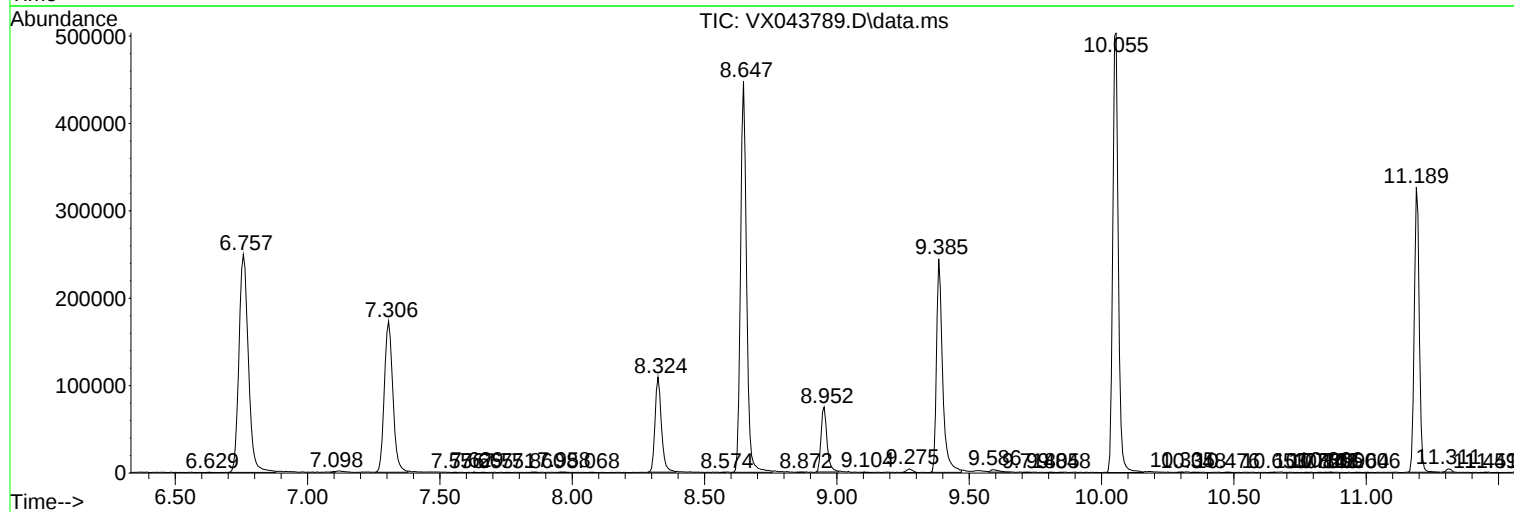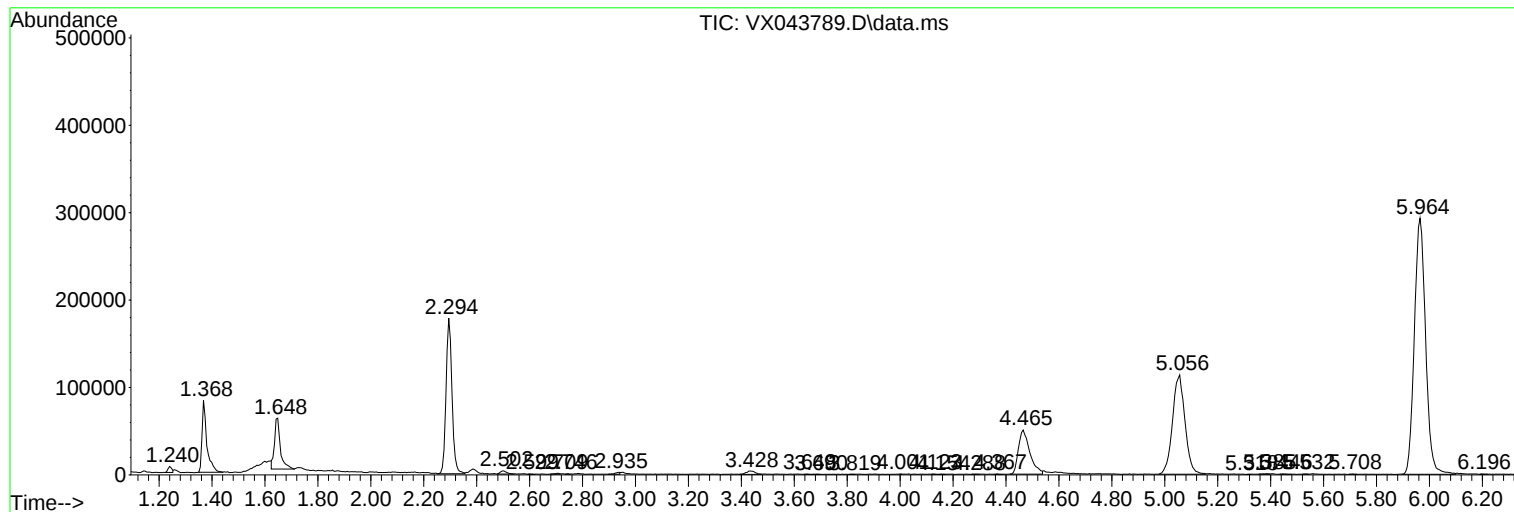

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043789.D
Acq On : 11 Nov 2024 14:08
Operator : JC/MD
Sample : P4786-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27M4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043789.D
Acq On : 11 Nov 2024 14:08
Operator : JC/MD
Sample : P4786-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27M4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
