

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043791.D
 Acq On : 11 Nov 2024 14:54
 Operator : JC/MD
 Sample : P4786-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27M6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043791.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	23	25	32	rVB2	4990	7350	1.32%	0.170%
2	1.368	43	46	53	rVB	55765	60702	10.87%	1.405%
3	1.648	89	92	103	rVB	53960	70742	12.67%	1.637%
4	2.300	192	199	209	rBV	106307	166204	29.76%	3.846%
5	2.569	238	243	249	rVB4	999	2049	0.37%	0.047%
6	2.611	249	250	253	rBV2	316	328	0.06%	0.008%
7	2.648	254	256	258	rVV	464	315	0.06%	0.007%
8	2.672	258	260	262	rVV3	333	353	0.06%	0.008%
9	2.709	265	266	269	rVV2	578	454	0.08%	0.011%
10	2.788	275	279	283	rVB2	797	1213	0.22%	0.028%
11	2.904	295	298	299	rBV2	298	349	0.06%	0.008%
12	2.940	299	304	311	rVB2	2829	6042	1.08%	0.140%
13	3.087	325	328	330	rBV2	430	438	0.08%	0.010%
14	3.178	341	343	346	rVB	577	512	0.09%	0.012%
15	3.361	370	373	376	rBV2	558	693	0.12%	0.016%
16	3.440	379	386	394	rVV4	2354	5437	0.97%	0.126%
17	3.837	447	451	452	rBV2	280	417	0.07%	0.010%
18	3.977	473	474	478	rVV2	373	340	0.06%	0.008%
19	4.044	483	485	487	rBV	357	376	0.07%	0.009%
20	4.154	501	503	506	rVB	578	503	0.09%	0.012%
21	4.312	527	529	530	rBV	458	306	0.05%	0.007%
22	4.465	546	554	569	rBV2	31438	97676	17.49%	2.260%
23	4.800	607	609	613	rBV4	405	569	0.10%	0.013%
24	4.873	618	621	624	rBV3	372	480	0.09%	0.011%
25	5.050	639	650	671	rVB	73834	229206	41.04%	5.304%
26	5.391	704	706	708	rBV3	369	385	0.07%	0.009%
27	5.550	730	732	738	rVB3	338	564	0.10%	0.013%
28	5.702	756	757	762	rVB2	440	539	0.10%	0.012%
29	5.964	790	800	818	rBV3	187570	558472	100.00%	12.922%
30	6.251	845	847	850	rVB2	628	606	0.11%	0.014%
31	6.287	850	853	854	rBV2	364	400	0.07%	0.009%
32	6.354	863	864	869	rVB2	577	407	0.07%	0.009%
33	6.525	890	892	895	rBV2	324	349	0.06%	0.008%
34	6.757	920	930	948	rBV	159186	402727	72.11%	9.319%
35	7.104	982	987	988	rBV2	328	506	0.09%	0.012%
36	7.123	988	990	994	rVB3	958	1201	0.22%	0.028%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043791.D
 Acq On : 11 Nov 2024 14:54
 Operator : JC/MD
 Sample : P4786-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27M6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.153	994	995	998	rBV3	698	658	0.12%	0.015%
38	7.305	1012	1020	1036	rBV	114448	254447	45.56%	5.888%
39	7.476	1045	1048	1049	rBV2	348	339	0.06%	0.008%
40	7.549	1059	1060	1063	rBV	444	456	0.08%	0.011%
41	7.580	1063	1065	1067	rVV2	440	410	0.07%	0.009%
42	7.787	1096	1099	1103	rBV3	318	578	0.10%	0.013%
43	7.860	1109	1111	1114	rVB2	390	351	0.06%	0.008%
44	7.903	1114	1118	1120	rBV2	344	470	0.08%	0.011%
45	8.000	1132	1134	1136	rVB2	356	315	0.06%	0.007%
46	8.055	1141	1143	1145	rVV2	326	362	0.06%	0.008%
47	8.074	1145	1146	1149	rVV2	540	364	0.07%	0.008%
48	8.324	1181	1187	1204	rBV	68558	119285	21.36%	2.760%
49	8.531	1219	1221	1225	rBV4	497	620	0.11%	0.014%
50	8.574	1225	1228	1231	rVB3	291	344	0.06%	0.008%
51	8.647	1234	1240	1256	rBV	282173	451556	80.86%	10.449%
52	8.799	1264	1265	1270	rVB3	581	533	0.10%	0.012%
53	8.952	1285	1290	1302	rBV	47769	73179	13.10%	1.693%
54	9.128	1316	1319	1321	rVB2	323	396	0.07%	0.009%
55	9.214	1330	1333	1334	rVB2	337	320	0.06%	0.007%
56	9.275	1337	1343	1347	rBV3	1996	2695	0.48%	0.062%
57	9.384	1356	1361	1383	rBV	152183	239640	42.91%	5.545%
58	9.592	1393	1395	1397	rVB3	615	533	0.10%	0.012%
59	9.616	1397	1399	1400	rBV	441	455	0.08%	0.011%
60	9.756	1421	1422	1425	rBV2	429	402	0.07%	0.009%
61	9.805	1428	1430	1432	rVB	464	403	0.07%	0.009%
62	9.842	1434	1436	1439	rBV3	281	323	0.06%	0.007%
63	9.994	1459	1461	1465	rBV2	279	390	0.07%	0.009%
64	10.055	1465	1471	1483	rBV	337339	483189	86.52%	11.180%
65	10.177	1490	1491	1493	rBV2	557	326	0.06%	0.008%
66	10.220	1496	1498	1500	rVB2	608	464	0.08%	0.011%
67	10.256	1502	1504	1509	rBV3	408	523	0.09%	0.012%
68	10.439	1531	1534	1537	rVB2	329	458	0.08%	0.011%
69	10.890	1606	1608	1612	rVB2	433	398	0.07%	0.009%
70	11.012	1627	1628	1630	rBV	454	307	0.05%	0.007%
71	11.189	1652	1657	1673	rBV	202722	266171	47.66%	6.159%
72	11.311	1673	1677	1682	rVB3	1959	2556	0.46%	0.059%
73	11.415	1691	1694	1697	rBV2	372	425	0.08%	0.010%
74	11.719	1740	1744	1746	rVV2	231	309	0.06%	0.007%
75	11.890	1771	1772	1774	rVB2	512	365	0.07%	0.008%
76	11.921	1774	1777	1780	rBV2	305	407	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043791.D
 Acq On : 11 Nov 2024 14:54
 Operator : JC/MD
 Sample : P4786-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27M6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	11.975	1784	1786	1788	rBV2	466	475	0.09%	0.011%
78	12.018	1788	1793	1808	rVV	312867	409686	73.36%	9.480%
79	12.158	1814	1816	1818	rVB2	530	324	0.06%	0.007%
80	12.268	1832	1834	1837	rBV2	379	443	0.08%	0.010%
81	12.317	1837	1842	1854	rBV	287066	373982	66.97%	8.654%
82	12.542	1878	1879	1883	rBV2	282	342	0.06%	0.008%
83	12.664	1897	1899	1902	rBV2	332	414	0.07%	0.010%
84	12.878	1930	1934	1938	rVV3	707	1311	0.23%	0.030%
85	13.274	1998	1999	2001	rBV	375	322	0.06%	0.007%
86	13.841	2091	2092	2094	rBV2	350	316	0.06%	0.007%
87	13.938	2107	2108	2116	rVB3	477	500	0.09%	0.012%
88	14.127	2134	2139	2142	rBV3	833	1331	0.24%	0.031%
89	14.219	2152	2154	2156	rBV2	417	399	0.07%	0.009%
90	14.268	2161	2162	2166	rBV3	526	606	0.11%	0.014%
91	14.524	2202	2204	2206	rVB	422	306	0.05%	0.007%
92	14.792	2245	2248	2249	rBV2	236	305	0.05%	0.007%
93	15.164	2307	2309	2312	rBV2	541	512	0.09%	0.012%
94	15.487	2358	2362	2365	rBV3	696	1126	0.20%	0.026%
95	15.859	2422	2423	2426	rVB3	831	635	0.11%	0.015%
96	16.255	2486	2488	2489	rBV2	568	445	0.08%	0.010%
97	16.328	2497	2500	2503	rBV3	732	1154	0.21%	0.027%
98	16.450	2518	2520	2523	rVB3	674	467	0.08%	0.011%
99	16.517	2529	2531	2537	rBV5	585	880	0.16%	0.020%
100	16.779	2572	2574	2575	rBV2	706	511	0.09%	0.012%

Sum of corrected areas: 4321724




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043791.D
Acq On : 11 Nov 2024 14:54
Operator : JC/MD
Sample : P4786-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

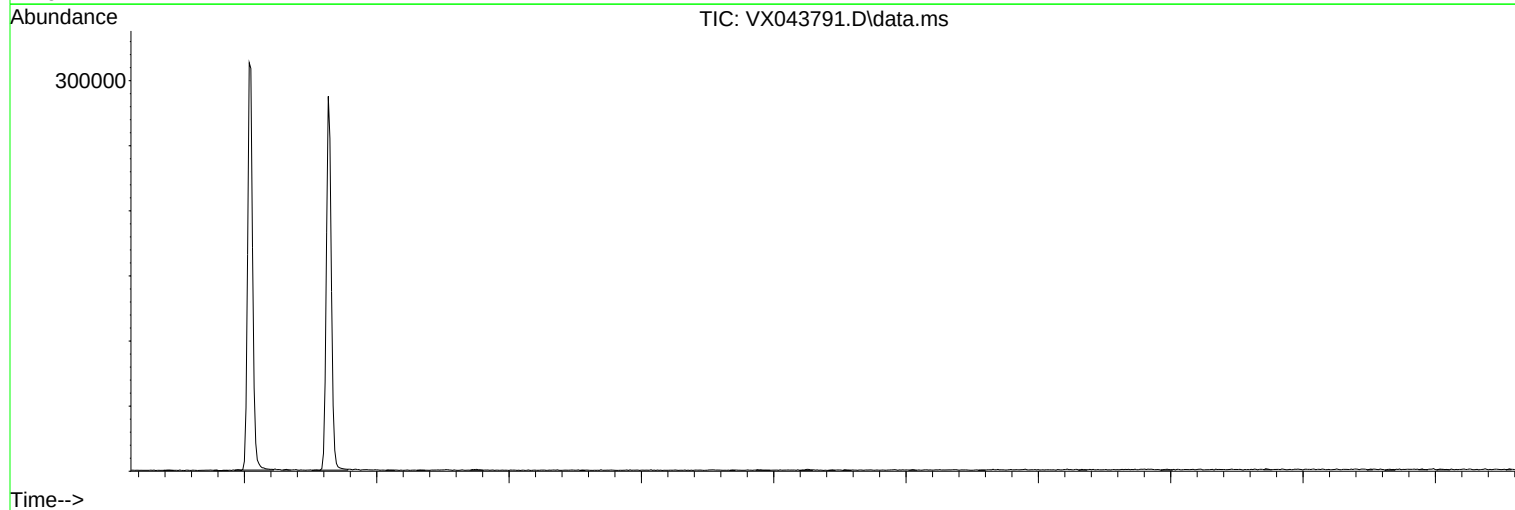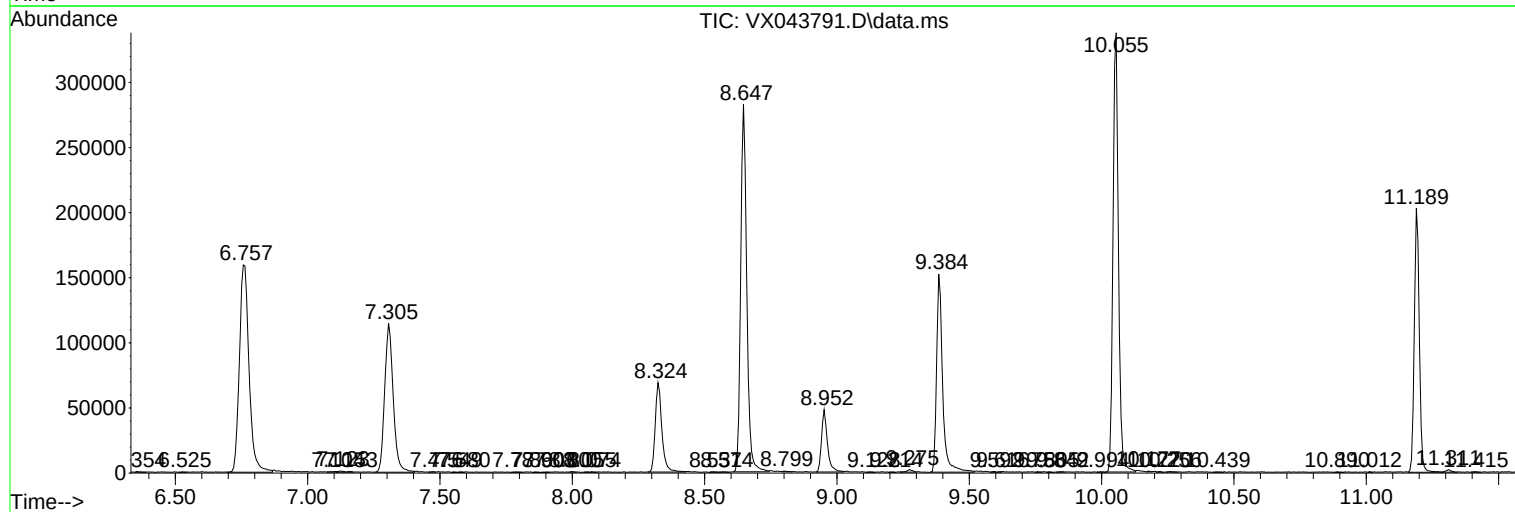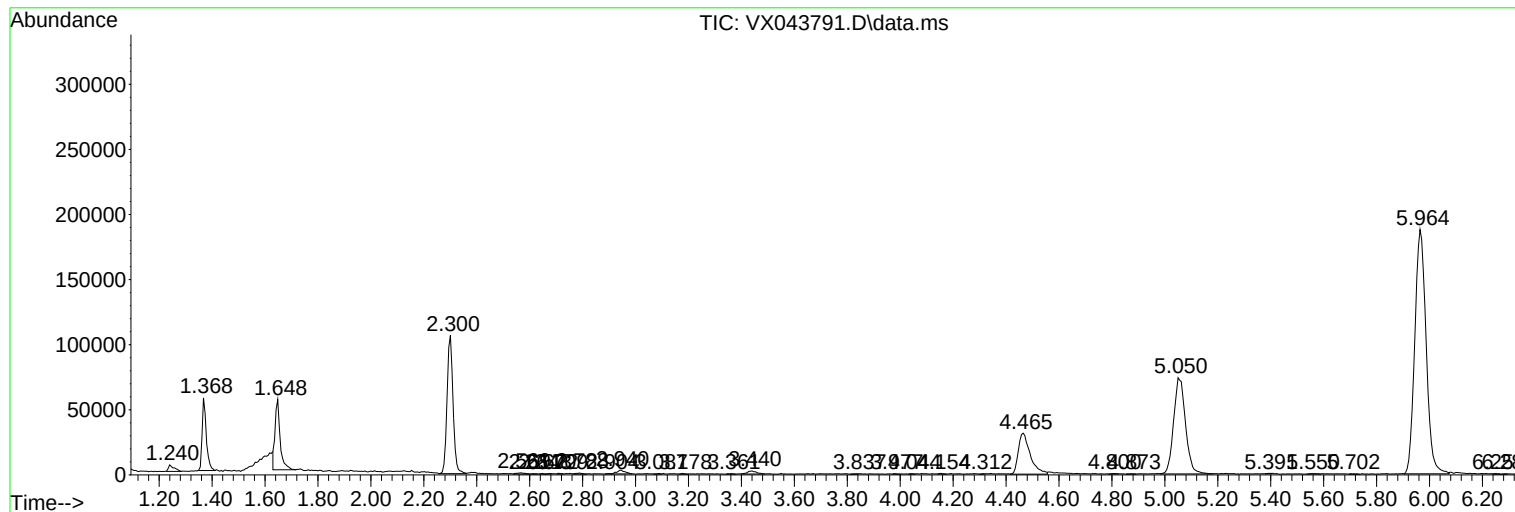

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043791.D
Acq On : 11 Nov 2024 14:54
Operator : JC/MD
Sample : P4786-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043791.D
Acq On : 11 Nov 2024 14:54
Operator : JC/MD
Sample : P4786-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
