

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043800.D
 Acq On : 11 Nov 2024 18:22
 Operator : JC/MD
 Sample : P4786-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27N5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043800.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	13	rBV	3247	3104	0.06%	0.026%
2	1.240	22	25	31	rBV	20481	26961	0.50%	0.227%
3	1.368	43	46	56	rBV	77761	94738	1.74%	0.798%
4	1.642	89	91	101	rVB	67766	91434	1.68%	0.770%
5	2.294	192	198	210	rBV	161704	259913	4.78%	2.189%
6	2.941	297	304	312	rVB2	3620	8992	0.17%	0.076%
7	3.087	324	328	332	rVB5	1067	1842	0.03%	0.016%
8	3.123	332	334	339	rVB4	405	528	0.01%	0.004%
9	3.312	363	365	367	rBV2	509	343	0.01%	0.003%
10	3.440	379	386	393	rBV5	3226	7999	0.15%	0.067%
11	3.898	459	461	464	rBV3	344	383	0.01%	0.003%
12	4.129	495	499	500	rVB3	548	502	0.01%	0.004%
13	4.288	521	525	528	rBV3	519	908	0.02%	0.008%
14	4.471	546	555	569	rBV2	63007	215481	3.96%	1.815%
15	4.843	613	616	618	rBV2	324	508	0.01%	0.004%
16	4.891	621	624	628	rBV2	724	910	0.02%	0.008%
17	4.965	630	636	638	rBV3	545	946	0.02%	0.008%
18	5.050	639	650	666	rBV	103561	325136	5.98%	2.738%
19	5.373	696	703	704	rBV3	1272	2189	0.04%	0.018%
20	5.666	749	751	754	rBV3	406	406	0.01%	0.003%
21	5.879	785	786	789	rBV3	319	346	0.01%	0.003%
22	5.964	789	800	815	rBV2	270113	802020	14.75%	6.754%
23	6.233	842	844	847	rVB2	458	368	0.01%	0.003%
24	6.385	866	869	871	rBV3	349	342	0.01%	0.003%
25	6.440	875	878	881	rBV3	375	529	0.01%	0.004%
26	6.757	921	930	945	rBV2	246044	612513	11.27%	5.158%
27	7.025	972	974	976	rBV2	400	347	0.01%	0.003%
28	7.123	980	990	1011	rBV	2484100	5435997	100.00%	45.779%
29	7.306	1012	1020	1036	rVB	162906	364374	6.70%	3.069%
30	7.793	1095	1100	1101	rBV3	329	454	0.01%	0.004%
31	7.940	1122	1124	1125	rBV2	545	420	0.01%	0.004%
32	7.976	1128	1130	1133	rVV3	641	685	0.01%	0.006%
33	8.007	1133	1135	1137	rVV3	653	538	0.01%	0.005%
34	8.055	1140	1143	1145	rVB3	406	461	0.01%	0.004%
35	8.196	1164	1166	1169	rBV4	425	550	0.01%	0.005%
36	8.257	1174	1176	1178	rBV3	313	340	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043800.D
 Acq On : 11 Nov 2024 18:22
 Operator : JC/MD
 Sample : P4786-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27N5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	8.324	1181	1187	1198	rBV	104420	172637	3.18%	1.454%
38	8.574	1226	1228	1231	rBV3	537	519	0.01%	0.004%
39	8.647	1234	1240	1250	rBV	413037	652321	12.00%	5.494%
40	8.952	1284	1290	1299	rBV	69903	113578	2.09%	0.956%
41	9.098	1311	1314	1317	rBV5	509	735	0.01%	0.006%
42	9.226	1333	1335	1338	rVB2	411	377	0.01%	0.003%
43	9.275	1338	1343	1351	rBV	10979	18312	0.34%	0.154%
44	9.385	1356	1361	1379	rBV	226655	357152	6.57%	3.008%
45	9.586	1392	1394	1395	rBV2	523	386	0.01%	0.003%
46	9.604	1395	1397	1402	rBV4	567	799	0.01%	0.007%
47	9.695	1409	1412	1415	rBV3	339	443	0.01%	0.004%
48	10.055	1465	1471	1486	rVV	490875	699503	12.87%	5.891%
49	10.238	1498	1501	1503	rBV4	368	510	0.01%	0.004%
50	10.311	1510	1513	1514	rBV3	603	662	0.01%	0.006%
51	10.384	1522	1525	1527	rBV3	365	386	0.01%	0.003%
52	10.567	1553	1555	1559	rBV3	400	607	0.01%	0.005%
53	10.634	1565	1566	1571	rVB3	423	417	0.01%	0.004%
54	10.933	1612	1615	1616	rBV2	398	352	0.01%	0.003%
55	11.067	1634	1637	1639	rVB	500	401	0.01%	0.003%
56	11.189	1652	1657	1671	rVV	300339	394167	7.25%	3.319%
57	11.311	1673	1677	1685	rVB2	3534	5596	0.10%	0.047%
58	11.567	1715	1719	1722	rVB4	297	395	0.01%	0.003%
59	11.957	1780	1783	1788	rBV2	331	552	0.01%	0.005%
60	12.018	1788	1793	1802	rBV	471541	613178	11.28%	5.164%
61	12.317	1837	1842	1855	rBV	430251	554128	10.19%	4.667%
62	12.494	1870	1871	1874	rVB2	434	363	0.01%	0.003%
63	12.524	1874	1876	1879	rVB3	583	563	0.01%	0.005%
64	12.683	1899	1902	1905	rBV2	394	504	0.01%	0.004%
65	12.707	1905	1906	1908	rVV	597	423	0.01%	0.004%
66	12.725	1908	1909	1911	rVV2	523	397	0.01%	0.003%
67	12.756	1911	1914	1921	rVV4	1368	2281	0.04%	0.019%
68	12.896	1933	1937	1938	rVV3	448	485	0.01%	0.004%
69	12.969	1942	1949	1952	rBV3	500	856	0.02%	0.007%
70	13.097	1966	1970	1973	rBV3	488	705	0.01%	0.006%
71	13.207	1985	1988	1989	rBV2	394	470	0.01%	0.004%
72	13.225	1989	1991	1996	rVB3	440	528	0.01%	0.004%
73	13.390	2016	2018	2023	rVV2	386	426	0.01%	0.004%
74	13.426	2023	2024	2028	rVV	437	507	0.01%	0.004%
75	13.469	2030	2031	2033	rVV2	520	323	0.01%	0.003%
76	13.518	2036	2039	2042	rVB3	494	637	0.01%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
 Data File : VX043800.D
 Acq On : 11 Nov 2024 18:22
 Operator : JC/MD
 Sample : P4786-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27N5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	13.542	2042	2043	2047	rBV3	382	467	0.01%	0.004%
78	13.652	2059	2061	2065	rVB3	351	389	0.01%	0.003%
79	13.792	2082	2084	2086	rVV2	388	360	0.01%	0.003%
80	13.817	2086	2088	2091	rVB2	470	361	0.01%	0.003%
81	13.853	2091	2094	2096	rBV4	321	349	0.01%	0.003%
82	13.926	2103	2106	2109	rBV4	383	569	0.01%	0.005%
83	14.054	2123	2127	2128	rBV3	404	560	0.01%	0.005%
84	14.378	2177	2180	2181	rVB	434	333	0.01%	0.003%
85	14.506	2199	2201	2204	rBV2	335	364	0.01%	0.003%
86	14.579	2208	2213	2214	rBV4	390	539	0.01%	0.005%
87	14.725	2236	2237	2238	rBV	819	421	0.01%	0.004%
88	14.816	2250	2252	2255	rBV3	435	448	0.01%	0.004%
89	14.865	2258	2260	2262	rVB	450	330	0.01%	0.003%
90	14.896	2263	2265	2269	rBV3	445	439	0.01%	0.004%
91	15.164	2308	2309	2314	rBV4	646	818	0.02%	0.007%
92	15.438	2352	2354	2357	rVB2	603	426	0.01%	0.004%
93	15.566	2373	2375	2377	rBV3	734	796	0.01%	0.007%
94	15.609	2379	2382	2385	rBV3	643	1030	0.02%	0.009%
95	15.963	2437	2440	2442	rBV2	714	792	0.01%	0.007%
96	16.036	2450	2452	2455	rVB4	771	832	0.02%	0.007%
97	16.341	2498	2502	2503	rBV3	692	1068	0.02%	0.009%
98	16.462	2521	2522	2525	rBV2	441	448	0.01%	0.004%
99	16.621	2546	2548	2550	rBV2	965	784	0.01%	0.007%
100	16.773	2571	2573	2574	rVB2	739	389	0.01%	0.003%

Sum of corrected areas: 11874400




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043800.D
Acq On : 11 Nov 2024 18:22
Operator : JC/MD
Sample : P4786-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27N5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

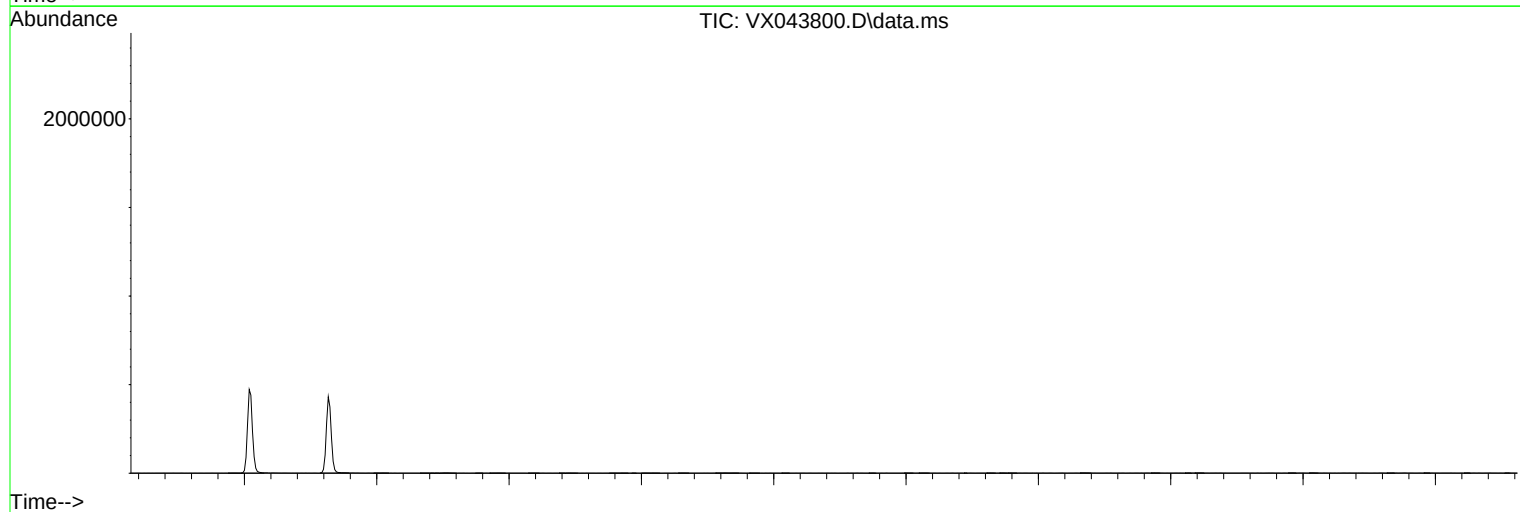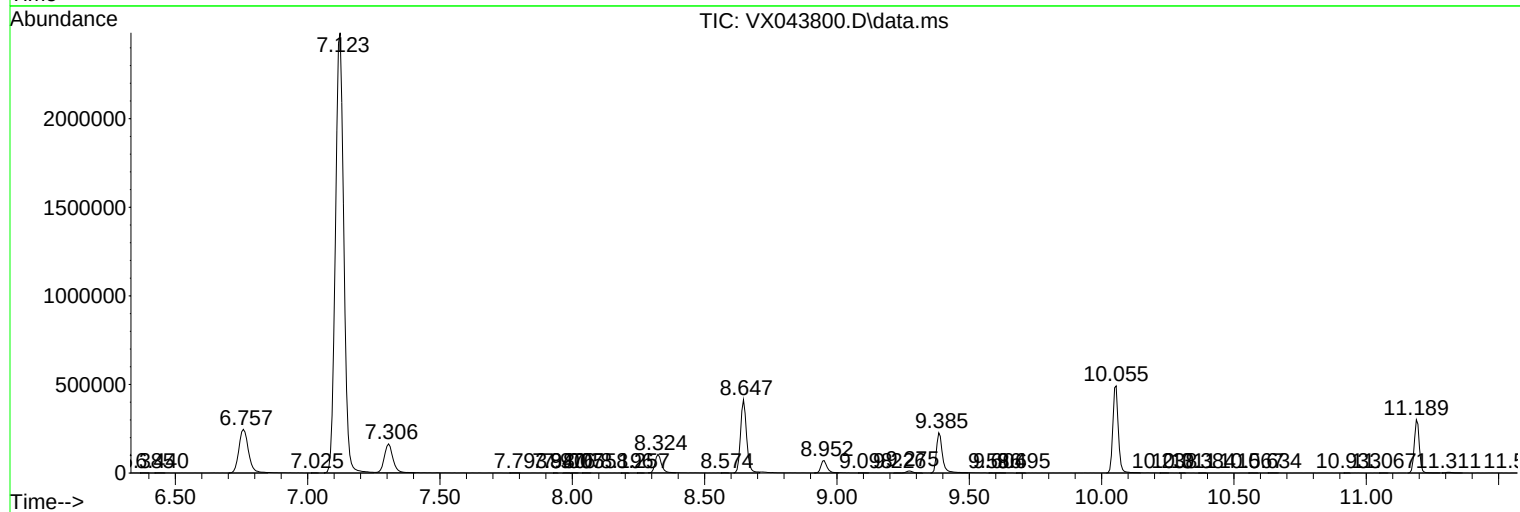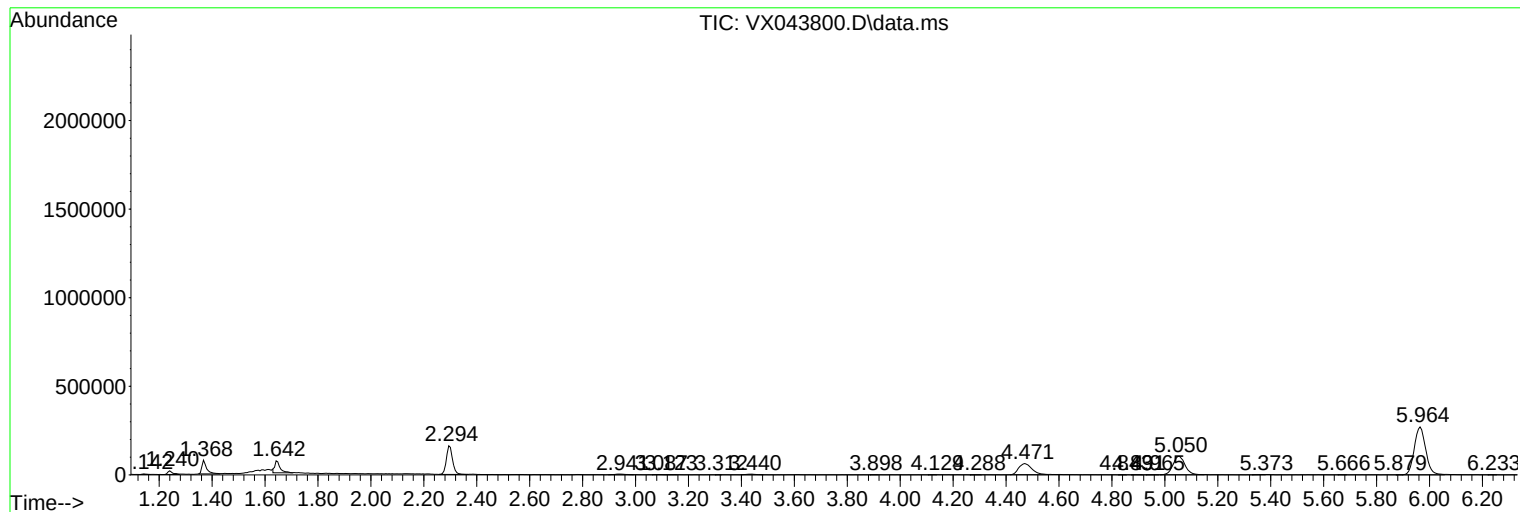

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043800.D
Acq On : 11 Nov 2024 18:22
Operator : JC/MD
Sample : P4786-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27N5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043800.D
Acq On : 11 Nov 2024 18:22
Operator : JC/MD
Sample : P4786-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27N5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------