
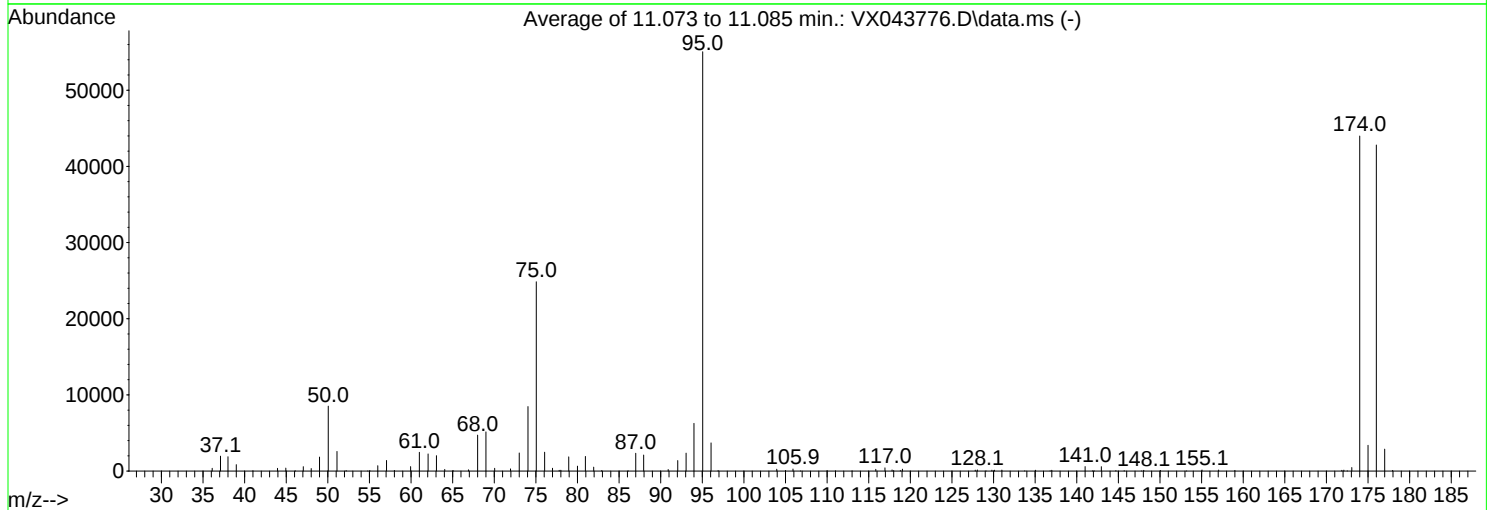


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111124\
Data File : VX043776.D
Acq On : 11 Nov 2024 08:31
Operator : JC/MD
Sample : BFB696
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB696

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Title : VOC Analysis
Last Update : Tue Nov 12 00:51:02 2024

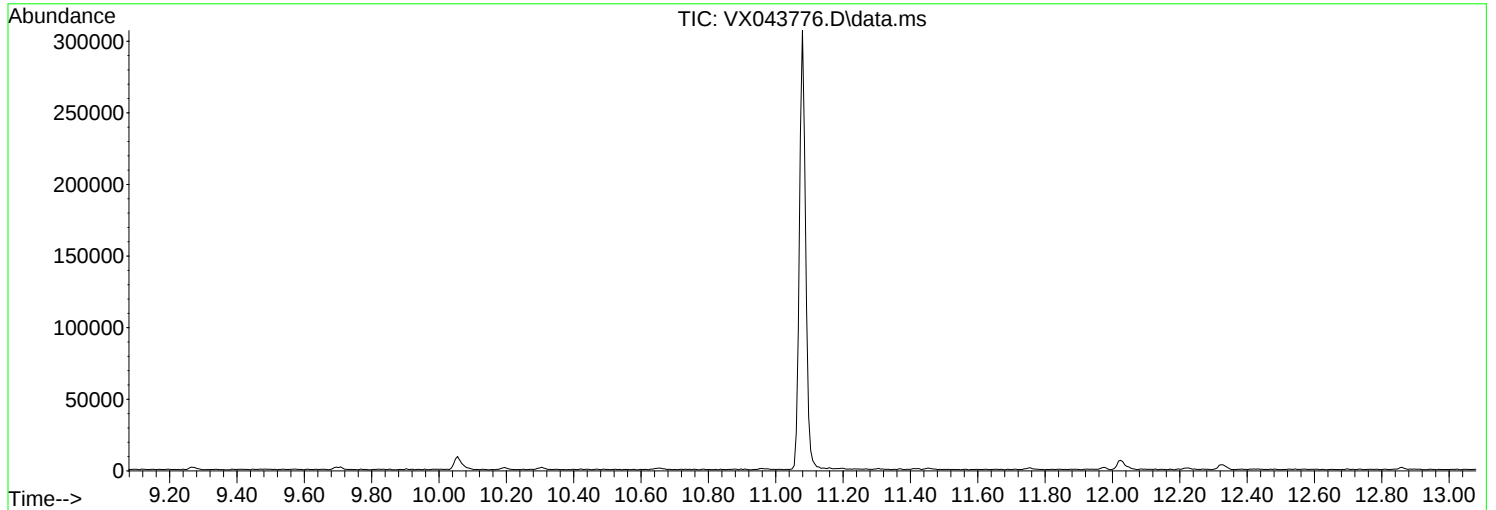

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	8528	PASS
75	95	30	80	45.1	24856	PASS
95	95	100	100	100.0	55053	PASS
96	95	5	9	6.7	3702	PASS
173	174	0.00	2	1.1	465	PASS
174	95	50	120	79.9	43989	PASS
175	174	5	9	7.7	3382	PASS
176	174	95	101	97.3	42808	PASS
177	176	5	9	6.7	2880	PASS

m/z	Abundance
36.10	67.0
39.00	64.0
39.90	555.0
44.10	404.0

Instrument :
MSVOA_X
ClientSampleId :
BFB696

m/z	Abundance
36.10	464.0
37.10	2218.0
38.00	2055.0
39.00	924.0
40.10	505.0
44.00	490.0
45.00	453.0
46.10	93.0
47.00	531.0
48.10	279.0
49.10	1794.0
50.10	9291.0
51.10	2624.0
52.20	80.0
54.80	62.0
55.90	728.0
57.10	1525.0
58.10	59.0
59.90	583.0
61.00	2429.0
62.00	2276.0
63.10	1901.0
64.10	220.0
65.10	68.0
66.90	141.0
68.00	5048.0
69.00	5405.0
70.00	455.0
71.90	259.0
73.00	2429.0
74.10	8758.0
75.00	22864.0
76.00	2834.0
77.00	397.0
77.80	313.0
78.90	1905.0
80.00	607.0
80.90	1671.0
81.90	374.0
87.00	2098.0
88.00	1833.0
90.90	219.0
92.10	1124.0
93.00	2255.0
94.00	5802.0
95.00	51808.0
96.00	3481.0
104.00	320.0
105.80	201.0
109.90	55.0
111.00	79.0
113.00	59.0
115.80	272.0
117.00	484.0
117.70	111.0
118.80	224.0
128.10	181.0
130.10	210.0
131.00	120.0
133.70	57.0
136.80	110.0
141.10	535.0
143.00	549.0
144.70	56.0
145.70	110.0
148.00	108.0
150.10	53.0
155.00	76.0
157.10	162.0
159.00	97.0
171.80	108.0
172.50	113.0
173.10	466.0
174.00	36080.0
175.00	2915.0
176.00	33960.0
177.00	2525.0
178.00	67.0

Instrument :
MSVOA_X
ClientSampleId :
BFB696

m/z	Abundance
36.20	503.0
37.10	2352.0
38.00	2055.0
39.10	1177.0
40.00	483.0
41.00	119.0
43.90	590.0
44.90	451.0
47.10	716.0
48.00	422.0
49.00	2306.0
50.00	9644.0
51.10	3069.0
52.20	136.0
55.00	71.0
56.00	735.0
57.00	1721.0
58.00	181.0
60.00	633.0
61.00	2793.0
62.10	2437.0
63.10	2544.0
64.10	317.0
65.00	58.0
66.90	274.0
68.00	5356.0
69.00	5971.0
70.10	387.0
71.90	337.0
73.00	2919.0
74.00	9347.0
75.10	30272.0
76.00	2456.0
77.00	475.0
78.00	222.0
78.90	2047.0
80.00	783.0
81.00	2359.0
82.00	843.0
82.90	81.0
87.00	3011.0
88.00	2385.0
90.90	340.0
92.10	1847.0
93.10	2797.0
94.00	7611.0
95.10	66248.0
96.00	4214.0
103.90	262.0
105.00	116.0
105.90	356.0
106.80	64.0
110.00	59.0
115.80	243.0
117.00	429.0
117.80	352.0
119.00	368.0
127.80	382.0
129.80	360.0
131.10	145.0
133.80	61.0
135.00	215.0
137.00	166.0
141.00	728.0
141.90	103.0
143.00	625.0
144.70	135.0
145.70	61.0
148.10	202.0
150.00	84.0
153.20	78.0
155.00	129.0
157.00	182.0
159.00	105.0
171.90	204.0
173.10	497.0
174.00	53344.0
175.00	4044.0
176.00	51568.0
177.00	3566.0
178.00	96.0

Instrument :
MSVOA_X
ClientSampleId :
BFB696

m/z	Abundance
36.00	335.0
37.10	1312.0
38.00	1550.0
39.10	628.0
40.10	573.0
44.20	574.0
45.00	280.0
47.10	486.0
47.90	294.0
48.90	1423.0
50.10	6648.0
51.10	2051.0
55.10	100.0
56.10	665.0
57.00	931.0
60.00	535.0
61.00	2166.0
62.00	2034.0
63.00	1633.0
63.90	128.0
65.00	100.0
66.90	102.0
68.00	3766.0
69.00	4072.0
70.00	260.0
72.00	281.0
73.00	1775.0
74.00	7312.0
75.10	21432.0
76.10	2146.0
76.90	241.0
78.00	121.0
79.00	1648.0
79.80	282.0
80.10	284.0
81.00	1740.0
81.90	329.0
82.90	85.0
86.10	85.0
87.00	1903.0
87.90	2094.0
90.90	62.0
92.00	1174.0
93.00	2023.0
94.00	5384.0
95.10	47104.0
96.10	3410.0
96.90	187.0
104.00	159.0
105.00	79.0
106.00	253.0
110.10	54.0
115.90	191.0
116.90	350.0
118.00	194.0
119.10	393.0
128.00	270.0
129.10	69.0
130.10	154.0
130.90	133.0
135.10	125.0
137.00	163.0
140.90	513.0
142.10	86.0
142.90	566.0
147.80	60.0
150.00	107.0
155.10	229.0
157.00	80.0
159.00	62.0
172.10	375.0
173.00	433.0
174.00	42544.0
175.00	3188.0
176.00	42896.0
177.00	2548.0
177.90	89.0

Instrument :
MSVOA_X
ClientSampleId :
BFB696