

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
 Data File : VX025142.D
 Acq On : 12 Nov 2021 09:46
 Operator : JC/MD
 Sample : VX1112MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 12 10:44:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 12 05:08:01 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	204669	50.00	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	183628	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	91066	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	65865	47.63	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	95.26%		
7) Chloroethane-d5	1.672	69	44346	56.27	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	112.54%		
11) 1,1-Dichloroethene-d2	2.306	63	82273	34.60	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	69.20%		
21) 2-Butanone-d5	4.458	46	104769	100.27	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	100.27%		
24) Chloroform-d	5.056	84	113314	46.58	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.16%		
26) 1,2-Dichloroethane-d4	6.080	65	184	0.12	ug/L	0.12
Spiked Amount 50.000	Range 70 - 125		Recovery =	0.24%#		
32) Benzene-d6	5.976	84	244003	48.69	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.38%		
36) 1,2-Dichloropropane-d6	7.312	67	75984	49.65	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	99.30%		
41) Toluene-d8	8.653	98	227722	47.58	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.16%		
43) trans-1,3-Dichloroprop...	8.951	79	39128	47.10	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.20%		
47) 2-Hexanone-d5	9.384	63	80586	98.07	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	98.07%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	104219	47.28	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	94.56%		
66) 1,2-Dichlorobenzene-d4	12.323	152	88768	49.17	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.34%		
Target Compounds						
37) 1,2-Dichloropropane	7.305	63	8073	5.71	ug/L #	85
44) trans-1,3-Dichloropropene	8.951	75	1708	0.76	ug/L #	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
Data File : VX025142.D
Acq On : 12 Nov 2021 09:46
Operator : JC/MD
Sample : VX1112MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 12 10:44:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 12 05:08:01 2021
Response via : Initial Calibration




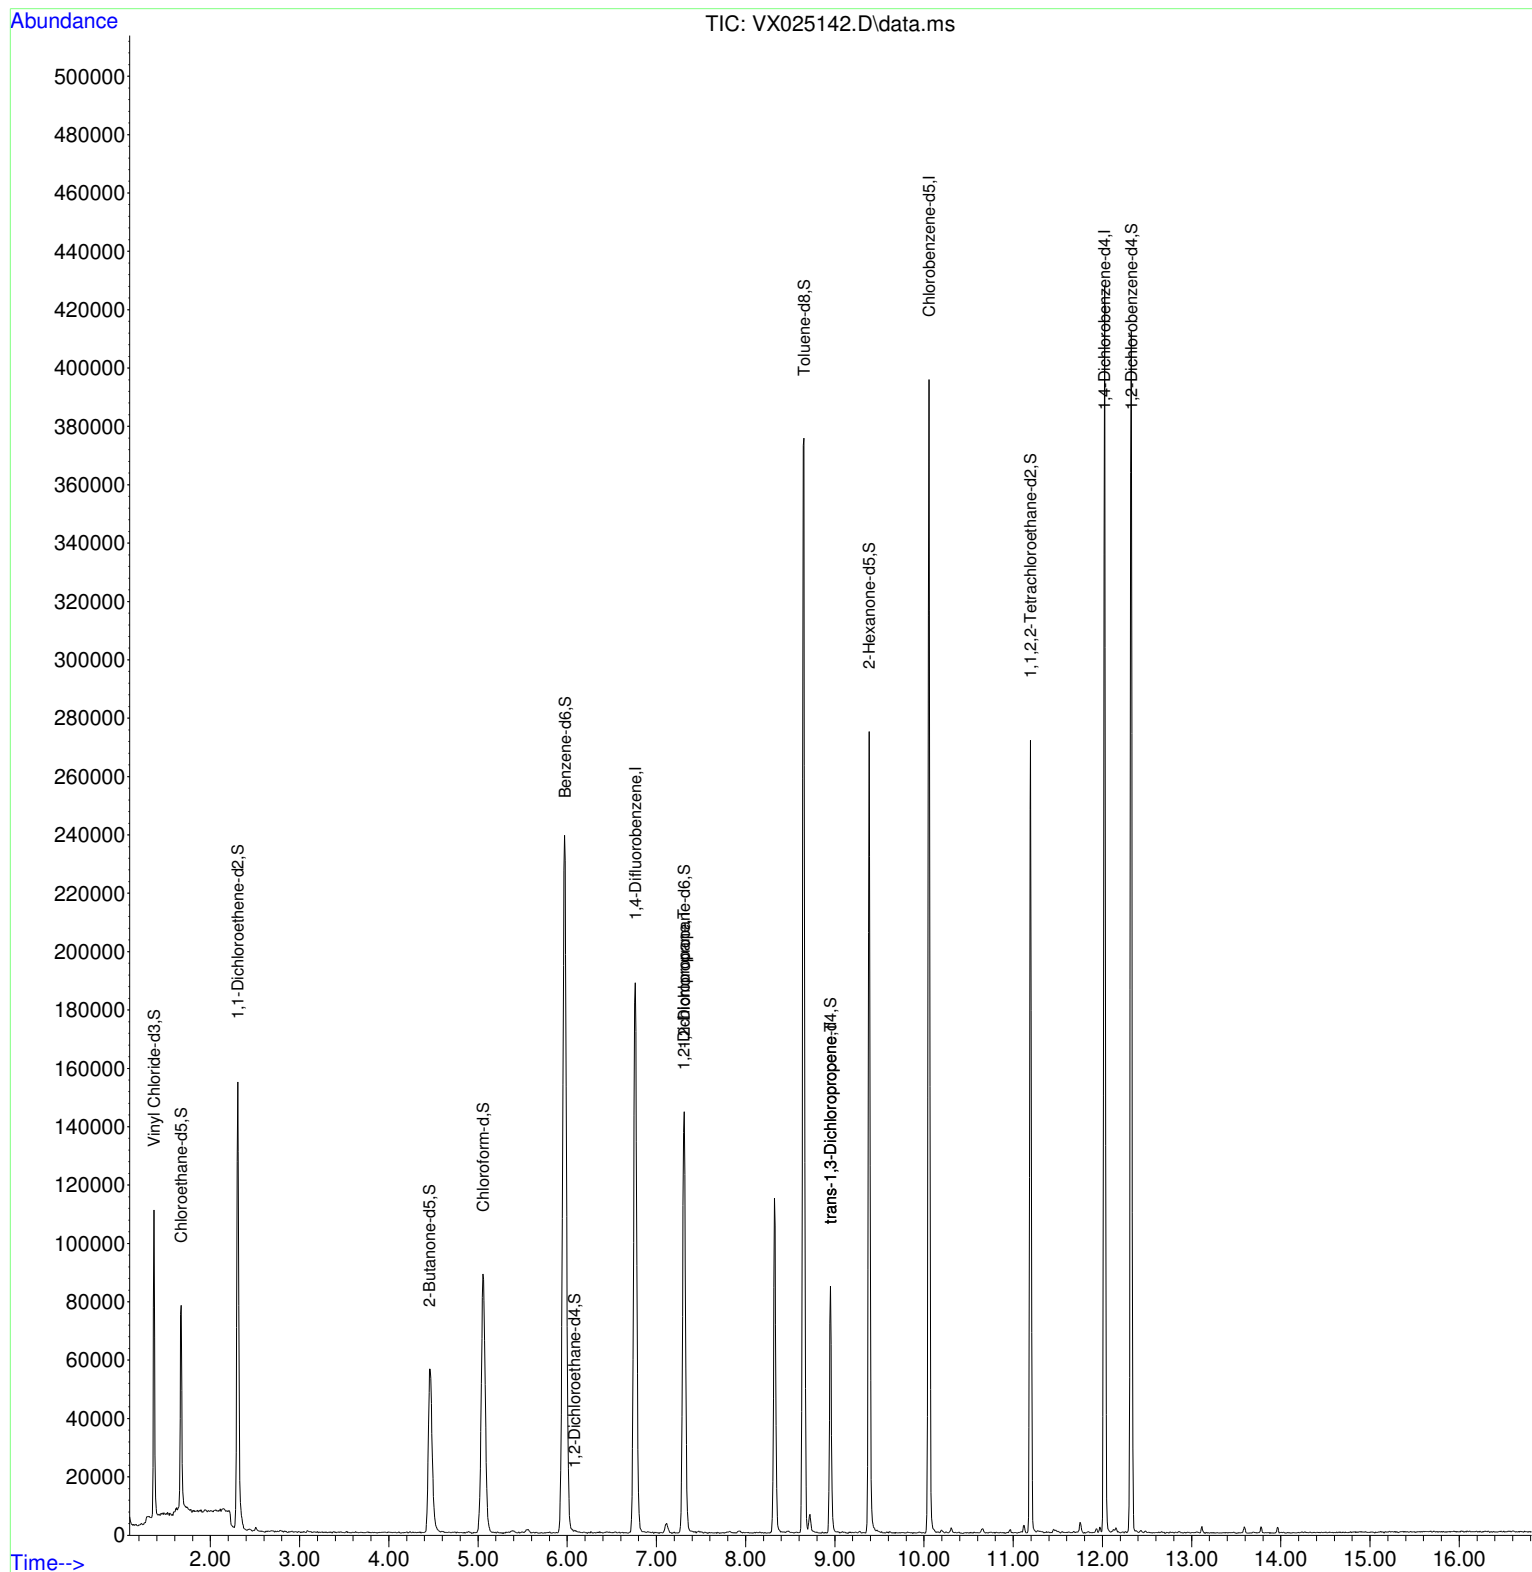


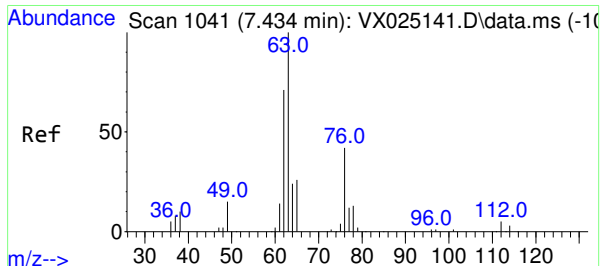

#37
1,2-Dichloropropane
Concen: 5.71 ug/L
RT: 7.305 min Scan# 1
Delta R.T. -0.128 min
Lab File: VX025142.D
Acq: 12 Nov 2021 09:46

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 63 Resp: 8073
Ion Ratio Lower Upper
63 100
112 0.0 4.0 6.0#

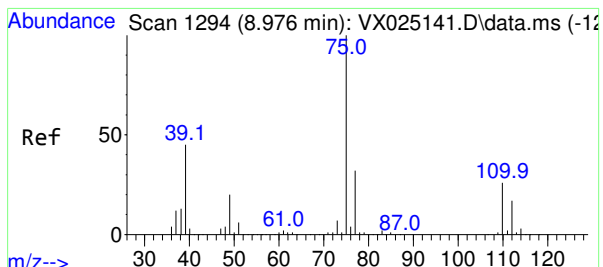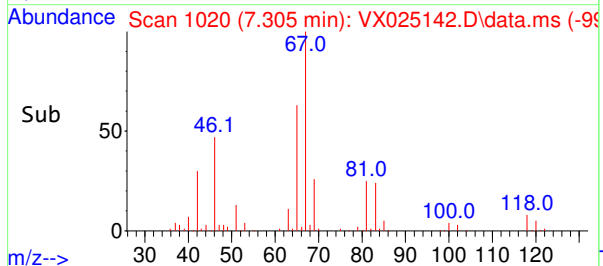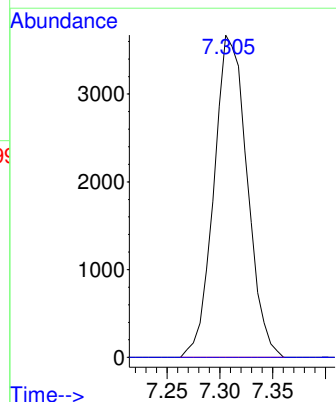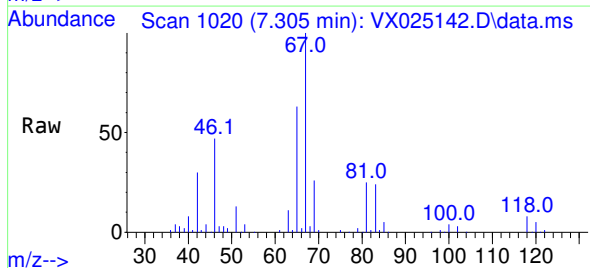

#44
trans-1,3-Dichloropropene
Concen: 0.76 ug/L
RT: 8.951 min Scan# 1290
Delta R.T. -0.025 min
Lab File: VX025142.D
Acq: 12 Nov 2021 09:46

Tgt Ion: 75 Resp: 1708
Ion Ratio Lower Upper
75 100
77 50.3 23.4 43.6#

