

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
 Data File : VX025143.D
 Acq On : 12 Nov 2021 10:09
 Operator : JC/MD
 Sample : VX1112WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 12 10:45:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 12 05:08:01 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	198958	50.00	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	181310	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	89945	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	62436	46.45	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	92.90%		
7) Chloroethane-d5	1.672	69	44606	58.23	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	116.46%		
11) 1,1-Dichloroethene-d2	2.306	63	79069	34.20	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	68.40%		
21) 2-Butanone-d5	4.458	46	104479	102.86	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	102.86%		
24) Chloroform-d	5.068	84	110879	46.89	ug/L	0.01
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.78%		
26) 1,2-Dichloroethane-d4	5.958	65	70143	48.94	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.88%		
32) Benzene-d6	5.976	84	236724	47.84	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.68%		
36) 1,2-Dichloropropane-d6	7.312	67	73750	48.81	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.62%		
41) Toluene-d8	8.653	98	222966	47.18	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.36%		
43) trans-1,3-Dichloroprop...	8.951	79	38692	47.17	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.34%		
47) 2-Hexanone-d5	9.384	63	81279	100.17	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	100.17%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	103714	47.66	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	95.32%		
66) 1,2-Dichlorobenzene-d4	12.323	152	87055	48.82	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.64%		
Target Compounds						
44) trans-1,3-Dichloropropene	8.951	75	1878	0.84	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
Data File : VX025143.D
Acq On : 12 Nov 2021 10:09
Operator : JC/MD
Sample : VX1112WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 12 10:45:12 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 12 05:08:01 2021
Response via : Initial Calibration

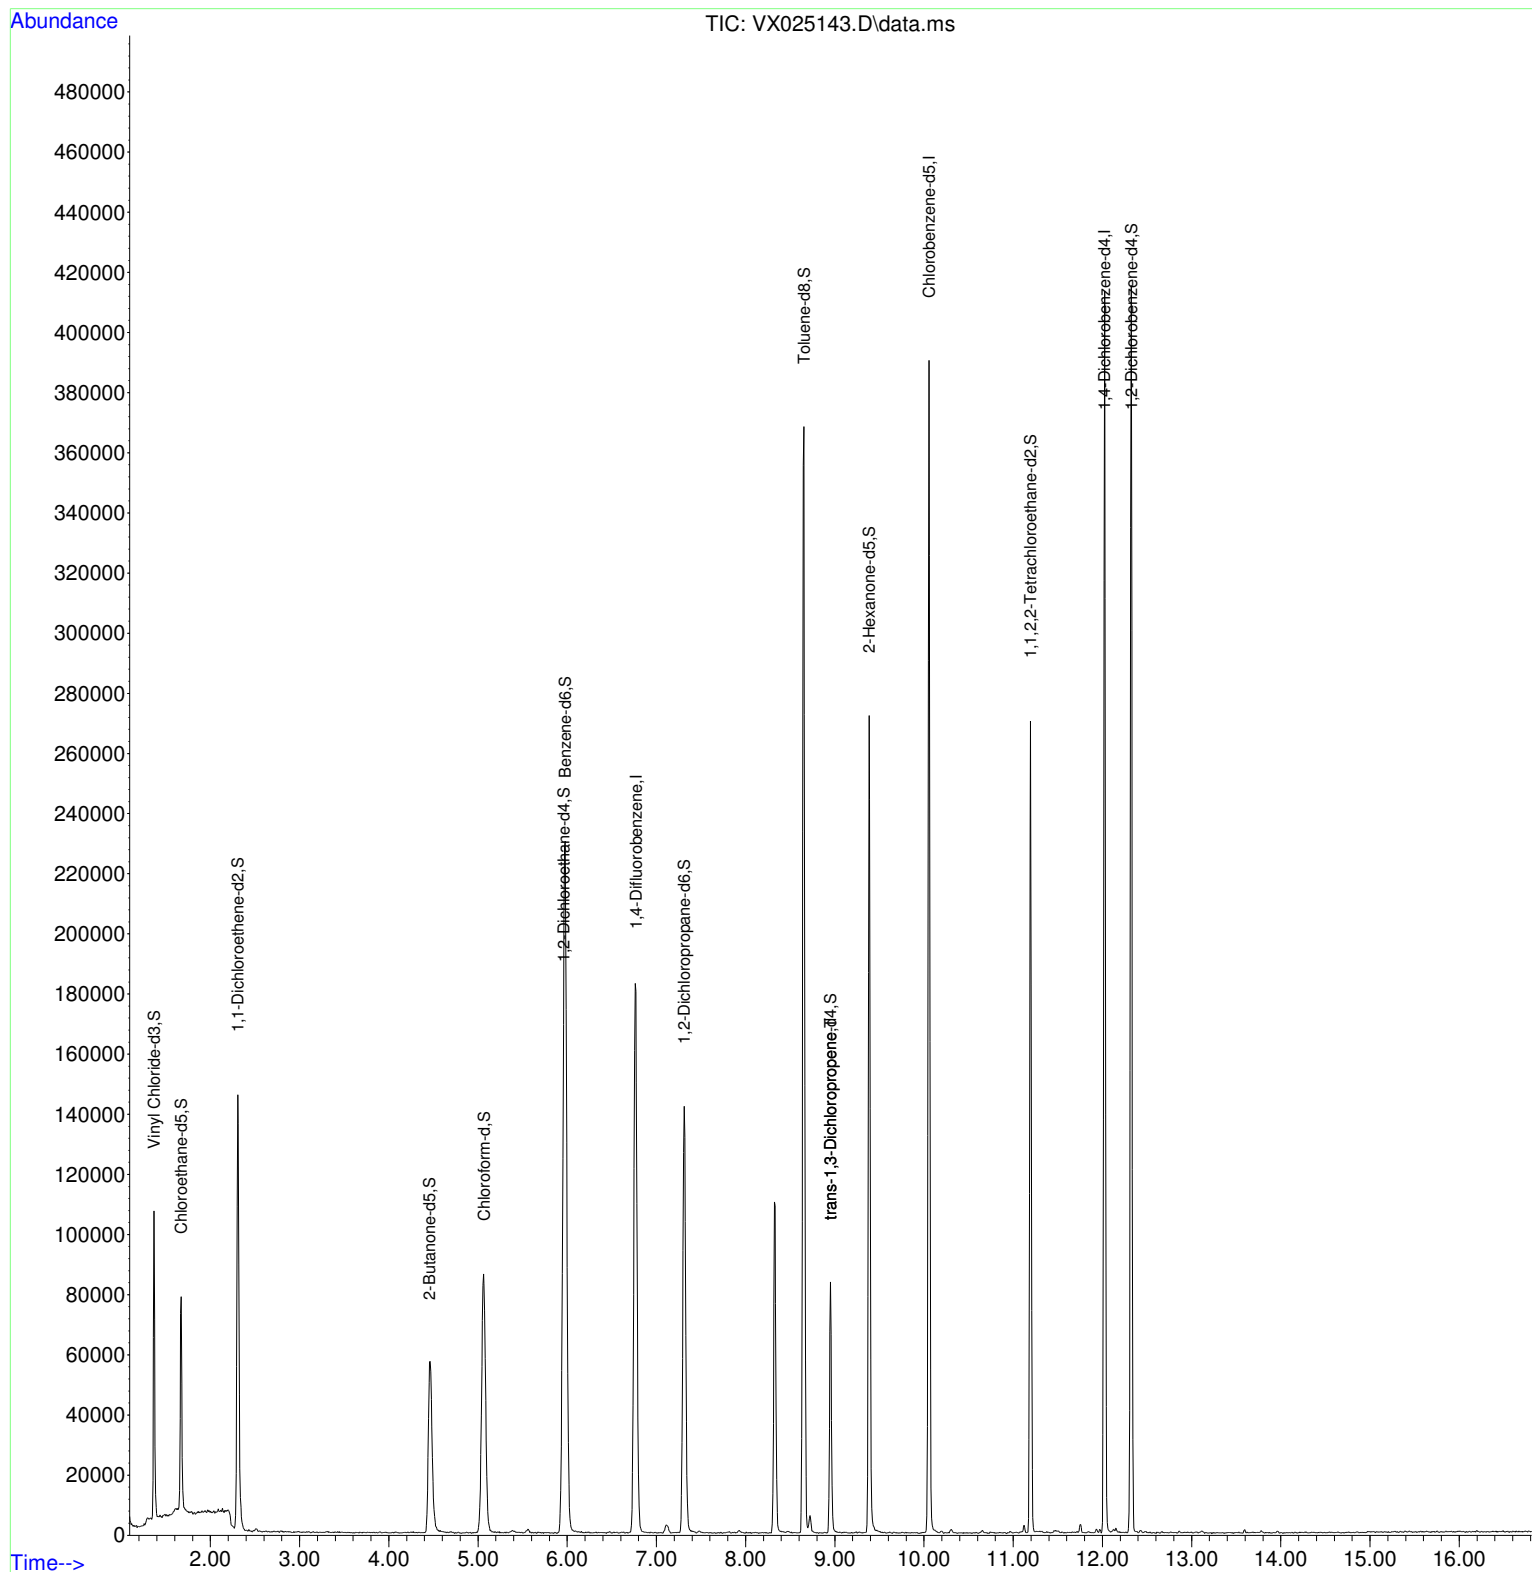

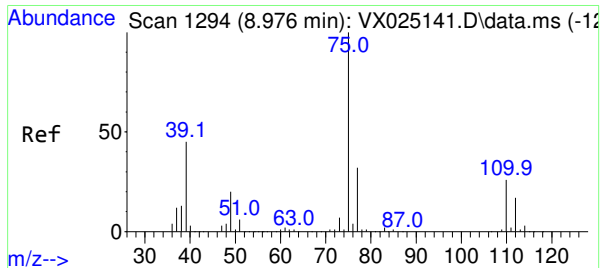

#44
trans-1,3-Dichloropropene
Concen: 0.84 ug/L
RT: 8.951 min Scan# 1
Delta R.T. -0.025 min
Lab File: VX025143.D
Acq: 12 Nov 2021 10:09

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 75 Resp: 1878
Ion Ratio Lower Upper
75 100
77 33.8 23.4 43.6

