

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
 Data File : VX025145.D
 Acq On : 12 Nov 2021 11:02
 Operator : JC/MD
 Sample : M4615-02 40X
 Misc : 4.07g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 12 12:08:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 12 12:01:23 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	209570	50.00	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	191869	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	95666	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	60938	43.04	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	86.08%		
7) Chloroethane-d5	1.666	69	37232	46.14	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	92.28%		
11) 1,1-Dichloroethene-d2	2.306	63	77865	31.98	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	63.96%		
21) 2-Butanone-d5	4.458	46	98496	92.06	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	92.06%		
24) Chloroform-d	5.062	84	109695	44.04	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.08%		
26) 1,2-Dichloroethane-d4	5.958	65	68322	45.25	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.50%		
32) Benzene-d6	5.976	84	234868	44.85	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.70%		
36) 1,2-Dichloropropane-d6	7.311	67	72545	45.37	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	90.74%		
41) Toluene-d8	8.652	98	219528	43.90	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.80%		
43) trans-1,3-Dichloroprop...	8.951	79	38405	44.25	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	88.50%		
47) 2-Hexanone-d5	9.384	63	78093	90.95	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	90.95%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	101406	44.03	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	88.06%		
66) 1,2-Dichlorobenzene-d4	12.323	152	86722	45.73	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.46%		
Target Compounds						
37) 1,2-Dichloropropane	7.311	63	7451	5.05	ug/L	# 85
44) trans-1,3-Dichloropropene	8.951	75	1838	0.78	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
Data File : VX025145.D
Acq On : 12 Nov 2021 11:02
Operator : JC/MD
Sample : M4615-02 40X
Misc : 4.07g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 12 12:08:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 12 12:01:23 2021
Response via : Initial Calibration




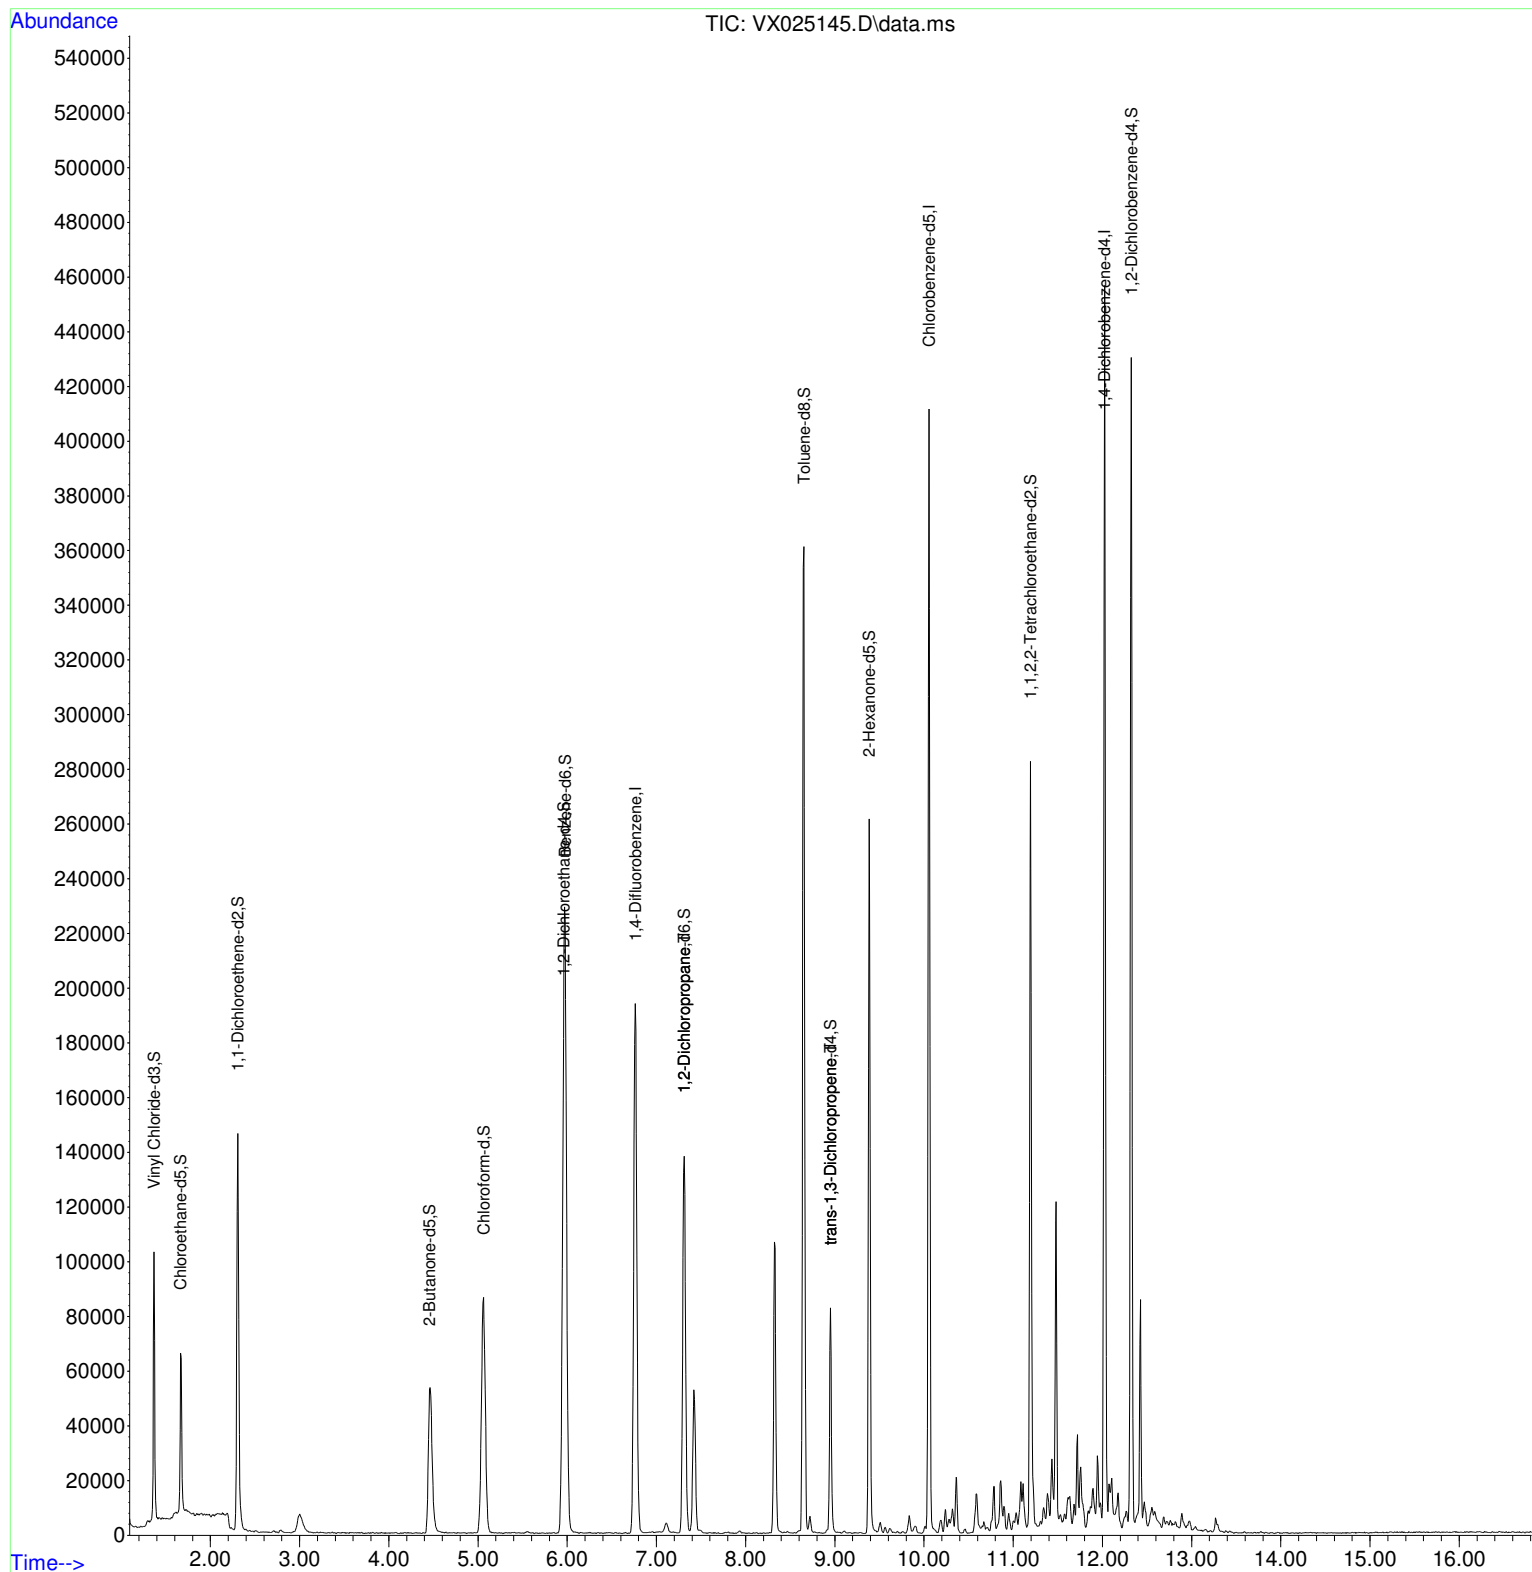


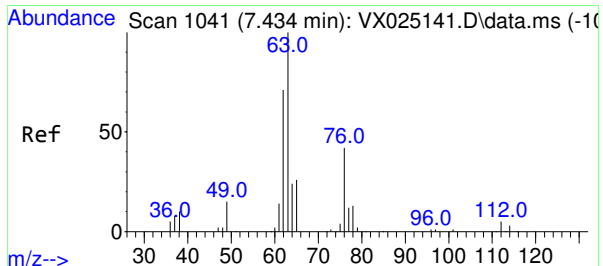

#37
 1,2-Dichloropropane
 Concen: 5.05 ug/L
 RT: 7.311 min Scan# 1
 Delta R.T. -0.122 min
 Lab File: VX025145.D
 Acq: 12 Nov 2021 11:02

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 63 Resp: 7451
 Ion Ratio Lower Upper
 63 100
 112 0.0 4.0 6.0#

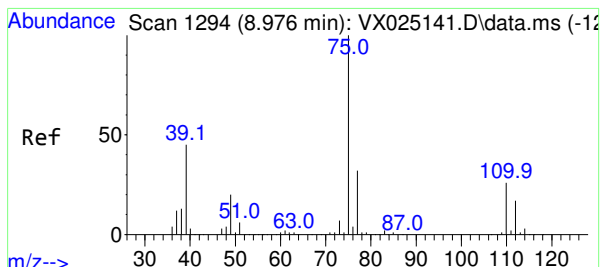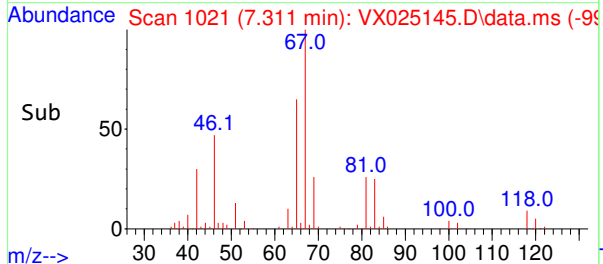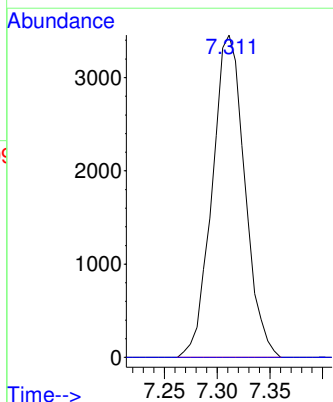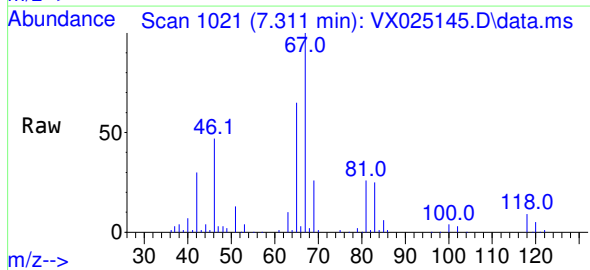

#44
 trans-1,3-Dichloropropene
 Concen: 0.78 ug/L
 RT: 8.951 min Scan# 1290
 Delta R.T. -0.025 min
 Lab File: VX025145.D
 Acq: 12 Nov 2021 11:02

Tgt Ion: 75 Resp: 1838
 Ion Ratio Lower Upper
 75 100
 77 43.4 23.4 43.6

