

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
 Data File : VX025148.D
 Acq On : 12 Nov 2021 12:47
 Operator : JC/MD
 Sample : M4615-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM11121WMA.M
 Title : VOC Analysis

Signal : TIC: VX025148.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	111702	113948	15.22%	1.829%
2	1.672	92	96	104	rVB	73633	94735	12.65%	1.521%
3	2.307	194	200	212	rVB	161770	259951	34.72%	4.173%
4	2.685	260	262	264	rBV2	366	307	0.04%	0.005%
5	2.880	292	294	297	rVB3	414	472	0.06%	0.008%
6	2.983	308	311	315	rBV4	359	663	0.09%	0.011%
7	3.105	329	331	334	rBV4	366	294	0.04%	0.005%
8	3.215	347	349	350	rBV	429	302	0.04%	0.005%
9	3.270	356	358	360	rBV2	602	555	0.07%	0.009%
10	3.300	360	363	365	rVB4	304	352	0.05%	0.006%
11	3.489	391	394	397	rBV4	401	621	0.08%	0.010%
12	3.623	412	416	417	rBV2	380	414	0.06%	0.007%
13	3.678	422	425	426	rBV2	394	407	0.05%	0.007%
14	3.764	437	439	441	rBV2	264	285	0.04%	0.005%
15	3.898	460	461	465	rVB3	363	322	0.04%	0.005%
16	3.934	465	467	469	rBV3	336	322	0.04%	0.005%
17	4.032	481	483	486	rVB3	489	403	0.05%	0.006%
18	4.087	490	492	495	rVB3	357	424	0.06%	0.007%
19	4.129	495	499	503	rBV5	438	519	0.07%	0.008%
20	4.209	510	512	516	rVB2	279	369	0.05%	0.006%
21	4.245	516	518	522	rBV3	333	501	0.07%	0.008%
22	4.465	545	554	569	rBV	61563	176922	23.63%	2.840%
23	5.068	641	653	668	rBV	96882	294242	39.30%	4.723%
24	5.202	673	675	677	rVB3	432	302	0.04%	0.005%
25	5.251	681	683	688	rVB5	393	445	0.06%	0.007%
26	5.416	708	710	712	rVB3	356	305	0.04%	0.005%
27	5.495	721	723	727	rVB3	335	417	0.06%	0.007%
28	5.556	728	733	739	rVV4	853	1575	0.21%	0.025%
29	5.678	750	753	754	rBV3	569	372	0.05%	0.006%
30	5.842	776	780	783	rVB4	458	472	0.06%	0.008%
31	5.977	788	802	820	rBV2	249442	748743	100.00%	12.019%
32	6.208	836	840	842	rBV2	419	544	0.07%	0.009%
33	6.233	842	844	845	rVB2	499	318	0.04%	0.005%
34	6.355	862	864	866	rBV3	515	411	0.05%	0.007%
35	6.678	914	917	920	rBV4	259	344	0.05%	0.006%
36	6.763	921	931	947	rBV	197891	475457	63.50%	7.632%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
 Data File : VX025148.D
 Acq On : 12 Nov 2021 12:47
 Operator : JC/MD
 Sample : M4615-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

37	7.312	1012	1021	1031	rBV	152680	335670	44.83%	5.388%
38	7.421	1032	1039	1047	rBV	94888	198454	26.50%	3.186%
39	7.927	1118	1122	1125	rBV4	740	1257	0.17%	0.020%
40	7.982	1127	1131	1133	rBV5	508	634	0.08%	0.010%
41	8.165	1159	1161	1163	rBV3	390	351	0.05%	0.006%
42	8.275	1178	1179	1181	rBV2	395	284	0.04%	0.005%
43	8.330	1181	1188	1200	rVV	117958	199326	26.62%	3.200%
44	8.653	1234	1241	1249	rBV	405219	636773	85.05%	10.222%
45	8.720	1249	1252	1259	rVB	6421	9346	1.25%	0.150%
46	8.952	1284	1290	1302	rBV	92474	132945	17.76%	2.134%
47	9.263	1339	1341	1342	rBV2	416	396	0.05%	0.006%
48	9.385	1355	1361	1373	rBV	283162	402610	53.77%	6.463%
49	9.653	1403	1405	1406	rBV2	557	375	0.05%	0.006%
50	9.750	1420	1421	1423	rBV2	423	298	0.04%	0.005%
51	10.055	1465	1471	1481	rBV	425852	569632	76.08%	9.144%
52	10.195	1491	1494	1495	rBV2	430	422	0.06%	0.007%
53	10.305	1509	1512	1516	rVB3	964	1220	0.16%	0.020%
54	10.500	1541	1544	1546	rBV3	334	408	0.05%	0.007%
55	10.598	1556	1560	1563	rVB3	399	584	0.08%	0.009%
56	10.634	1563	1566	1569	rBV4	643	867	0.12%	0.014%
57	10.860	1598	1603	1604	rBV4	390	558	0.07%	0.009%
58	10.970	1617	1621	1623	rBV4	333	430	0.06%	0.007%
59	11.085	1638	1640	1641	rVV2	557	336	0.04%	0.005%
60	11.122	1642	1646	1651	rVB	2889	3836	0.51%	0.062%
61	11.195	1652	1658	1668	rBV	294922	371064	49.56%	5.957%
62	11.378	1684	1688	1691	rBV4	500	770	0.10%	0.012%
63	11.482	1701	1705	1711	rVB	4209	6228	0.83%	0.100%
64	11.549	1711	1716	1719	rBV4	526	939	0.13%	0.015%
65	11.628	1727	1729	1733	rBV4	629	667	0.09%	0.011%
66	11.719	1740	1744	1746	rBV5	1575	2145	0.29%	0.034%
67	11.750	1746	1749	1754	rVB2	2729	3493	0.47%	0.056%
68	11.884	1770	1771	1774	rVB3	382	332	0.04%	0.005%
69	11.939	1776	1780	1784	rVB6	1258	2067	0.28%	0.033%
70	11.969	1784	1785	1789	rBV4	559	367	0.05%	0.006%
71	12.024	1789	1794	1805	rBV	468340	579326	77.37%	9.300%
72	12.238	1826	1829	1830	rBV3	400	314	0.04%	0.005%
73	12.323	1837	1843	1850	rBV	446247	566853	75.71%	9.100%
74	12.427	1856	1860	1865	rVB2	5512	6784	0.91%	0.109%
75	12.475	1865	1868	1874	rVB5	740	1333	0.18%	0.021%
76	12.664	1895	1899	1901	rBV4	573	738	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
 Data File : VX025148.D
 Acq On : 12 Nov 2021 12:47
 Operator : JC/MD
 Sample : M4615-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM11121WMA.M
 Title : VOC Analysis

77	12.860	1928	1931	1933	rBV3	616	865	0.12%	0.014%
78	12.920	1940	1941	1944	rBV3	364	387	0.05%	0.006%
79	13.006	1953	1955	1957	rVB2	471	357	0.05%	0.006%
80	13.036	1958	1960	1966	rVB5	435	747	0.10%	0.012%
81	13.237	1989	1993	1996	rBV4	322	535	0.07%	0.009%
82	13.268	1996	1998	2002	rVB3	629	678	0.09%	0.011%
83	13.414	2021	2022	2025	rBV2	313	281	0.04%	0.005%
84	13.634	2056	2058	2060	rBV3	224	289	0.04%	0.005%
85	13.713	2069	2071	2073	rVV2	418	334	0.04%	0.005%
86	13.859	2093	2095	2100	rBV4	350	534	0.07%	0.009%
87	14.036	2121	2124	2128	rVB3	445	547	0.07%	0.009%
88	14.067	2128	2129	2132	rBV3	352	374	0.05%	0.006%
89	14.134	2138	2140	2142	rBV3	415	405	0.05%	0.007%
90	14.182	2145	2148	2149	rBV	451	390	0.05%	0.006%
91	14.286	2163	2165	2168	rVV3	301	326	0.04%	0.005%
92	14.390	2179	2182	2183	rBV2	314	378	0.05%	0.006%
93	14.853	2256	2258	2261	rBV3	362	443	0.06%	0.007%
94	14.896	2263	2265	2269	rBV3	530	738	0.10%	0.012%
95	15.115	2298	2301	2305	rBV5	566	967	0.13%	0.016%
96	15.274	2325	2327	2330	rBV3	359	338	0.05%	0.005%
97	15.652	2387	2389	2392	rBV3	401	561	0.07%	0.009%
98	16.139	2467	2469	2473	rVB3	556	599	0.08%	0.010%
99	16.292	2493	2494	2496	rBV2	702	519	0.07%	0.008%
100	16.438	2516	2518	2519	rBV	627	405	0.05%	0.007%




Sum of corrected areas: 6229464

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
Data File : VX025148.D
Acq On : 12 Nov 2021 12:47
Operator : JC/MD
Sample : M4615-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

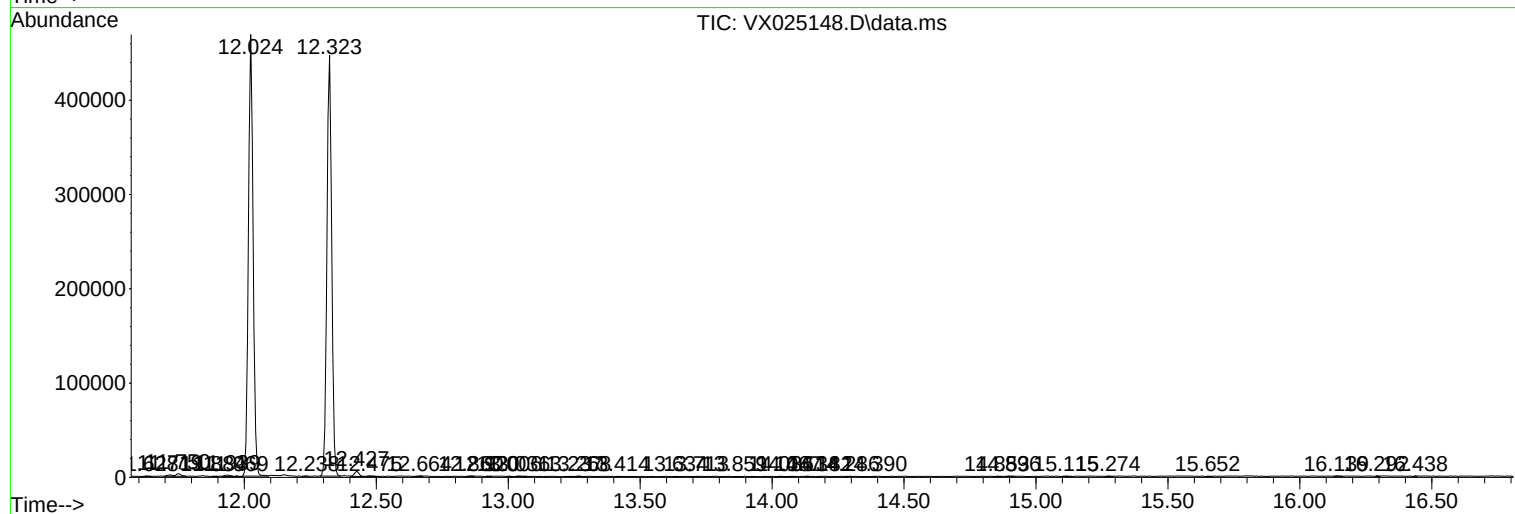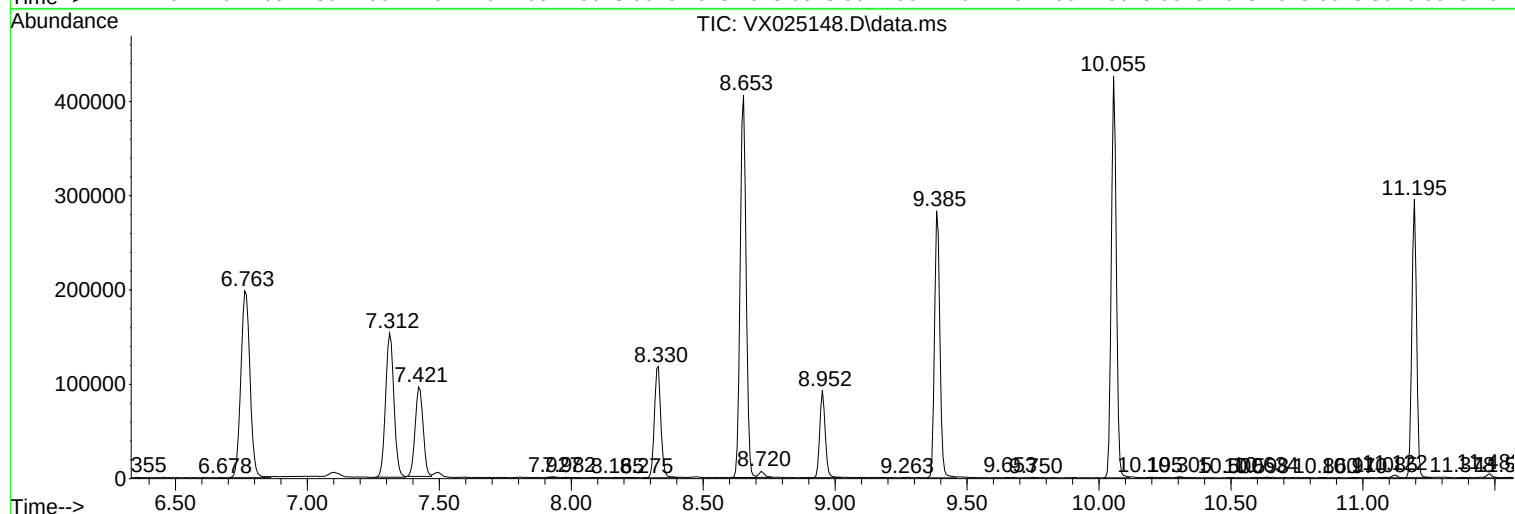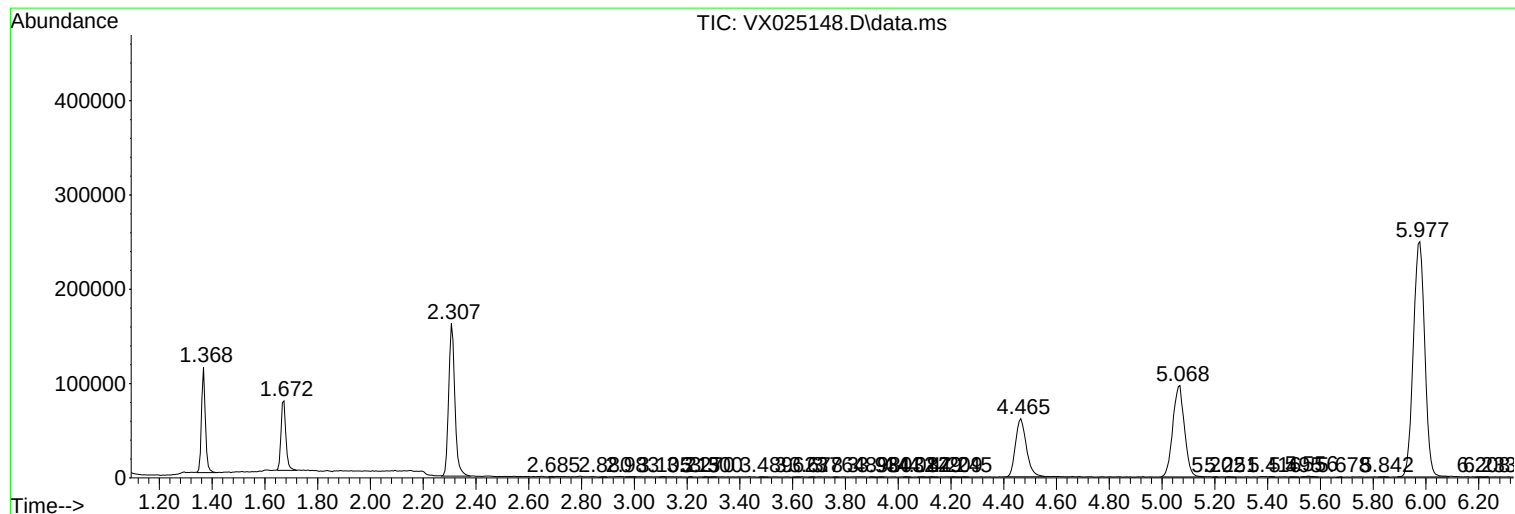

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
Data File : VX025148.D
Acq On : 12 Nov 2021 12:47
Operator : JC/MD
Sample : M4615-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
Data File : VX025148.D
Acq On : 12 Nov 2021 12:47
Operator : JC/MD
Sample : M4615-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
