

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
 Data File : VX025149.D
 Acq On : 12 Nov 2021 13:12
 Operator : JC/MD
 Sample : M4645-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM11121WMA.M
 Title : VOC Analysis

Signal : TIC: VX025149.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	53	rBV	101879	102470	14.39%	1.749%
2	1.672	92	96	103	rVB	69063	85897	12.06%	1.467%
3	2.306	194	200	215	rVB	151752	243594	34.20%	4.159%
4	3.550	400	404	406	rVB5	352	434	0.06%	0.007%
5	3.593	406	411	413	rVB3	568	662	0.09%	0.011%
6	3.617	413	415	420	rBV5	427	702	0.10%	0.012%
7	3.702	427	429	430	rBV2	326	200	0.03%	0.003%
8	3.757	435	438	440	rBV3	407	496	0.07%	0.008%
9	3.873	456	457	460	rBV3	415	271	0.04%	0.005%
10	4.105	493	495	496	rBV2	364	355	0.05%	0.006%
11	4.464	543	554	575	rBV	59216	175294	24.61%	2.993%
12	4.714	593	595	596	rVB2	366	258	0.04%	0.004%
13	4.909	625	627	628	rBV2	313	237	0.03%	0.004%
14	5.062	638	652	667	rBV	90026	278530	39.11%	4.755%
15	5.226	676	679	681	rBV4	318	355	0.05%	0.006%
16	5.391	700	706	711	rVB5	629	1358	0.19%	0.023%
17	5.446	713	715	717	rBV2	302	231	0.03%	0.004%
18	5.537	727	730	731	rBV2	471	556	0.08%	0.009%
19	5.635	744	746	749	rBV3	362	466	0.07%	0.008%
20	5.873	782	785	786	rBV2	285	300	0.04%	0.005%
21	5.970	789	801	819	rVV2	237526	712214	100.00%	12.160%
22	6.208	838	840	845	rVB4	352	398	0.06%	0.007%
23	6.269	848	850	851	rBV2	300	293	0.04%	0.005%
24	6.312	855	857	858	rBV	308	242	0.03%	0.004%
25	6.458	879	881	883	rVV2	322	203	0.03%	0.003%
26	6.763	920	931	942	rBV	190661	453762	63.71%	7.747%
27	7.311	1013	1021	1032	rBV	148760	318036	44.65%	5.430%
28	7.421	1032	1039	1048	rVV2	40897	84994	11.93%	1.451%
29	7.543	1057	1059	1062	rVB4	448	421	0.06%	0.007%
30	7.763	1093	1095	1096	rBV2	391	304	0.04%	0.005%
31	7.933	1116	1123	1131	rBV8	855	2222	0.31%	0.038%
32	8.049	1140	1142	1145	rBV2	264	222	0.03%	0.004%
33	8.104	1148	1151	1153	rBV3	486	653	0.09%	0.011%
34	8.208	1166	1168	1171	rBV3	381	542	0.08%	0.009%
35	8.256	1175	1176	1178	rBV2	291	262	0.04%	0.004%
36	8.330	1181	1188	1198	rVV	112650	192009	26.96%	3.278%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
 Data File : VX025149.D
 Acq On : 12 Nov 2021 13:12
 Operator : JC/MD
 Sample : M4645-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM11121WMA.M
 Title : VOC Analysis

37	8.653	1233	1241	1248	rBV	381265	605716	85.05%	10.341%
38	8.720	1248	1252	1262	rVB2	5618	10828	1.52%	0.185%
39	8.951	1284	1290	1300	rVV	88559	128711	18.07%	2.197%
40	9.086	1311	1312	1315	rBV2	314	293	0.04%	0.005%
41	9.268	1341	1342	1345	rVB2	262	204	0.03%	0.003%
42	9.384	1356	1361	1371	rBV	271161	390062	54.77%	6.659%
43	9.713	1413	1415	1417	rBV2	416	414	0.06%	0.007%
44	9.915	1446	1448	1450	rBV2	328	289	0.04%	0.005%
45	9.988	1457	1460	1462	rBV3	245	245	0.03%	0.004%
46	10.055	1464	1471	1480	rBV	402901	543453	76.30%	9.278%
47	10.189	1491	1493	1495	rBV3	368	279	0.04%	0.005%
48	10.305	1509	1512	1518	rVB4	1079	1387	0.19%	0.024%
49	10.445	1533	1535	1538	rVB3	309	282	0.04%	0.005%
50	10.488	1538	1542	1544	rBV4	419	536	0.08%	0.009%
51	10.555	1549	1553	1556	rBV4	351	547	0.08%	0.009%
52	10.604	1559	1561	1564	rBV2	297	250	0.04%	0.004%
53	10.701	1574	1577	1578	rBV2	238	238	0.03%	0.004%
54	10.762	1584	1587	1588	rVB3	404	357	0.05%	0.006%
55	10.780	1588	1590	1594	rVB5	212	244	0.03%	0.004%
56	10.914	1609	1612	1615	rBV4	392	625	0.09%	0.011%
57	11.091	1639	1641	1642	rBV2	362	210	0.03%	0.004%
58	11.122	1642	1646	1652	rVB2	2667	3490	0.49%	0.060%
59	11.195	1652	1658	1669	rBV	291473	359162	50.43%	6.132%
60	11.384	1686	1689	1691	rBV4	377	523	0.07%	0.009%
61	11.481	1701	1705	1710	rBV2	2708	3493	0.49%	0.060%
62	11.719	1741	1744	1746	rBV4	1123	1253	0.18%	0.021%
63	11.750	1746	1749	1752	rVB3	2028	2472	0.35%	0.042%
64	11.841	1762	1764	1768	rVB4	685	780	0.11%	0.013%
65	11.933	1776	1779	1784	rBV2	1362	2001	0.28%	0.034%
66	12.024	1789	1794	1805	rVV	446637	564297	79.23%	9.634%
67	12.103	1805	1807	1809	rVV2	656	696	0.10%	0.012%
68	12.146	1813	1814	1818	rVB2	1121	1071	0.15%	0.018%
69	12.323	1837	1843	1852	rBV	444699	556627	78.15%	9.503%
70	12.426	1856	1860	1863	rVB2	3533	4279	0.60%	0.073%
71	12.579	1881	1885	1888	rBV3	503	717	0.10%	0.012%
72	12.743	1910	1912	1913	rBV2	275	219	0.03%	0.004%
73	12.823	1923	1925	1928	rBV3	373	466	0.07%	0.008%
74	12.859	1928	1931	1932	rVV	539	568	0.08%	0.010%
75	12.908	1935	1939	1941	rVB4	370	542	0.08%	0.009%
76	13.097	1968	1970	1971	rBV2	246	222	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
 Data File : VX025149.D
 Acq On : 12 Nov 2021 13:12
 Operator : JC/MD
 Sample : M4645-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
 Title : VOC Analysis

77	13.213	1987	1989	1991	rVB3	390	323	0.05%	0.006%
78	13.268	1995	1998	2002	rVV5	685	936	0.13%	0.016%
79	13.384	2015	2017	2020	rBV3	324	391	0.05%	0.007%
80	13.512	2036	2038	2039	rBV2	367	223	0.03%	0.004%
81	13.597	2050	2052	2054	rBV2	281	330	0.05%	0.006%
82	13.646	2057	2060	2062	rBV3	343	356	0.05%	0.006%
83	13.694	2067	2068	2071	rBV3	439	473	0.07%	0.008%
84	13.774	2079	2081	2082	rVV2	331	241	0.03%	0.004%
85	13.847	2089	2093	2097	rVB2	357	602	0.08%	0.010%
86	13.883	2097	2099	2100	rBV	324	302	0.04%	0.005%
87	13.932	2105	2107	2110	rBV2	372	442	0.06%	0.008%
88	13.969	2110	2113	2115	rBV3	337	493	0.07%	0.008%
89	14.085	2131	2132	2134	rBV2	451	308	0.04%	0.005%
90	14.121	2134	2138	2140	rBV3	337	481	0.07%	0.008%
91	14.255	2158	2160	2161	rBV2	406	362	0.05%	0.006%
92	14.682	2228	2230	2234	rVB3	250	296	0.04%	0.005%
93	14.719	2234	2236	2237	rBV2	391	338	0.05%	0.006%
94	14.847	2255	2257	2259	rBV3	431	451	0.06%	0.008%
95	14.902	2263	2266	2268	rBV3	402	429	0.06%	0.007%
96	15.164	2307	2309	2312	rVB	327	230	0.03%	0.004%
97	15.700	2395	2397	2400	rVB3	519	385	0.05%	0.007%
98	15.853	2420	2422	2423	rBV2	476	329	0.05%	0.006%
99	16.224	2481	2483	2485	rBV	405	304	0.04%	0.005%
100	16.316	2495	2498	2500	rBV2	632	734	0.10%	0.013%




Sum of corrected areas: 5857250

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
Data File : VX025149.D
Acq On : 12 Nov 2021 13:12
Operator : JC/MD
Sample : M4645-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

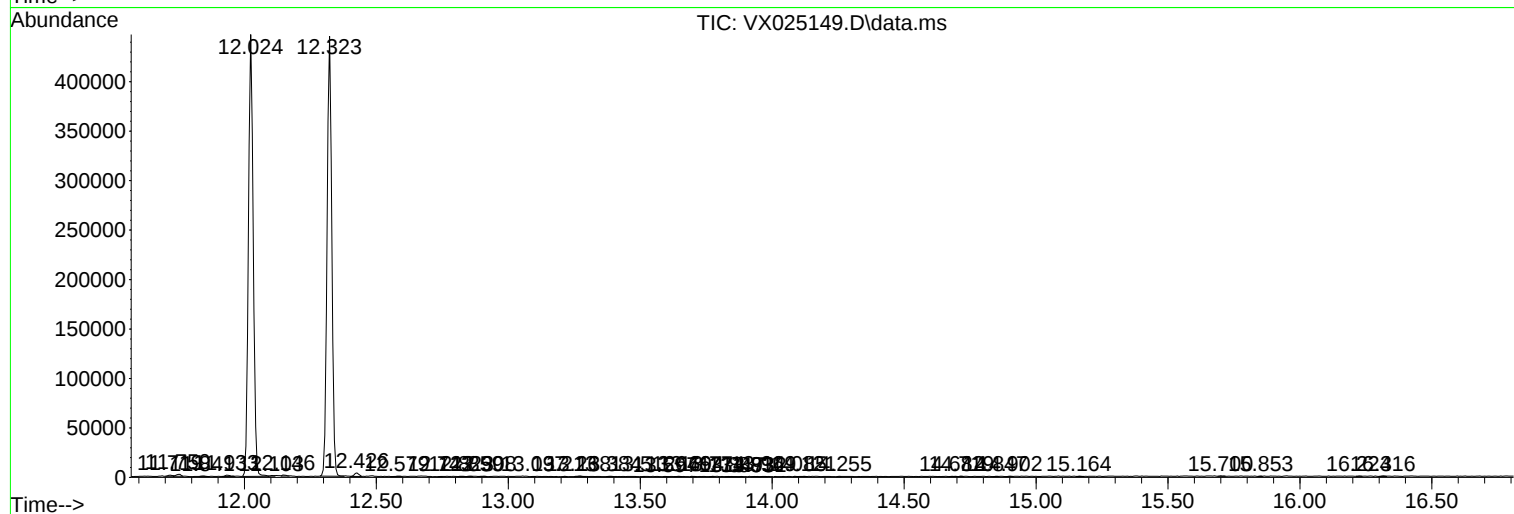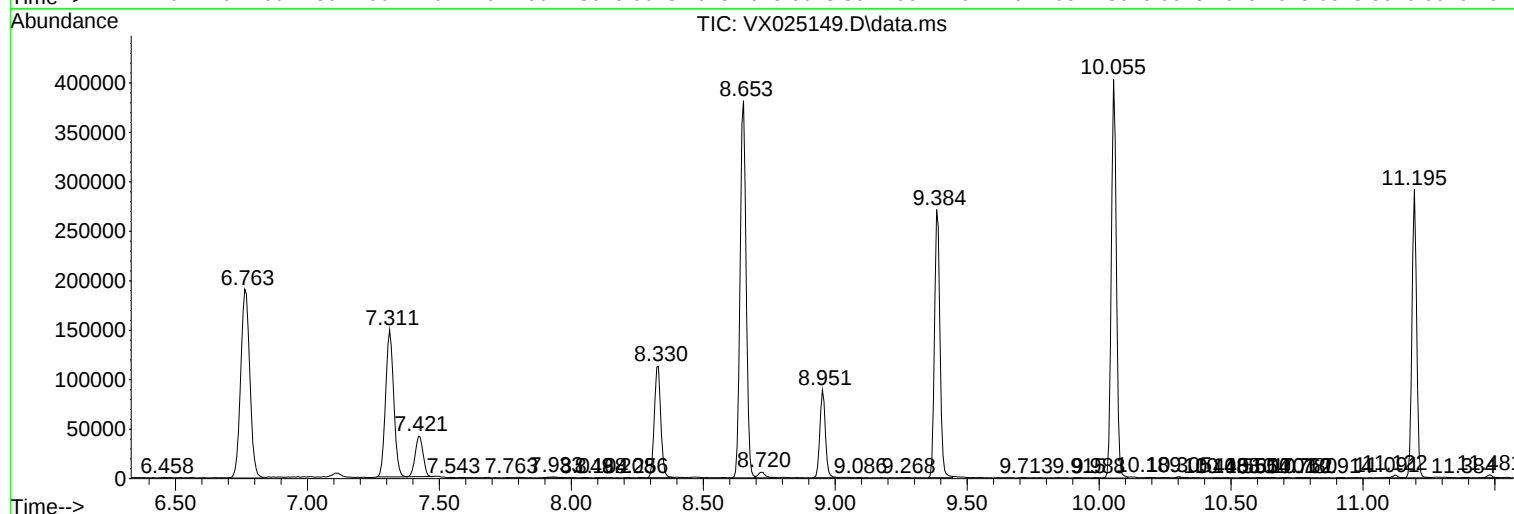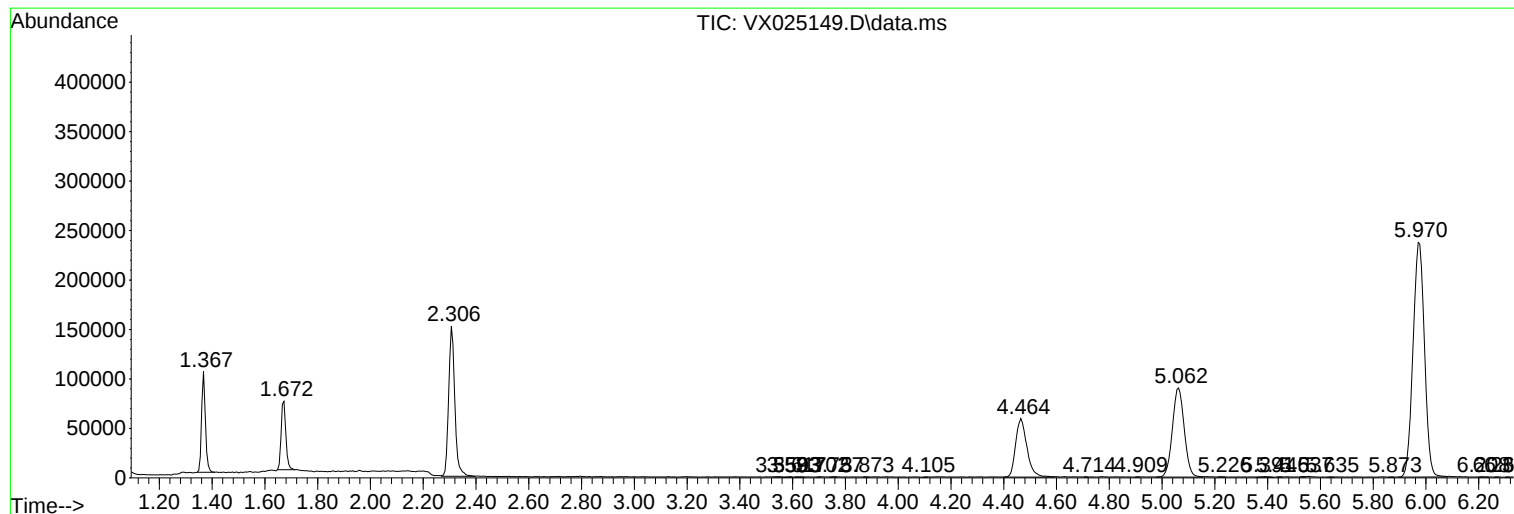

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
Data File : VX025149.D
Acq On : 12 Nov 2021 13:12
Operator : JC/MD
Sample : M4645-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
Data File : VX025149.D
Acq On : 12 Nov 2021 13:12
Operator : JC/MD
Sample : M4645-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc