

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
 Data File : VX025152.D
 Acq On : 12 Nov 2021 14:22
 Operator : JC/MD
 Sample : M4672-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A42A7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM11121WMA.M
 Title : VOC Analysis

Signal : TIC: VX025152.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.203	18	19	22	rBV2	464	445	0.06%	0.008%
2	1.294	28	34	36	rBV5	4768	9501	1.37%	0.161%
3	1.368	42	46	51	rBV	102111	102257	14.74%	1.734%
4	1.666	91	95	104	rVB	76523	102568	14.79%	1.739%
5	2.306	194	200	214	rVV	148443	242038	34.90%	4.105%
6	2.398	214	215	219	rVB3	751	517	0.07%	0.009%
7	2.562	238	242	244	rBV5	404	500	0.07%	0.008%
8	2.745	269	272	275	rVB4	394	577	0.08%	0.010%
9	2.825	283	285	290	rVB4	331	543	0.08%	0.009%
10	2.940	300	304	307	rVV4	620	879	0.13%	0.015%
11	3.038	319	320	326	rVB3	402	573	0.08%	0.010%
12	3.203	344	347	350	rBV5	400	537	0.08%	0.009%
13	3.318	363	366	368	rBV2	341	439	0.06%	0.007%
14	3.392	374	378	380	rBV2	453	584	0.08%	0.010%
15	3.538	399	402	403	rVV2	516	479	0.07%	0.008%
16	3.873	455	457	460	rVB3	409	429	0.06%	0.007%
17	3.904	460	462	466	rBV2	484	679	0.10%	0.012%
18	4.178	503	507	509	rBV3	379	405	0.06%	0.007%
19	4.465	544	554	567	rBV	54793	158841	22.90%	2.694%
20	4.727	593	597	600	rVB5	370	624	0.09%	0.011%
21	4.757	600	602	606	rBV3	291	456	0.07%	0.008%
22	5.062	640	652	669	rVB	88131	276122	39.81%	4.683%
23	5.263	684	685	689	rBV2	370	412	0.06%	0.007%
24	5.385	701	705	710	rVB5	463	828	0.12%	0.014%
25	5.544	727	731	732	rBV3	662	577	0.08%	0.010%
26	5.794	768	772	776	rBV5	384	529	0.08%	0.009%
27	5.855	778	782	783	rVB3	513	639	0.09%	0.011%
28	5.976	789	802	820	rBV2	232432	693533	100.00%	11.762%
29	6.092	820	821	826	rVB3	652	761	0.11%	0.013%
30	6.141	826	829	834	rBV5	405	531	0.08%	0.009%
31	6.458	878	881	882	rBV2	405	488	0.07%	0.008%
32	6.665	912	915	920	rVB3	336	509	0.07%	0.009%
33	6.763	920	931	944	rBV	197511	475126	68.51%	8.058%
34	6.982	964	967	969	rVV3	532	775	0.11%	0.013%
35	7.013	970	972	973	rVV2	567	436	0.06%	0.007%
36	7.025	973	974	977	rVV3	528	449	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
 Data File : VX025152.D
 Acq On : 12 Nov 2021 14:22
 Operator : JC/MD
 Sample : M4672-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A42A7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM11121WMA.M
 Title : VOC Analysis

37	7.110	977	988	998	rVV6	4592	12428	1.79%	0.211%
38	7.202	1001	1003	1008	rVV3	509	680	0.10%	0.012%
39	7.312	1012	1021	1032	rVV	142524	312389	45.04%	5.298%
40	7.421	1032	1039	1047	rVV	19116	41601	6.00%	0.706%
41	7.494	1047	1051	1058	rVV6	1843	3967	0.57%	0.067%
42	7.799	1099	1101	1105	rBV5	494	459	0.07%	0.008%
43	7.927	1115	1122	1124	rBV3	1078	1801	0.26%	0.031%
44	8.000	1132	1134	1136	rBV2	528	548	0.08%	0.009%
45	8.031	1136	1139	1143	rVV5	359	575	0.08%	0.010%
46	8.330	1181	1188	1200	rBV	111734	186697	26.92%	3.166%
47	8.470	1209	1211	1214	rVB4	458	508	0.07%	0.009%
48	8.653	1234	1241	1249	rBV	376788	596113	85.95%	10.110%
49	8.726	1249	1253	1263	rVB	5544	9421	1.36%	0.160%
50	8.799	1263	1265	1270	rVB4	597	819	0.12%	0.014%
51	8.878	1276	1278	1283	rVB6	331	393	0.06%	0.007%
52	8.952	1283	1290	1297	rBV	85322	125335	18.07%	2.126%
53	9.037	1302	1304	1305	rVV2	644	428	0.06%	0.007%
54	9.049	1305	1306	1309	rVB3	543	445	0.06%	0.008%
55	9.147	1316	1322	1323	rBV6	560	729	0.11%	0.012%
56	9.275	1340	1343	1347	rBV4	663	944	0.14%	0.016%
57	9.317	1347	1350	1353	rBV4	528	503	0.07%	0.009%
58	9.384	1355	1361	1376	rBV	259972	366355	52.82%	6.213%
59	9.525	1380	1384	1388	rVB6	945	1428	0.21%	0.024%
60	9.573	1391	1392	1397	rVB3	368	413	0.06%	0.007%
61	9.622	1397	1400	1402	rBV4	702	761	0.11%	0.013%
62	9.671	1405	1408	1410	rBV3	385	466	0.07%	0.008%
63	9.799	1422	1429	1430	rBV6	741	1513	0.22%	0.026%
64	9.988	1458	1460	1464	rVB5	658	819	0.12%	0.014%
65	10.055	1464	1471	1486	rBV	424398	573382	82.68%	9.724%
66	10.244	1500	1502	1504	rBV3	465	418	0.06%	0.007%
67	10.305	1509	1512	1516	rVB5	2035	2226	0.32%	0.038%
68	10.342	1516	1518	1520	rBV3	690	674	0.10%	0.011%
69	10.409	1527	1529	1533	rBV4	536	743	0.11%	0.013%
70	10.439	1533	1534	1537	rVV3	618	665	0.10%	0.011%
71	10.567	1554	1555	1556	rBV	719	423	0.06%	0.007%
72	10.585	1556	1558	1560	rVV3	784	624	0.09%	0.011%
73	10.628	1563	1565	1566	rVB	810	447	0.06%	0.008%
74	10.683	1572	1574	1577	rVB3	1040	887	0.13%	0.015%
75	10.750	1584	1585	1588	rVV3	649	673	0.10%	0.011%
76	10.774	1588	1589	1592	rVB3	863	590	0.09%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
 Data File : VX025152.D
 Acq On : 12 Nov 2021 14:22
 Operator : JC/MD
 Sample : M4672-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A42A7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
 Title : VOC Analysis

77	10.945	1616	1617	1619	rBV	718	656	0.09%	0.011%
78	11.012	1626	1628	1629	rBV2	908	540	0.08%	0.009%
79	11.085	1638	1640	1643	rVB3	593	476	0.07%	0.008%
80	11.122	1643	1646	1650	rBV3	2183	3109	0.45%	0.053%
81	11.195	1652	1658	1666	rBV	269537	341032	49.17%	5.784%
82	11.256	1666	1668	1670	rBV3	559	391	0.06%	0.007%
83	11.286	1670	1673	1674	rBV3	1159	1195	0.17%	0.020%
84	11.390	1684	1690	1691	rBV6	1263	1825	0.26%	0.031%
85	11.756	1746	1750	1753	rBV6	3475	4432	0.64%	0.075%
86	11.817	1759	1760	1762	rBV2	1235	636	0.09%	0.011%
87	12.024	1789	1794	1803	rBV	484549	595480	85.86%	10.099%
88	12.219	1822	1826	1834	rVB	8754	14710	2.12%	0.249%
89	12.323	1837	1843	1851	rVB	431813	538629	77.66%	9.135%
90	12.420	1857	1859	1863	rBV4	2188	3113	0.45%	0.053%
91	15.316	2332	2334	2336	rBV3	1478	1806	0.26%	0.031%
92	15.560	2368	2374	2381	rBV2	22448	36222	5.22%	0.614%
93	16.097	2456	2462	2467	rBV2	9383	18119	2.61%	0.307%
94	16.176	2472	2475	2478	rBV5	658	852	0.12%	0.014%
95	16.267	2488	2490	2491	rBV2	843	717	0.10%	0.012%
96	16.401	2510	2512	2513	rBV2	555	426	0.06%	0.007%
97	16.487	2524	2526	2527	rBV	853	642	0.09%	0.011%
98	16.542	2530	2535	2538	rVV6	1416	2258	0.33%	0.038%
99	16.590	2541	2543	2549	rVB7	1696	2488	0.36%	0.042%
100	16.633	2549	2550	2553	rBV3	754	854	0.12%	0.014%


Sum of corrected areas: 5896484

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
Data File : VX025152.D
Acq On : 12 Nov 2021 14:22
Operator : JC/MD
Sample : M4672-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A42A7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

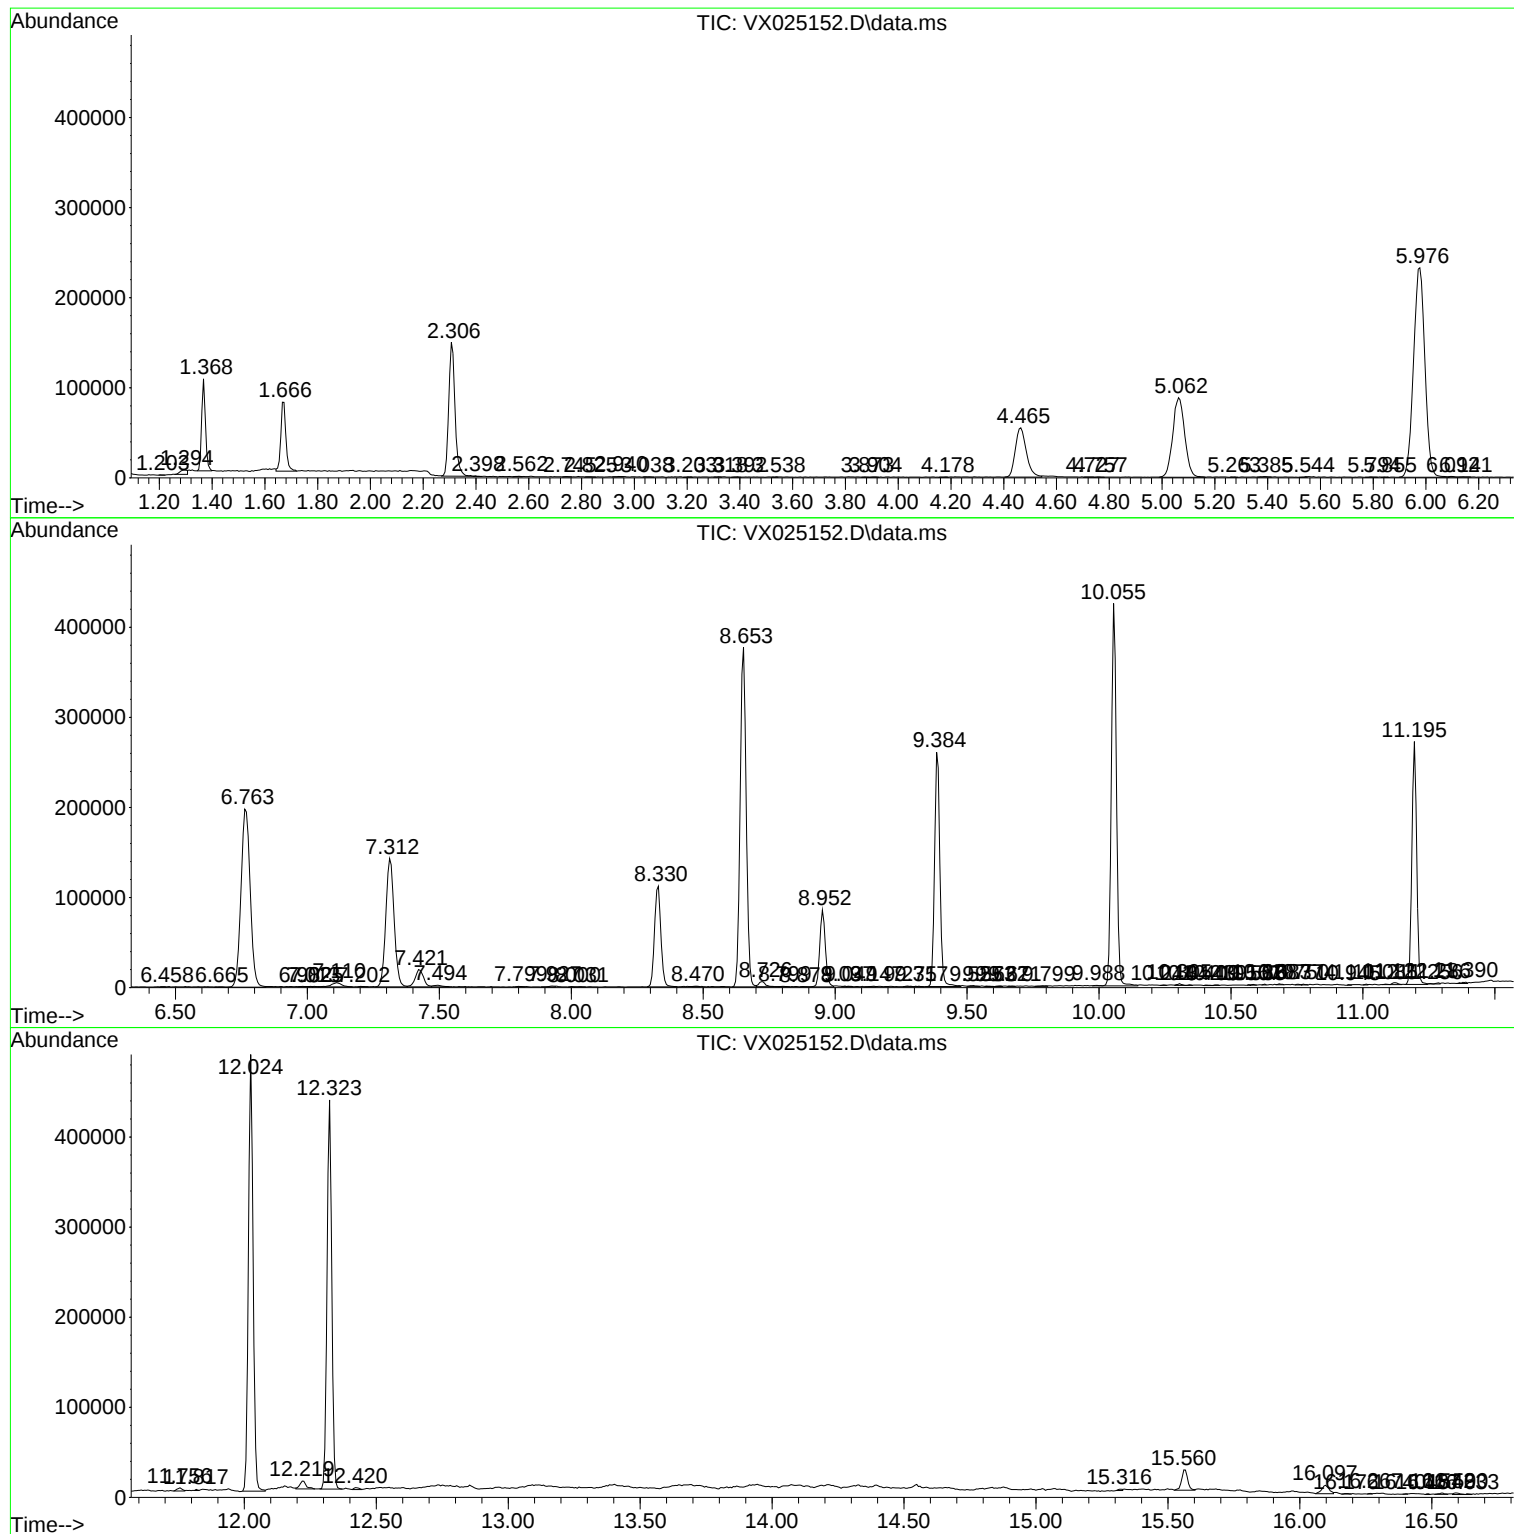

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
Data File : VX025152.D
Acq On : 12 Nov 2021 14:22
Operator : JC/MD
Sample : M4672-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A42A7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
Data File : VX025152.D
Acq On : 12 Nov 2021 14:22
Operator : JC/MD
Sample : M4672-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A42A7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
