

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
 Data File : VX025156.D
 Acq On : 12 Nov 2021 16:21
 Operator : JC/MD
 Sample : M4672-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM11121WMA.M
 Title : VOC Analysis

Signal : TIC: VX025156.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rBV	104754	102770	14.57%	1.753%
2	1.672	92	96	104	rVB	79319	100898	14.30%	1.721%
3	2.306	194	200	213	rVB	150788	241586	34.24%	4.121%
4	2.666	257	259	261	rBV	329	239	0.03%	0.004%
5	2.733	268	270	272	rVB3	401	225	0.03%	0.004%
6	2.794	276	280	284	rVV6	1018	1718	0.24%	0.029%
7	2.843	286	288	289	rBV	489	242	0.03%	0.004%
8	2.861	289	291	294	rVV3	348	303	0.04%	0.005%
9	2.886	294	295	297	rVB2	315	199	0.03%	0.003%
10	3.081	325	327	330	rBV2	257	217	0.03%	0.004%
11	3.209	346	348	353	rVB4	355	560	0.08%	0.010%
12	3.251	353	355	357	rBV3	299	386	0.05%	0.007%
13	3.489	392	394	397	rVV4	185	190	0.03%	0.003%
14	3.556	404	405	406	rBV	477	198	0.03%	0.003%
15	3.581	406	409	412	rVV4	254	386	0.05%	0.007%
16	3.776	439	441	443	rVB2	239	238	0.03%	0.004%
17	4.020	478	481	484	rBV3	485	571	0.08%	0.010%
18	4.276	521	523	524	rBV2	351	262	0.04%	0.004%
19	4.330	529	532	534	rBV2	257	315	0.04%	0.005%
20	4.458	543	553	568	rBV	55317	158039	22.40%	2.696%
21	4.708	590	594	597	rVV5	311	455	0.06%	0.008%
22	4.739	597	599	601	rVB	272	194	0.03%	0.003%
23	4.891	623	624	628	rVB	241	258	0.04%	0.004%
24	5.062	637	652	666	rBV	89809	279394	39.60%	4.766%
25	5.312	691	693	695	rVB3	322	253	0.04%	0.004%
26	5.422	708	711	712	rBV2	260	267	0.04%	0.005%
27	5.970	788	801	815	rBV2	236680	705486	100.00%	12.036%
28	6.239	843	845	848	rVB2	334	282	0.04%	0.005%
29	6.306	853	856	859	rBV3	233	414	0.06%	0.007%
30	6.446	876	879	881	rBV4	336	403	0.06%	0.007%
31	6.513	886	890	892	rBV3	209	232	0.03%	0.004%
32	6.543	892	895	896	rBV2	373	384	0.05%	0.007%
33	6.641	910	911	916	rBV4	341	421	0.06%	0.007%
34	6.763	921	931	945	rBV	198422	464648	65.86%	7.927%
35	7.110	981	988	996	rBV4	3318	7807	1.11%	0.133%
36	7.312	1011	1021	1032	rBV	142531	318036	45.08%	5.426%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
 Data File : VX025156.D
 Acq On : 12 Nov 2021 16:21
 Operator : JC/MD
 Sample : M4672-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM11121WMA.M
 Title : VOC Analysis

37	7.421	1033	1039	1046	rVB	7613	15920	2.26%	0.272%
38	7.525	1054	1056	1059	rVB3	481	428	0.06%	0.007%
39	7.665	1077	1079	1082	rVB3	260	243	0.03%	0.004%
40	7.696	1082	1084	1087	rBV4	299	348	0.05%	0.006%
41	7.927	1116	1122	1127	rBV4	1027	2479	0.35%	0.042%
42	8.031	1135	1139	1142	rVV4	249	337	0.05%	0.006%
43	8.092	1147	1149	1151	rBV3	244	202	0.03%	0.003%
44	8.269	1176	1178	1180	rBV2	213	210	0.03%	0.004%
45	8.324	1180	1187	1200	rVV	114557	187123	26.52%	3.192%
46	8.421	1201	1203	1204	rVB2	537	290	0.04%	0.005%
47	8.470	1204	1211	1218	rBV5	710	2034	0.29%	0.035%
48	8.653	1234	1241	1248	rBV	381424	606567	85.98%	10.348%
49	8.720	1248	1252	1261	rVB	5769	10081	1.43%	0.172%
50	8.854	1272	1274	1275	rVB2	345	202	0.03%	0.003%
51	8.872	1275	1277	1278	rBV2	333	235	0.03%	0.004%
52	8.952	1282	1290	1298	rBV	84432	124570	17.66%	2.125%
53	9.116	1314	1317	1322	rVB3	303	442	0.06%	0.008%
54	9.202	1329	1331	1335	rBV2	311	451	0.06%	0.008%
55	9.293	1343	1346	1347	rBV3	253	265	0.04%	0.005%
56	9.336	1350	1353	1355	rBV3	214	293	0.04%	0.005%
57	9.384	1355	1361	1369	rBV	267578	359503	50.96%	6.133%
58	9.580	1391	1393	1396	rVB3	355	433	0.06%	0.007%
59	9.610	1396	1398	1401	rVB2	269	230	0.03%	0.004%
60	9.653	1401	1405	1409	rVB3	416	761	0.11%	0.013%
61	9.701	1409	1413	1417	rBV4	467	985	0.14%	0.017%
62	9.762	1422	1423	1424	rBV	358	189	0.03%	0.003%
63	9.903	1444	1446	1450	rVB4	219	288	0.04%	0.005%
64	9.970	1455	1457	1458	rBV2	248	222	0.03%	0.004%
65	10.006	1460	1463	1465	rBV3	452	552	0.08%	0.009%
66	10.055	1465	1471	1483	rVV	418827	556508	78.88%	9.494%
67	10.201	1490	1495	1499	rBV4	502	1021	0.14%	0.017%
68	10.238	1499	1501	1504	rBV4	391	251	0.04%	0.004%
69	10.305	1509	1512	1514	rVV	1258	1573	0.22%	0.027%
70	10.360	1517	1521	1525	rBV3	2090	2787	0.40%	0.048%
71	10.476	1538	1540	1546	rVB3	464	449	0.06%	0.008%
72	10.543	1546	1551	1554	rBV4	394	678	0.10%	0.012%
73	10.579	1554	1557	1561	rBV3	624	1011	0.14%	0.017%
74	10.653	1566	1569	1571	rBV3	464	686	0.10%	0.012%
75	10.750	1583	1585	1587	rBV2	417	530	0.08%	0.009%
76	10.781	1588	1590	1595	rVB3	1747	2062	0.29%	0.035%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
 Data File : VX025156.D
 Acq On : 12 Nov 2021 16:21
 Operator : JC/MD
 Sample : M4672-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM11121WMA.M
 Title : VOC Analysis

77	10.951	1613	1618	1620	rBV4	647	1033	0.15%	0.018%
78	11.030	1628	1631	1635	rBV4	1287	1512	0.21%	0.026%
79	11.085	1638	1640	1642	rBV	1703	1511	0.21%	0.026%
80	11.195	1652	1658	1666	rBV	275153	350030	49.62%	5.972%
81	11.390	1689	1690	1692	rVB	603	242	0.03%	0.004%
82	11.433	1694	1697	1700	rBV4	2104	3114	0.44%	0.053%
83	11.476	1701	1704	1712	rVB	18824	23840	3.38%	0.407%
84	11.549	1712	1716	1717	rBV3	664	687	0.10%	0.012%
85	11.713	1740	1743	1747	rBV	5831	6734	0.95%	0.115%
86	11.750	1747	1749	1752	rVB2	2501	2549	0.36%	0.043%
87	12.024	1789	1794	1800	rBV	488818	596474	84.55%	10.176%
88	12.103	1805	1807	1812	rVB3	2919	3269	0.46%	0.056%
89	12.323	1837	1843	1850	rBV	451321	568827	80.63%	9.704%
90	12.427	1856	1860	1864	rVB	19560	21907	3.11%	0.374%
91	12.542	1875	1879	1883	rBV4	1367	3213	0.46%	0.055%
92	13.268	1995	1998	2003	rVB5	1678	2044	0.29%	0.035%
93	13.372	2013	2015	2016	rBV2	418	230	0.03%	0.004%
94	13.628	2055	2057	2059	rBV3	281	214	0.03%	0.004%
95	13.774	2080	2081	2082	rBV	506	285	0.04%	0.005%
96	14.012	2118	2120	2121	rBV2	325	258	0.04%	0.004%
97	14.054	2126	2127	2129	rBV2	553	337	0.05%	0.006%
98	14.127	2136	2139	2142	rBV3	508	677	0.10%	0.012%
99	14.993	2279	2281	2283	rBV3	496	521	0.07%	0.009%
100	16.133	2466	2468	2469	rBV	415	208	0.03%	0.004%




Sum of corrected areas: 5861631

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
Data File : VX025156.D
Acq On : 12 Nov 2021 16:21
Operator : JC/MD
Sample : M4672-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

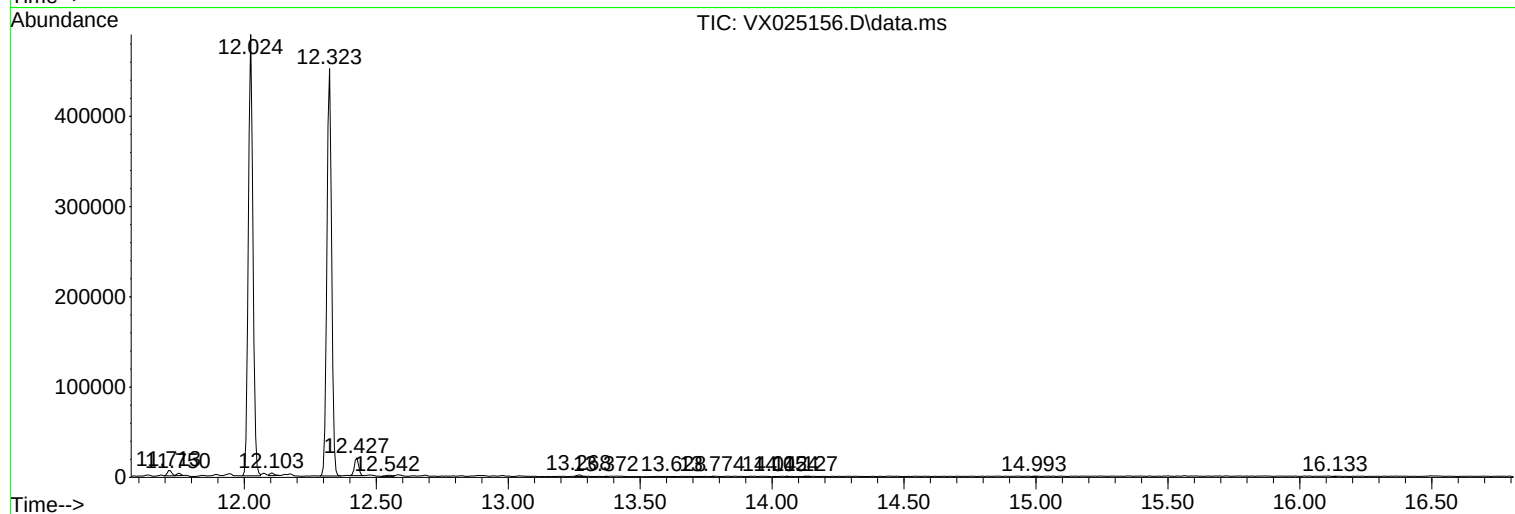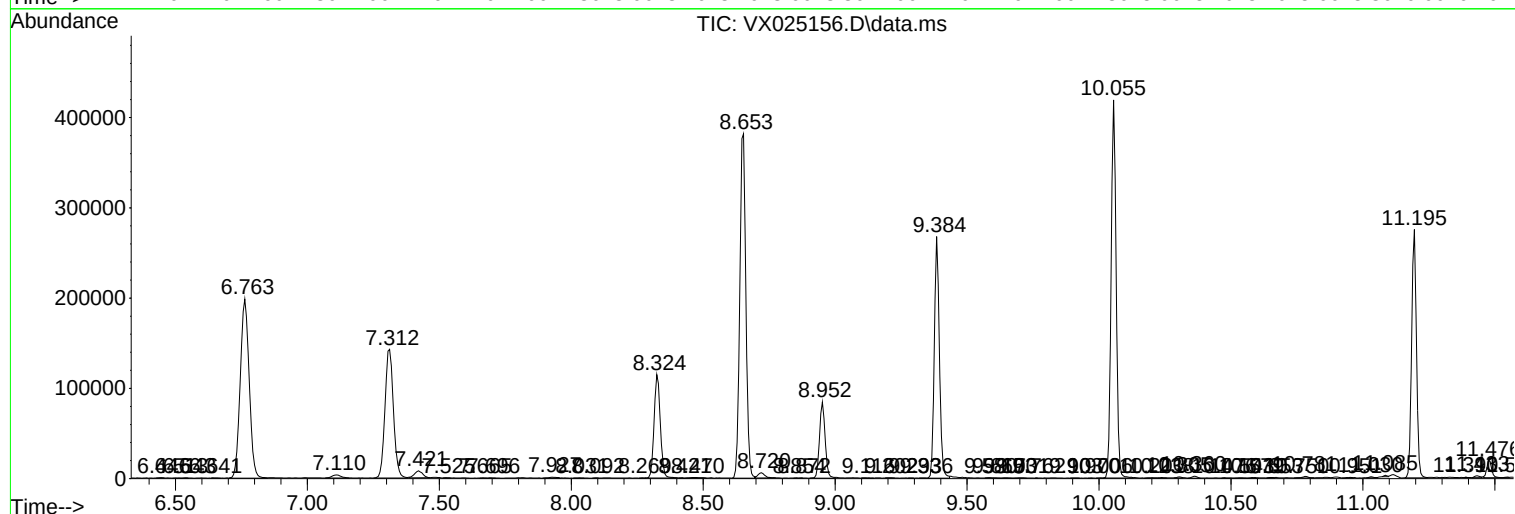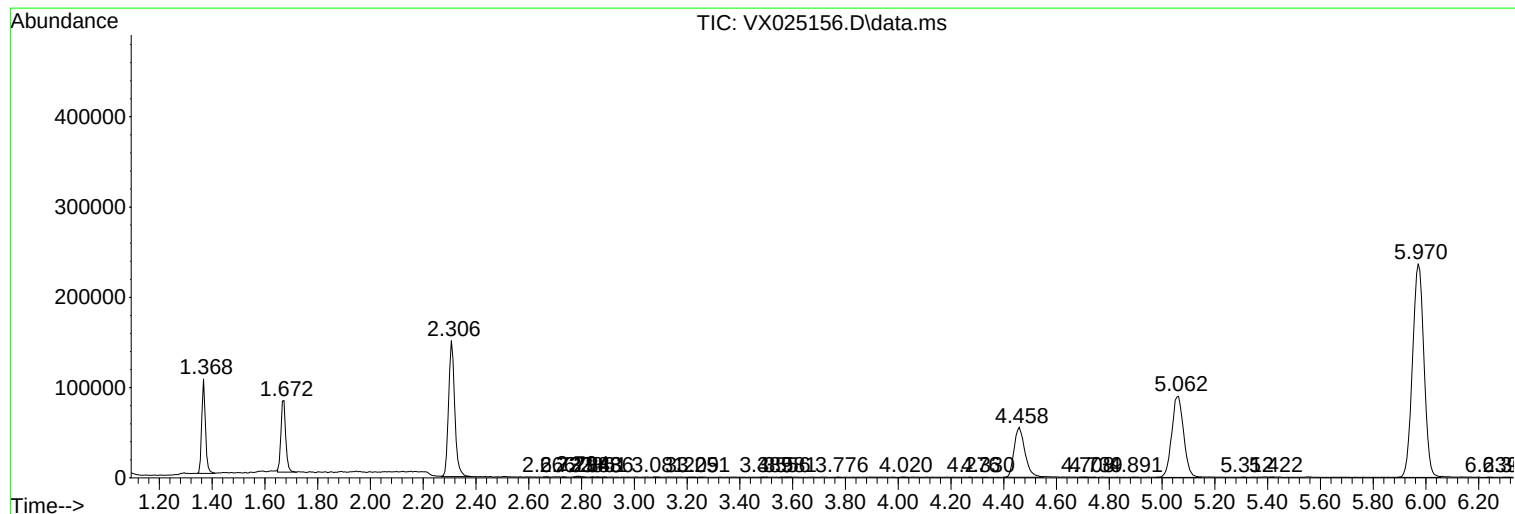

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
Data File : VX025156.D
Acq On : 12 Nov 2021 16:21
Operator : JC/MD
Sample : M4672-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
Data File : VX025156.D
Acq On : 12 Nov 2021 16:21
Operator : JC/MD
Sample : M4672-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
