
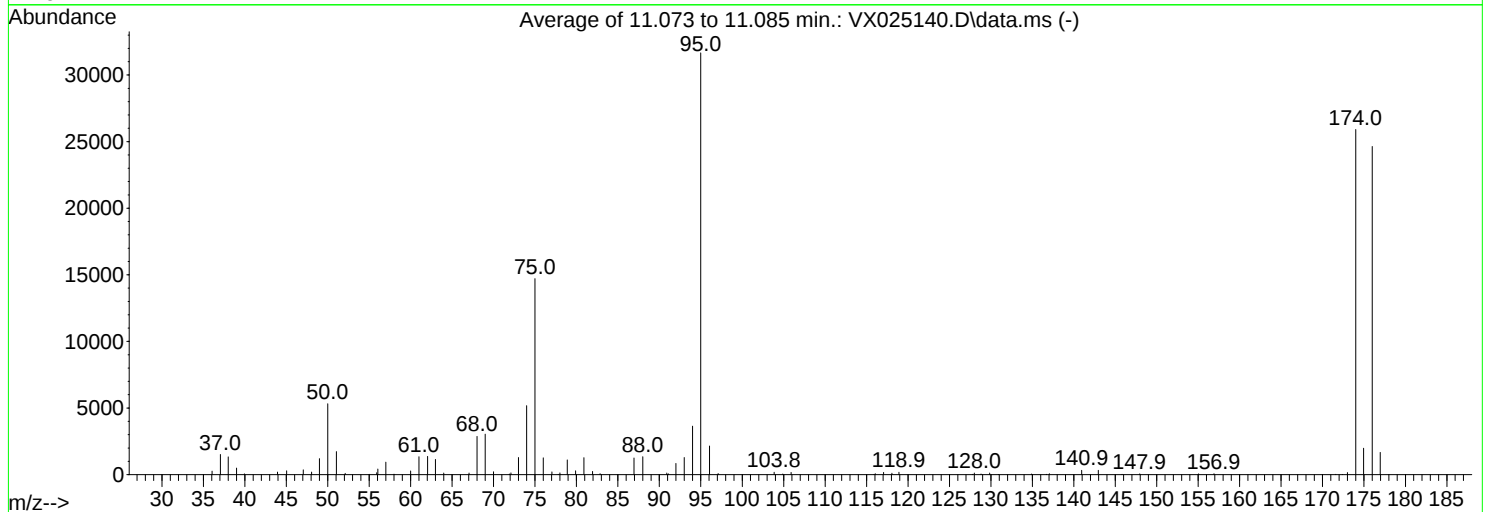


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111221\
Data File : VX025140.D
Acq On : 12 Nov 2021 08:44
Operator : JC/MD
Sample : BFB614
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB614

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Title : VOC Analysis
Last Update : Fri Nov 12 12:01:23 2021

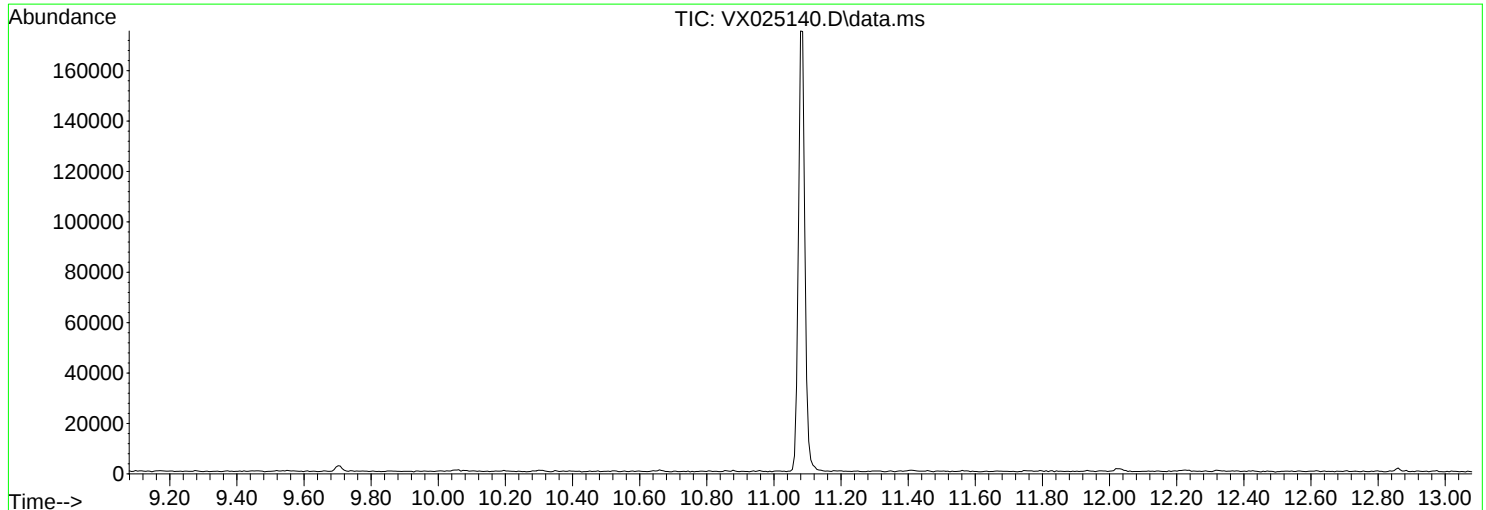

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	5317	PASS
75	95	30	80	46.5	14716	PASS
95	95	100	100	100.0	31664	PASS
96	95	5	9	6.8	2148	PASS
173	174	0.00	2	0.6	162	PASS
174	95	50	120	81.8	25913	PASS
175	174	5	9	7.7	1985	PASS
176	174	95	101	95.1	24639	PASS
177	176	5	9	6.8	1669	PASS

m/z	Abundance
39.00	67.0
40.00	226.0
41.00	171.0
42.10	59.0
43.00	124.0
43.90	270.0
55.00	129.0
70.00	51.0

Instrument :
MSVOA_X
ClientSampleId :
BFB614

m/z	Abundance
36.00	202.0
37.10	1136.0
38.00	1010.0
39.10	508.0
40.00	287.0
41.10	128.0
43.10	84.0
44.10	446.0
45.10	252.0
47.10	289.0
48.00	130.0
49.00	929.0
50.00	4083.0
51.00	1359.0
52.10	69.0
55.00	92.0
55.90	435.0
57.00	669.0
60.00	165.0
61.00	903.0
62.00	1140.0
63.00	826.0
64.00	117.0
67.00	126.0
68.00	2092.0
69.00	2326.0
70.10	216.0
71.90	137.0
73.00	874.0
74.00	3898.0
75.00	11081.0
76.00	920.0
77.20	139.0
77.80	86.0
78.90	744.0
79.90	240.0
80.90	854.0
81.90	172.0
82.80	75.0
86.90	863.0
88.00	1064.0
90.90	152.0
92.00	666.0
93.00	911.0
94.00	2310.0
95.00	21944.0
96.00	1663.0
97.20	88.0
103.90	102.0
105.80	123.0
115.90	90.0
117.00	115.0
118.10	82.0
118.80	108.0
127.80	74.0
129.90	97.0
137.10	64.0
140.90	185.0
143.00	235.0
147.90	52.0
156.80	67.0
172.40	51.0
174.00	15522.0
174.90	1185.0
176.00	14374.0
176.90	1018.0
178.00	55.0

Instrument :
MSVOA_X
ClientSampleId :
BFB614

m/z	Abundance
36.10	332.0
37.00	1782.0
38.00	1640.0
39.00	565.0
39.90	252.0
41.10	126.0
43.10	117.0
44.00	483.0
45.00	353.0
47.00	422.0
48.00	238.0
49.00	1440.0
50.00	6228.0
51.00	2073.0
52.10	121.0
55.10	176.0
56.10	658.0
57.00	1133.0
58.00	58.0
60.00	335.0
61.00	1659.0
62.10	1613.0
63.00	1313.0
63.90	112.0
67.00	98.0
68.00	3400.0
69.00	3695.0
70.00	274.0
72.10	227.0
73.00	1513.0
74.00	6013.0
75.00	17168.0
76.00	1573.0
77.00	293.0
78.00	211.0
78.90	1384.0
79.90	357.0
80.90	1400.0
82.00	340.0
82.80	73.0
87.00	1554.0
88.00	1512.0
90.90	228.0
92.00	951.0
93.00	1527.0
94.00	4562.0
95.00	36904.0
96.00	2517.0
97.10	84.0
103.90	189.0
104.90	66.0
105.90	175.0
116.10	135.0
117.10	222.0
118.00	134.0
118.90	220.0
128.00	164.0
128.80	66.0
129.90	148.0
135.00	84.0
136.70	76.0
137.10	88.0
141.00	312.0
142.90	345.0
148.00	78.0
155.00	83.0
156.90	61.0
171.60	64.0
173.00	221.0
174.00	29152.0
174.90	2335.0
176.00	28352.0
177.00	1875.0

Instrument :
MSVOA_X
ClientSampleId :
BFB614

m/z	Abundance
36.00	253.0
37.00	1620.0
38.00	1364.0
39.10	623.0
40.00	309.0
41.10	113.0
42.10	53.0
43.10	124.0
44.00	450.0
45.00	268.0
47.00	369.0
48.10	203.0
49.00	1232.0
50.00	5639.0
51.10	1748.0
52.10	104.0
55.10	209.0
56.00	596.0
57.00	1007.0
58.00	66.0
60.00	345.0
61.00	1475.0
62.00	1367.0
63.00	1280.0
64.10	142.0
67.10	144.0
68.00	3133.0
69.00	3086.0
70.00	305.0
72.10	183.0
73.00	1470.0
74.00	5618.0
75.00	15900.0
76.00	1283.0
77.00	176.0
78.00	175.0
78.90	1192.0
79.90	284.0
80.90	1569.0
82.00	224.0
82.90	90.0
87.00	1332.0
88.00	1452.0
91.10	189.0
92.00	919.0
93.00	1401.0
94.00	4030.0
95.00	36144.0
96.10	2265.0
97.00	86.0
103.80	245.0
104.90	76.0
106.00	216.0
116.00	93.0
117.00	167.0
118.00	119.0
119.00	203.0
128.00	207.0
128.80	67.0
129.80	114.0
130.90	58.0
134.80	54.0
137.00	65.0
140.90	492.0
142.90	390.0
145.80	61.0
148.00	64.0
155.10	98.0
157.00	79.0
173.00	266.0
174.00	33064.0
175.00	2435.0
176.00	31192.0
176.90	2115.0

Instrument :
MSVOA_X
ClientSampleId :
BFB614