

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043804.D
 Acq On : 12 Nov 2024 12:42
 Operator : JC/MD
 Sample : VX1112MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 13 02:05:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 13 02:04:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	257500	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	223207	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	96465	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	59886	43.655	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.320%
7) Chloroethane-d5	1.642	69	36937	62.642	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	125.280%
11) 1,1-Dichloroethene-d2	2.294	65	27980	44.183	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.360%
21) 2-Butanone-d5	4.464	46	90801	101.094	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.090%
24) Chloroform-d	5.050	84	140251	47.426	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.860%
26) 1,2-Dichloroethane-d4	5.952	65	92288	49.124	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.240%
32) Benzene-d6	5.964	84	293485	50.857	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.720%
36) 1,2-Dichloropropane-d6	7.305	67	88153	50.210	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.420%
41) Toluene-d8	8.647	98	258104	49.235	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.480%
43) trans-1,3-Dichloroprop...	8.951	79	37596	44.777	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.560%
47) 2-Hexanone-d5	9.384	63	73476	105.748	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	105.750%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	125651	55.779	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	111.560%
66) 1,2-Dichlorobenzene-d4	12.317	152	100786	60.302	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	120.600%#
Target Compounds						
					Qvalue	
61) 1,2,3-Trichloropropane	12.018	75	10334	5.519	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043804.D
Acq On : 12 Nov 2024 12:42
Operator : JC/MD
Sample : VX1112MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Nov 13 02:05:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 13 02:04:29 2024
Response via : Initial Calibration

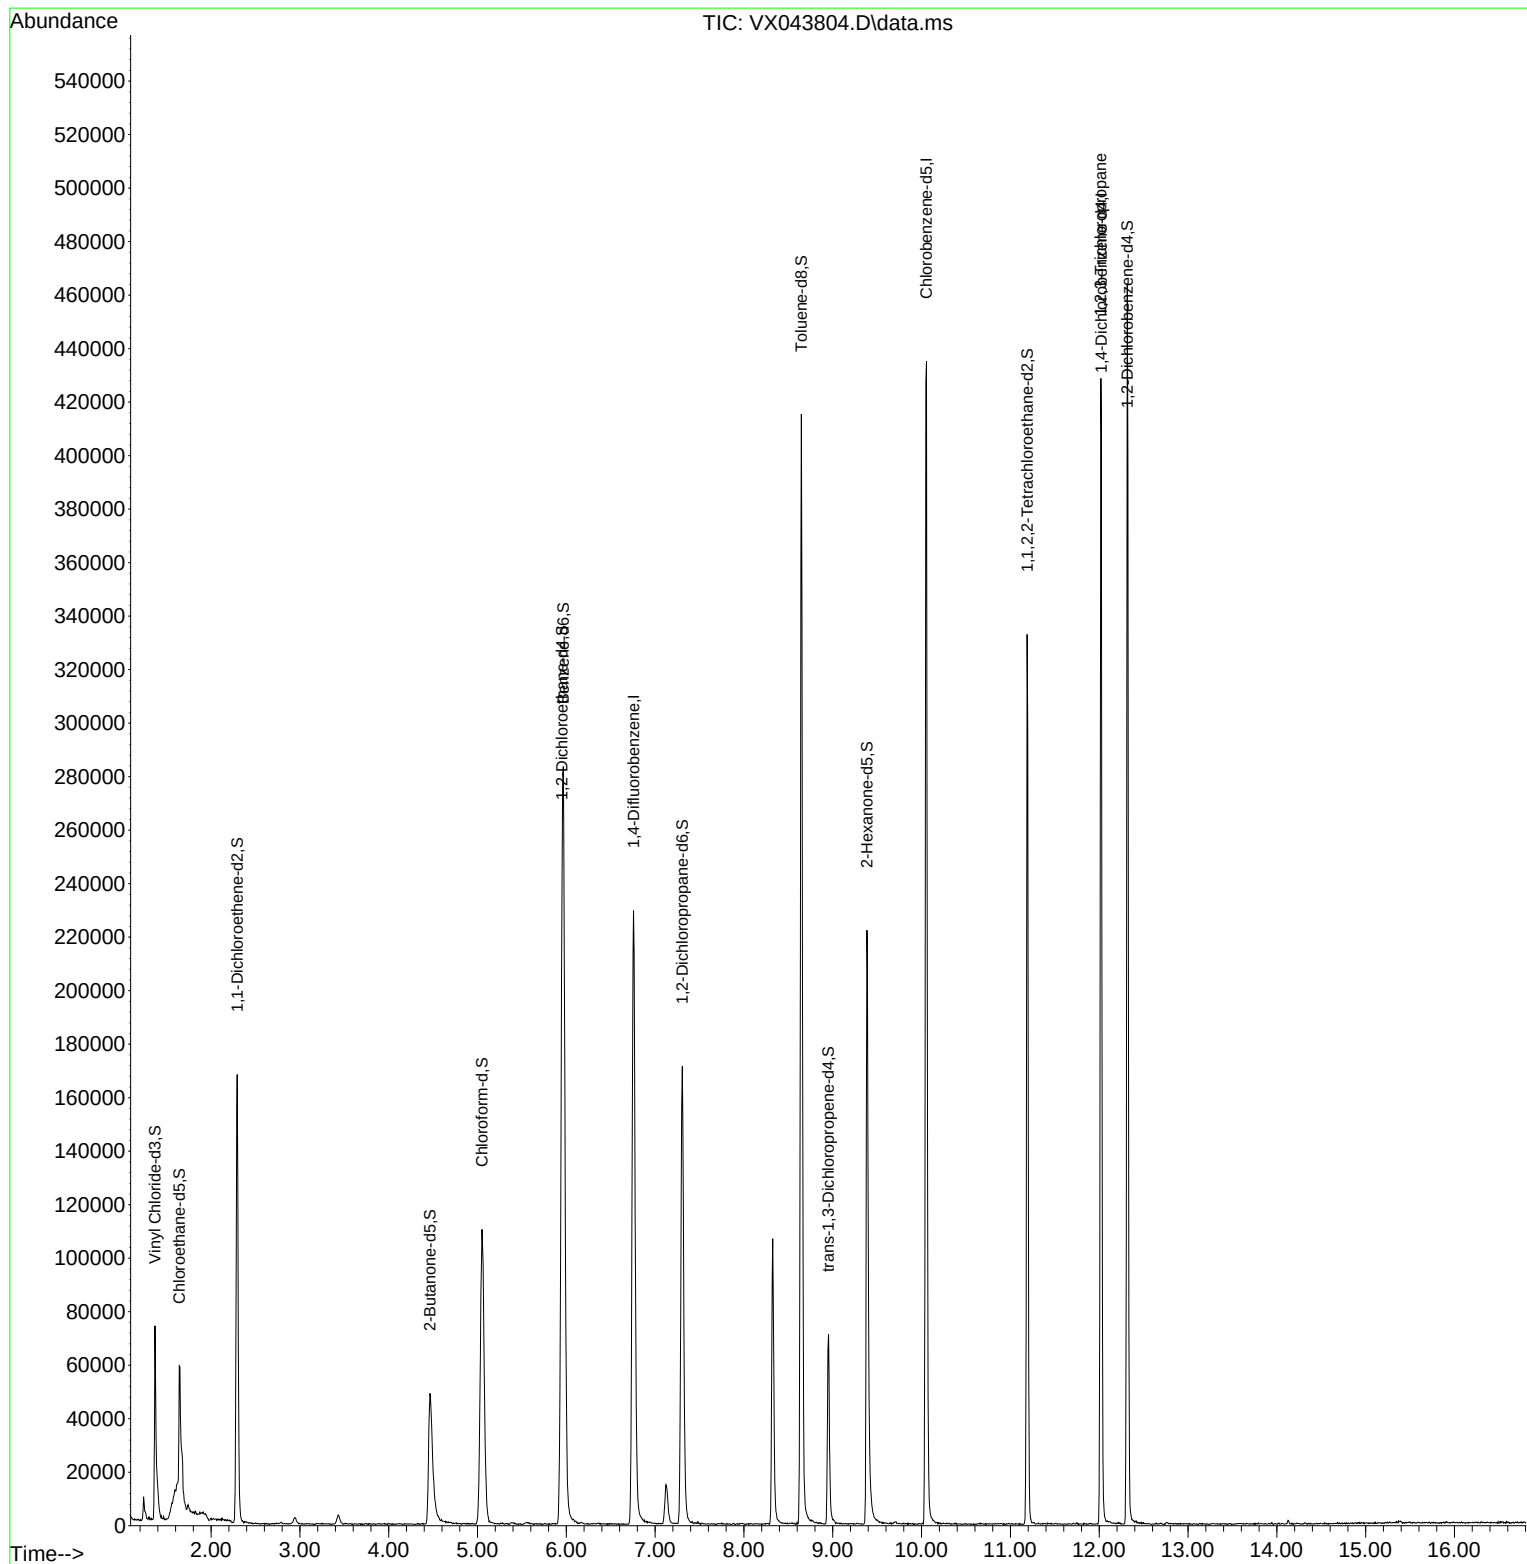

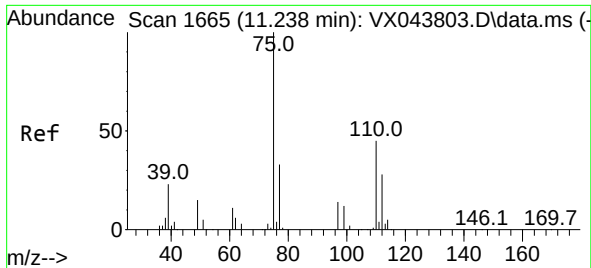

#61
 1,2,3-Trichloropropane
 Concen: 5.519 ug/L
 RT: 12.018 min Scan# 11
 Delta R.T. 0.780 min
 Lab File: VX043804.D
 Acq: 12 Nov 2024 12:42

Instrument :
 MSVOA_X
 ClientSampleId :

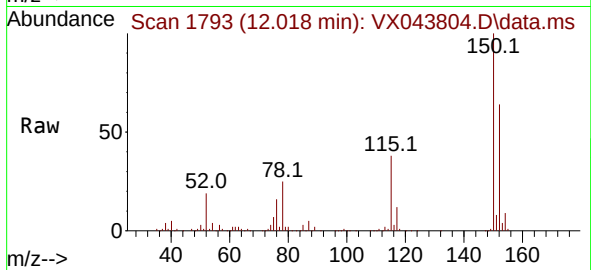

Tgt Ion: 75 Resp: 10334
 Ion Ratio Lower Upper
 75 100
 77 30.5 25.4 38.0
 110 2.7 33.6 50.4#

