

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043809.D
 Acq On : 12 Nov 2024 14:45
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 13 02:06:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 13 02:04:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	214273	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	192898	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	85251	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	45200	39.597	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 79.200%			
7) Chloroethane-d5	1.642	69	29021	59.146	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 118.300%			
11) 1,1-Dichloroethene-d2	2.294	65	22818	43.301	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 86.600%			
21) 2-Butanone-d5	4.459	46	90106	120.558	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 120.560%			
24) Chloroform-d	5.050	84	124412	50.557	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 101.120%			
26) 1,2-Dichloroethane-d4	5.952	65	87123	55.731	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 111.460%			
32) Benzene-d6	5.964	84	245897	49.306	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 98.620%			
36) 1,2-Dichloropropane-d6	7.299	67	78019	51.420	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 102.840%			
41) Toluene-d8	8.647	98	216714	47.835	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 95.680%			
43) trans-1,3-Dichloroprop...	8.946	79	33378	45.999	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 92.000%			
47) 2-Hexanone-d5	9.384	63	71725	119.448	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 119.450%			
56) 1,1,2,2-Tetrachloroeth...	11.189	84	120429	61.861	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 123.720%#			
66) 1,2-Dichlorobenzene-d4	12.317	152	88254	59.749	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 119.500%			
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	12.018	75	9040	5.463	ug/L	# 64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043809.D
Acq On : 12 Nov 2024 14:45
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 13 02:06:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 13 02:04:29 2024
Response via : Initial Calibration

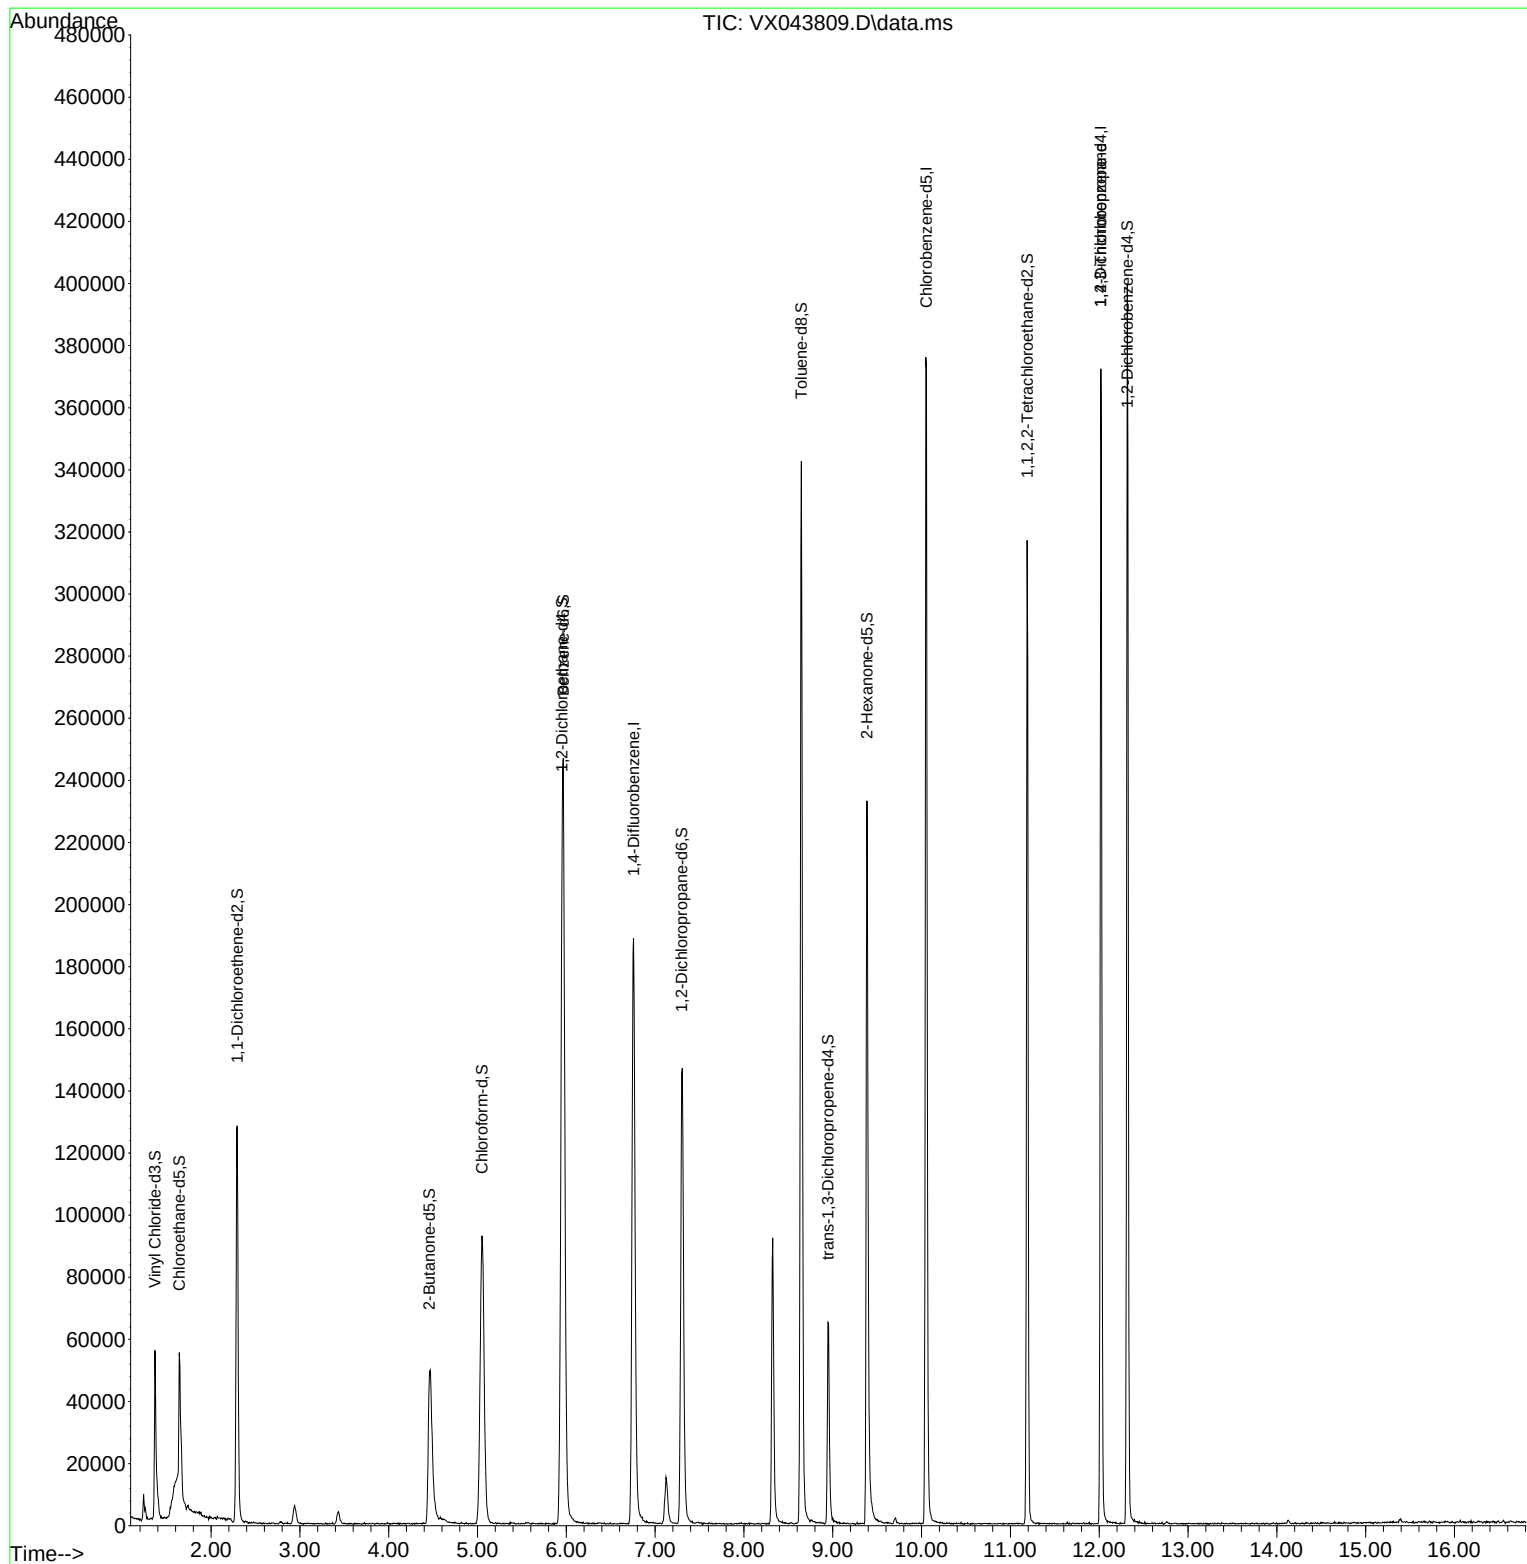

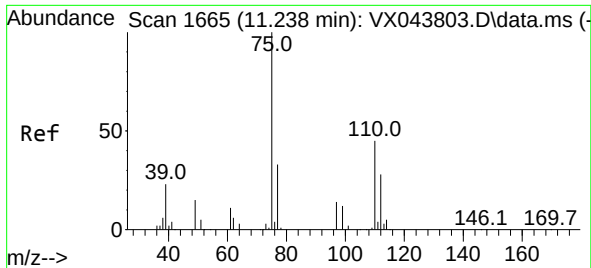

#61

1,2,3-Trichloropropane

Concen: 5.463 ug/L

RT: 12.018 min Scan# 11

Delta R.T. 0.780 min


Lab File: VX043809.D

Acq: 12 Nov 2024 14:45

Instrument :

MSVOA_X

ClientSampleId :

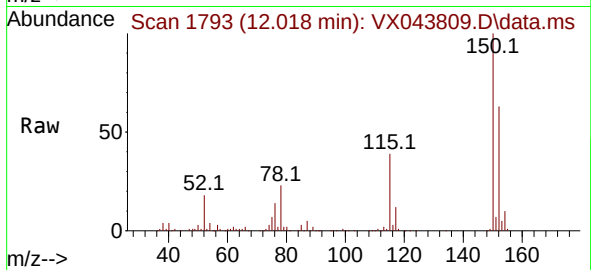

Tgt Ion: 75 Resp: 9040

Ion Ratio Lower Upper

75 100

77 31.1 25.4 38.0

110 2.1 33.6 50.4#

