

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX111224\  
 Data File : VX043816.D  
 Acq On : 12 Nov 2024 17:27  
 Operator : JC/MD  
 Sample : P4786-18  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :

Quant Time: Nov 13 02:08:24 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXLM110424WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Wed Nov 13 02:04:29 2024  
 Response via : Initial Calibration


| Compound                      | R.T.    | QIon  | Response | Conc     | Units | Dev(Min)    |
|-------------------------------|---------|-------|----------|----------|-------|-------------|
| -----                         |         |       |          |          |       |             |
| Internal Standards            |         |       |          |          |       |             |
| 1) 1,4-Difluorobenzene        | 6.757   | 114   | 293617   | 50.000   | ug/L  | 0.00        |
| 28) Chlorobenzene-d5          | 10.055  | 117   | 256658   | 50.000   | ug/L  | 0.00        |
| 58) 1,4-Dichlorobenzene-d4    | 12.018  | 152   | 112950   | 50.000   | ug/L  | 0.00        |
| System Monitoring Compounds   |         |       |          |          |       |             |
| 4) Vinyl Chloride-d3          | 1.368   | 65    | 50239    | 32.118   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 60 - 135 | Recovery | =     | 64.240%     |
| 7) Chloroethane-d5            | 1.642   | 69    | 33052    | 49.158   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 70 - 130 | Recovery | =     | 98.320%     |
| 11) 1,1-Dichloroethene-d2     | 2.294   | 65    | 25424    | 35.209   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 60 - 125 | Recovery | =     | 70.420%     |
| 21) 2-Butanone-d5             | 4.465   | 46    | 76980    | 75.164   | ug/L  | 0.00        |
| Spiked Amount                 | 100.000 | Range | 40 - 130 | Recovery | =     | 75.160%     |
| 24) Chloroform-d              | 5.050   | 84    | 131329   | 38.946   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 70 - 125 | Recovery | =     | 77.900%     |
| 26) 1,2-Dichloroethane-d4     | 5.952   | 65    | 83967    | 39.197   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 70 - 125 | Recovery | =     | 78.400%     |
| 32) Benzene-d6                | 5.964   | 84    | 262009   | 39.485   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 70 - 125 | Recovery | =     | 78.980%     |
| 36) 1,2-Dichloropropane-d6    | 7.306   | 67    | 77660    | 38.468   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 70 - 120 | Recovery | =     | 76.940%     |
| 41) Toluene-d8                | 8.647   | 98    | 233297   | 38.703   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 80 - 120 | Recovery | =     | 77.400%#    |
| 43) trans-1,3-Dichloroprop... | 8.952   | 79    | 33390    | 34.584   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 60 - 125 | Recovery | =     | 69.160%     |
| 47) 2-Hexanone-d5             | 9.385   | 63    | 66611    | 83.373   | ug/L  | 0.00        |
| Spiked Amount                 | 100.000 | Range | 45 - 130 | Recovery | =     | 83.370%     |
| 56) 1,1,2,2-Tetrachloroeth... | 11.189  | 84    | 111503   | 43.047   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 65 - 120 | Recovery | =     | 86.100%     |
| 66) 1,2-Dichlorobenzene-d4    | 12.317  | 152   | 92158    | 47.092   | ug/L  | 0.00        |
| Spiked Amount                 | 50.000  | Range | 80 - 120 | Recovery | =     | 94.180%     |
| Target Compounds              |         |       |          |          |       |             |
| 61) 1,2,3-Trichloropropane    | 12.018  | 75    | 12171    | 5.551    | ug/L  | Qvalue # 63 |
| -----                         |         |       |          |          |       |             |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX111224\  
Data File : VX043816.D  
Acq On : 12 Nov 2024 17:27  
Operator : JC/MD  
Sample : P4786-18  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :


Quant Time: Nov 13 02:08:24 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXML110424WMA.M  
Quant Title : VOC Analysis  
QLast Update : Wed Nov 13 02:04:29 2024  
Response via : Initial Calibration

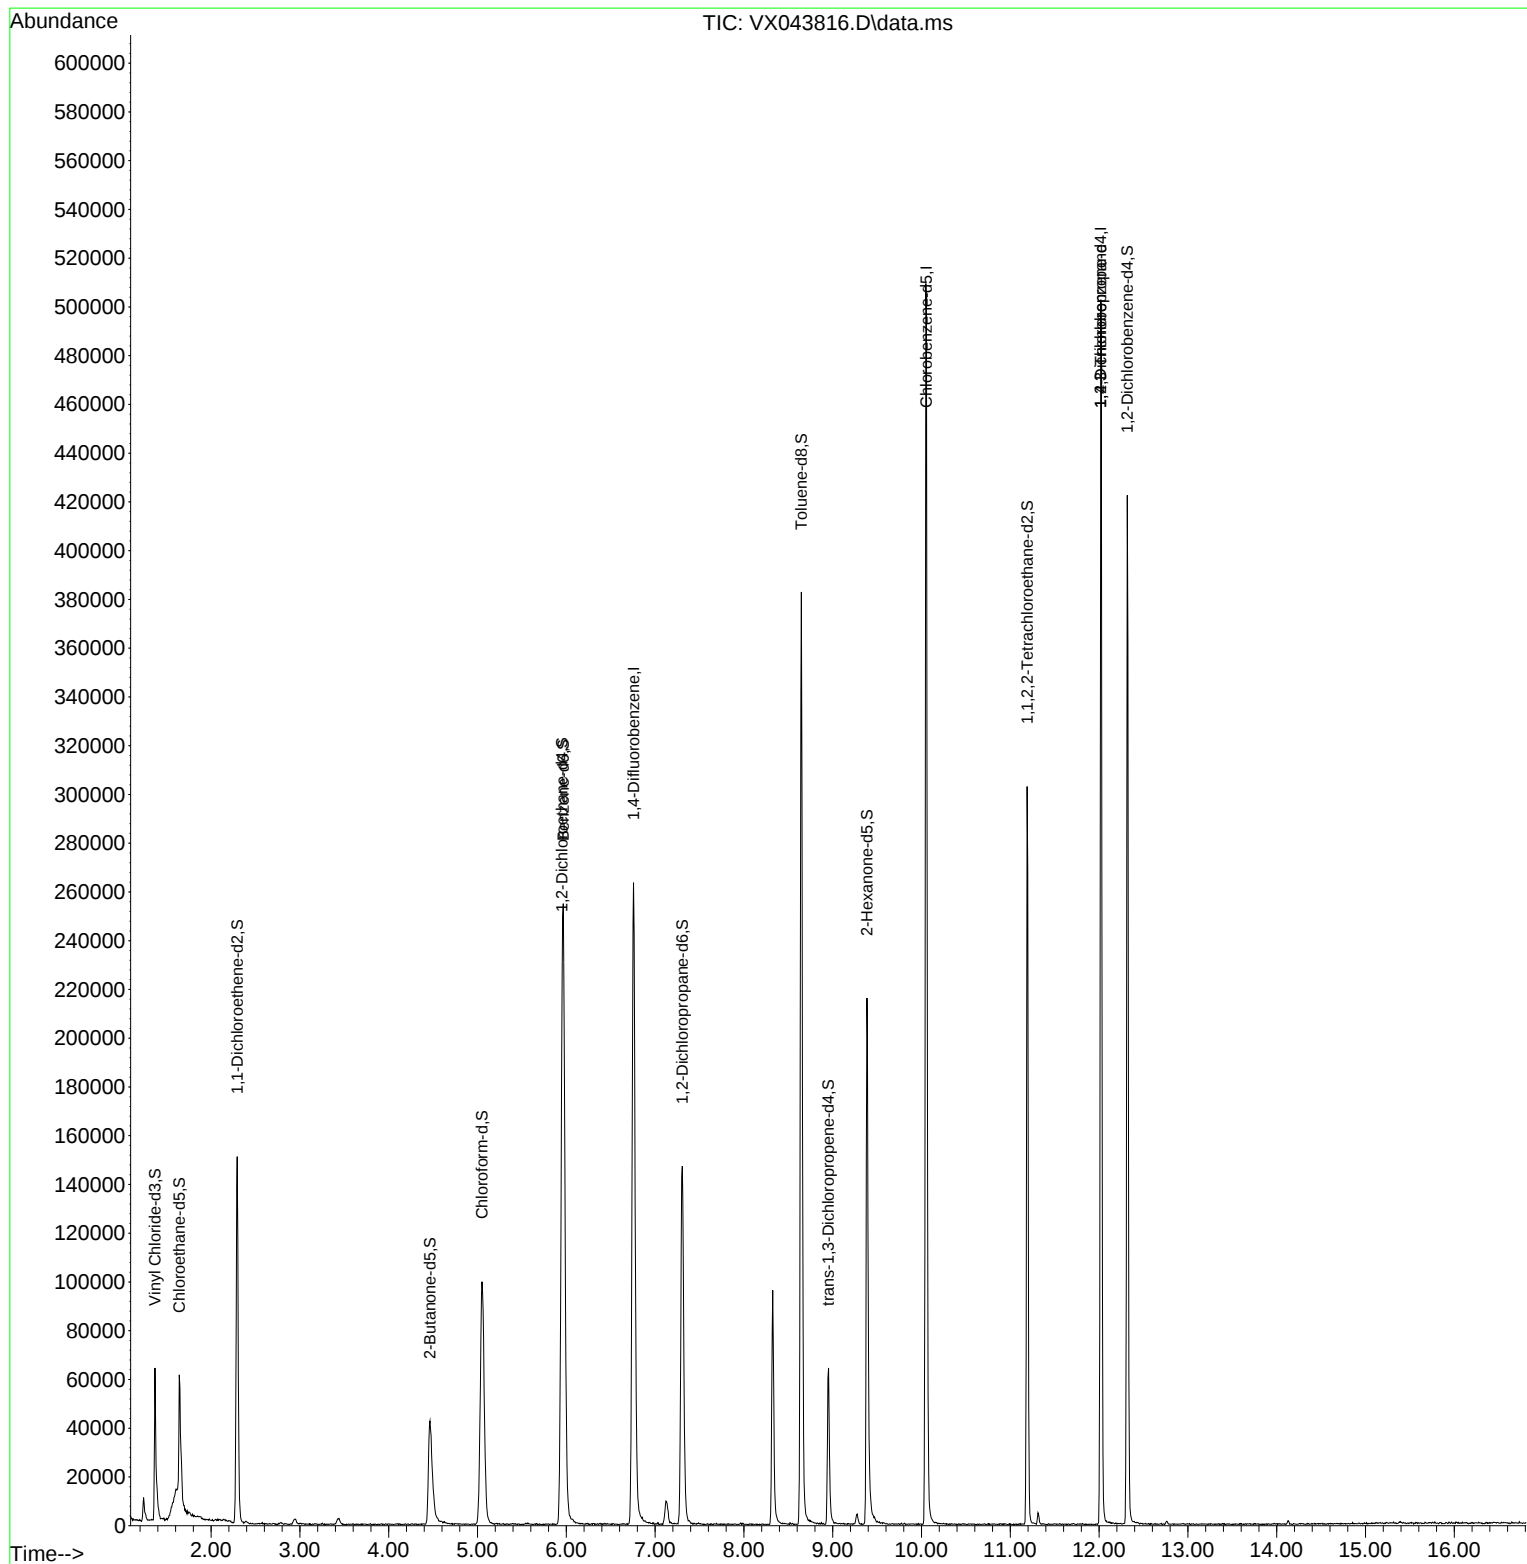

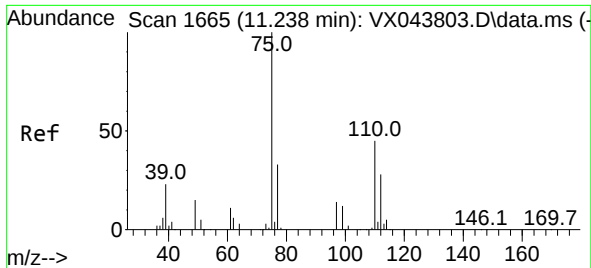

#61  
1,2,3-Trichloropropane  
Concen: 5.551 ug/L  
RT: 12.018 min Scan# 11  
Delta R.T. 0.781 min  
Lab File: VX043816.D  
Acq: 12 Nov 2024 17:27

Instrument :  
MSVOA\_X  
ClientSampleId :

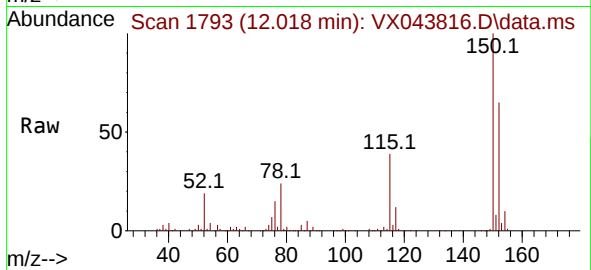

Tgt Ion: 75 Resp: 12171  
Ion Ratio Lower Upper  
75 100  
77 34.8 25.4 38.0  
110 3.4 33.6 50.4#

