

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043823.D
 Acq On : 12 Nov 2024 20:08
 Operator : JC/MD
 Sample : P4785-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 13 02:11:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 13 02:04:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	289789	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.049	117	255444	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	112419	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	47867	31.006	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	62.020%
7) Chloroethane-d5	1.648	69	31692	47.758	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	95.520%
11) 1,1-Dichloroethene-d2	2.294	65	25149	35.288	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.580%
21) 2-Butanone-d5	4.459	46	79961	79.106	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	79.110%
24) Chloroform-d	5.050	84	129211	38.824	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.640%
26) 1,2-Dichloroethane-d4	5.952	65	84501	39.968	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.940%
32) Benzene-d6	5.964	84	256877	38.896	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.800%
36) 1,2-Dichloropropane-d6	7.306	67	78188	38.914	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	77.820%
41) Toluene-d8	8.647	98	229241	38.211	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	76.420%#
43) trans-1,3-Dichloroprop...	8.952	79	33694	35.065	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.140%
47) 2-Hexanone-d5	9.385	63	68782	86.500	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	86.500%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	111644	43.306	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.620%
66) 1,2-Dichlorobenzene-d4	12.317	152	88273	45.320	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.640%
Target Compounds						
					Qvalue	
61) 1,2,3-Trichloropropane	12.018	75	11742	5.381	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043823.D
Acq On : 12 Nov 2024 20:08
Operator : JC/MD
Sample : P4785-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Nov 13 02:11:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 13 02:04:29 2024
Response via : Initial Calibration

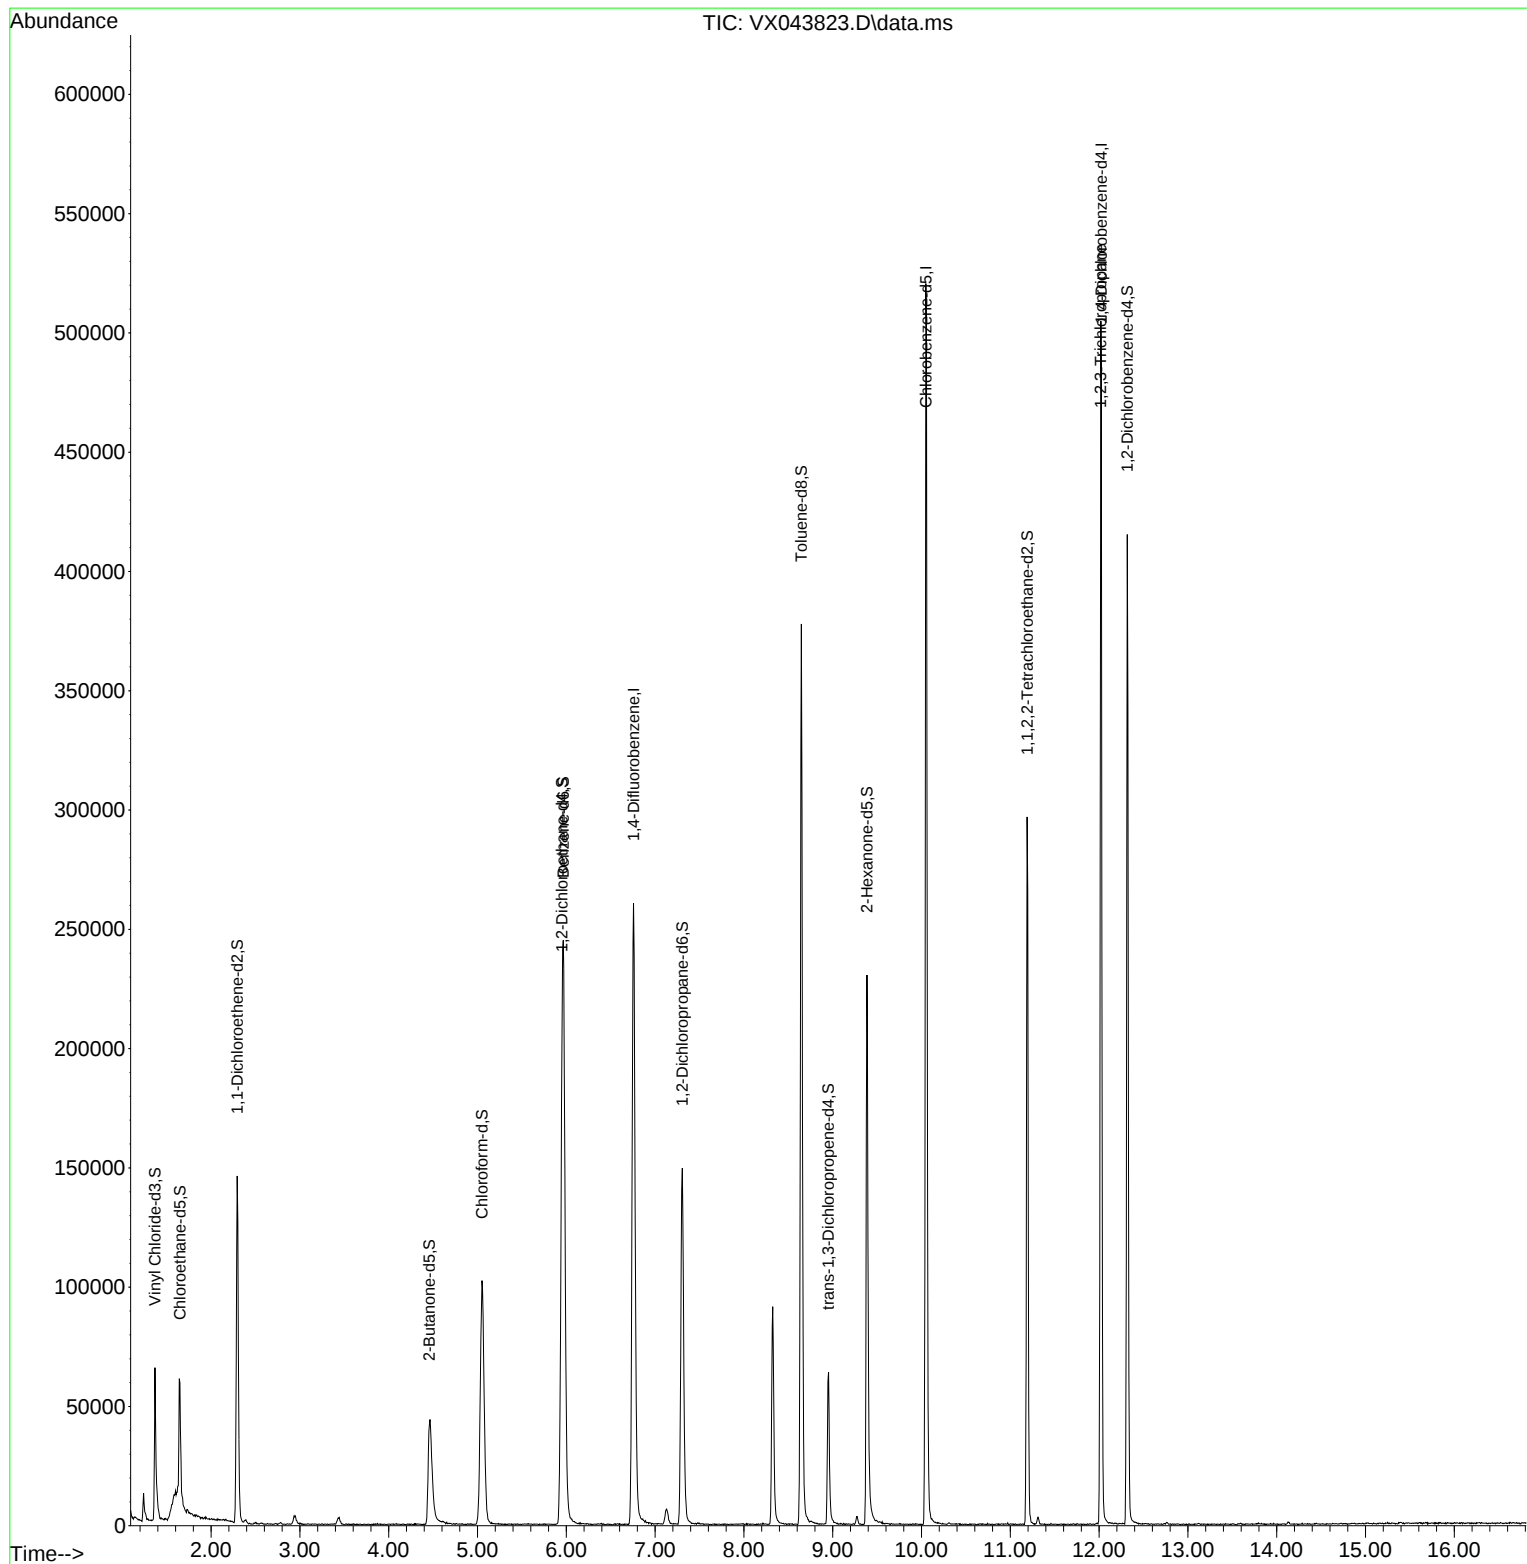

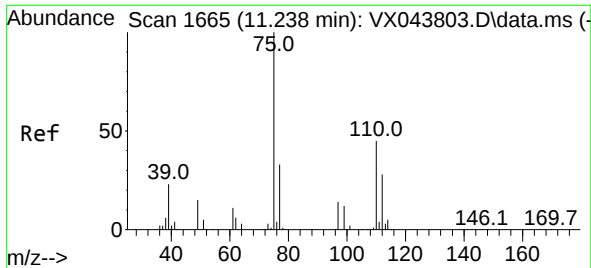

#61
 1,2,3-Trichloropropane
 Concen: 5.381 ug/L
 RT: 12.018 min Scan# 11
 Delta R.T. 0.780 min
 Lab File: VX043823.D
 Acq: 12 Nov 2024 20:08

Instrument :
 MSVOA_X
 ClientSampleId :

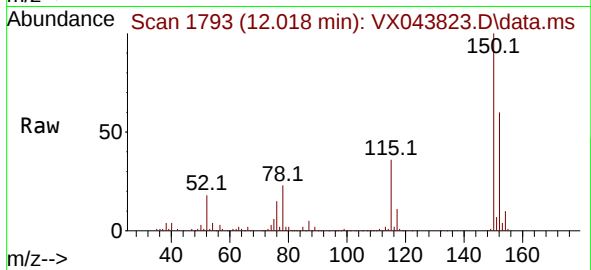

Tgt Ion: 75 Resp: 11742
 Ion Ratio Lower Upper
 75 100
 77 35.5 25.4 38.0
 110 3.7 33.6 50.4#

