

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043824.D
 Acq On : 12 Nov 2024 20:31
 Operator : JC/MD
 Sample : P4785-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 13 02:11:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 13 02:04:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	286845	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	251495	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	111509	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	46615	30.505	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	61.000%
7) Chloroethane-d5	1.648	69	32605	49.638	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	99.280%
11) 1,1-Dichloroethene-d2	2.294	65	24489	34.715	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.420%
21) 2-Butanone-d5	4.465	46	77394	77.352	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	77.350%
24) Chloroform-d	5.050	84	128426	38.985	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.960%
26) 1,2-Dichloroethane-d4	5.952	65	82014	39.190	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.380%
32) Benzene-d6	5.970	84	253128	38.930	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.860%
36) 1,2-Dichloropropane-d6	7.306	67	77672	39.264	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	78.520%
41) Toluene-d8	8.647	98	228194	38.633	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	77.260%#
43) trans-1,3-Dichloroprop...	8.952	79	32058	33.887	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.780%
47) 2-Hexanone-d5	9.384	63	64824	82.802	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	82.800%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	108584	42.781	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.560%
66) 1,2-Dichlorobenzene-d4	12.317	152	88650	45.885	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.760%
Target Compounds						
37) 1,2-Dichloropropane	7.306	63	8601	4.504	ug/L	Qvalue # 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043824.D
Acq On : 12 Nov 2024 20:31
Operator : JC/MD
Sample : P4785-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 13 02:11:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 13 02:04:29 2024
Response via : Initial Calibration

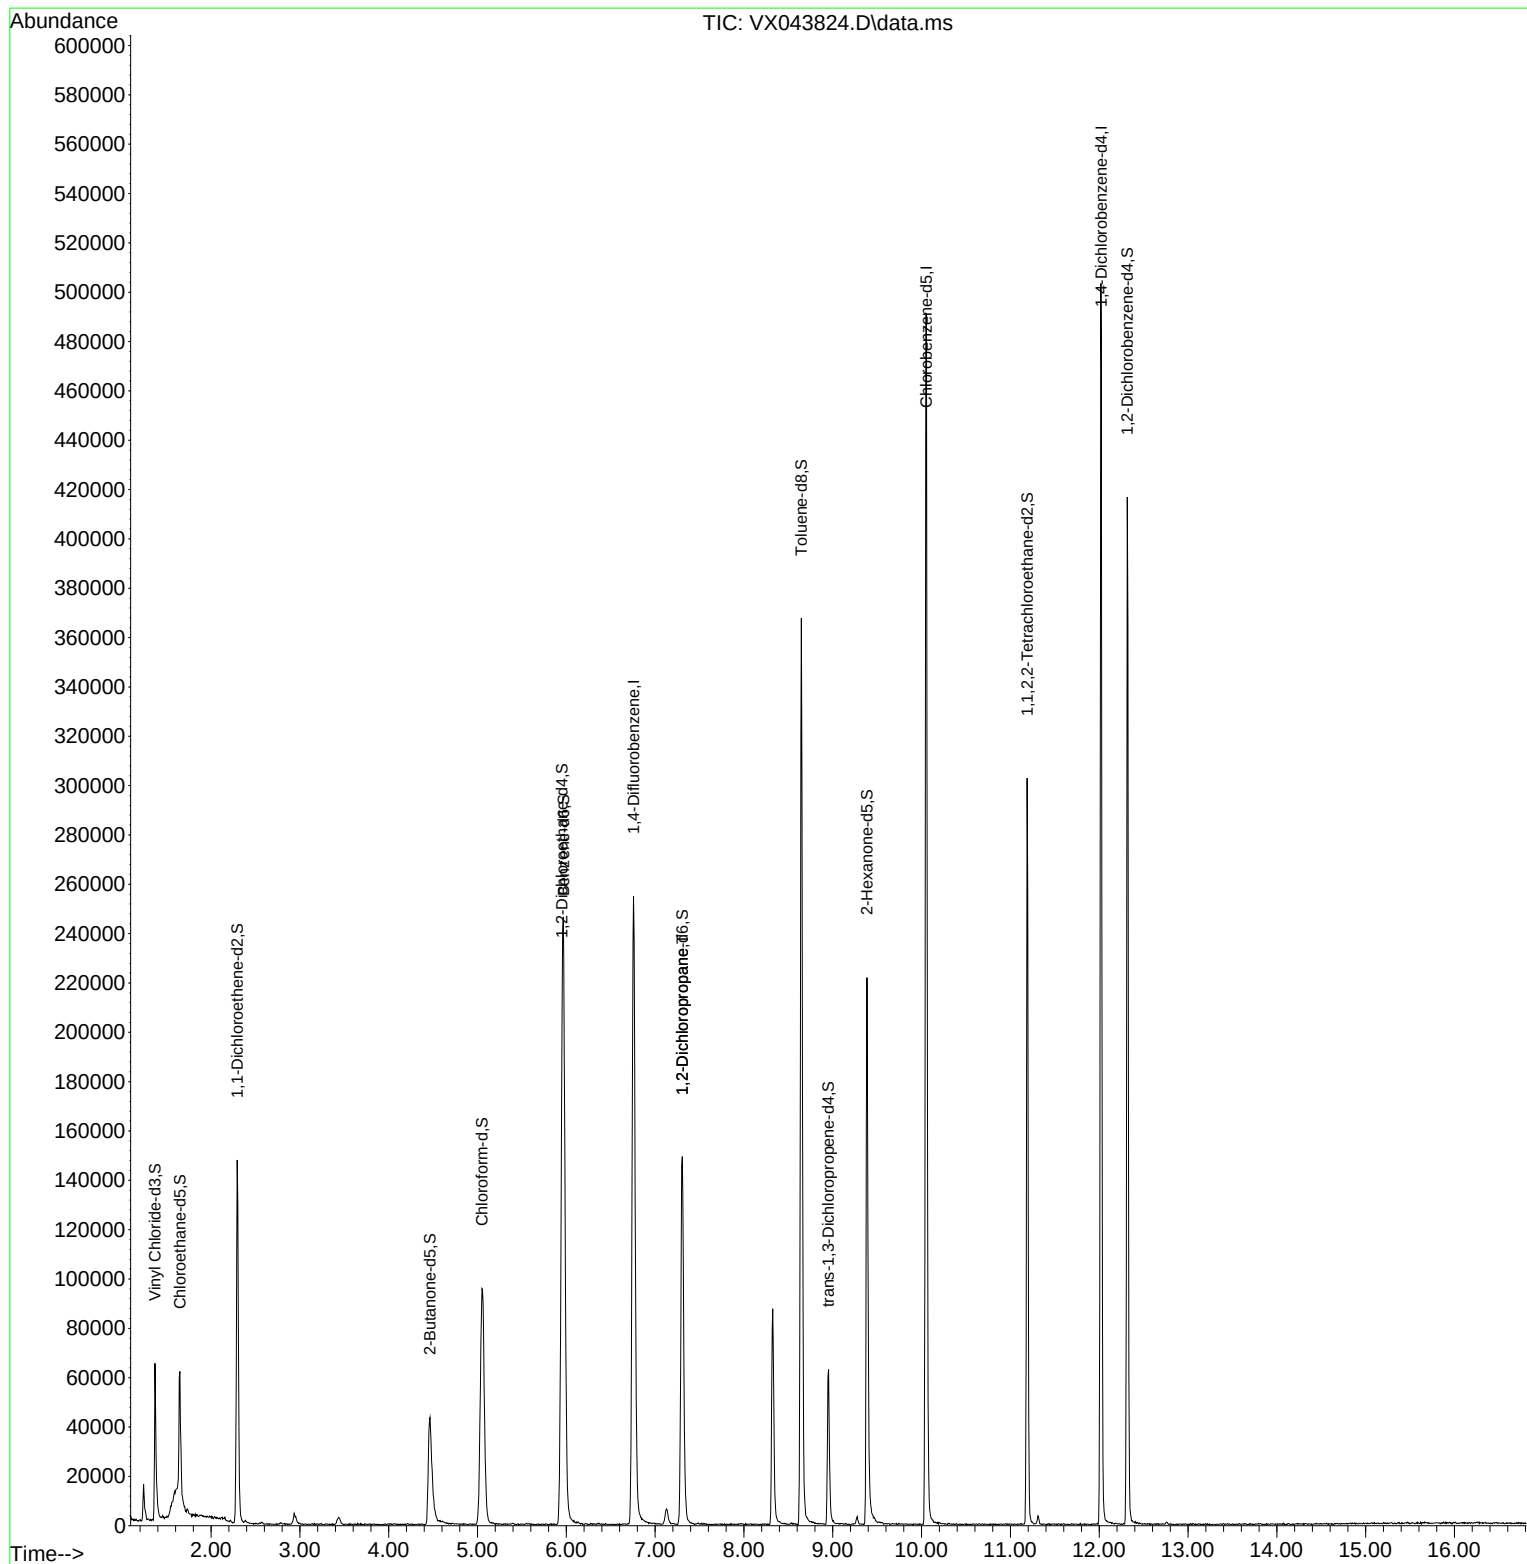

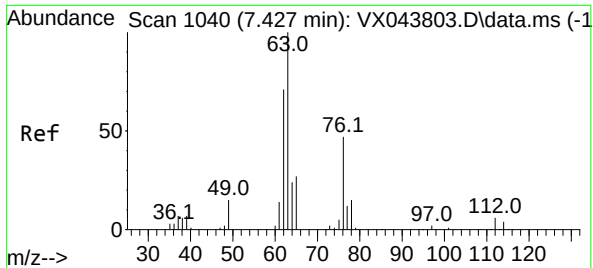

#37
1,2-Dichloropropane
Concen: 4.504 ug/L
RT: 7.306 min Scan# 10
Delta R.T. -0.122 min
Lab File: VX043824.D
Acq: 12 Nov 2024 20:31

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 63 Resp: 8601
Ion Ratio Lower Upper
63 100
112 0.0 3.8 5.8#

