

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043825.D
 Acq On : 12 Nov 2024 20:54
 Operator : JC/MD
 Sample : P4785-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 13 02:11:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 13 02:04:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	281814	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	248472	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	111504	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	45939	30.599	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	61.200%		
7) Chloroethane-d5	1.642	69	31580	48.936	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	97.880%		
11) 1,1-Dichloroethene-d2	2.294	65	24712	35.656	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	71.320%		
21) 2-Butanone-d5	4.459	46	75570	76.877	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	76.880%		
24) Chloroform-d	5.056	84	126690	39.144	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	78.280%		
26) 1,2-Dichloroethane-d4	5.946	65	82632	40.190	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.380%		
32) Benzene-d6	5.964	84	253698	39.492	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	78.980%		
36) 1,2-Dichloropropane-d6	7.306	67	76048	38.911	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	77.820%		
41) Toluene-d8	8.647	98	226559	38.823	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	77.640%#		
43) trans-1,3-Dichloroprop...	8.952	79	32240	34.494	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	68.980%		
47) 2-Hexanone-d5	9.385	63	63589	82.213	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	82.210%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	107695	42.947	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	85.900%		
66) 1,2-Dichlorobenzene-d4	12.317	152	88790	45.959	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.920%		
Target Compounds						Qvalue
35) Methylcyclohexane	7.300	83	20150	7.083	ug/L #	20
61) 1,2,3-Trichloropropane	12.018	75	11948	5.520	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043825.D
Acq On : 12 Nov 2024 20:54
Operator : JC/MD
Sample : P4785-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 13 02:11:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 13 02:04:29 2024
Response via : Initial Calibration




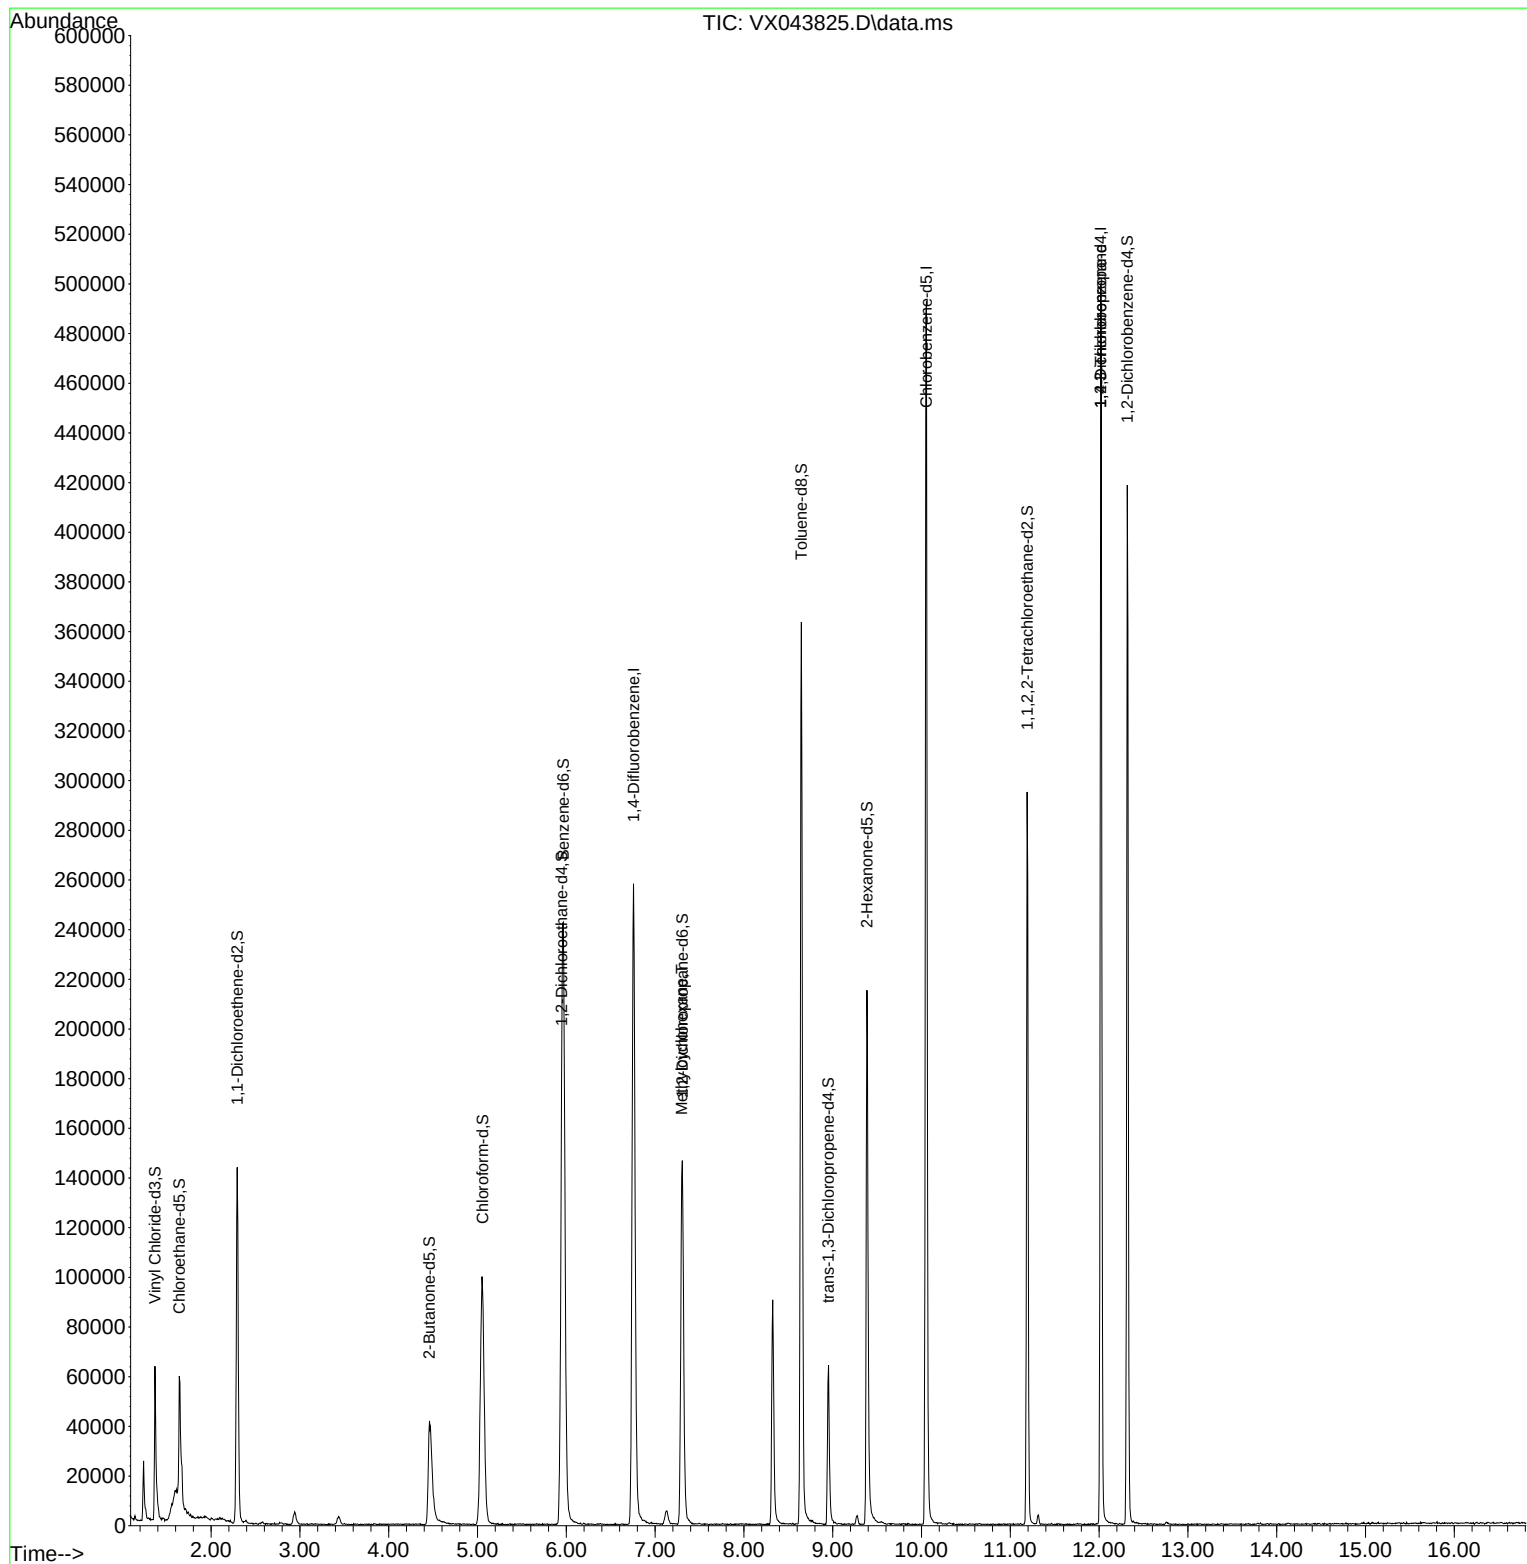


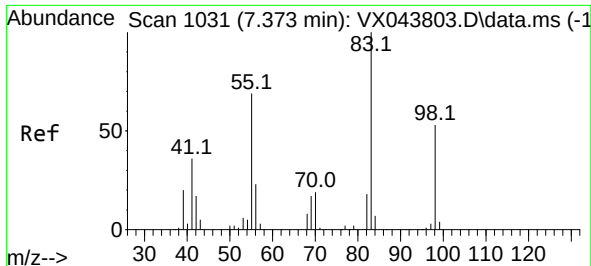

#35
Methylcyclohexane
Concen: 7.083 ug/L
RT: 7.300 min Scan# 1031
Delta R.T. -0.073 min
Lab File: VX043825.D
Acq: 12 Nov 2024 20:54

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 83 Resp: 20150
Ion Ratio Lower Upper
83 100
55 0.3 58.6 88.0#
98 1.8 39.0 58.4#

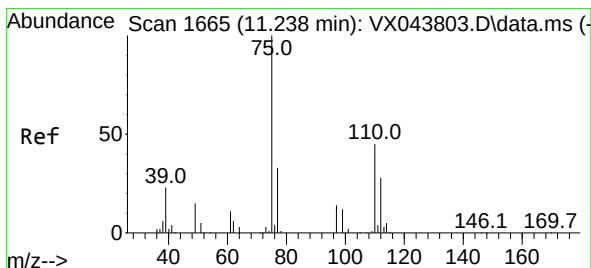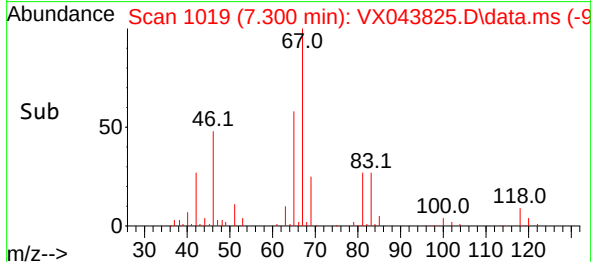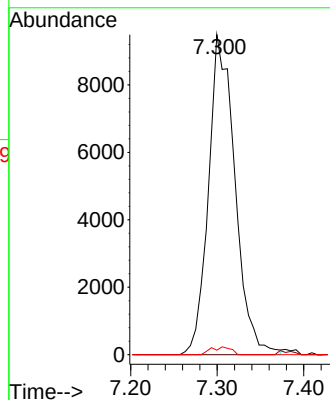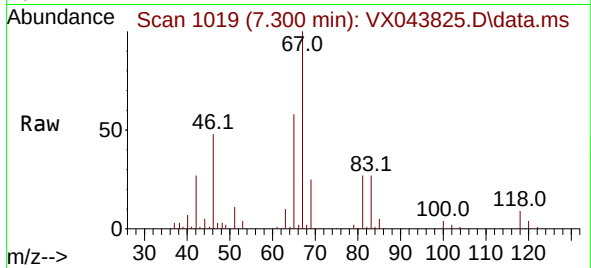

#61
1,2,3-Trichloropropane
Concen: 5.520 ug/L
RT: 12.018 min Scan# 1793
Delta R.T. 0.781 min
Lab File: VX043825.D
Acq: 12 Nov 2024 20:54

Tgt Ion: 75 Resp: 11948
Ion Ratio Lower Upper
75 100
77 32.7 25.4 38.0
110 3.8 33.6 50.4#

