

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043805.D
 Acq On : 12 Nov 2024 13:05
 Operator : JC/MD
 Sample : VX1112WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK724

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043805.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	33	rBV2	8381	11314	1.27%	0.167%
2	1.368	43	46	61	rVB	75975	97637	10.94%	1.440%
3	1.642	88	91	104	rVB	64645	110085	12.34%	1.624%
4	2.294	192	198	209	rBV	179009	274419	30.76%	4.049%
5	2.508	230	233	236	rBV2	667	878	0.10%	0.013%
6	2.587	244	246	248	rVB2	523	332	0.04%	0.005%
7	2.623	248	252	253	rBV2	263	293	0.03%	0.004%
8	2.715	264	267	268	rVB	551	395	0.04%	0.006%
9	2.782	274	278	284	rVB4	998	1660	0.19%	0.024%
10	2.892	292	296	297	rBV	381	372	0.04%	0.005%
11	2.940	299	304	305	rBV2	2582	3757	0.42%	0.055%
12	3.032	317	319	322	rVB2	560	571	0.06%	0.008%
13	3.056	322	323	325	rBV	487	360	0.04%	0.005%
14	3.166	339	341	343	rVV	376	334	0.04%	0.005%
15	3.312	364	365	367	rBV	355	291	0.03%	0.004%
16	3.428	374	384	390	rBV5	3488	8192	0.92%	0.121%
17	3.702	426	429	432	rBV2	387	550	0.06%	0.008%
18	3.812	446	447	451	rBV2	535	524	0.06%	0.008%
19	3.904	458	462	467	rVB3	332	638	0.07%	0.009%
20	4.148	500	502	506	rBV	341	491	0.06%	0.007%
21	4.245	513	518	519	rBV2	321	507	0.06%	0.007%
22	4.343	531	534	535	rVB2	313	281	0.03%	0.004%
23	4.391	537	542	544	rBV3	259	321	0.04%	0.005%
24	4.465	544	554	573	rBV2	51338	171076	19.18%	2.524%
25	4.775	603	605	609	rVB3	490	431	0.05%	0.006%
26	4.861	616	619	622	rBV4	402	532	0.06%	0.008%
27	5.050	638	650	668	rBV	114960	361259	40.49%	5.330%
28	5.202	673	675	676	rBV	387	291	0.03%	0.004%
29	5.379	700	704	706	rBV3	682	973	0.11%	0.014%
30	5.550	728	732	733	rBV2	779	981	0.11%	0.014%
31	5.672	750	752	755	rVV2	321	289	0.03%	0.004%
32	5.714	755	759	760	rVB2	410	367	0.04%	0.005%
33	5.964	789	800	824	rVV2	298170	892113	100.00%	13.161%
34	6.470	880	883	884	rBV2	531	354	0.04%	0.005%
35	6.550	893	896	898	rBV2	352	409	0.05%	0.006%
36	6.696	918	920	921	rBV	410	292	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043805.D
 Acq On : 12 Nov 2024 13:05
 Operator : JC/MD
 Sample : VX1112WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK724

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	6.757	921	930	950	rBV	234472	586991	65.80%	8.660%
38	7.129	982	991	1003	rBV5	16061	40561	4.55%	0.598%
39	7.305	1011	1020	1035	rBV	180996	401844	45.04%	5.928%
40	7.427	1038	1040	1042	rVV3	703	650	0.07%	0.010%
41	7.641	1073	1075	1078	rBV2	310	318	0.04%	0.005%
42	7.708	1083	1086	1090	rVB	356	465	0.05%	0.007%
43	7.811	1101	1103	1107	rVV2	347	403	0.05%	0.006%
44	7.842	1107	1108	1111	rVV	332	317	0.04%	0.005%
45	7.915	1118	1120	1122	rBV2	287	313	0.04%	0.005%
46	7.970	1126	1129	1132	rVB2	486	614	0.07%	0.009%
47	8.080	1144	1147	1149	rBV2	375	410	0.05%	0.006%
48	8.238	1171	1173	1178	rBV3	216	341	0.04%	0.005%
49	8.324	1181	1187	1203	rBV	115212	191978	21.52%	2.832%
50	8.500	1213	1216	1217	rBV2	495	413	0.05%	0.006%
51	8.647	1233	1240	1256	rBV	444915	711892	79.80%	10.503%
52	8.952	1285	1290	1303	rBV	77803	122976	13.78%	1.814%
53	9.201	1328	1331	1334	rBV	316	319	0.04%	0.005%
54	9.384	1356	1361	1379	rBV	257930	397537	44.56%	5.865%
55	9.543	1385	1387	1389	rBV2	639	443	0.05%	0.007%
56	9.707	1410	1414	1417	rVB3	878	1451	0.16%	0.021%
57	9.762	1421	1423	1425	rBV2	279	287	0.03%	0.004%
58	9.933	1449	1451	1453	rBV2	378	283	0.03%	0.004%
59	9.964	1453	1456	1459	rBV3	262	317	0.04%	0.005%
60	10.055	1465	1471	1486	rBV	461722	676722	75.86%	9.984%
61	10.238	1498	1501	1505	rBV2	475	637	0.07%	0.009%
62	10.305	1510	1512	1514	rBV2	361	323	0.04%	0.005%
63	10.476	1538	1540	1543	rVB2	373	466	0.05%	0.007%
64	10.561	1551	1554	1556	rVB3	382	318	0.04%	0.005%
65	10.622	1563	1564	1566	rBV2	331	331	0.04%	0.005%
66	10.695	1574	1576	1579	rBV3	294	398	0.04%	0.006%
67	10.841	1596	1600	1603	rVV3	252	408	0.05%	0.006%
68	10.957	1612	1619	1622	rBV3	399	950	0.11%	0.014%
69	11.061	1633	1636	1638	rBV2	247	337	0.04%	0.005%
70	11.189	1652	1657	1666	rBV	350700	454212	50.91%	6.701%
71	11.317	1674	1678	1680	rBV2	429	642	0.07%	0.009%
72	11.360	1683	1685	1687	rVB2	487	289	0.03%	0.004%
73	11.396	1689	1691	1694	rBV	287	320	0.04%	0.005%
74	12.018	1788	1793	1805	rVV	447910	593785	66.56%	8.760%
75	12.207	1821	1824	1825	rBV2	556	457	0.05%	0.007%
76	12.317	1837	1842	1851	rBV	489731	630484	70.67%	9.302%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043805.D
 Acq On : 12 Nov 2024 13:05
 Operator : JC/MD
 Sample : VX1112WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK724

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	12.469	1865	1867	1870	rVV3	642	689	0.08%	0.010%
78	12.768	1912	1916	1920	rBV4	705	1209	0.14%	0.018%
79	12.939	1942	1944	1949	rBV3	316	530	0.06%	0.008%
80	13.012	1954	1956	1960	rVB3	429	549	0.06%	0.008%
81	13.067	1963	1965	1967	rVB2	648	515	0.06%	0.008%
82	13.097	1967	1970	1974	rBV2	479	604	0.07%	0.009%
83	13.353	2010	2012	2014	rBV2	320	305	0.03%	0.004%
84	13.463	2028	2030	2032	rVB2	336	306	0.03%	0.005%
85	13.542	2041	2043	2046	rBV2	189	298	0.03%	0.004%
86	13.634	2055	2058	2060	rBV2	245	296	0.03%	0.004%
87	13.841	2090	2092	2094	rBV	383	362	0.04%	0.005%
88	14.091	2131	2133	2136	rBV2	263	360	0.04%	0.005%
89	14.127	2136	2139	2143	rVV4	1258	1607	0.18%	0.024%
90	14.201	2149	2151	2154	rVB2	342	294	0.03%	0.004%
91	14.298	2163	2167	2168	rBV2	296	299	0.03%	0.004%
92	14.335	2168	2173	2177	rVB3	472	714	0.08%	0.011%
93	14.371	2177	2179	2182	rBV3	364	404	0.05%	0.006%
94	14.554	2208	2209	2212	rBV2	344	315	0.04%	0.005%
95	14.804	2249	2250	2252	rBV2	573	463	0.05%	0.007%
96	15.712	2397	2399	2401	rBV3	569	514	0.06%	0.008%
97	16.255	2486	2488	2489	rBV2	513	379	0.04%	0.006%
98	16.548	2533	2536	2539	rBV3	557	651	0.07%	0.010%
99	16.609	2544	2546	2548	rBV2	593	474	0.05%	0.007%
100	16.767	2571	2572	2575	rBV	534	323	0.04%	0.005%




Sum of corrected areas: 6778231

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043805.D
Acq On : 12 Nov 2024 13:05
Operator : JC/MD
Sample : VX1112WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK724

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

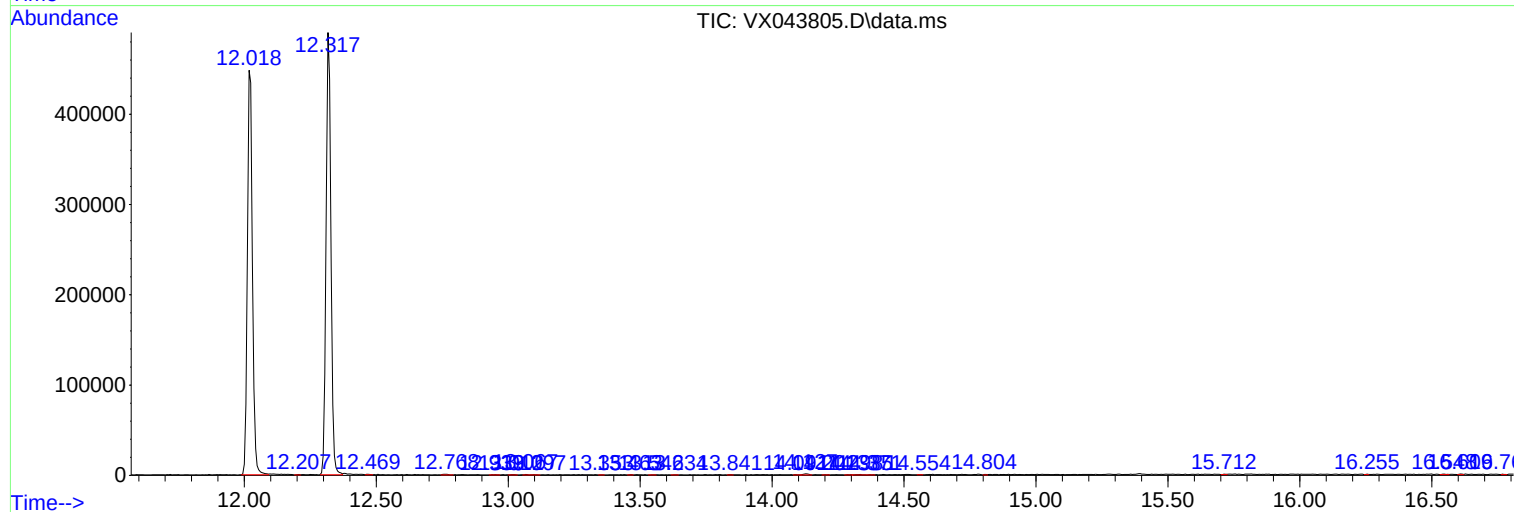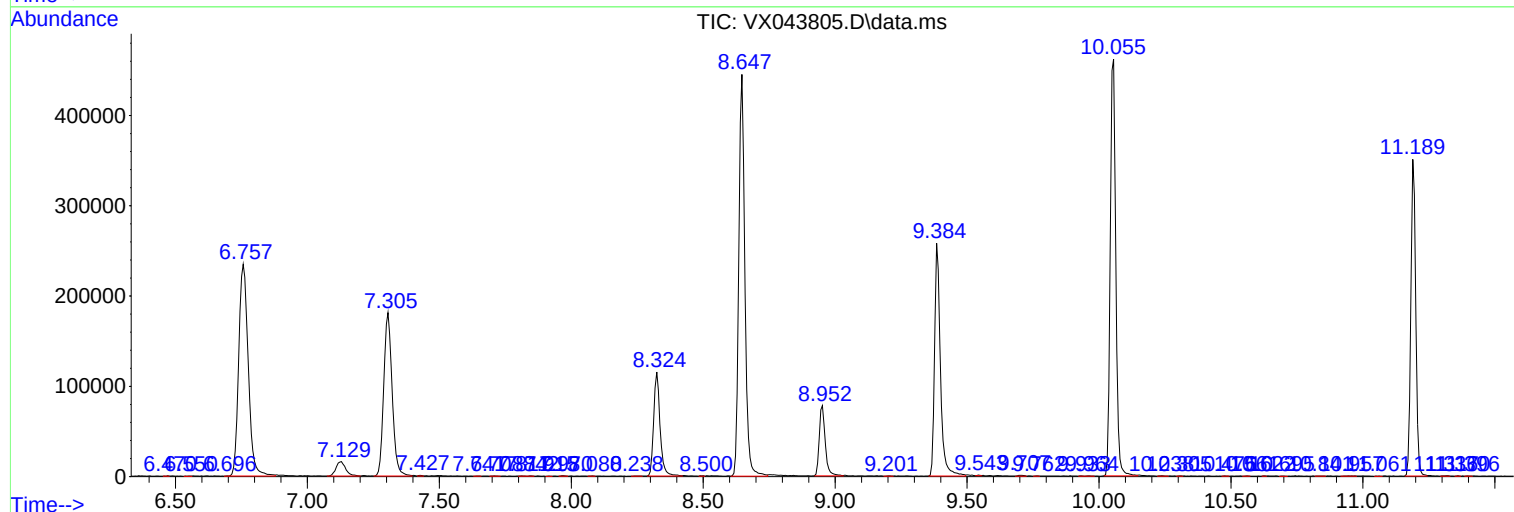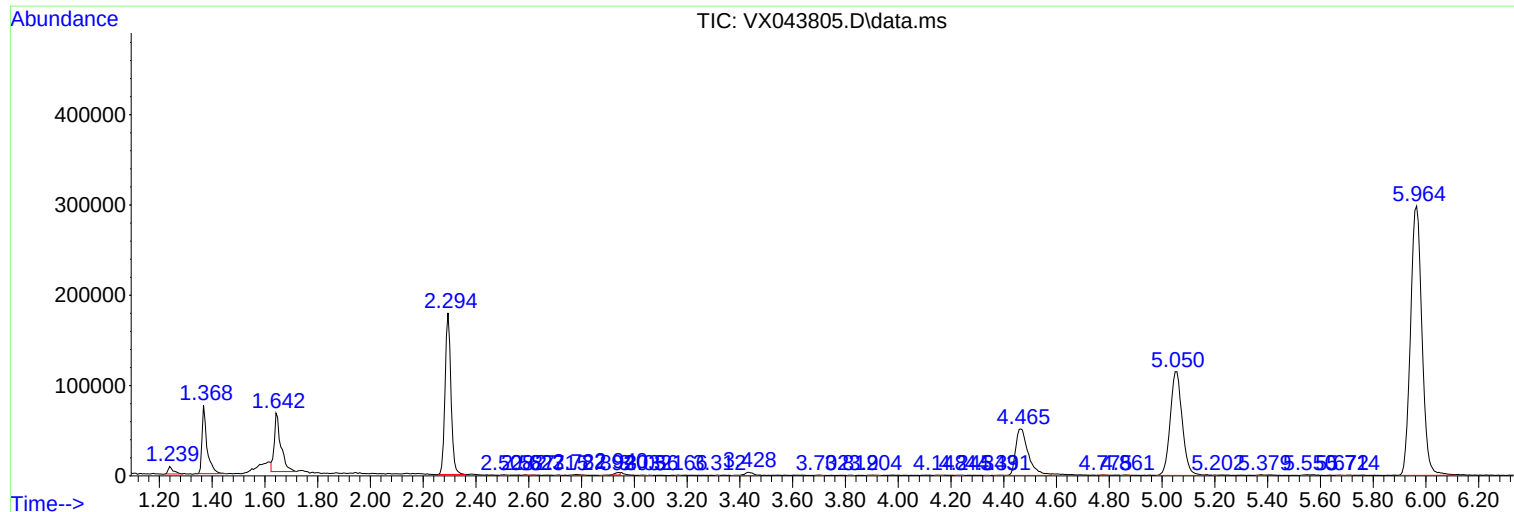

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043805.D
Acq On : 12 Nov 2024 13:05
Operator : JC/MD
Sample : VX1112WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK724

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043805.D
Acq On : 12 Nov 2024 13:05
Operator : JC/MD
Sample : VX1112WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK724

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc