

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043806.D
 Acq On : 12 Nov 2024 13:34
 Operator : JC/MD
 Sample : P4786-13DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27N5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043806.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	27	rBV	9076	9255	1.02%	0.126%
2	1.368	43	46	59	rVB	71768	100441	11.07%	1.364%
3	1.642	88	91	104	rVB	57403	103255	11.38%	1.402%
4	2.294	191	198	211	rVB	179637	289214	31.86%	3.928%
5	2.660	257	258	261	rBV2	369	377	0.04%	0.005%
6	2.703	263	265	267	rBV3	475	511	0.06%	0.007%
7	2.782	274	278	284	rVB3	1883	2831	0.31%	0.038%
8	2.941	298	304	314	rVB3	6213	14983	1.65%	0.204%
9	3.093	324	329	330	rBV3	758	1149	0.13%	0.016%
10	3.434	377	385	392	rVV5	3399	8304	0.91%	0.113%
11	3.544	401	403	407	rVB2	407	389	0.04%	0.005%
12	3.575	407	408	410	rBV2	477	440	0.05%	0.006%
13	3.605	410	413	418	rVV3	562	919	0.10%	0.012%
14	3.922	464	465	468	rVB2	538	395	0.04%	0.005%
15	4.087	490	492	495	rBV2	304	417	0.05%	0.006%
16	4.361	535	537	540	rBV	404	367	0.04%	0.005%
17	4.459	545	553	571	rBV	53261	176069	19.40%	2.391%
18	4.891	622	624	626	rBV2	390	330	0.04%	0.004%
19	4.958	633	635	638	rBV3	218	330	0.04%	0.004%
20	5.050	638	650	668	rVV	122550	376073	41.43%	5.108%
21	5.269	682	686	687	rBV2	485	346	0.04%	0.005%
22	5.464	714	718	719	rBV4	690	1046	0.12%	0.014%
23	5.550	727	732	734	rBV4	745	1432	0.16%	0.019%
24	5.641	743	747	748	rVV2	400	446	0.05%	0.006%
25	5.666	749	751	753	rVV2	722	570	0.06%	0.008%
26	5.861	779	783	784	rBV2	268	364	0.04%	0.005%
27	5.879	784	786	788	rVB2	520	346	0.04%	0.005%
28	5.958	788	799	816	rBV2	310616	907724	100.00%	12.329%
29	6.288	851	853	856	rBV2	280	340	0.04%	0.005%
30	6.342	859	862	863	rBV	362	332	0.04%	0.005%
31	6.452	877	880	882	rBV2	584	482	0.05%	0.007%
32	6.477	882	884	887	rVB2	446	377	0.04%	0.005%
33	6.672	912	916	918	rBV3	254	338	0.04%	0.005%
34	6.757	920	930	950	rBV	271807	680313	74.95%	9.241%
35	6.964	962	964	969	rVB2	660	586	0.06%	0.008%
36	7.123	983	990	1006	rVB5	15780	39755	4.38%	0.540%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043806.D
 Acq On : 12 Nov 2024 13:34
 Operator : JC/MD
 Sample : P4786-13DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27N5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

37	7.300	1011	1019	1034	rBV	180333	412785	45.47%	5.607%
38	7.519	1053	1055	1057	rBV2	597	469	0.05%	0.006%
39	7.726	1088	1089	1094	rVB2	439	375	0.04%	0.005%
40	7.775	1094	1097	1099	rBV2	440	558	0.06%	0.008%
41	7.830	1102	1106	1110	rVB5	580	1060	0.12%	0.014%
42	8.324	1181	1187	1200	rBV	110255	199803	22.01%	2.714%
43	8.464	1207	1210	1213	rVB	552	720	0.08%	0.010%
44	8.580	1225	1229	1233	rBV4	1175	1793	0.20%	0.024%
45	8.647	1233	1240	1249	rBV	449715	735175	80.99%	9.986%
46	8.952	1283	1290	1304	rBV	78341	129404	14.26%	1.758%
47	9.098	1311	1314	1315	rBV2	298	372	0.04%	0.005%
48	9.159	1321	1324	1330	rBV5	1290	1988	0.22%	0.027%
49	9.275	1340	1343	1350	rVB3	2244	3345	0.37%	0.045%
50	9.385	1356	1361	1378	rBV	271998	434279	47.84%	5.899%
51	9.884	1441	1443	1446	rBV	582	477	0.05%	0.006%
52	10.049	1465	1470	1488	rVV	556112	798347	87.95%	10.844%
53	10.195	1490	1494	1501	rVV4	2567	4624	0.51%	0.063%
54	10.250	1501	1503	1506	rVB2	596	571	0.06%	0.008%
55	10.305	1508	1512	1523	rVB4	2143	4409	0.49%	0.060%
56	10.415	1528	1530	1533	rVB2	531	478	0.05%	0.006%
57	10.482	1539	1541	1544	rBV2	342	319	0.04%	0.004%
58	10.518	1545	1547	1551	rVB2	427	452	0.05%	0.006%
59	10.561	1551	1554	1557	rBV2	394	402	0.04%	0.005%
60	10.610	1559	1562	1563	rBV2	301	313	0.03%	0.004%
61	10.653	1564	1569	1579	rVB5	2652	6626	0.73%	0.090%
62	10.799	1591	1593	1599	rVV3	427	583	0.06%	0.008%
63	10.884	1605	1607	1609	rVB2	636	550	0.06%	0.007%
64	10.964	1616	1620	1624	rVV	3004	3777	0.42%	0.051%
65	11.000	1624	1626	1627	rVV	417	345	0.04%	0.005%
66	11.018	1627	1629	1630	rVV	552	414	0.05%	0.006%
67	11.104	1639	1643	1647	rVB2	256	489	0.05%	0.007%
68	11.189	1652	1657	1671	rVB	365943	478259	52.69%	6.496%
69	11.451	1695	1700	1705	rBV3	2665	3434	0.38%	0.047%
70	11.756	1747	1750	1755	rVB2	2307	3284	0.36%	0.045%
71	11.969	1782	1785	1788	rBV2	2122	2522	0.28%	0.034%
72	12.018	1788	1793	1802	rBV	555438	720836	79.41%	9.791%
73	12.256	1830	1832	1835	rBV2	387	398	0.04%	0.005%
74	12.317	1837	1842	1855	rVV	535731	663717	73.12%	9.015%
75	12.762	1909	1915	1919	rBV3	1438	2147	0.24%	0.029%
76	12.884	1931	1935	1939	rVB3	378	674	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043806.D
 Acq On : 12 Nov 2024 13:34
 Operator : JC/MD
 Sample : P4786-13DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27N5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	12.951	1942	1946	1950	rBV3	538	761	0.08%	0.010%
78	13.122	1971	1974	1977	rBV3	1526	1818	0.20%	0.025%
79	13.317	2003	2006	2010	rVB3	326	498	0.05%	0.007%
80	13.536	2038	2042	2045	rVB2	439	492	0.05%	0.007%
81	13.597	2048	2052	2056	rBV2	1295	1548	0.17%	0.021%
82	13.676	2062	2065	2069	rBV3	498	564	0.06%	0.008%
83	13.786	2079	2083	2087	rBV3	1628	2600	0.29%	0.035%
84	13.908	2101	2103	2106	rVB	394	356	0.04%	0.005%
85	13.939	2106	2108	2109	rBV	405	370	0.04%	0.005%
86	13.963	2109	2112	2119	rVB4	1276	2029	0.22%	0.028%
87	14.042	2122	2125	2128	rBV3	439	584	0.06%	0.008%
88	14.121	2134	2138	2145	rBV2	2069	3275	0.36%	0.044%
89	14.420	2185	2187	2190	rBV2	397	593	0.07%	0.008%
90	14.554	2205	2209	2212	rBV2	457	640	0.07%	0.009%
91	14.603	2216	2217	2221	rVB2	606	455	0.05%	0.006%
92	14.640	2221	2223	2225	rBV2	393	404	0.04%	0.005%
93	14.951	2270	2274	2275	rBV3	494	564	0.06%	0.008%
94	15.505	2363	2365	2366	rBV2	566	461	0.05%	0.006%
95	15.639	2386	2387	2390	rBV	574	357	0.04%	0.005%
96	16.024	2449	2450	2453	rVB2	793	753	0.08%	0.010%
97	16.048	2453	2454	2456	rBV2	470	436	0.05%	0.006%
98	16.225	2481	2483	2486	rVB3	566	445	0.05%	0.006%
99	16.402	2511	2512	2516	rVB	604	437	0.05%	0.006%
100	16.694	2558	2560	2561	rBV	646	425	0.05%	0.006%




Sum of corrected areas: 7362284

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043806.D
Acq On : 12 Nov 2024 13:34
Operator : JC/MD
Sample : P4786-13DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27N5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

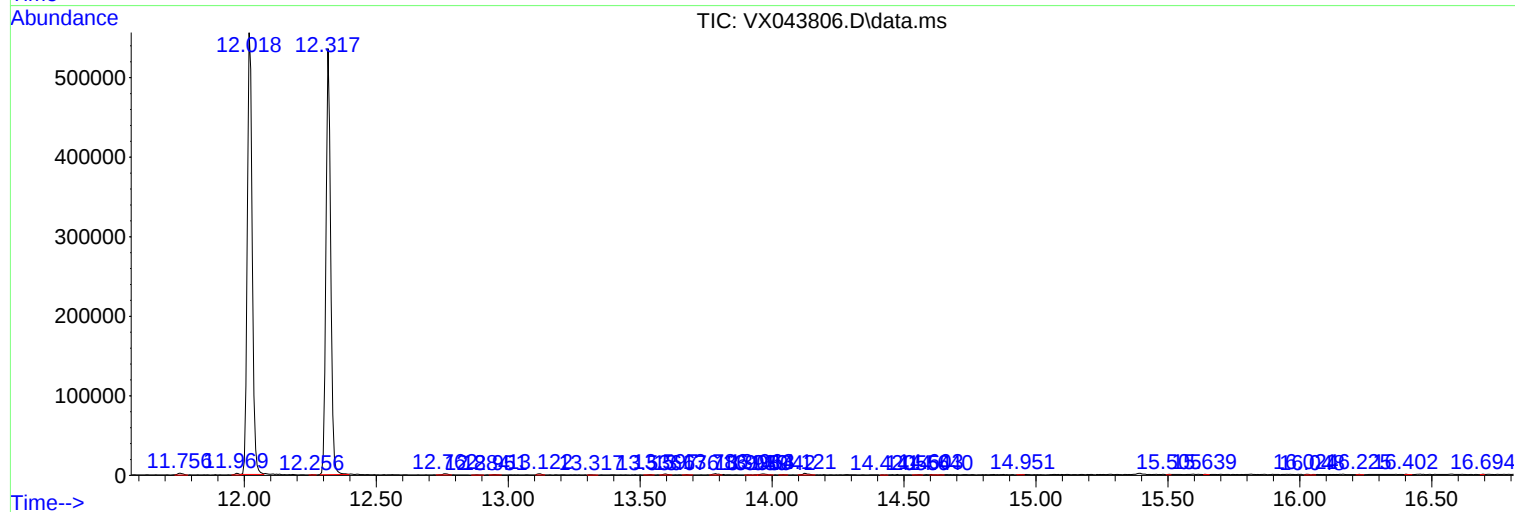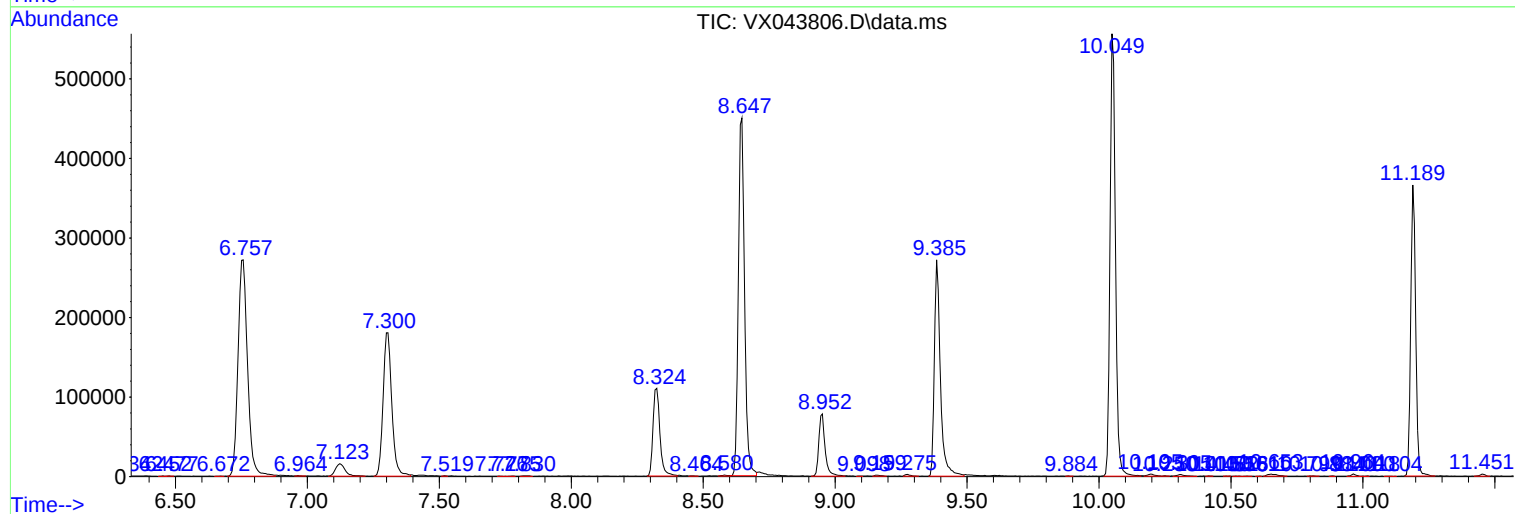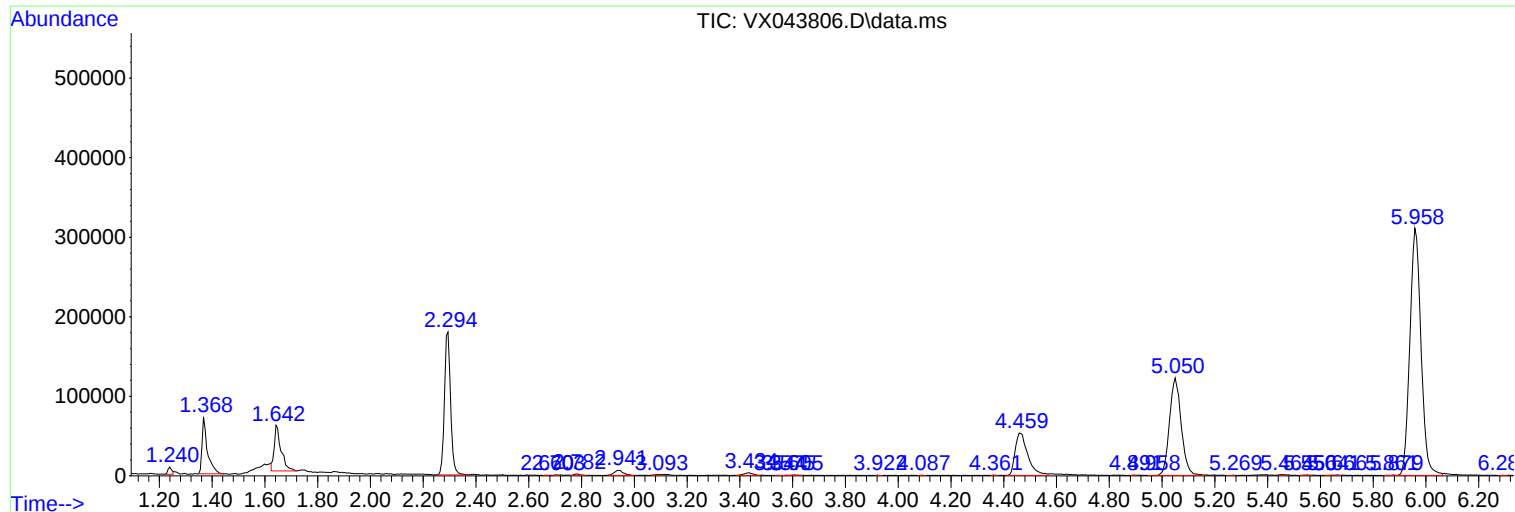

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043806.D
Acq On : 12 Nov 2024 13:34
Operator : JC/MD
Sample : P4786-13DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27N5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043806.D
Acq On : 12 Nov 2024 13:34
Operator : JC/MD
Sample : P4786-13DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27N5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc