

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043807.D
 Acq On : 12 Nov 2024 13:57
 Operator : JC/MD
 Sample : P4786-05DL 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27M7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M

Title : VOC Analysis

Signal : TIC: VX043807.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	32	rBV2	7732	12059	1.55%	0.167%
2	1.368	43	46	61	rVB2	73761	102609	13.20%	1.423%
3	1.642	88	91	104	rVB	53939	90250	11.61%	1.252%
4	2.294	191	198	211	rBV	158171	242945	31.25%	3.370%
5	2.581	243	245	246	rVB	583	314	0.04%	0.004%
6	2.697	262	264	269	rBV3	395	499	0.06%	0.007%
7	2.782	275	278	279	rBV	595	580	0.07%	0.008%
8	2.947	297	305	314	rBV2	4885	12360	1.59%	0.171%
9	3.081	322	327	334	rBV3	2918	5306	0.68%	0.074%
10	3.282	356	360	363	rBV	275	394	0.05%	0.005%
11	3.440	377	386	394	rVB5	3644	8482	1.09%	0.118%
12	3.599	411	412	414	rBV	524	260	0.03%	0.004%
13	3.623	414	416	418	rBV	477	252	0.03%	0.003%
14	4.032	481	483	486	rVB3	298	303	0.04%	0.004%
15	4.080	489	491	494	rBV3	264	344	0.04%	0.005%
16	4.123	496	498	500	rBV2	284	251	0.03%	0.003%
17	4.196	509	510	513	rVB2	443	387	0.05%	0.005%
18	4.227	513	515	516	rBV	385	361	0.05%	0.005%
19	4.257	518	520	521	rVV2	361	262	0.03%	0.004%
20	4.373	537	539	541	rVB	521	374	0.05%	0.005%
21	4.398	541	543	546	rBV2	337	379	0.05%	0.005%
22	4.477	546	556	570	rBV2	155344	481398	61.92%	6.677%
23	4.788	605	607	608	rBV	384	314	0.04%	0.004%
24	4.897	623	625	626	rBV	302	275	0.04%	0.004%
25	5.056	639	651	669	rBV	102112	313621	40.34%	4.350%
26	5.190	671	673	675	rVB	435	310	0.04%	0.004%
27	5.275	685	687	689	rVB2	320	255	0.03%	0.004%
28	5.294	689	690	695	rBV4	332	553	0.07%	0.008%
29	5.373	699	703	704	rBV2	419	410	0.05%	0.006%
30	5.391	704	706	708	rVV	402	418	0.05%	0.006%
31	5.416	708	710	712	rVB3	516	376	0.05%	0.005%
32	5.477	718	720	723	rVB	406	334	0.04%	0.005%
33	5.635	744	746	750	rBV2	249	333	0.04%	0.005%
34	5.958	788	799	815	rBV2	255786	772676	99.39%	10.717%
35	6.330	859	860	862	rBV	431	308	0.04%	0.004%
36	6.373	864	867	868	rVB2	389	376	0.05%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043807.D
 Acq On : 12 Nov 2024 13:57
 Operator : JC/MD
 Sample : P4786-05DL 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27M7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	6.458	878	881	882	rBV	384	304	0.04%	0.004%
38	6.592	902	903	908	rBV	347	422	0.05%	0.006%
39	6.665	911	915	916	rBV	424	349	0.04%	0.005%
40	6.684	916	918	920	rVB2	357	262	0.03%	0.004%
41	6.757	921	930	946	rBV	272062	665661	85.63%	9.233%
42	7.117	981	989	1007	rBV	199210	450462	57.94%	6.248%
43	7.306	1011	1020	1035	rVV	154545	346061	44.51%	4.800%
44	7.513	1053	1054	1057	rBV2	401	326	0.04%	0.005%
45	7.610	1067	1070	1071	rBV2	262	267	0.03%	0.004%
46	7.927	1120	1122	1124	rBV2	318	316	0.04%	0.004%
47	7.952	1124	1126	1127	rBV2	333	289	0.04%	0.004%
48	8.092	1145	1149	1150	rBV	447	424	0.05%	0.006%
49	8.324	1179	1187	1200	rBV2	97924	168652	21.69%	2.339%
50	8.647	1233	1240	1256	rBV	385168	624777	80.37%	8.666%
51	8.952	1285	1290	1299	rBV	63737	102924	13.24%	1.428%
52	9.104	1313	1315	1318	rBV2	405	492	0.06%	0.007%
53	9.244	1334	1338	1340	rBV2	293	380	0.05%	0.005%
54	9.275	1340	1343	1345	rBV2	540	553	0.07%	0.008%
55	9.384	1356	1361	1378	rBV	212209	359048	46.19%	4.980%
56	9.701	1410	1413	1416	rBV3	793	1038	0.13%	0.014%
57	9.817	1430	1432	1435	rVB2	527	507	0.07%	0.007%
58	9.903	1444	1446	1448	rVB	365	274	0.04%	0.004%
59	9.939	1448	1452	1455	rBV3	558	719	0.09%	0.010%
60	10.049	1465	1470	1490	rBV	528656	777405	100.00%	10.783%
61	10.311	1511	1513	1517	rVB3	603	840	0.11%	0.012%
62	10.457	1535	1537	1542	rVB2	409	539	0.07%	0.007%
63	10.500	1542	1544	1548	rBV2	304	352	0.05%	0.005%
64	10.622	1562	1564	1567	rVV2	246	272	0.03%	0.004%
65	10.738	1579	1583	1585	rBV2	306	335	0.04%	0.005%
66	10.848	1599	1601	1603	rVV2	431	440	0.06%	0.006%
67	10.951	1616	1618	1620	rBV3	274	255	0.03%	0.004%
68	11.098	1640	1642	1643	rBV	647	341	0.04%	0.005%
69	11.189	1652	1657	1668	rBV	296356	392708	50.52%	5.447%
70	11.311	1674	1677	1681	rVB3	1529	1938	0.25%	0.027%
71	11.506	1706	1709	1710	rBV	293	250	0.03%	0.003%
72	11.573	1718	1720	1722	rBV	277	262	0.03%	0.004%
73	11.591	1722	1723	1726	rVB2	273	288	0.04%	0.004%
74	11.616	1726	1727	1729	rBV	487	322	0.04%	0.004%
75	11.658	1732	1734	1738	rVV2	287	368	0.05%	0.005%
76	11.719	1742	1744	1748	rVB3	376	416	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043807.D
 Acq On : 12 Nov 2024 13:57
 Operator : JC/MD
 Sample : P4786-05DL 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27M7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	12.018	1788	1793	1803	rVV	538105	687303	88.41%	9.533%
78	12.207	1822	1824	1829	rVB4	391	516	0.07%	0.007%
79	12.250	1829	1831	1833	rBV	250	272	0.03%	0.004%
80	12.317	1837	1842	1850	rBV	421075	548811	70.60%	7.612%
81	12.530	1873	1877	1879	rBV3	530	813	0.10%	0.011%
82	12.573	1883	1884	1887	rBV3	441	539	0.07%	0.007%
83	12.762	1911	1915	1920	rVB3	1968	3196	0.41%	0.044%
84	12.872	1930	1933	1934	rBV	428	512	0.07%	0.007%
85	12.920	1937	1941	1943	rVB2	275	354	0.05%	0.005%
86	13.231	1990	1992	1995	rBV2	380	496	0.06%	0.007%
87	13.762	2076	2079	2081	rBV	260	272	0.03%	0.004%
88	13.951	2108	2110	2112	rBV2	332	326	0.04%	0.005%
89	13.993	2116	2117	2119	rBV2	289	270	0.03%	0.004%
90	14.127	2135	2139	2144	rBV	3514	5101	0.66%	0.071%
91	14.207	2150	2152	2153	rBV2	395	270	0.03%	0.004%
92	14.329	2169	2172	2174	rVB3	404	420	0.05%	0.006%
93	14.353	2174	2176	2178	rBV2	554	524	0.07%	0.007%
94	14.371	2178	2179	2182	rVB3	471	395	0.05%	0.005%
95	14.505	2199	2201	2204	rBV2	541	616	0.08%	0.009%
96	14.908	2265	2267	2269	rVB2	580	361	0.05%	0.005%
97	15.389	2343	2346	2351	rVB4	2478	3944	0.51%	0.055%
98	15.761	2404	2407	2408	rVB2	486	376	0.05%	0.005%
99	15.841	2417	2420	2422	rBV2	668	926	0.12%	0.013%
100	16.438	2516	2518	2520	rVB2	823	383	0.05%	0.005%




Sum of corrected areas: 7209762

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043807.D
Acq On : 12 Nov 2024 13:57
Operator : JC/MD
Sample : P4786-05DL 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27M7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

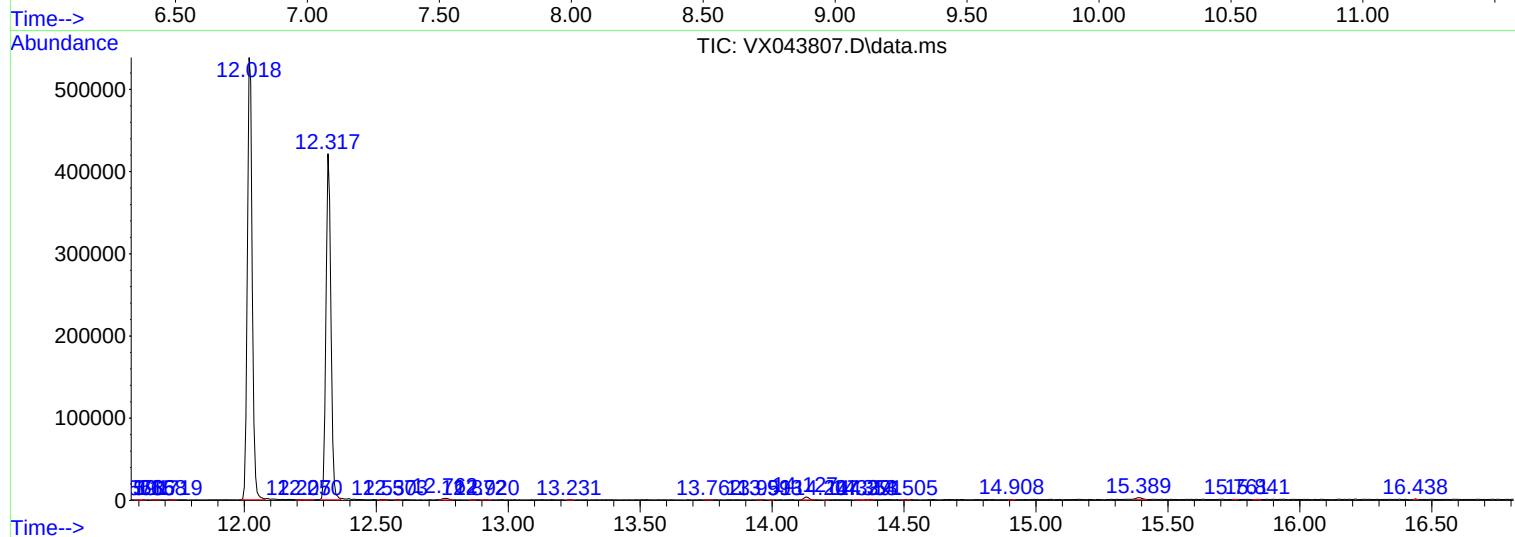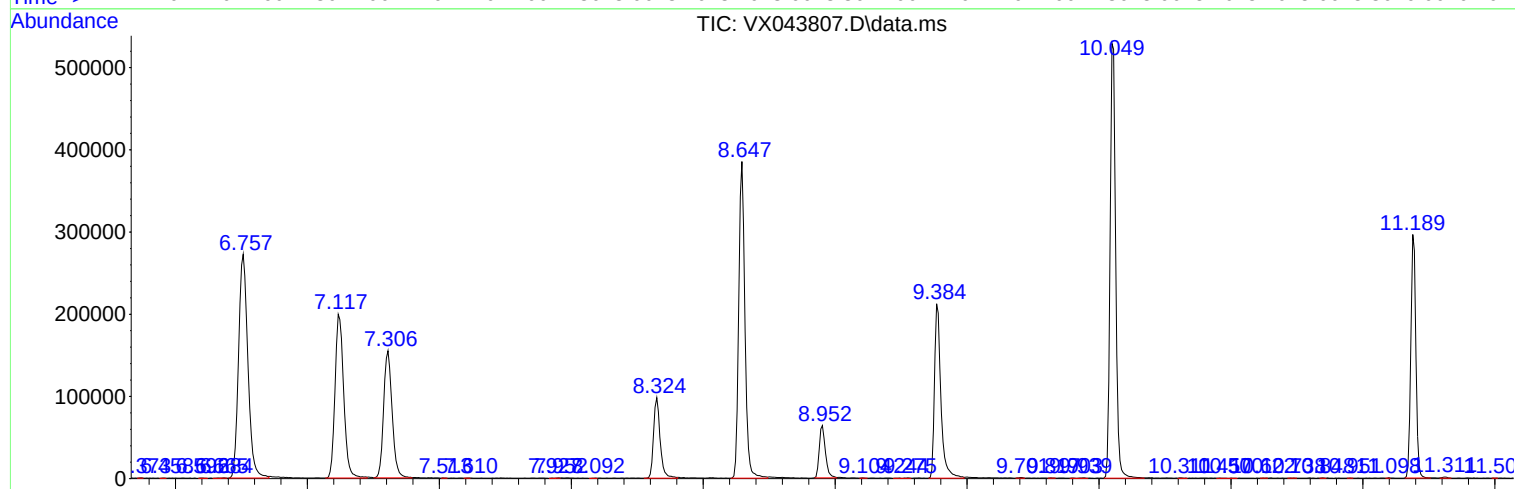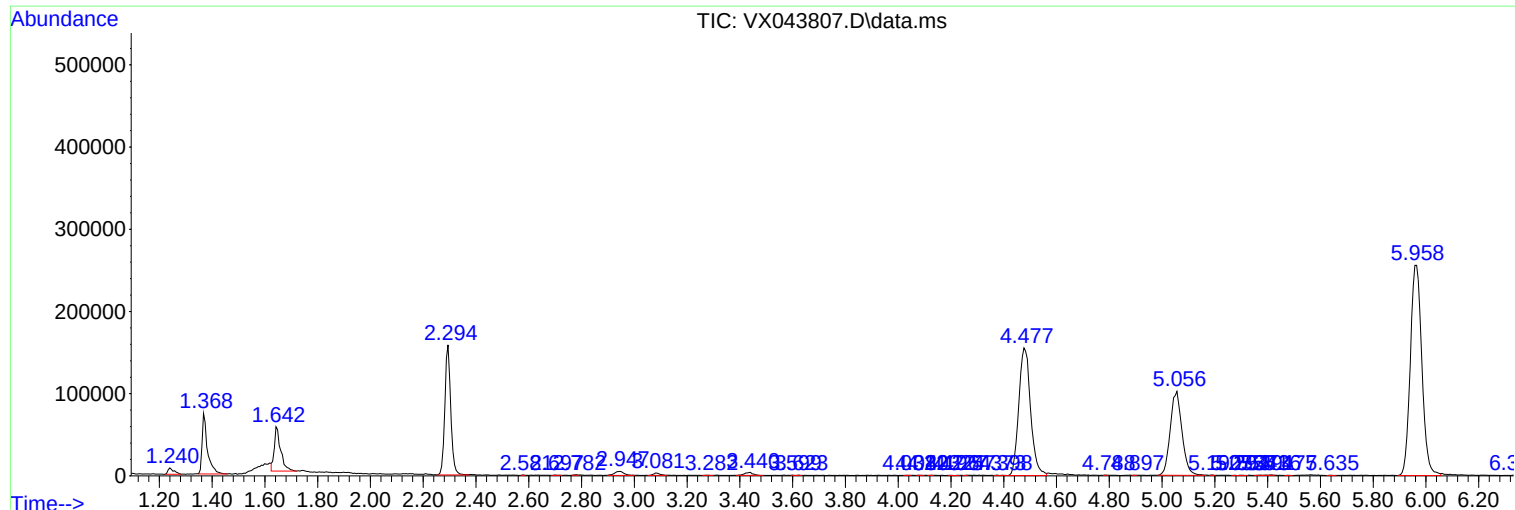

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043807.D
Acq On : 12 Nov 2024 13:57
Operator : JC/MD
Sample : P4786-05DL 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27M7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043807.D
Acq On : 12 Nov 2024 13:57
Operator : JC/MD
Sample : P4786-05DL 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27M7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------