

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043811.D
 Acq On : 12 Nov 2024 15:31
 Operator : JC/MD
 Sample : P4786-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27M5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043811.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	33	rVB2	8841	12224	1.58%	0.193%
2	1.368	43	46	57	rVB	65607	86562	11.19%	1.363%
3	1.642	88	91	104	rVB	56573	83815	10.83%	1.320%
4	2.294	192	198	209	rVB	163432	245139	31.69%	3.861%
5	2.593	246	247	251	rVB3	387	454	0.06%	0.007%
6	2.764	272	275	276	rBV	598	506	0.07%	0.008%
7	2.946	298	305	309	rBV3	2675	4985	0.64%	0.079%
8	3.373	373	375	377	rVV2	322	316	0.04%	0.005%
9	3.434	379	385	394	rBV4	3620	7718	1.00%	0.122%
10	3.574	407	408	413	rBV2	293	376	0.05%	0.006%
11	3.648	418	420	423	rVV	324	292	0.04%	0.005%
12	3.757	436	438	440	rBV2	533	602	0.08%	0.009%
13	3.812	446	447	449	rBV	476	285	0.04%	0.004%
14	4.007	475	479	480	rBV3	427	543	0.07%	0.009%
15	4.160	500	504	507	rVB3	374	509	0.07%	0.008%
16	4.245	515	518	520	rVV	469	398	0.05%	0.006%
17	4.300	525	527	529	rBV2	343	366	0.05%	0.006%
18	4.349	533	535	540	rVB2	236	305	0.04%	0.005%
19	4.465	546	554	569	rBV	46020	141459	18.28%	2.228%
20	5.050	640	650	665	rBV	101526	318783	41.21%	5.021%
21	5.367	699	702	703	rBV	415	394	0.05%	0.006%
22	5.477	717	720	721	rVV2	389	443	0.06%	0.007%
23	5.556	729	733	738	rVV4	706	1658	0.21%	0.026%
24	5.635	740	746	747	rVV	292	387	0.05%	0.006%
25	5.842	779	780	783	rBV2	217	301	0.04%	0.005%
26	5.879	785	786	789	rBV2	362	428	0.06%	0.007%
27	5.964	789	800	815	rBV2	261113	773640	100.00%	12.186%
28	6.190	836	837	840	rBV2	437	428	0.06%	0.007%
29	6.245	844	846	849	rVV2	601	601	0.08%	0.009%
30	6.269	849	850	853	rVV2	485	481	0.06%	0.008%
31	6.604	904	905	908	rBV	327	290	0.04%	0.005%
32	6.647	911	912	916	rVB2	341	322	0.04%	0.005%
33	6.757	921	930	947	rBV	265288	646738	83.60%	10.187%
34	6.946	959	961	966	rVB2	792	937	0.12%	0.015%
35	7.129	981	991	1002	rVB5	12209	29621	3.83%	0.467%
36	7.305	1012	1020	1038	rBV	157077	347720	44.95%	5.477%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043811.D
 Acq On : 12 Nov 2024 15:31
 Operator : JC/MD
 Sample : P4786-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27M5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.464	1044	1046	1047	rBV2	396	366	0.05%	0.006%
38	7.635	1072	1074	1078	rBV2	517	495	0.06%	0.008%
39	7.726	1087	1089	1092	rVB2	365	417	0.05%	0.007%
40	7.811	1099	1103	1104	rBV2	276	305	0.04%	0.005%
41	7.964	1122	1128	1130	rBV3	478	757	0.10%	0.012%
42	8.141	1156	1157	1160	rBV3	308	387	0.05%	0.006%
43	8.232	1169	1172	1173	rVB2	451	308	0.04%	0.005%
44	8.324	1181	1187	1200	rBV	99947	169597	21.92%	2.671%
45	8.647	1234	1240	1255	rBV	387872	631543	81.63%	9.947%
46	8.878	1276	1278	1279	rVB	600	384	0.05%	0.006%
47	8.952	1285	1290	1299	rBV	67061	104894	13.56%	1.652%
48	9.269	1339	1342	1347	rVB3	3281	4457	0.58%	0.070%
49	9.384	1356	1361	1377	rBV	227619	358110	46.29%	5.641%
50	9.616	1397	1399	1402	rVB2	403	348	0.04%	0.005%
51	9.781	1422	1426	1430	rBV2	409	559	0.07%	0.009%
52	10.055	1465	1471	1493	rVV	511404	742493	95.97%	11.695%
53	10.287	1506	1509	1511	rVB2	353	351	0.05%	0.006%
54	10.311	1511	1513	1517	rVB2	536	546	0.07%	0.009%
55	10.366	1517	1522	1523	rBV	199	288	0.04%	0.005%
56	10.421	1530	1531	1534	rVB2	384	302	0.04%	0.005%
57	10.463	1534	1538	1539	rBV2	466	529	0.07%	0.008%
58	10.494	1539	1543	1544	rVB2	321	353	0.05%	0.006%
59	10.732	1580	1582	1585	rBV2	427	440	0.06%	0.007%
60	10.774	1587	1589	1593	rVV3	425	530	0.07%	0.008%
61	11.012	1625	1628	1629	rBV2	246	298	0.04%	0.005%
62	11.085	1636	1640	1642	rBV	370	393	0.05%	0.006%
63	11.189	1652	1657	1667	rBV	299845	392006	50.67%	6.174%
64	11.311	1674	1677	1684	rVB2	3849	4901	0.63%	0.077%
65	11.384	1688	1689	1692	rVV2	436	437	0.06%	0.007%
66	11.408	1692	1693	1696	rVB	544	291	0.04%	0.005%
67	11.451	1696	1700	1702	rBV2	407	567	0.07%	0.009%
68	11.707	1738	1742	1745	rBV2	382	540	0.07%	0.009%
69	11.780	1749	1754	1756	rBV	225	349	0.05%	0.005%
70	11.927	1774	1778	1781	rBV3	407	698	0.09%	0.011%
71	12.018	1788	1793	1807	rBV	506359	655928	84.78%	10.331%
72	12.219	1824	1826	1829	rBV3	670	771	0.10%	0.012%
73	12.256	1831	1832	1836	rVB3	433	303	0.04%	0.005%
74	12.317	1837	1842	1854	rVV	442673	548140	70.85%	8.634%
75	12.579	1882	1885	1888	rVB	529	583	0.08%	0.009%
76	12.609	1888	1890	1891	rBV	446	374	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043811.D
 Acq On : 12 Nov 2024 15:31
 Operator : JC/MD
 Sample : P4786-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27M5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

77	12.628	1891	1893	1896	rVB2	339	322	0.04%	0.005%
78	12.859	1928	1931	1938	rBV5	1366	2427	0.31%	0.038%
79	12.914	1938	1940	1944	rBV3	426	452	0.06%	0.007%
80	12.963	1946	1948	1950	rBV	491	423	0.05%	0.007%
81	13.621	2054	2056	2058	rVV	412	360	0.05%	0.006%
82	13.737	2073	2075	2077	rVB2	363	336	0.04%	0.005%
83	13.774	2077	2081	2082	rBV2	436	410	0.05%	0.006%
84	13.969	2110	2113	2114	rBV2	309	373	0.05%	0.006%
85	14.018	2118	2121	2124	rBV3	376	293	0.04%	0.005%
86	14.066	2128	2129	2132	rBV3	385	310	0.04%	0.005%
87	14.127	2137	2139	2144	rVB	1564	1765	0.23%	0.028%
88	14.316	2168	2170	2174	rVB2	280	308	0.04%	0.005%
89	14.505	2198	2201	2202	rBV	428	424	0.05%	0.007%
90	14.591	2212	2215	2217	rBV2	427	478	0.06%	0.008%
91	14.743	2238	2240	2241	rBV	528	434	0.06%	0.007%
92	14.877	2260	2262	2263	rBV2	418	296	0.04%	0.005%
93	14.926	2268	2270	2271	rBV2	447	435	0.06%	0.007%
94	15.042	2286	2289	2291	rBV3	721	897	0.12%	0.014%
95	15.280	2325	2328	2330	rVB3	527	585	0.08%	0.009%
96	15.481	2360	2361	2362	rBV	767	340	0.04%	0.005%
97	15.633	2385	2386	2389	rBV2	421	475	0.06%	0.007%
98	15.853	2421	2422	2425	rBV3	511	583	0.08%	0.009%
99	16.249	2485	2487	2489	rBV2	706	421	0.05%	0.007%
100	16.603	2544	2545	2546	rBV	468	319	0.04%	0.005%




Sum of corrected areas: 6348830

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043811.D
Acq On : 12 Nov 2024 15:31
Operator : JC/MD
Sample : P4786-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27M5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

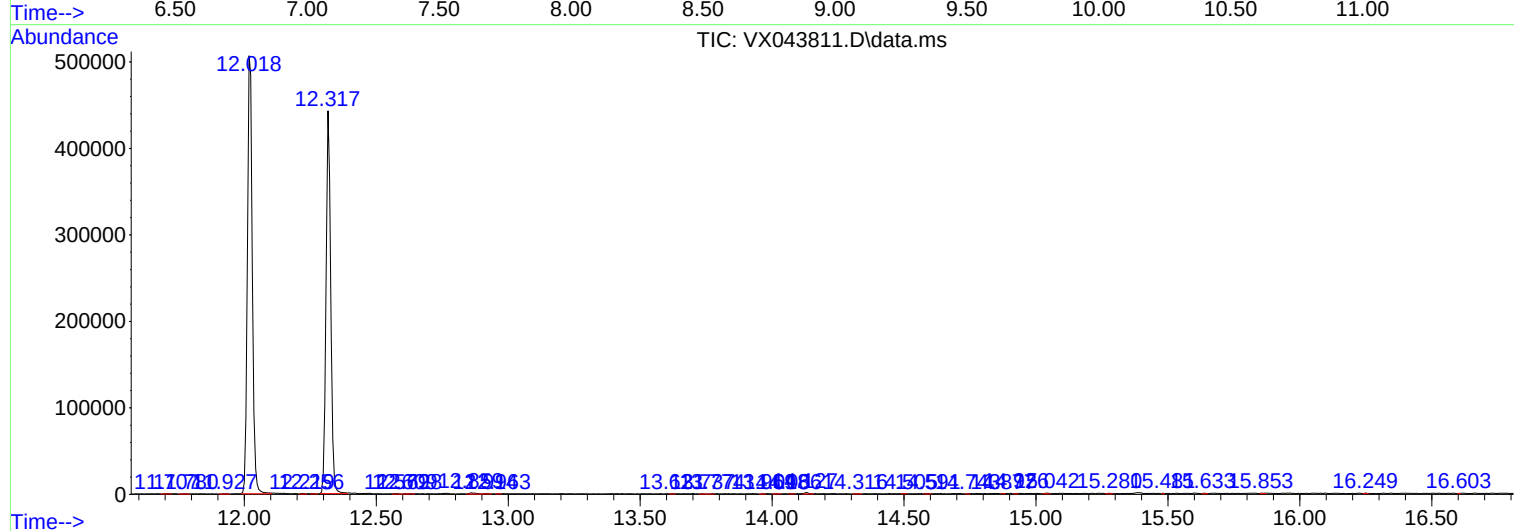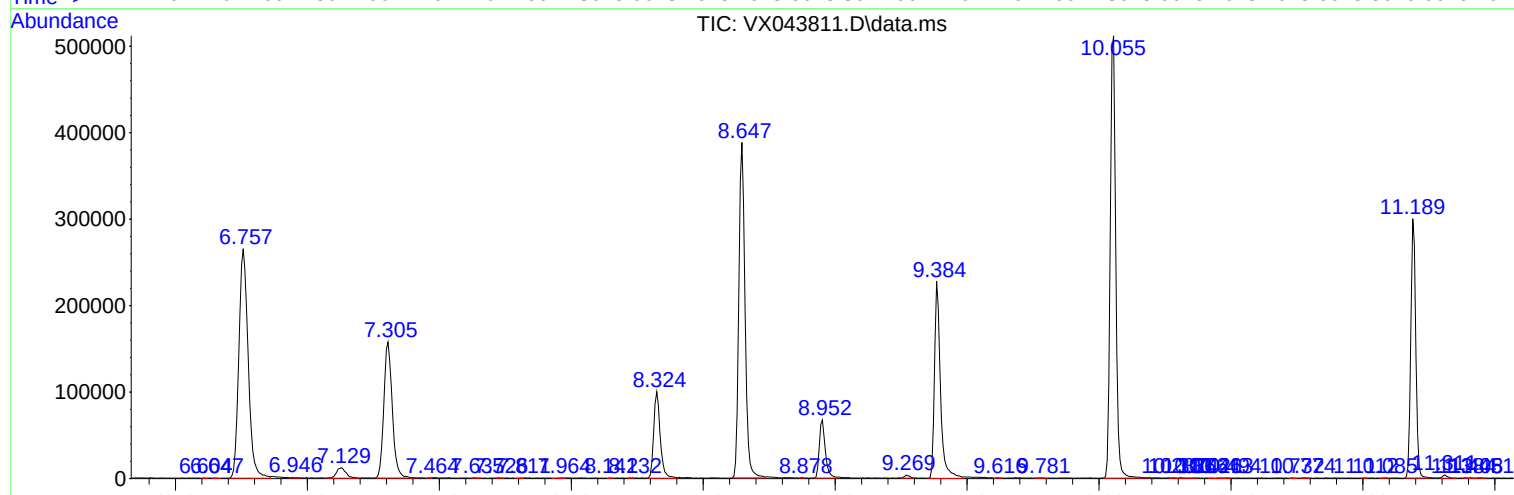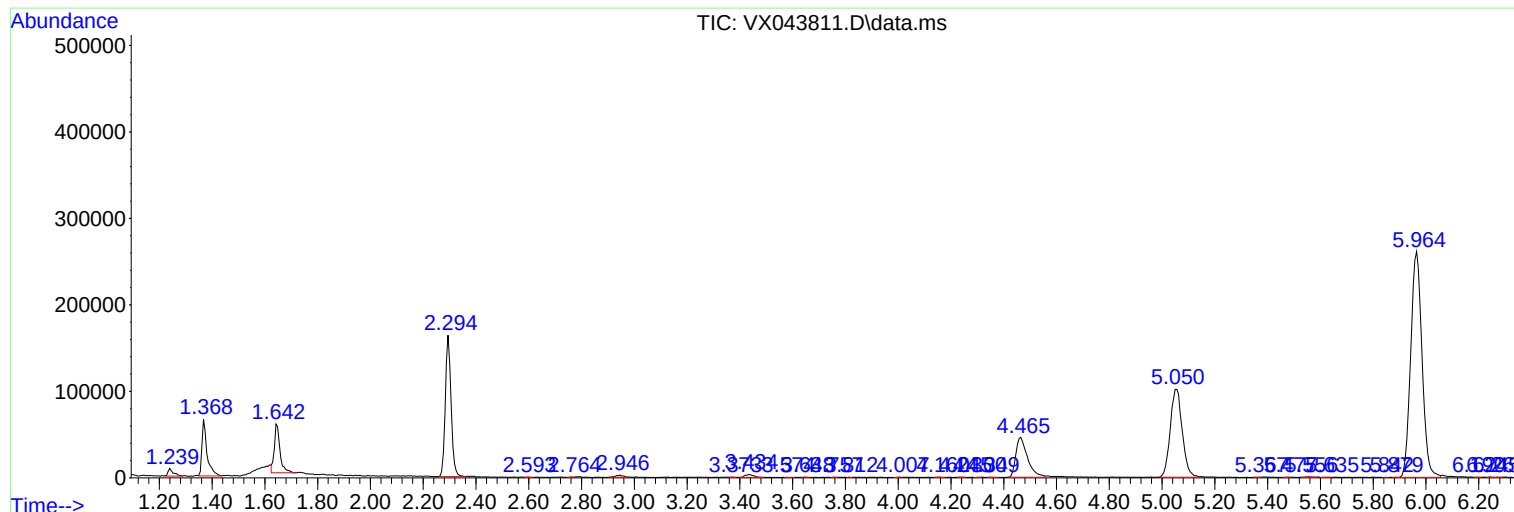

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043811.D
Acq On : 12 Nov 2024 15:31
Operator : JC/MD
Sample : P4786-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27M5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043811.D
Acq On : 12 Nov 2024 15:31
Operator : JC/MD
Sample : P4786-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27M5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------