

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043823.D
 Acq On : 12 Nov 2024 20:08
 Operator : JC/MD
 Sample : P4785-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27L1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043823.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	31	rBV	11915	15683	2.12%	0.254%
2	1.368	42	46	57	rBV	63822	79958	10.80%	1.293%
3	1.642	88	91	104	rVB	56056	87633	11.84%	1.418%
4	2.294	192	198	209	rBV	145373	228142	30.82%	3.690%
5	2.483	228	229	230	rBV	425	264	0.04%	0.004%
6	2.636	251	254	256	rBV3	322	288	0.04%	0.005%
7	2.782	272	278	282	rBV4	850	1655	0.22%	0.027%
8	2.855	288	290	293	rBV2	312	360	0.05%	0.006%
9	2.934	298	303	311	rVV2	3402	7732	1.04%	0.125%
10	3.093	326	329	331	rVB2	278	277	0.04%	0.004%
11	3.245	352	354	357	rVB	408	417	0.06%	0.007%
12	3.440	380	386	391	rVB5	2876	6083	0.82%	0.098%
13	3.520	396	399	402	rBV2	416	483	0.07%	0.008%
14	3.587	408	410	411	rBV	387	286	0.04%	0.005%
15	3.721	430	432	437	rVB3	204	285	0.04%	0.005%
16	3.764	437	439	443	rBV3	255	281	0.04%	0.005%
17	4.166	502	505	506	rBV	326	319	0.04%	0.005%
18	4.251	518	519	523	rVB2	303	299	0.04%	0.005%
19	4.288	523	525	528	rBV2	455	474	0.06%	0.008%
20	4.465	546	554	571	rBV	43923	141521	19.12%	2.289%
21	4.654	583	585	587	rBV2	695	478	0.06%	0.008%
22	4.757	601	602	607	rBV3	524	700	0.09%	0.011%
23	4.885	621	623	626	rBV2	406	518	0.07%	0.008%
24	5.050	638	650	667	rBV	102175	309335	41.79%	5.004%
25	5.318	691	694	696	rBV2	358	354	0.05%	0.006%
26	5.410	707	709	712	rBV2	316	344	0.05%	0.006%
27	5.574	733	736	737	rBV2	314	288	0.04%	0.005%
28	5.964	789	800	820	rVV3	244635	740160	100.00%	11.973%
29	6.355	862	864	867	rBV2	347	372	0.05%	0.006%
30	6.464	878	882	885	rBV2	302	389	0.05%	0.006%
31	6.544	891	895	896	rBV2	486	542	0.07%	0.009%
32	6.580	899	901	903	rVB	391	323	0.04%	0.005%
33	6.757	921	930	945	rBV	260307	633824	85.63%	10.253%
34	6.970	963	965	967	rBV2	453	476	0.06%	0.008%
35	7.129	983	991	1003	rBV5	6320	15894	2.15%	0.257%
36	7.306	1012	1020	1039	rBV	149339	335356	45.31%	5.425%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043823.D
 Acq On : 12 Nov 2024 20:08
 Operator : JC/MD
 Sample : P4785-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27L1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.482	1046	1049	1051	rBV5	634	661	0.09%	0.011%
38	7.653	1074	1077	1078	rBV2	298	371	0.05%	0.006%
39	7.775	1096	1097	1099	rBV	417	295	0.04%	0.005%
40	8.019	1134	1137	1138	rBV2	264	266	0.04%	0.004%
41	8.324	1181	1187	1201	rBV	91114	158544	21.42%	2.565%
42	8.507	1213	1217	1218	rBV2	445	492	0.07%	0.008%
43	8.525	1218	1220	1222	rVV	266	308	0.04%	0.005%
44	8.647	1233	1240	1255	rBV	377668	600993	81.20%	9.722%
45	8.952	1284	1290	1306	rVV	63633	102120	13.80%	1.652%
46	9.092	1312	1313	1317	rVB2	449	315	0.04%	0.005%
47	9.177	1325	1327	1334	rVB2	276	363	0.05%	0.006%
48	9.232	1334	1336	1338	rBV	348	292	0.04%	0.005%
49	9.275	1338	1343	1348	rBV2	3317	5082	0.69%	0.082%
50	9.385	1356	1361	1377	rBV	230207	352291	47.60%	5.699%
51	9.659	1404	1406	1409	rBV2	487	606	0.08%	0.010%
52	9.866	1438	1440	1443	rBV2	298	373	0.05%	0.006%
53	9.903	1443	1446	1447	rBV2	461	376	0.05%	0.006%
54	10.049	1465	1470	1487	rBV	520157	739758	99.95%	11.967%
55	10.305	1508	1512	1516	rBV4	652	1056	0.14%	0.017%
56	10.543	1549	1551	1554	rBV2	384	337	0.05%	0.005%
57	10.744	1582	1584	1585	rBV	534	265	0.04%	0.004%
58	10.896	1607	1609	1613	rBV2	296	424	0.06%	0.007%
59	10.970	1620	1621	1623	rVB	689	280	0.04%	0.005%
60	11.000	1623	1626	1628	rBV	350	353	0.05%	0.006%
61	11.134	1646	1648	1652	rVB3	307	360	0.05%	0.006%
62	11.189	1652	1657	1670	rBV	296678	392131	52.98%	6.343%
63	11.311	1673	1677	1683	rVB4	2983	4488	0.61%	0.073%
64	11.457	1700	1701	1705	rVB2	419	298	0.04%	0.005%
65	11.604	1722	1725	1728	rBV2	278	328	0.04%	0.005%
66	11.683	1736	1738	1739	rBV2	375	279	0.04%	0.005%
67	11.707	1739	1742	1744	rVV2	425	410	0.06%	0.007%
68	11.750	1748	1749	1751	rBV	380	286	0.04%	0.005%
69	11.817	1758	1760	1763	rBV3	377	323	0.04%	0.005%
70	11.933	1776	1779	1781	rVB3	305	286	0.04%	0.005%
71	11.957	1781	1783	1784	rBV	372	301	0.04%	0.005%
72	11.976	1784	1786	1788	rVV2	494	420	0.06%	0.007%
73	12.018	1788	1793	1808	rVV	504240	657379	88.82%	10.634%
74	12.317	1837	1842	1855	rBV	414861	534470	72.21%	8.646%
75	12.738	1907	1911	1912	rBV2	413	394	0.05%	0.006%
76	12.762	1912	1915	1919	rVV3	853	1179	0.16%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043823.D
 Acq On : 12 Nov 2024 20:08
 Operator : JC/MD
 Sample : P4785-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27L1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

77	12.829	1923	1926	1928	rBV2	400	401	0.05%	0.006%
78	13.012	1952	1956	1958	rBV	399	345	0.05%	0.006%
79	13.244	1991	1994	1996	rBV2	251	373	0.05%	0.006%
80	13.335	2007	2009	2013	rBV2	290	380	0.05%	0.006%
81	13.420	2022	2023	2026	rBV	343	280	0.04%	0.005%
82	13.506	2034	2037	2039	rBV2	358	423	0.06%	0.007%
83	13.567	2044	2047	2048	rBV2	548	580	0.08%	0.009%
84	13.792	2083	2084	2086	rBV2	518	336	0.05%	0.005%
85	14.012	2116	2120	2121	rVB2	468	499	0.07%	0.008%
86	14.036	2121	2124	2125	rBV2	311	316	0.04%	0.005%
87	14.128	2136	2139	2143	rBV3	987	1308	0.18%	0.021%
88	14.445	2189	2191	2193	rVV2	415	300	0.04%	0.005%
89	14.499	2198	2200	2202	rBV2	299	326	0.04%	0.005%
90	14.628	2219	2221	2225	rBV4	320	340	0.05%	0.005%
91	15.091	2295	2297	2298	rBV	447	287	0.04%	0.005%
92	15.249	2322	2323	2325	rVB2	594	313	0.04%	0.005%
93	15.371	2341	2343	2344	rBV	578	329	0.04%	0.005%
94	15.652	2387	2389	2390	rBV2	494	362	0.05%	0.006%
95	15.713	2397	2399	2401	rBV3	518	625	0.08%	0.010%
96	15.920	2432	2433	2435	rBV2	534	446	0.06%	0.007%
97	16.078	2457	2459	2461	rVB3	544	455	0.06%	0.007%
98	16.188	2475	2477	2478	rBV	455	291	0.04%	0.005%
99	16.304	2495	2496	2501	rBV3	487	588	0.08%	0.010%
100	16.761	2568	2571	2573	rBV2	518	649	0.09%	0.010%

Sum of corrected areas: 6181898




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043823.D
Acq On : 12 Nov 2024 20:08
Operator : JC/MD
Sample : P4785-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27L1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

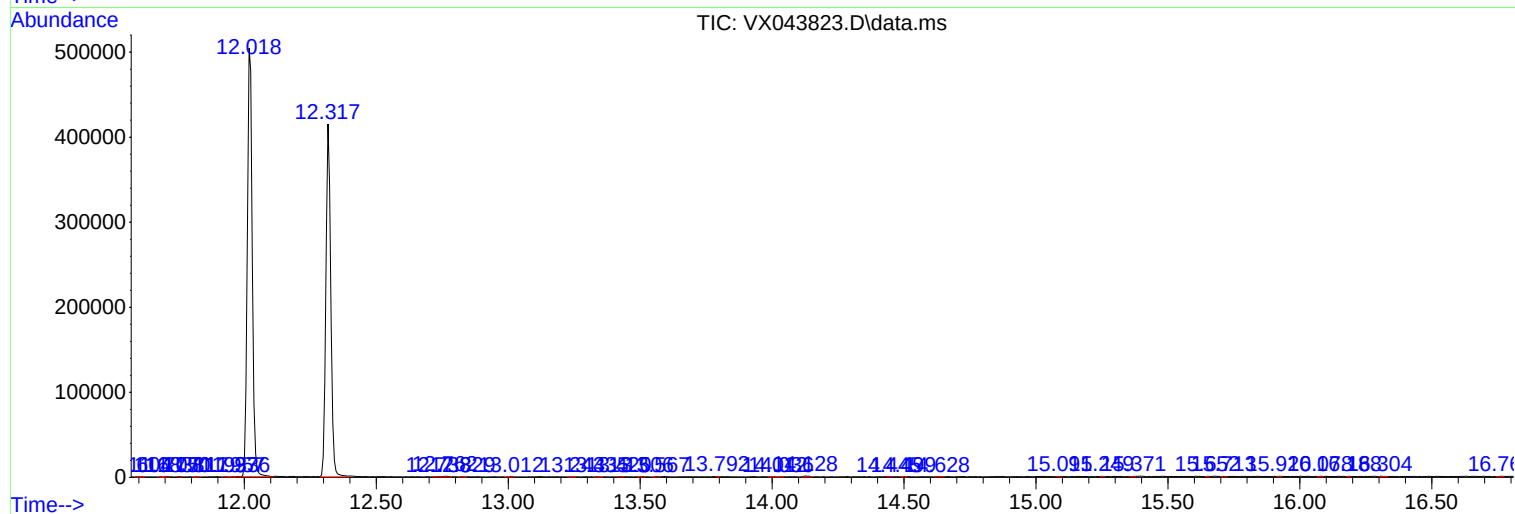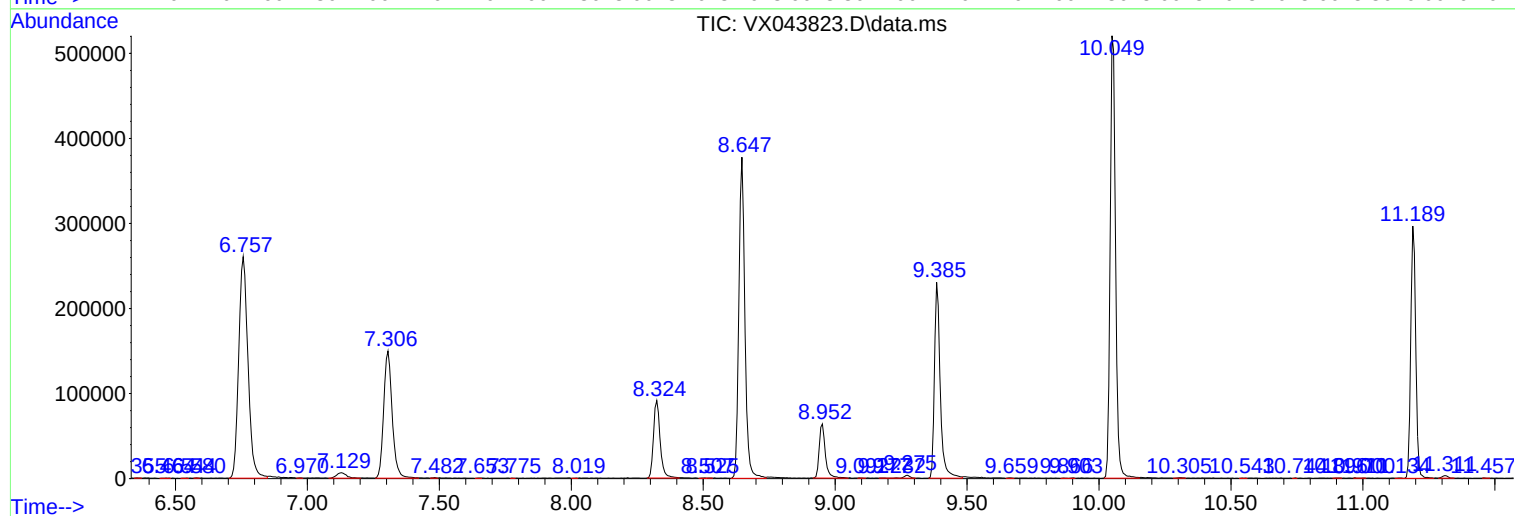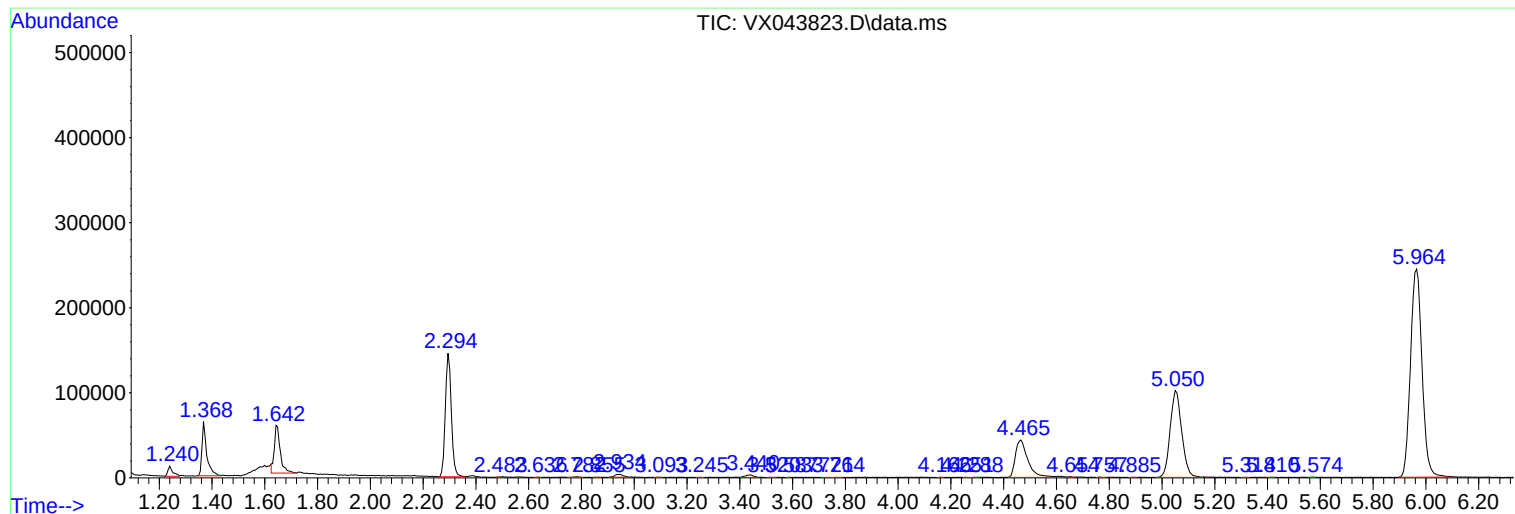

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043823.D
Acq On : 12 Nov 2024 20:08
Operator : JC/MD
Sample : P4785-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27L1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043823.D
Acq On : 12 Nov 2024 20:08
Operator : JC/MD
Sample : P4785-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27L1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc