

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043825.D
 Acq On : 12 Nov 2024 20:54
 Operator : JC/MD
 Sample : P4785-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27L3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043825.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	12	rBB3	1666	1234	0.17%	0.020%
2	1.240	22	25	32	rBV	23968	28871	3.95%	0.477%
3	1.368	43	46	58	rVB	61860	77441	10.58%	1.279%
4	1.642	88	91	101	rVB	53692	89558	12.24%	1.479%
5	2.294	190	198	209	rBV	143341	224549	30.69%	3.709%
6	2.550	237	240	241	rBV2	447	539	0.07%	0.009%
7	2.617	250	251	253	rBV2	451	344	0.05%	0.006%
8	2.770	274	276	277	rBV2	676	426	0.06%	0.007%
9	2.941	297	304	313	rVV2	5101	11785	1.61%	0.195%
10	3.117	330	333	334	rBV	303	323	0.04%	0.005%
11	3.325	366	367	370	rBV2	419	321	0.04%	0.005%
12	3.434	380	385	394	rVB4	3078	6786	0.93%	0.112%
13	3.684	423	426	428	rBV	338	394	0.05%	0.007%
14	3.831	449	450	452	rBV2	365	346	0.05%	0.006%
15	4.184	506	508	510	rVV	314	283	0.04%	0.005%
16	4.264	519	521	524	rVB2	244	275	0.04%	0.005%
17	4.306	524	528	529	rBV3	278	283	0.04%	0.005%
18	4.459	544	553	571	rBV	41791	133738	18.28%	2.209%
19	4.721	594	596	601	rVB3	329	365	0.05%	0.006%
20	4.782	603	606	608	rVB3	337	349	0.05%	0.006%
21	4.837	612	615	616	rBV3	357	379	0.05%	0.006%
22	5.050	637	650	668	rBV	99901	306222	41.85%	5.058%
23	5.233	678	680	681	rVB2	583	410	0.06%	0.007%
24	5.282	685	688	691	rVB2	486	450	0.06%	0.007%
25	5.385	703	705	708	rVB2	282	285	0.04%	0.005%
26	5.556	730	733	735	rBV2	353	358	0.05%	0.006%
27	5.580	735	737	739	rVV2	355	308	0.04%	0.005%
28	5.617	741	743	745	rVB	297	300	0.04%	0.005%
29	5.666	750	751	755	rVV3	374	351	0.05%	0.006%
30	5.757	763	766	768	rBV2	307	316	0.04%	0.005%
31	5.964	788	800	818	rBV2	242348	731664	100.00%	12.086%
32	6.196	836	838	842	rVB4	423	380	0.05%	0.006%
33	6.385	866	869	871	rVV3	402	462	0.06%	0.008%
34	6.428	874	876	880	rVB2	286	326	0.04%	0.005%
35	6.562	897	898	906	rBV3	226	462	0.06%	0.008%
36	6.623	906	908	910	rBV2	304	303	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043825.D
 Acq On : 12 Nov 2024 20:54
 Operator : JC/MD
 Sample : P4785-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27L3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

37	6.757	921	930	946	rBV	257759	618329	84.51%	10.214%
38	7.129	983	991	998	rBV6	5464	14429	1.97%	0.238%
39	7.306	1011	1020	1038	rBV	146512	332634	45.46%	5.494%
40	7.562	1061	1062	1065	rBV	449	416	0.06%	0.007%
41	7.665	1076	1079	1081	rVB3	250	291	0.04%	0.005%
42	7.696	1081	1084	1085	rBV2	332	346	0.05%	0.006%
43	7.757	1092	1094	1099	rVV2	421	539	0.07%	0.009%
44	7.848	1107	1109	1111	rVB2	335	275	0.04%	0.005%
45	7.958	1123	1127	1129	rBV3	310	453	0.06%	0.007%
46	8.068	1142	1145	1146	rBV2	332	319	0.04%	0.005%
47	8.135	1154	1156	1158	rBV2	310	273	0.04%	0.005%
48	8.324	1181	1187	1204	rBV	90456	155697	21.28%	2.572%
49	8.549	1222	1224	1228	rVB2	588	566	0.08%	0.009%
50	8.586	1228	1230	1233	rBV2	404	554	0.08%	0.009%
51	8.647	1233	1240	1255	rBV	363087	589747	80.60%	9.741%
52	8.952	1285	1290	1300	rBV	64109	98507	13.46%	1.627%
53	9.061	1306	1308	1311	rBV2	268	396	0.05%	0.007%
54	9.275	1338	1343	1347	rVV2	3468	5456	0.75%	0.090%
55	9.385	1356	1361	1382	rBV	214909	330234	45.13%	5.455%
56	9.635	1398	1402	1405	rVB3	345	526	0.07%	0.009%
57	9.756	1420	1422	1424	rVB	444	331	0.05%	0.005%
58	9.842	1435	1436	1437	rBV	491	276	0.04%	0.005%
59	10.055	1465	1471	1485	rBV	492434	713504	97.52%	11.786%
60	10.317	1509	1514	1518	rBV3	699	1395	0.19%	0.023%
61	10.360	1520	1521	1526	rBV2	504	373	0.05%	0.006%
62	10.543	1549	1551	1553	rBV2	340	285	0.04%	0.005%
63	10.653	1565	1569	1572	rVB3	367	491	0.07%	0.008%
64	11.116	1642	1645	1648	rBV2	427	394	0.05%	0.007%
65	11.189	1652	1657	1670	rVV	294949	380744	52.04%	6.289%
66	11.317	1673	1678	1682	rVB	3895	5584	0.76%	0.092%
67	11.348	1682	1683	1686	rBV3	318	281	0.04%	0.005%
68	11.433	1695	1697	1700	rBV	211	285	0.04%	0.005%
69	11.463	1700	1702	1706	rVB2	574	467	0.06%	0.008%
70	11.524	1709	1712	1713	rBV	403	302	0.04%	0.005%
71	11.543	1713	1715	1719	rVB2	316	358	0.05%	0.006%
72	11.969	1784	1785	1788	rBV2	329	318	0.04%	0.005%
73	12.018	1788	1793	1808	rVV	499428	639489	87.40%	10.563%
74	12.189	1819	1821	1825	rVB4	426	483	0.07%	0.008%
75	12.317	1837	1842	1851	rBV	418062	523021	71.48%	8.639%
76	12.494	1869	1871	1874	rBV2	293	381	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
 Data File : VX043825.D
 Acq On : 12 Nov 2024 20:54
 Operator : JC/MD
 Sample : P4785-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27L3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

77	12.756	1910	1914	1916	rBV3	1010	1393	0.19%	0.023%
78	12.902	1935	1938	1943	rBV3	240	468	0.06%	0.008%
79	13.128	1972	1975	1976	rBV2	345	373	0.05%	0.006%
80	13.225	1989	1991	1996	rBV3	301	495	0.07%	0.008%
81	13.280	1998	2000	2007	rVV2	245	345	0.05%	0.006%
82	13.786	2079	2083	2085	rVV3	570	780	0.11%	0.013%
83	13.817	2086	2088	2090	rVV2	643	431	0.06%	0.007%
84	13.896	2097	2101	2104	rVB2	413	615	0.08%	0.010%
85	13.933	2104	2107	2109	rBV3	506	521	0.07%	0.009%
86	14.128	2135	2139	2143	rBV5	491	945	0.13%	0.016%
87	14.329	2170	2172	2173	rVB2	496	293	0.04%	0.005%
88	14.457	2191	2193	2194	rBV	375	273	0.04%	0.005%
89	14.518	2201	2203	2205	rVB2	466	397	0.05%	0.007%
90	14.536	2205	2206	2210	rBV2	641	674	0.09%	0.011%
91	14.628	2218	2221	2223	rBV3	410	447	0.06%	0.007%
92	14.853	2256	2258	2262	rVB3	291	378	0.05%	0.006%
93	15.036	2286	2288	2291	rVB3	657	493	0.07%	0.008%
94	15.073	2293	2294	2296	rBV2	554	318	0.04%	0.005%
95	15.243	2320	2322	2326	rBV3	482	675	0.09%	0.011%
96	15.426	2350	2352	2356	rVB3	603	632	0.09%	0.010%
97	15.463	2356	2358	2359	rBV	698	312	0.04%	0.005%
98	15.804	2412	2414	2415	rVB	807	425	0.06%	0.007%
99	16.255	2483	2488	2491	rBV3	802	1534	0.21%	0.025%
100	16.621	2544	2548	2550	rBV3	670	837	0.11%	0.014%




Sum of corrected areas: 6053989

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043825.D
Acq On : 12 Nov 2024 20:54
Operator : JC/MD
Sample : P4785-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27L3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

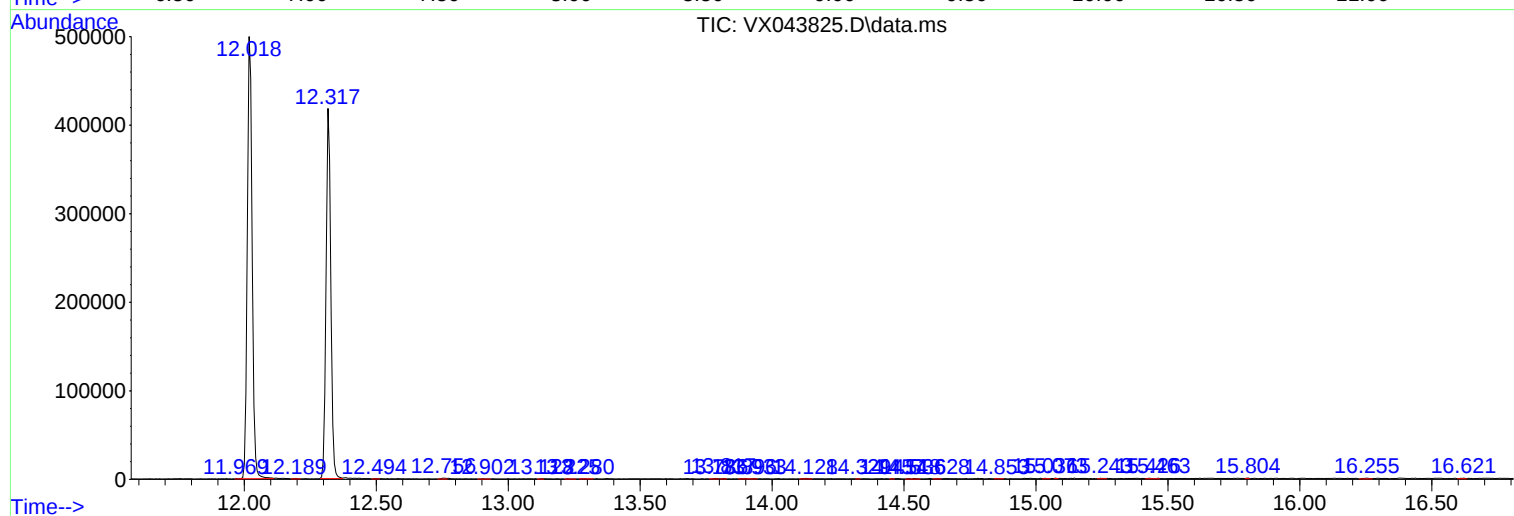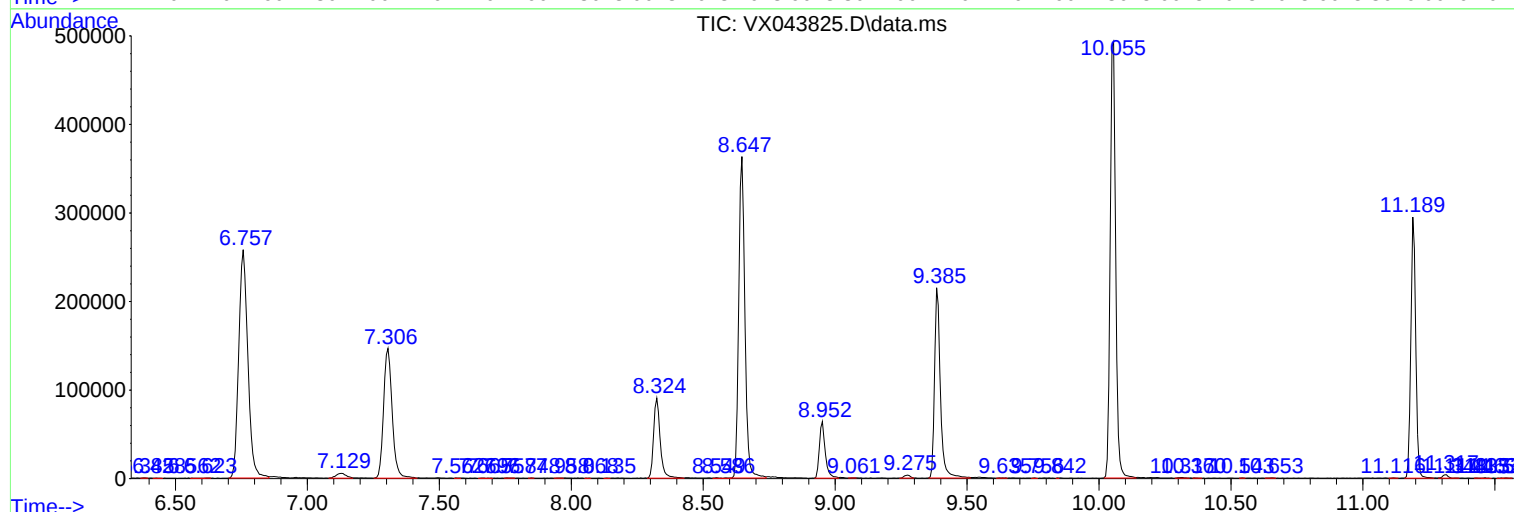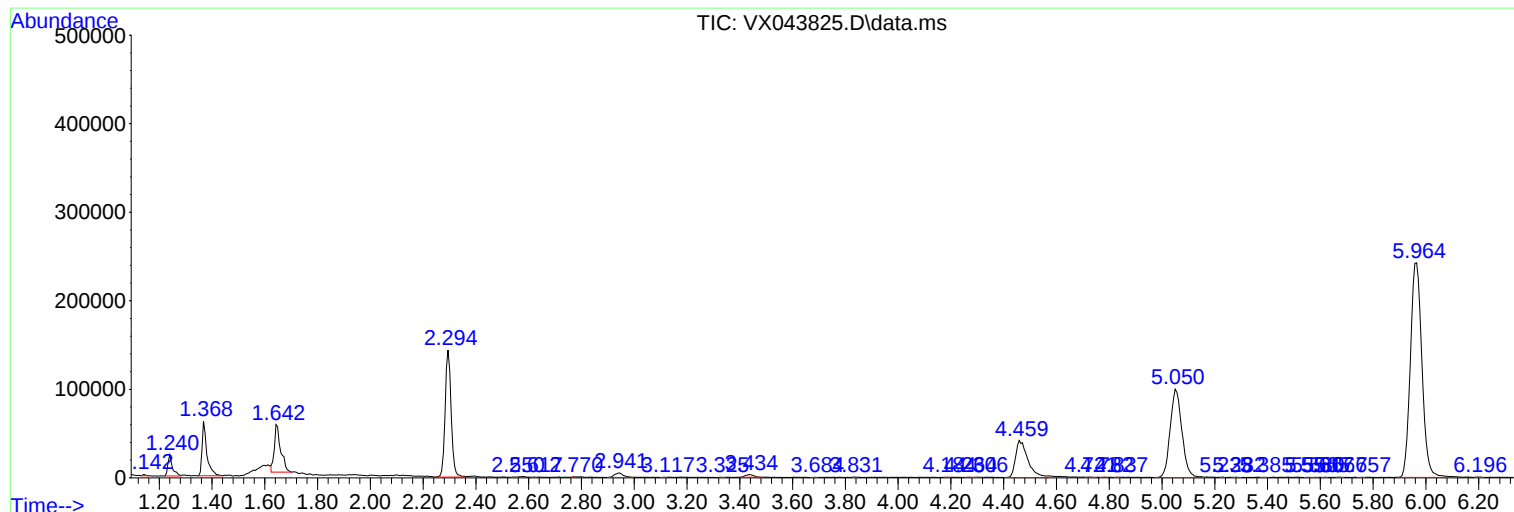

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043825.D
Acq On : 12 Nov 2024 20:54
Operator : JC/MD
Sample : P4785-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27L3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043825.D
Acq On : 12 Nov 2024 20:54
Operator : JC/MD
Sample : P4785-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27L3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc