
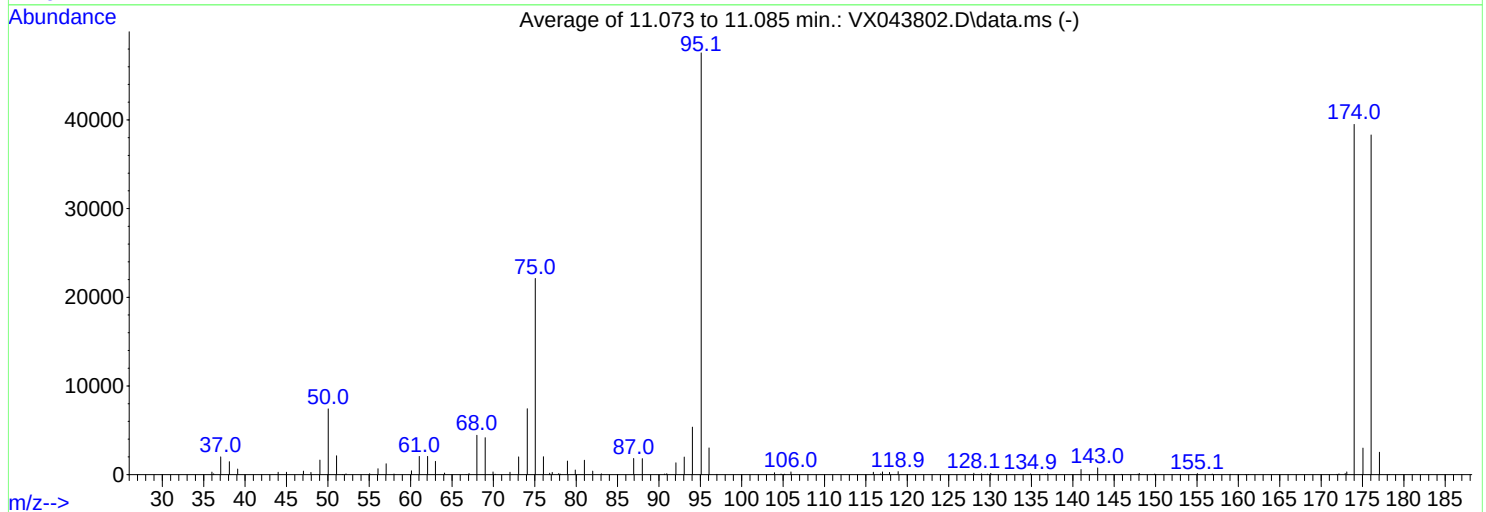


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111224\
Data File : VX043802.D
Acq On : 12 Nov 2024 09:46
Operator : JC/MD
Sample : BFB697
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB697

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Title : VOC Analysis
Last Update : Wed Nov 13 02:04:29 2024

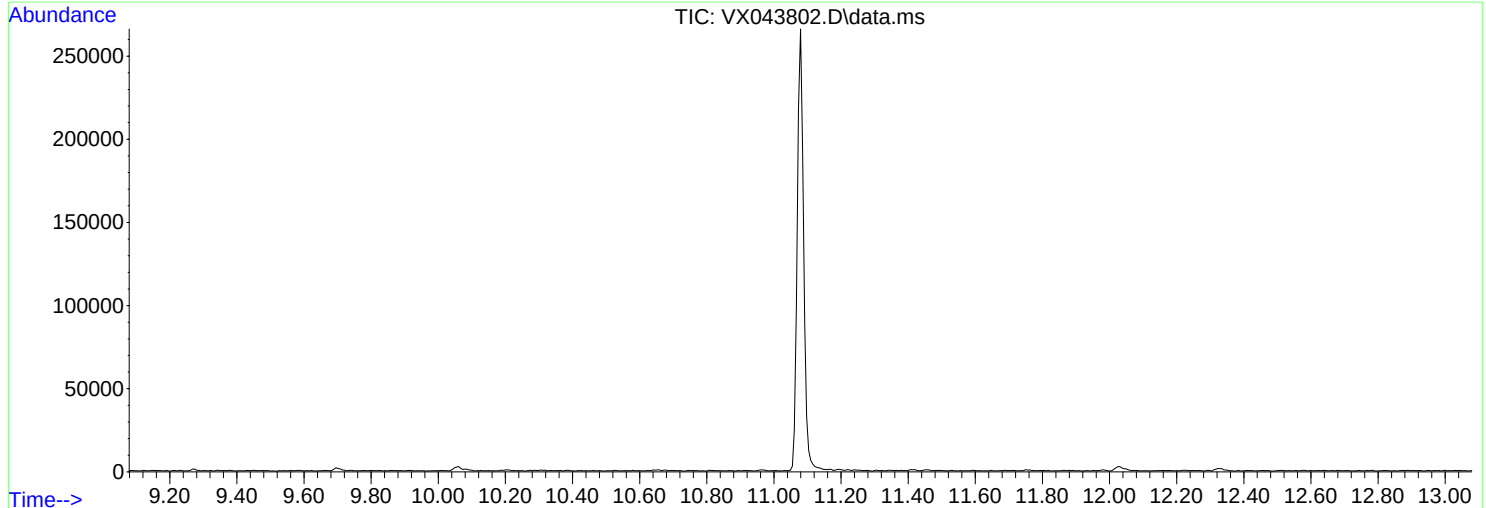

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.6	7415	PASS
75	95	30	80	46.5	22112	PASS
95	95	100	100	100.0	47565	PASS
96	95	5	9	6.3	3009	PASS
173	174	0.00	2	0.8	309	PASS
174	95	50	120	83.0	39499	PASS
175	174	5	9	7.6	3000	PASS
176	174	95	101	97.0	38315	PASS
177	176	5	9	6.6	2527	PASS

m/z	Abundance
39.10	82.0
40.10	518.0
43.90	169.0

Instrument :
MSVOA_X
ClientSampleId :
BFB697

m/z	Abundance
36.10	431.0
37.00	2251.0
38.10	1784.0
39.10	775.0
40.00	516.0
44.20	419.0
44.90	314.0
47.10	486.0
48.00	259.0
49.00	1603.0
50.10	8032.0
51.10	2479.0
52.20	187.0
55.00	85.0
56.10	632.0
57.00	1404.0
58.00	133.0
60.10	539.0
61.10	2183.0
62.00	2250.0
63.00	1752.0
64.10	171.0
67.10	184.0
68.00	5034.0
69.00	4095.0
70.00	471.0
72.00	354.0
73.00	2033.0
74.10	7929.0
75.10	22656.0
76.10	2014.0
77.10	537.0
78.00	161.0
78.90	1585.0
79.90	517.0
81.00	1794.0
82.10	398.0
83.10	100.0
87.00	1841.0
88.00	1793.0
90.70	60.0
91.10	116.0
92.10	1178.0
93.10	1814.0
94.10	5761.0
95.10	46912.0
96.00	3102.0
97.00	84.0
103.90	217.0
105.90	374.0
116.00	253.0
116.80	271.0
117.80	202.0
118.90	381.0
128.00	170.0
129.00	118.0
129.70	160.0
130.20	175.0
136.70	61.0
141.00	523.0
143.00	712.0
147.90	206.0
149.90	81.0
153.00	103.0
155.00	87.0
159.10	74.0
160.90	71.0
171.90	111.0
172.90	388.0
174.00	33328.0
175.10	2619.0
176.00	33840.0
177.10	2198.0
178.20	63.0

Instrument :
MSVOA_X
ClientSampleId :
BFB697

m/z	Abundance
35.90	454.0
37.10	2523.0
38.10	1540.0
39.10	730.0
39.90	434.0
44.00	575.0
45.00	297.0
47.00	428.0
48.00	254.0
49.10	2368.0
50.00	8506.0
51.10	2259.0
52.20	99.0
55.10	144.0
56.00	881.0
57.10	1314.0
58.00	106.0
60.10	555.0
61.00	2570.0
62.10	2355.0
63.00	1995.0
64.10	159.0
67.00	198.0
68.00	4901.0
69.00	4979.0
69.90	156.0
70.20	180.0
71.90	281.0
73.10	2396.0
74.10	8418.0
75.00	25696.0
76.00	2531.0
76.80	464.0
77.80	227.0
78.90	1725.0
79.90	730.0
81.00	1913.0
82.00	491.0
83.00	85.0
87.00	1987.0
88.00	2178.0
90.90	213.0
91.90	1805.0
93.00	2532.0
94.00	6258.0
95.10	55904.0
96.10	3845.0
104.00	231.0
104.70	100.0
105.20	108.0
105.90	292.0
115.90	258.0
117.00	453.0
117.80	316.0
118.90	329.0
128.10	186.0
129.00	73.0
130.00	173.0
134.90	130.0
136.90	94.0
141.00	613.0
143.00	1021.0
145.90	83.0
148.10	270.0
149.90	138.0
155.10	145.0
156.80	104.0
159.00	57.0
172.10	166.0
173.10	319.0
174.00	47504.0
175.00	3799.0
176.00	45456.0
177.00	3250.0

Instrument :
MSVOA_X
ClientSampleId :
BFB697

m/z	Abundance
36.20	253.0
37.00	1253.0
38.00	1071.0
39.10	649.0
40.00	451.0
42.00	68.0
44.00	334.0
45.10	208.0
47.10	293.0
47.80	225.0
49.00	971.0
50.00	5706.0
51.00	1664.0
51.80	64.0
55.10	107.0
56.00	490.0
57.10	992.0
60.00	197.0
61.10	1418.0
62.10	1582.0
62.90	741.0
64.10	192.0
66.70	54.0
68.00	3382.0
69.00	3450.0
69.90	272.0
72.10	205.0
73.00	1607.0
74.10	5953.0
75.00	17984.0
76.10	1507.0
77.10	203.0
78.10	181.0
79.00	1271.0
79.90	302.0
80.90	1169.0
81.90	326.0
83.00	83.0
86.90	1620.0
88.00	1466.0
90.70	169.0
92.10	1032.0
93.00	1638.0
94.10	4087.0
95.10	39880.0
96.10	2081.0
103.90	197.0
104.80	116.0
105.20	80.0
106.00	282.0
115.80	325.0
117.00	451.0
117.90	242.0
118.90	333.0
128.00	148.0
128.90	106.0
130.00	90.0
134.90	141.0
137.00	110.0
141.00	601.0
142.90	567.0
148.00	117.0
155.10	122.0
156.90	97.0
161.20	68.0
172.20	106.0
173.10	608.0
174.00	37664.0
175.10	2581.0
176.10	35648.0
177.00	2132.0

Instrument :
MSVOA_X
ClientSampleId :
BFB697