

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111225\
 Data File : VX048570.D
 Acq On : 12 Nov 2025 11:59
 Operator : JC/MD
 Sample : Q3574-01 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 304641-01 Liquid

Quant Time: Nov 14 00:26:41 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110725W.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 08 05:08:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.538	168	180966	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.745	114	374288	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	398973	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	210340	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	138697	55.003	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	110.000%
35) Dibromofluoromethane	5.379	113	121406	42.857	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	85.720%
50) Toluene-d8	8.635	98	437830	49.555	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	99.120%
62) 4-Bromofluorobenzene	11.061	95	192170	58.365	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	116.720%
Target Compounds						
					Qvalue	
10) Methyl Iodide	2.465	142	799	0.268	ug/l #	89
13) Acrolein	2.227	56	41	0.593	ug/l #	15
16) Acetone	2.373	43	6813	5.708	ug/l	98
17) Carbon Disulfide	2.526	76	1553	0.262	ug/l #	75
18) Methyl Acetate	2.703	43	1008	0.307	ug/l #	79
20) Methylene Chloride	2.782	84	803	0.327	ug/l #	68
25) 2-Butanone	4.586	43	1903	1.078	ug/l #	73
31) Cyclohexane	5.544	56	3368	0.995	ug/l #	1
36) 1,1-Dichloropropene	5.538	75	13815	3.642	ug/l #	49
38) Carbon Tetrachloride	5.538	117	18451	4.273	ug/l #	18
44) Trichloroethene	7.110	130	15611	5.554	ug/l	90
51) 4-Methyl-2-Pentanone	8.567	43	3959	0.927	ug/l	94
52) Toluene	8.702	92	18494	2.987	ug/l	98
55) 1,1,2-Trichloroethane	9.086	97	997	0.403	ug/l #	15
67) Ethyl Benzene	10.177	91	14586	0.917	ug/l	95
68) m/p-Xylenes	10.287	106	24941	4.164	ug/l	94
69) o-Xylene	10.628	106	17583	3.001	ug/l	94
75) 1,1,2,2-Tetrachloroethane	11.201	83	1304	0.242	ug/l #	25
76) 1,2,3-Trichloropropane	11.061	75	92800	18.313	ug/l #	31
78) n-propylbenzene	11.286	91	11305	0.630	ug/l	99
79) 2-Chlorotoluene	11.360	91	6619	0.610	ug/l #	43
80) 1,3,5-Trimethylbenzene	11.433	105	16913	1.359	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.061	75	92800	52.381	ug/l #	12
82) 4-Chlorotoluene	11.439	91	2905	0.228	ug/l #	64
84) 1,2,4-Trimethylbenzene	11.732	105	67514	5.376	ug/l	98
89) n-Butylbenzene	12.311	91	12631	1.007	ug/l #	60
90) Hexachloroethane	12.518	117	1230	0.483	ug/l #	14
93) 1,2,4-Trichlorobenzene	13.573	180	1075	0.228	ug/l #	2
94) Hexachlorobutadiene	13.701	225	417	0.212	ug/l	83
95) Naphthalene	13.756	128	27645	1.824	ug/l #	90
96) 1,2,3-Trichlorobenzene	13.951	180	1447	0.330	ug/l #	13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111225\
Data File : VX048570.D
Acq On : 12 Nov 2025 11:59
Operator : JC/MD
Sample : Q3574-01 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
304641-01 Liquid


Quant Time: Nov 14 00:26:41 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110725W.M
Quant Title : SW846 8260
QLast Update : Sat Nov 08 05:08:11 2025
Response via : Initial Calibration

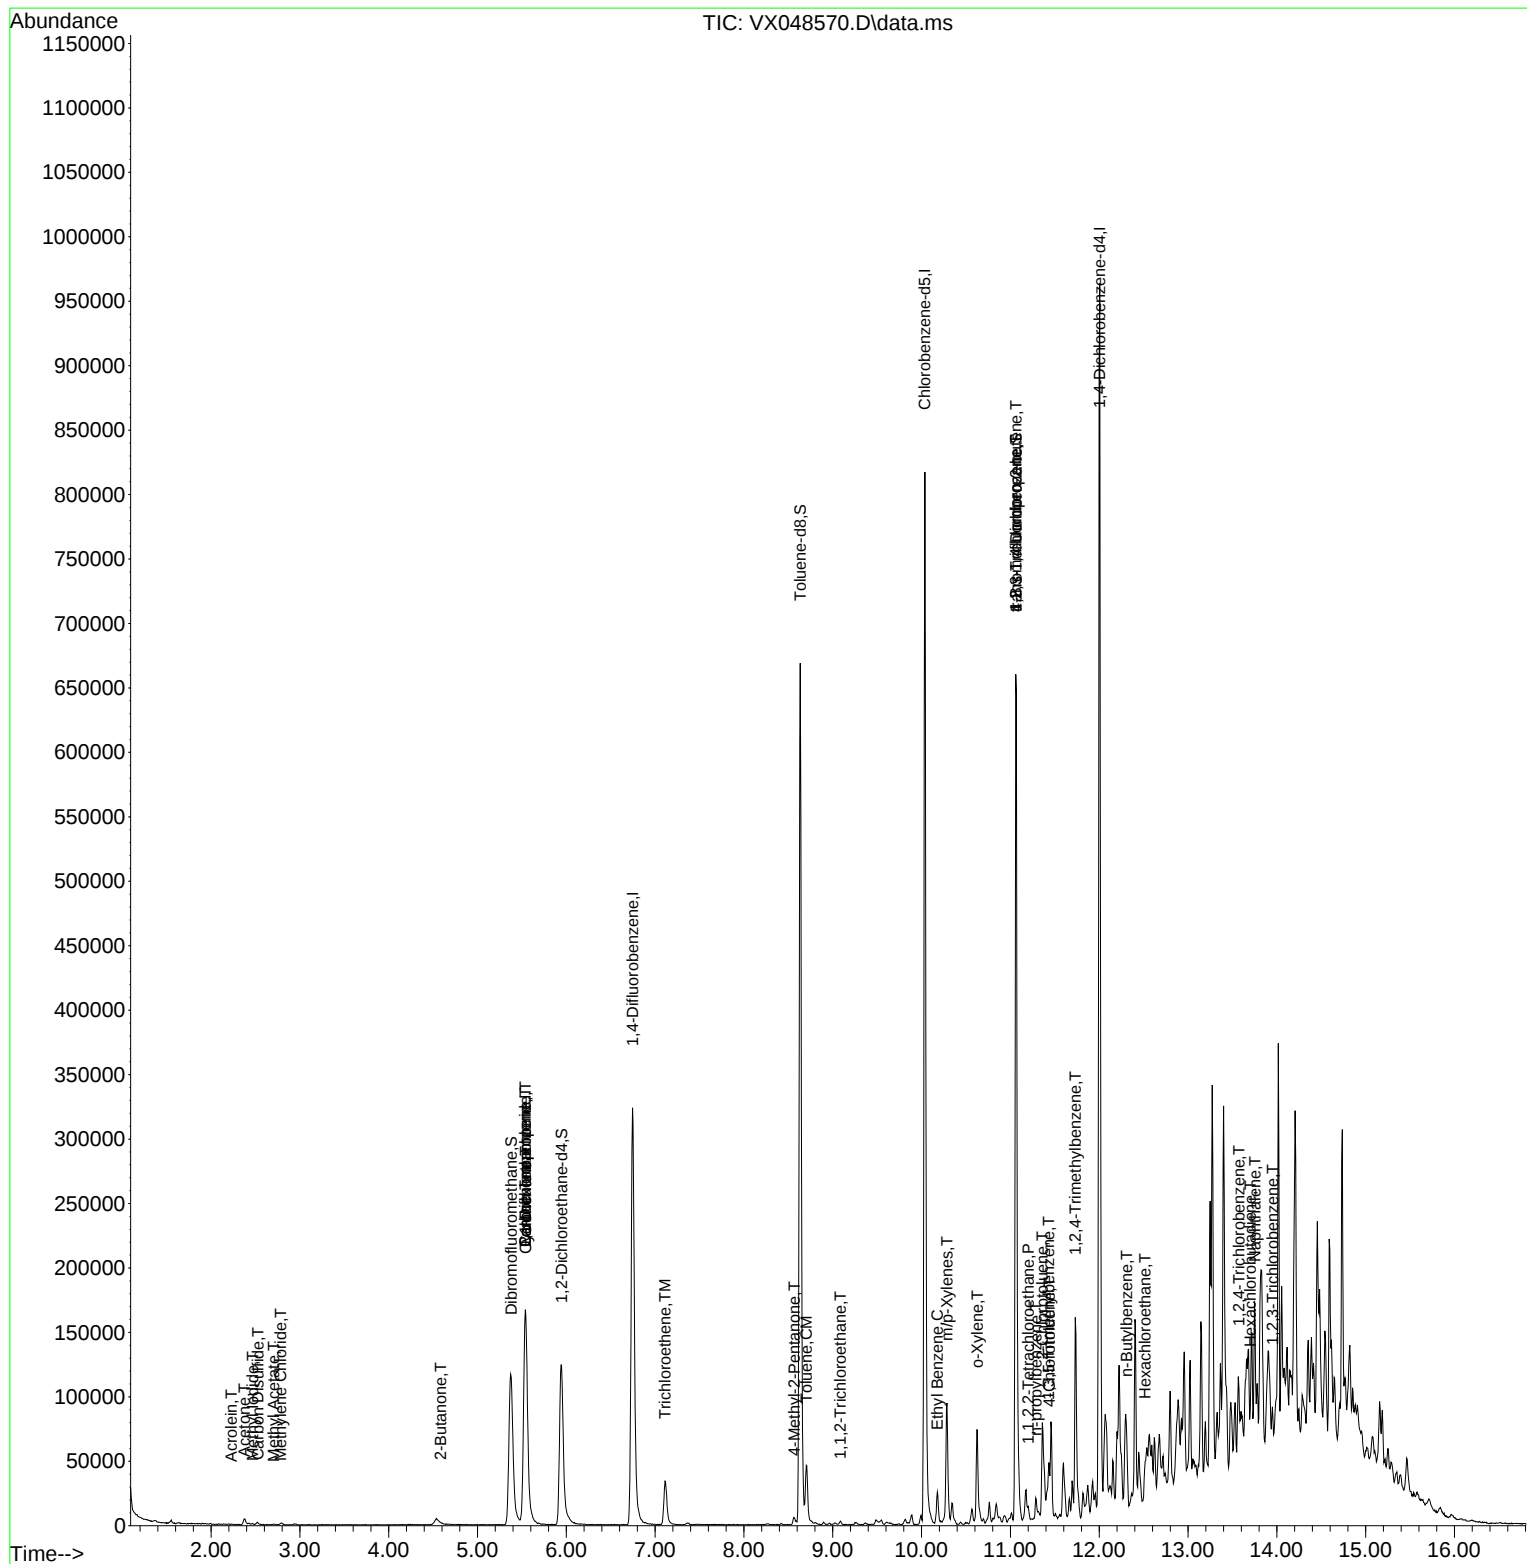



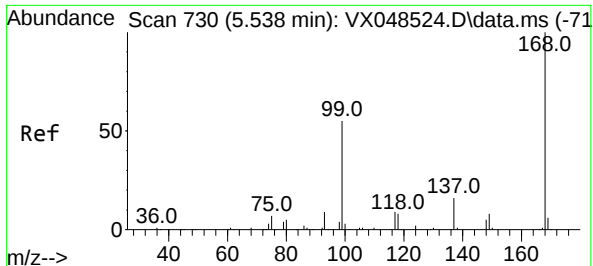


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.538 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59


Instrument :
MSVOA_X
ClientSampleId :
304641-01 Liquid

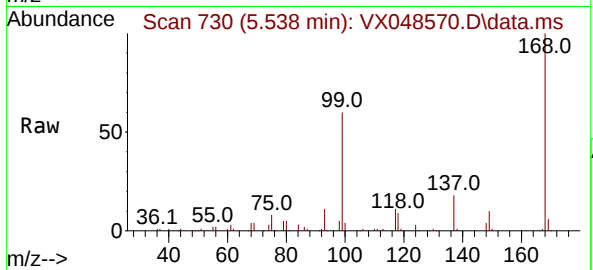



Tgt Ion:168 Resp: 180966
Ion Ratio Lower Upper
168 100
99 60.2 45.2 67.8

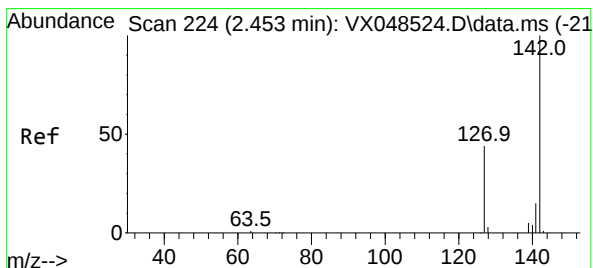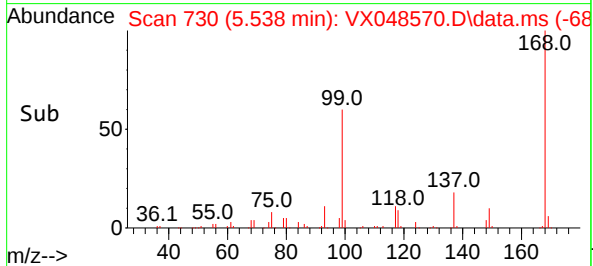


#10
Methyl Iodide
Concen: 0.268 ug/l
RT: 2.465 min Scan# 226
Delta R.T. 0.012 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59

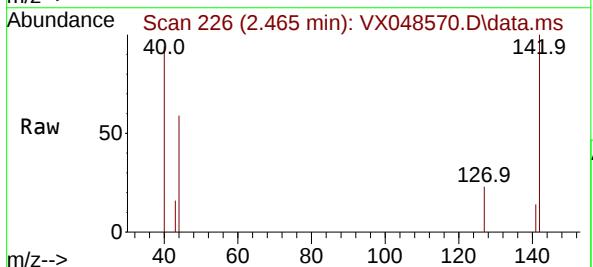

Tgt Ion:142 Resp: 799
Ion Ratio Lower Upper
142 100
127 38.0 35.8 53.6
141 9.0 11.4 17.0#



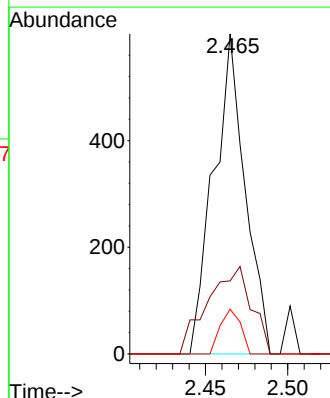
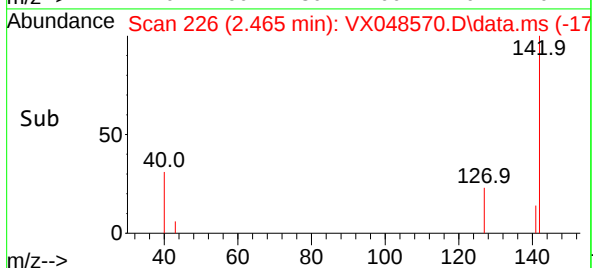




#13
Acrolein
Concen: 0.593 ug/l
RT: 2.227 min Scan# 187
Delta R.T. -0.012 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59




Instrument :
MSVOA_X
ClientSampleId :
304641-01 Liquid


Tgt Ion: 56 Resp: 41
Ion Ratio Lower Upper
56 100
55 0.0 54.9 82.3#



#16
Acetone
Concen: 5.708 ug/l
RT: 2.373 min Scan# 211
Delta R.T. -0.000 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59

Tgt Ion: 43 Resp: 6813
Ion Ratio Lower Upper
43 100
58 33.1 25.8 38.6









#17
Carbon Disulfide
Concen: 0.262 ug/l
RT: 2.526 min Scan# 21
Delta R.T. 0.012 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59




Instrument :
MSVOA_X
ClientSampleId :
304641-01 Liquid


Tgt Ion: 76 Resp: 1553
Ion Ratio Lower Upper
76 100
78 0.0 7.1 10.7#

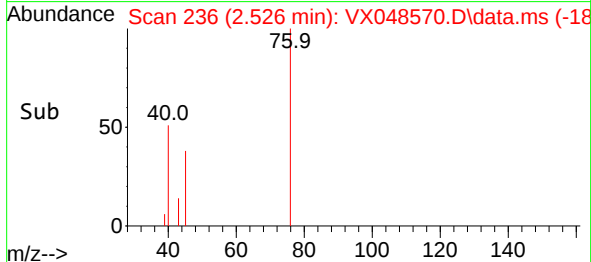

#18
Methyl Acetate
Concen: 0.307 ug/l
RT: 2.703 min Scan# 265
Delta R.T. 0.006 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59


Tgt Ion: 43 Resp: 1008
Ion Ratio Lower Upper
43 100
74 13.4 19.1 28.7#

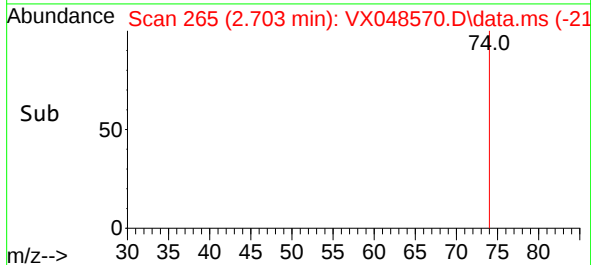






#20
Methylene Chloride
Concen: 0.327 ug/l
RT: 2.782 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59

Instrument :
MSVOA_X
ClientSampleId :
304641-01 Liquid







Tgt Ion: 84	Resp: 803
Ion Ratio	Lower Upper
84 100	
49 71.3	91.2 136.8#
51 23.5	28.3 42.5#
86 42.4	49.4 74.2#



#25
2-Butanone
Concen: 1.078 ug/l
RT: 4.586 min Scan# 574
Delta R.T. 0.049 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59


Tgt Ion: 43	Resp: 1903
Ion Ratio	Lower Upper
43 100	
72 13.0	21.5 32.3#

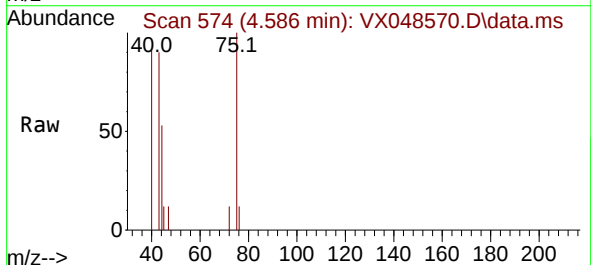






#31
Cyclohexane
Concen: 0.995 ug/l
RT: 5.544 min Scan# 717
Delta R.T. 0.085 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59

Instrument :
MSVOA_X
ClientSampleId :
304641-01 Liquid







Tgt Ion: 56 Resp: 3368
Ion Ratio Lower Upper
56 100
69 172.5 23.4 35.2#
84 129.6 66.3 99.5#



#33
1,2-Dichloroethane-d4
Concen: 55.003 ug/l
RT: 5.946 min Scan# 797
Delta R.T. -0.000 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59

Tgt Ion: 65 Resp: 138697
Ion Ratio Lower Upper
65 100
67 52.9 0.0 106.2


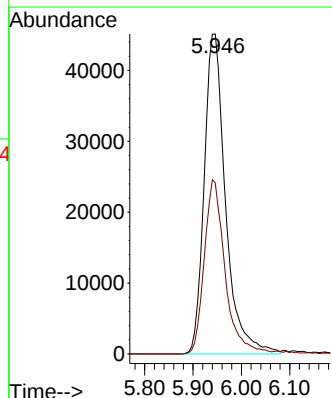






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.745 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59




Instrument :
MSVOA_X
ClientSampleId :
304641-01 Liquid


Tgt Ion:114 Resp: 374288
Ion Ratio Lower Upper
114 100
63 19.6 0.0 41.2
88 16.0 0.0 32.2

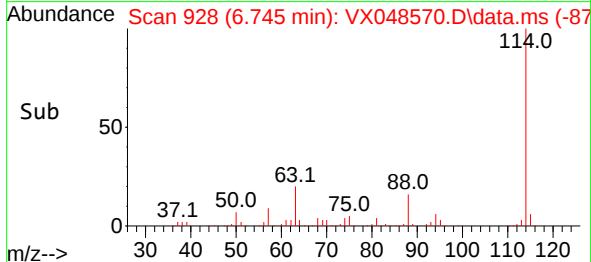

#35
Dibromofluoromethane
Concen: 42.857 ug/l
RT: 5.379 min Scan# 704
Delta R.T. 0.006 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59

Tgt Ion:113 Resp: 121406
Ion Ratio Lower Upper
113 100
111 102.8 81.9 122.9
192 19.8 15.8 23.6




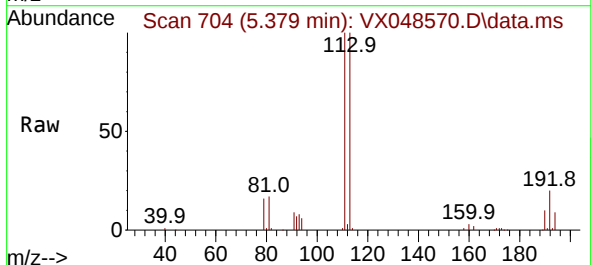




#36
1,1-Dichloropropene
Concen: 3.642 ug/l
RT: 5.538 min Scan# 710
Delta R.T. -0.140 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59




Instrument :
MSVOA_X
ClientSampleId :
304641-01 Liquid


Tgt Ion: 75 Resp: 13815
Ion Ratio Lower Upper
75 100
110 9.1 18.4 55.4#
77 0.0 24.6 37.0#

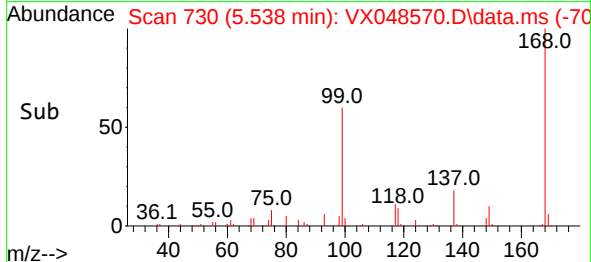

#38
Carbon Tetrachloride
Concen: 4.273 ug/l
RT: 5.538 min Scan# 730
Delta R.T. -0.128 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59

Tgt Ion: 117 Resp: 18451
Ion Ratio Lower Upper
117 100
119 6.1 74.5 111.7#
121 0.0 24.8 37.2#




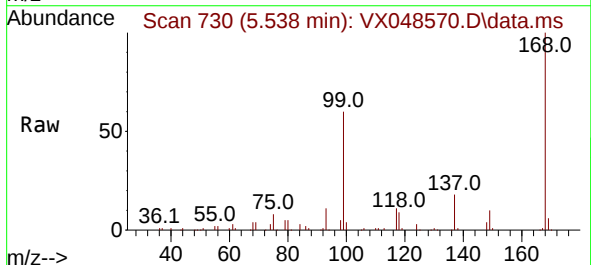




#44
Trichloroethene
Concen: 5.554 ug/l
RT: 7.110 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59




Instrument :
MSVOA_X
ClientSampleId :
304641-01 Liquid


Tgt Ion:130 Resp: 15611
Ion Ratio Lower Upper
130 100
95 104.8 0.0 190.2

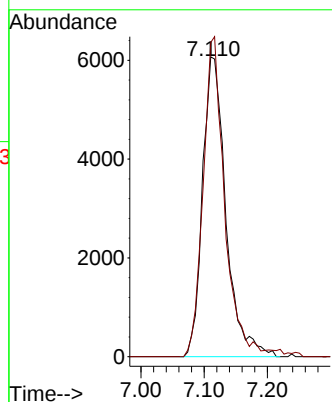

#50
Toluene-d8
Concen: 49.555 ug/l
RT: 8.635 min Scan# 1238
Delta R.T. -0.000 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59

Tgt Ion: 98 Resp: 437830
Ion Ratio Lower Upper
98 100
100 64.8 53.6 80.4









#51
4-Methyl-2-Pentanone
Concen: 0.927 ug/l
RT: 8.567 min Scan# 11
Delta R.T. 0.012 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59




Instrument :
MSVOA_X
ClientSampleId :
304641-01 Liquid


Tgt Ion: 43 Resp: 3959
Ion Ratio Lower Upper
43 100
58 36.5 32.3 48.5

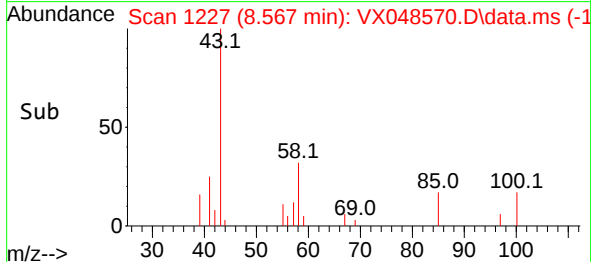

#52
Toluene
Concen: 2.987 ug/l
RT: 8.702 min Scan# 1249
Delta R.T. -0.000 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59

Tgt Ion: 92 Resp: 18494
Ion Ratio Lower Upper
92 100
91 174.4 137.0 205.6




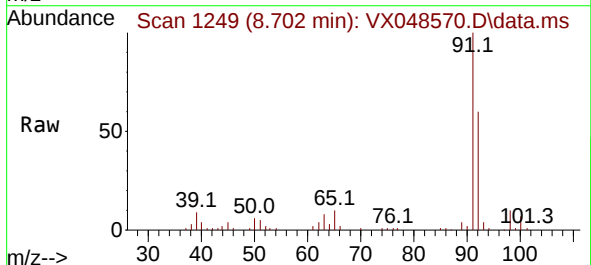




#55
 1,1,2-Trichloroethane
 Concen: 0.403 ug/l
 RT: 9.086 min Scan# 11
 Delta R.T. -0.049 min
 Lab File: VX048570.D
 Acq: 12 Nov 2025 11:59




Instrument :
 MSVOA_X
 ClientSampleId :
 304641-01 Liquid


Tgt Ion: 97	Resp: 997
Ion Ratio	Lower Upper
97 100	
83 0.0	69.2 103.8#
85 0.0	42.8 64.2#
99 0.0	49.7 74.5#

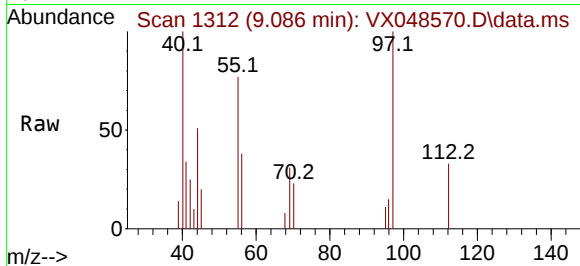

#62
 4-Bromofluorobenzene
 Concen: 58.365 ug/l
 RT: 11.061 min Scan# 1636
 Delta R.T. -0.000 min
 Lab File: VX048570.D
 Acq: 12 Nov 2025 11:59

Tgt Ion: 95	Resp: 192170
Ion Ratio	Lower Upper
95 100	
174 79.9	0.0 161.8
176 75.6	0.0 153.6



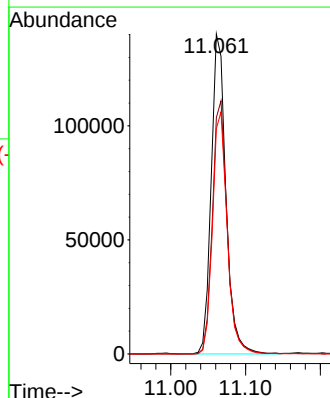
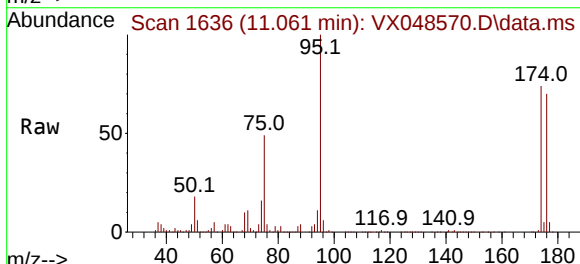




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. -0.000 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59




Instrument :
MSVOA_X
ClientSampleId :
304641-01 Liquid


Tgt Ion:117 Resp: 398973
Ion Ratio Lower Upper
117 100
82 56.2 44.4 66.6
119 32.1 25.1 37.7

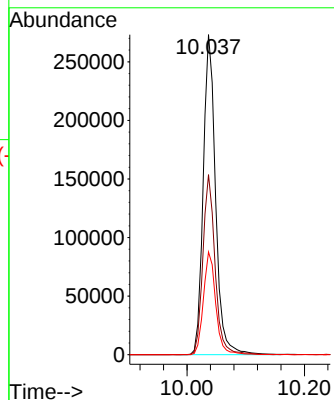

#67
Ethyl Benzene
Concen: 0.917 ug/l
RT: 10.177 min Scan# 1491
Delta R.T. -0.000 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59

Tgt Ion: 91 Resp: 14586
Ion Ratio Lower Upper
91 100
106 32.9 24.1 36.1



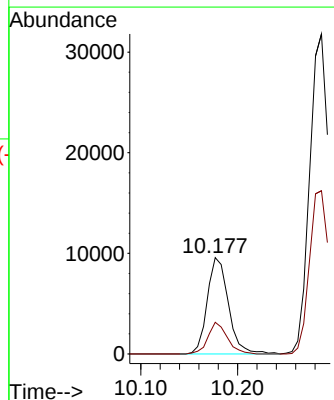





#68
m/p-Xylenes
Concen: 4.164 ug/l
RT: 10.287 min Scan# 1509
Delta R.T. -0.000 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59




Instrument :
MSVOA_X
ClientSampleId :
304641-01 Liquid


Tgt Ion:106 Resp: 24941
Ion Ratio Lower Upper
106 100
91 190.4 159.6 239.4



#69
o-Xylene
Concen: 3.001 ug/l
RT: 10.628 min Scan# 1565
Delta R.T. 0.006 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59

Tgt Ion:106 Resp: 17583
Ion Ratio Lower Upper
106 100
91 222.0 106.4 319.2









#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.006 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX048570.D
 Acq: 12 Nov 2025 11:59




Instrument :
 MSVOA_X
 ClientSampleId :
 304641-01 Liquid


Tgt Ion:152 Resp: 210340
 Ion Ratio Lower Upper
 152 100
 115 58.2 39.2 117.6
 150 155.9 0.0 347.0

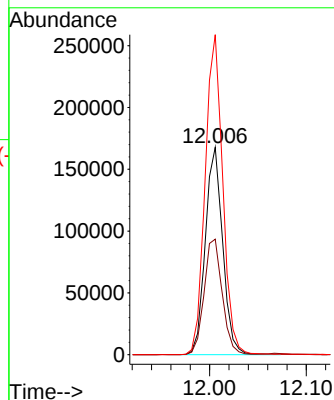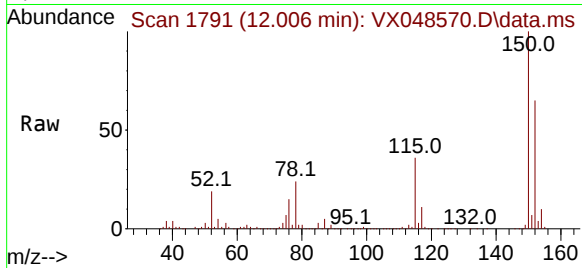

#75
 1,1,2,2-Tetrachloroethane
 Concen: 0.242 ug/l
 RT: 11.201 min Scan# 1659
 Delta R.T. 0.006 min
 Lab File: VX048570.D
 Acq: 12 Nov 2025 11:59

Tgt Ion: 83 Resp: 1304
 Ion Ratio Lower Upper
 83 100
 131 0.0 5.3 15.8#
 85 0.0 32.3 96.8#

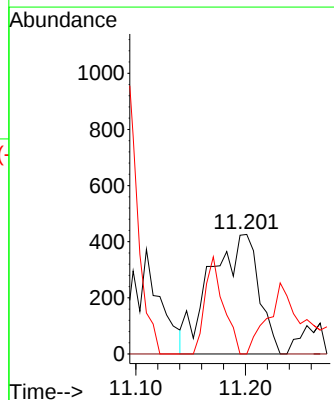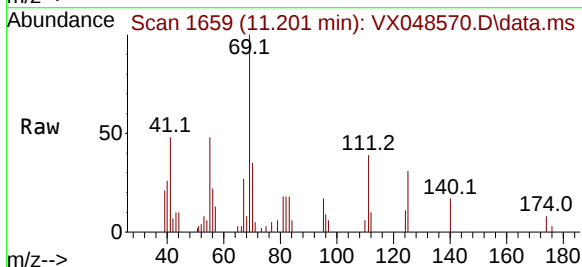



#76

1,2,3-Trichloropropane

Concen: 18.313 ug/l

RT: 11.061 min Scan# 1636

Delta R.T. -0.159 min

Lab File: VX048570.D

Acq: 12 Nov 2025 11:59

Instrument :

MSVOA_X

ClientSampleId :





304641-01 Liquid

Tgt Ion: 75 Resp: 92800

Ion Ratio Lower Upper

75 100

77 1.4 24.3 72.8#

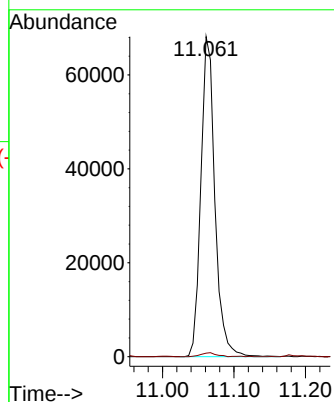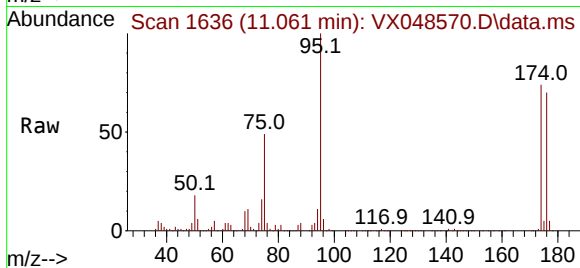

#78

n-propylbenzene

Concen: 0.630 ug/l

RT: 11.286 min Scan# 1673

Delta R.T. -0.000 min

Lab File: VX048570.D




Acq: 12 Nov 2025 11:59


Tgt Ion: 91 Resp: 11305

Ion Ratio Lower Upper

91 100

120 22.6 11.6 34.8


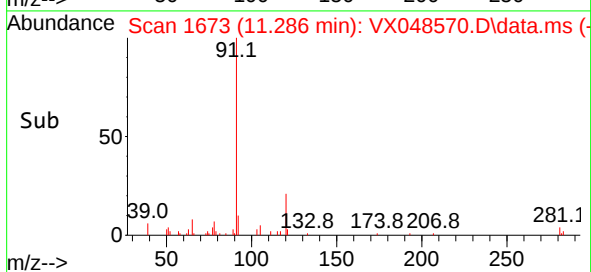
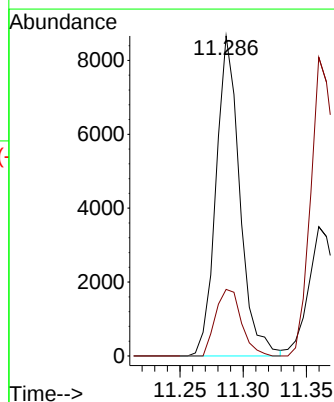
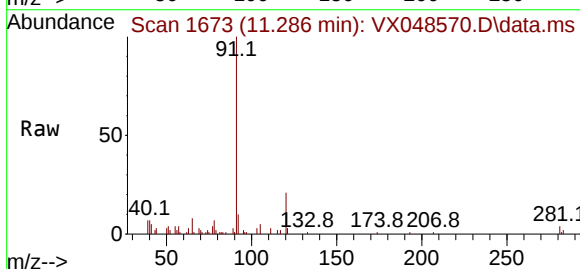




#79
2-Chlorotoluene
Concen: 0.610 ug/l
RT: 11.360 min Scan# 1685
Delta R.T. 0.012 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59




Instrument :
MSVOA_X
ClientSampleId :
304641-01 Liquid


Tgt Ion: 91 Resp: 6619
Ion Ratio Lower Upper
91 100
126 1.6 17.1 51.2#

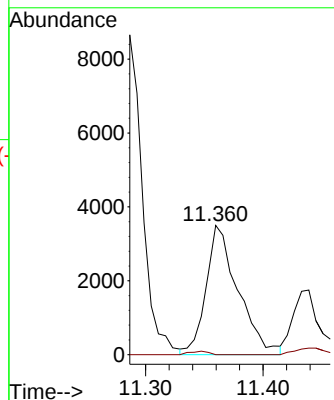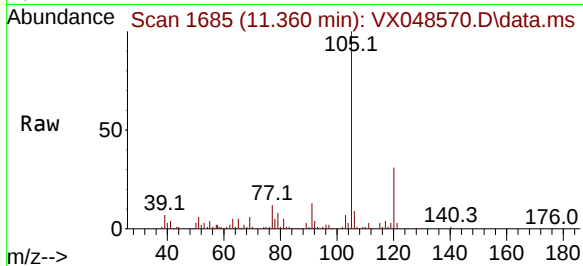

#80
1,3,5-Trimethylbenzene
Concen: 1.359 ug/l
RT: 11.433 min Scan# 1697
Delta R.T. -0.000 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59

Tgt Ion: 105 Resp: 16913
Ion Ratio Lower Upper
105 100
120 48.5 25.1 75.2



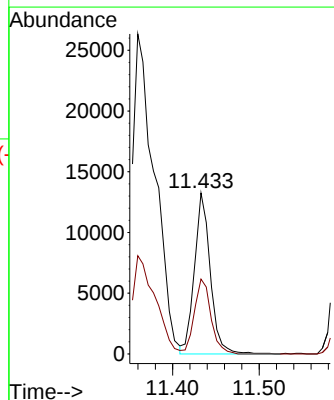
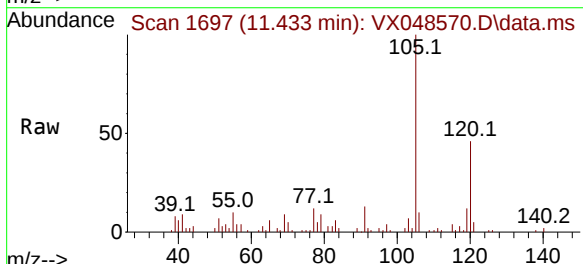




#81
trans-1,4-Dichloro-2-butene
Concen: 52.381 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. 0.061 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59




Instrument :
MSVOA_X
ClientSampleId :
304641-01 Liquid


Tgt Ion: 75 Resp: 92800
Ion Ratio Lower Upper
75 100
53 0.3 72.4 108.6#
89 0.0 43.6 65.4#

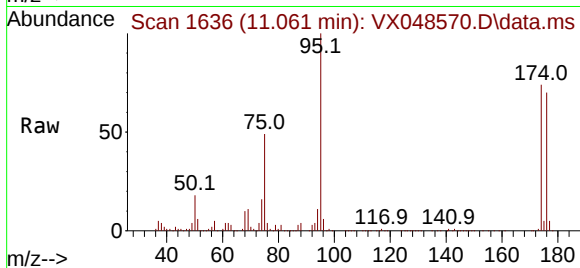

#82
4-Chlorotoluene
Concen: 0.228 ug/l
RT: 11.439 min Scan# 1698
Delta R.T. 0.006 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59

Tgt Ion: 91 Resp: 2905
Ion Ratio Lower Upper
91 100
126 10.5 14.9 44.7#

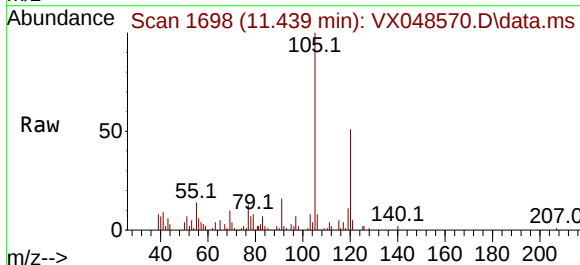



#84

1,2,4-Trimethylbenzene

Concen: 5.376 ug/l

RT: 11.732 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX048570.D

Acq: 12 Nov 2025 11:59

Instrument :

MSVOA_X

ClientSampleId :





304641-01 Liquid

Tgt Ion:105 Resp: 67514

Ion Ratio Lower Upper

105 100

120 46.1 22.4 67.0



#89

n-Butylbenzene

Concen: 1.007 ug/l

RT: 12.311 min Scan# 1841

Delta R.T. -0.000 min

Lab File: VX048570.D

Acq: 12 Nov 2025 11:59




Tgt Ion: 91 Resp: 12631


Ion Ratio Lower Upper

91 100

92 41.4 27.2 81.5

134 69.7 13.0 39.0#









#90
Hexachloroethane
Concen: 0.483 ug/l
RT: 12.518 min Scan# 117
Delta R.T. -0.000 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59




Instrument :
MSVOA_X
ClientSampleId :
304641-01 Liquid


Tgt Ion:117 Resp: 1230
Ion Ratio Lower Upper
117 100
201 0.0 35.9 107.8#

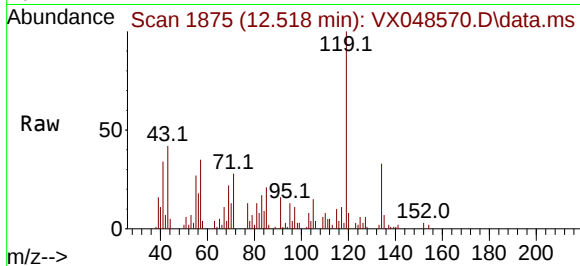

#93
1,2,4-Trichlorobenzene
Concen: 0.228 ug/l
RT: 13.573 min Scan# 2048
Delta R.T. 0.006 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59

Tgt Ion:180 Resp: 1075
Ion Ratio Lower Upper
180 100
182 81.6 47.5 142.6
145 226.1 15.9 47.7#




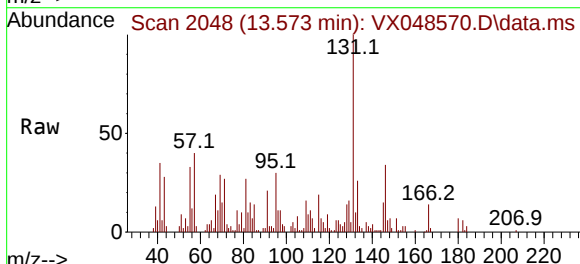




#94
Hexachlorobutadiene
Concen: 0.212 ug/l
RT: 13.701 min Scan# 2070
Delta R.T. -0.006 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59




Instrument :
MSVOA_X
ClientSampleId :
304641-01 Liquid


Tgt Ion:225 Resp: 417
Ion Ratio Lower Upper
225 100
223 70.7 30.6 92.0
227 48.0 32.5 97.4

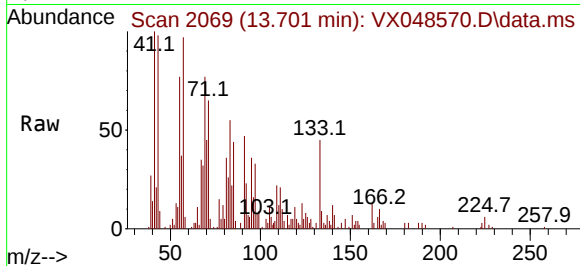

#95
Naphthalene
Concen: 1.824 ug/l
RT: 13.756 min Scan# 2078
Delta R.T. -0.000 min
Lab File: VX048570.D
Acq: 12 Nov 2025 11:59


Tgt Ion:128 Resp: 27645
Ion Ratio Lower Upper
128 100
127 16.3 10.1 15.1#
129 14.5 8.7 13.1#

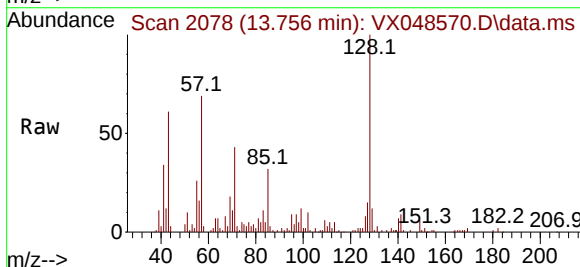



#96
 1,2,3-Trichlorobenzene
 Concen: 0.330 ug/l
 RT: 13.951 min Scan# 21
 Delta R.T. 0.012 min
 Lab File: VX048570.D
 Acq: 12 Nov 2025 11:59

Instrument :
 MSVOA_X
 ClientSampleId :
 304641-01 Liquid



Tgt Ion:180 Resp: 1447
 Ion Ratio Lower Upper
 180 100
 182 56.8 47.3 142.0
 145 160.0 16.7 50.0#

